

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
 Data File : PP035876.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 May 2021 3:01
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 5/14/2021 2:10:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 05:44:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.775	4.196	1088457	1695534	46.454	49.879
2) SA Decachlor...	10.609	9.432	665527	1070902	59.127m	50.640
Target Compounds						
26) L6 AR-1254-1	6.976	6.294	343824	774183	490.914	474.766
27) L6 AR-1254-2	7.204	6.449	536867	680404	487.821	494.882
28) L6 AR-1254-3	7.583	6.867	585766	1035780	495.009	499.041
29) L6 AR-1254-4	7.878	7.104	434806	787773	545.355	542.014
30) L6 AR-1254-5	8.302	7.525	482358	955129	511.189	497.816

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
Data File : PP035876.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 May 2021 3:01
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/14/2021 2:10:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 05:44:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

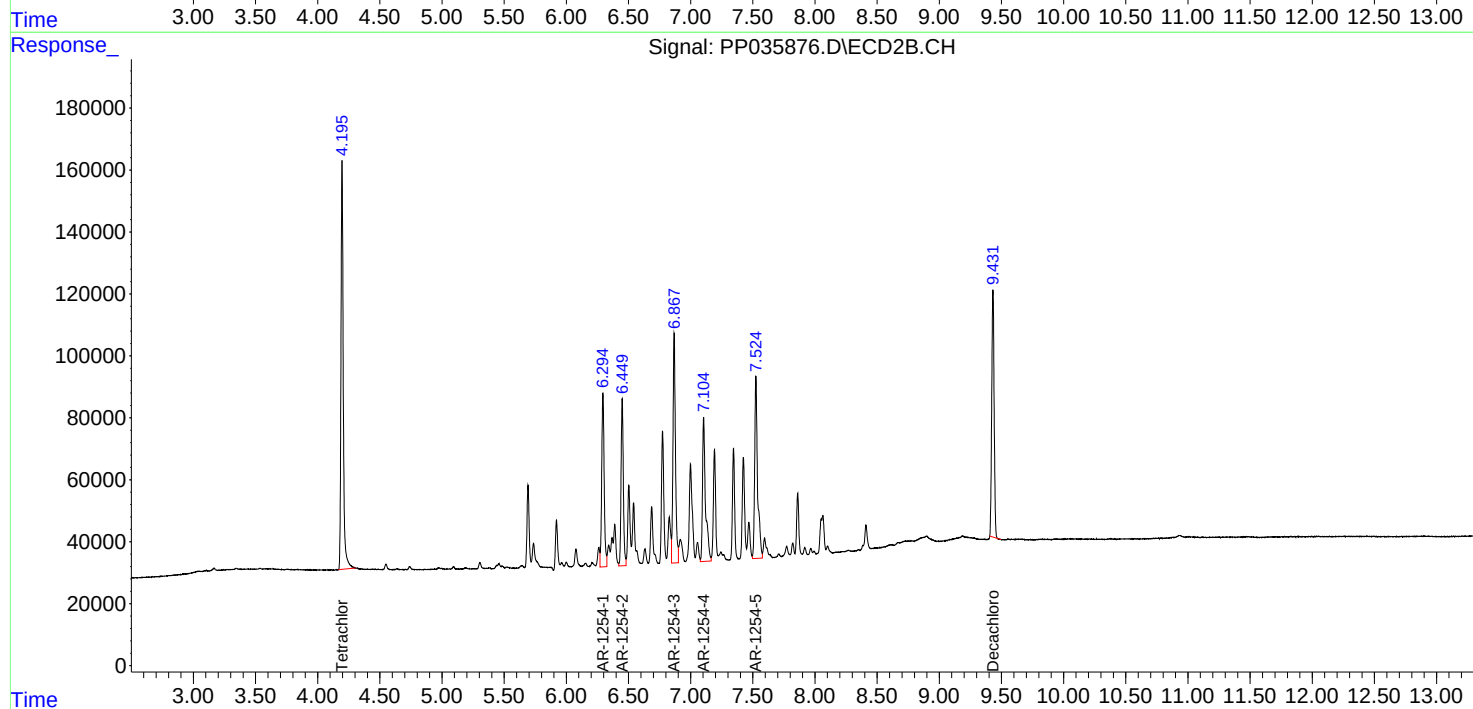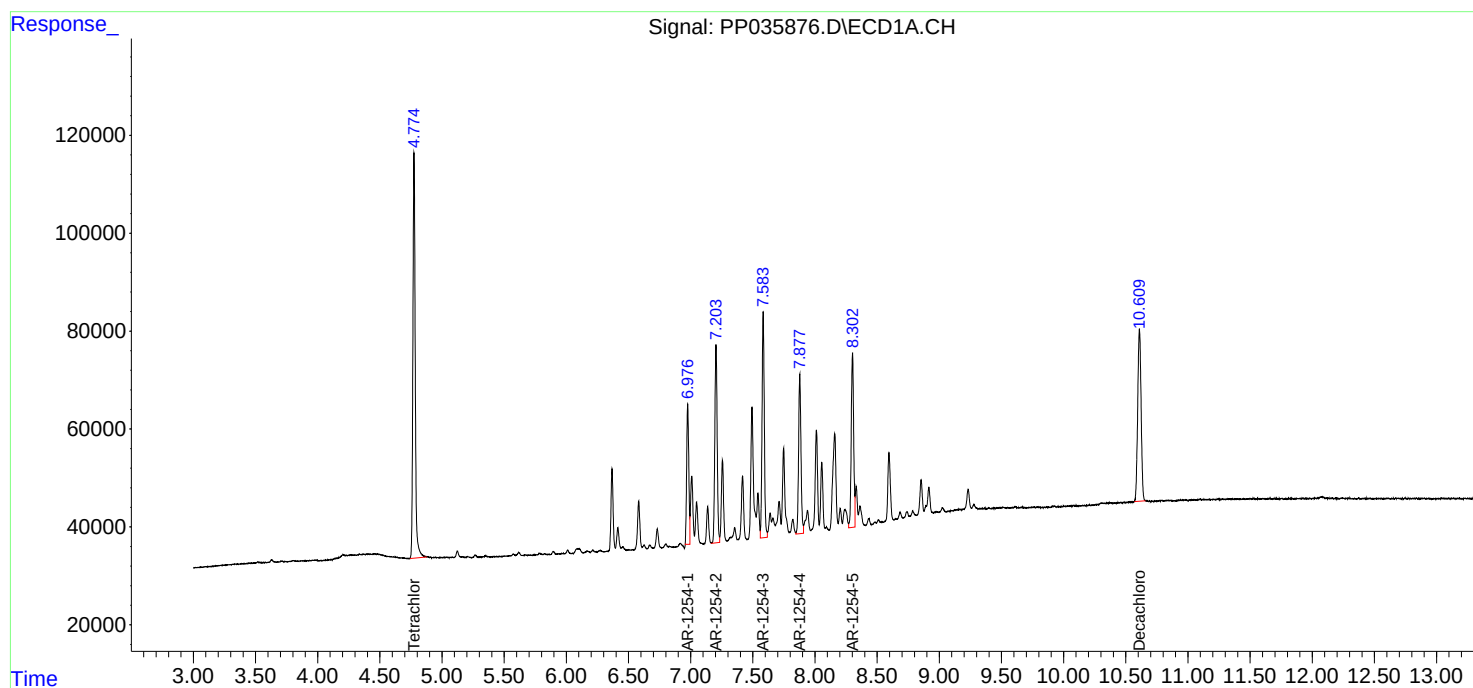

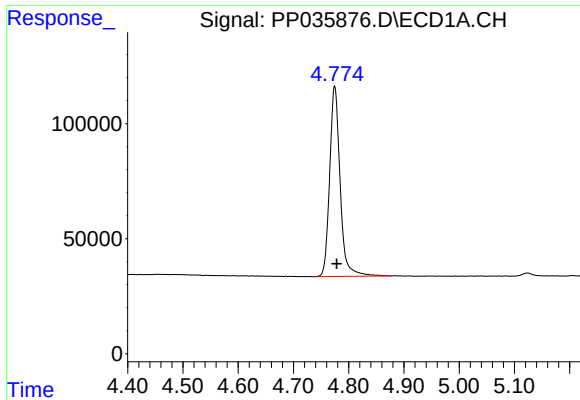


#1 Tetrachloro-m-xylene

R.T.: 4.775 min
Delta R.T.: -0.003 min
Response: 1088457
Conc: 46.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/14/2021 2:10:10 PM

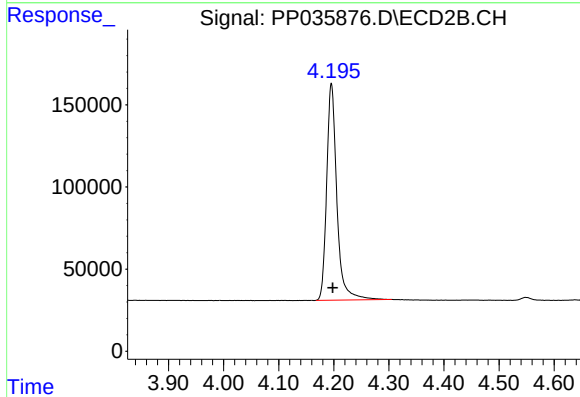


#1 Tetrachloro-m-xylene

R.T.: 4.196 min
Delta R.T.: -0.002 min
Response: 1695534
Conc: 49.88 ng/ml

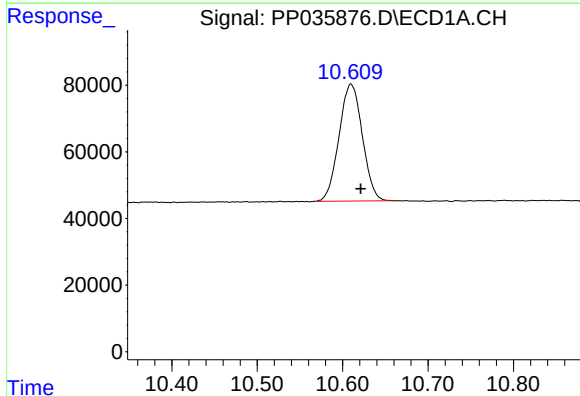


#2 Decachlorobiphenyl

R.T.: 10.609 min
Delta R.T.: -0.012 min
Response: 665527
Conc: 59.13 ng/ml m

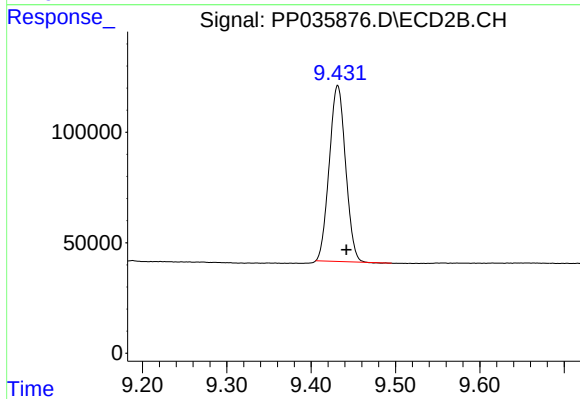

#2 Decachlorobiphenyl

R.T.: 9.432 min
Delta R.T.: -0.010 min
Response: 1070902
Conc: 50.64 ng/ml

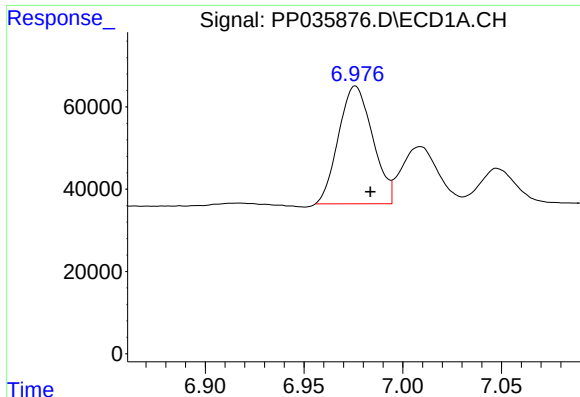


#26 AR-1254-1

R.T.: 6.976 min
Delta R.T.: -0.008 min
Response: 343824
Conc: 490.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/14/2021 2:10:10 PM

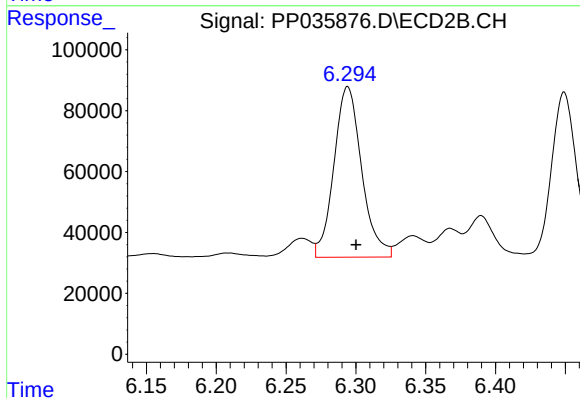


#26 AR-1254-1

R.T.: 6.294 min
Delta R.T.: -0.006 min
Response: 774183
Conc: 474.77 ng/ml

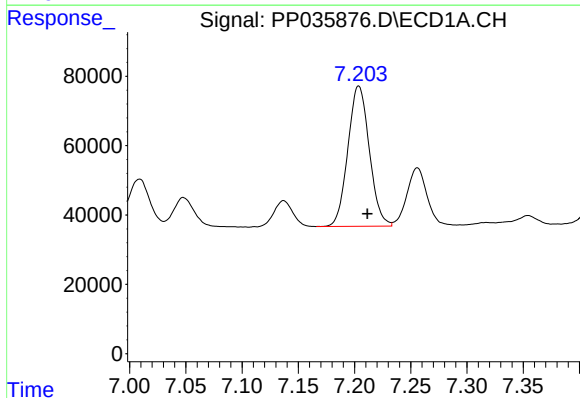


#27 AR-1254-2

R.T.: 7.204 min
Delta R.T.: -0.008 min
Response: 536867
Conc: 487.82 ng/ml

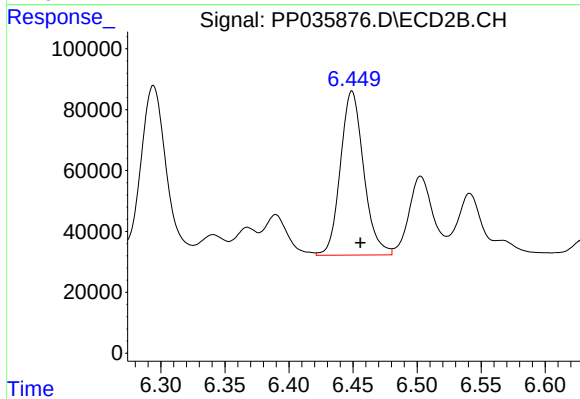

#27 AR-1254-2

R.T.: 6.449 min
Delta R.T.: -0.006 min
Response: 680404
Conc: 494.88 ng/ml

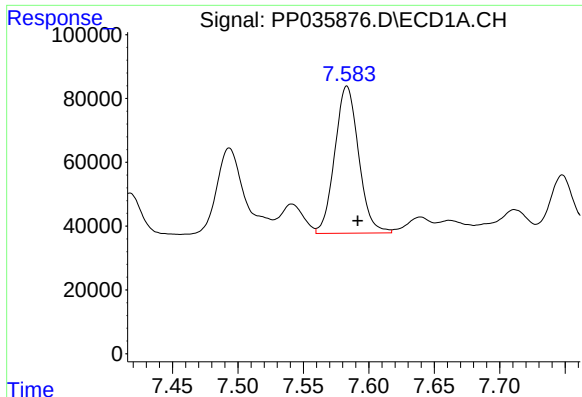


#28 AR-1254-3

R.T.: 7.583 min
Delta R.T.: -0.008 min
Response: 585766
Conc: 495.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/14/2021 2:10:10 PM

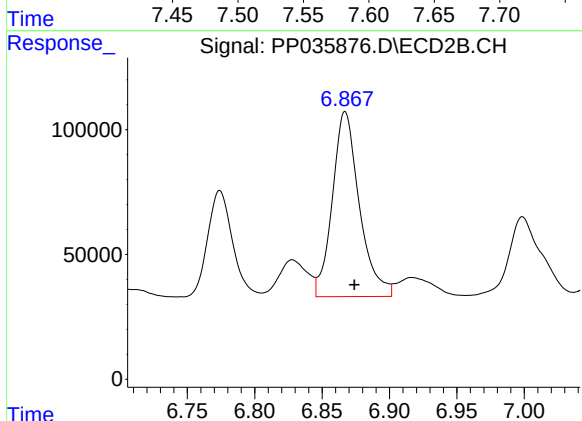


#28 AR-1254-3

R.T.: 6.867 min
Delta R.T.: -0.007 min
Response: 1035780
Conc: 499.04 ng/ml

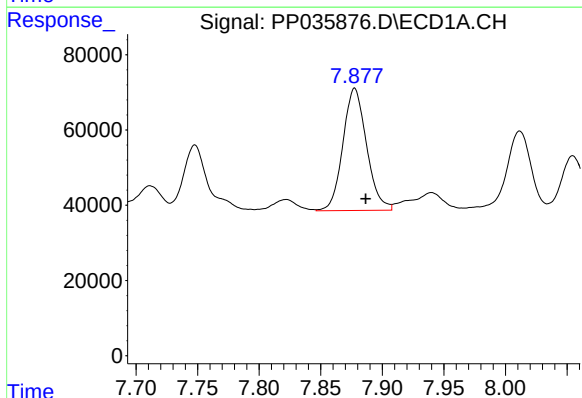


#29 AR-1254-4

R.T.: 7.878 min
Delta R.T.: -0.009 min
Response: 434806
Conc: 545.36 ng/ml

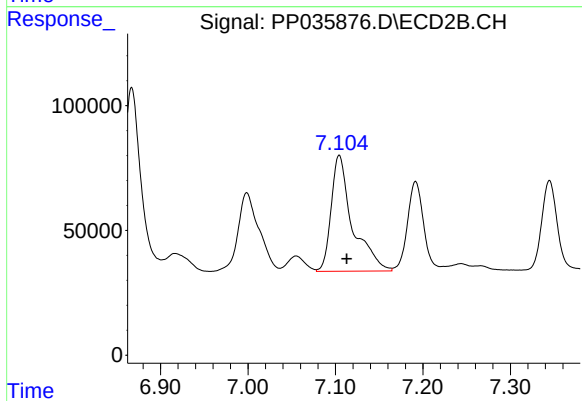

#29 AR-1254-4

R.T.: 7.104 min
Delta R.T.: -0.009 min
Response: 787773
Conc: 542.01 ng/ml

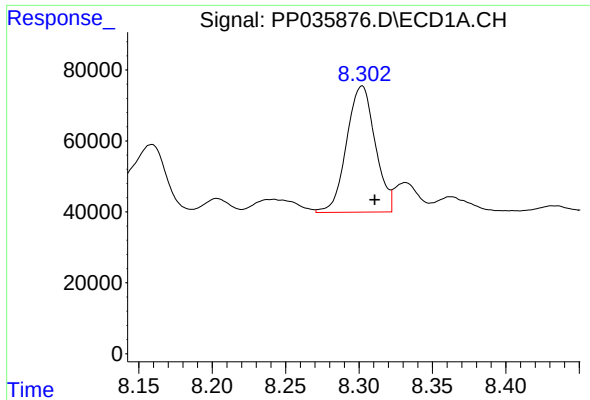


#30 AR-1254-5

R.T.: 8.302 min
Delta R.T.: -0.009 min
Response: 482358
Conc: 511.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
5/14/2021 2:10:10 PM

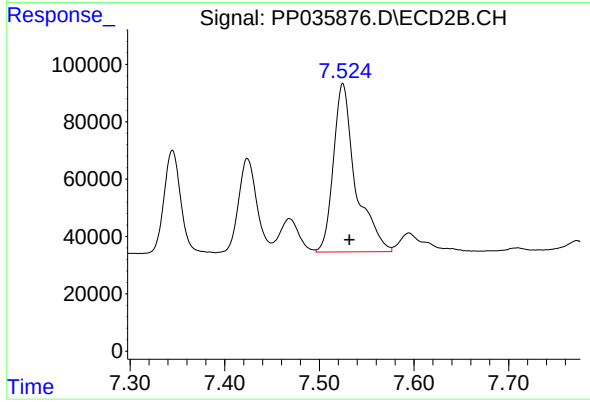

#30 AR-1254-5

R.T.: 7.525 min
Delta R.T.: -0.007 min
Response: 955129
Conc: 497.82 ng/ml