

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
 Data File : PP035889.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 May 2021 6:38
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 5/14/2021 2:10:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 07:10:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.773	4.195	1123639	1731935	47.956	50.950
2) SA Decachlor...	10.609	9.431	647033	973089	57.484m	46.014
Target Compounds						
26) L6 AR-1254-1	6.975	6.293	317045	735417	452.679	450.993
27) L6 AR-1254-2	7.203	6.448	503745	643694	457.725	468.182
28) L6 AR-1254-3	7.583	6.866	548745	952208	463.724	458.775
29) L6 AR-1254-4	7.878	7.103	393688	694638	493.783	477.934
30) L6 AR-1254-5	8.301	7.524	433954	831167	459.891	433.207

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
Data File : PP035889.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 May 2021 6:38
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/14/2021 2:10:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 07:10:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

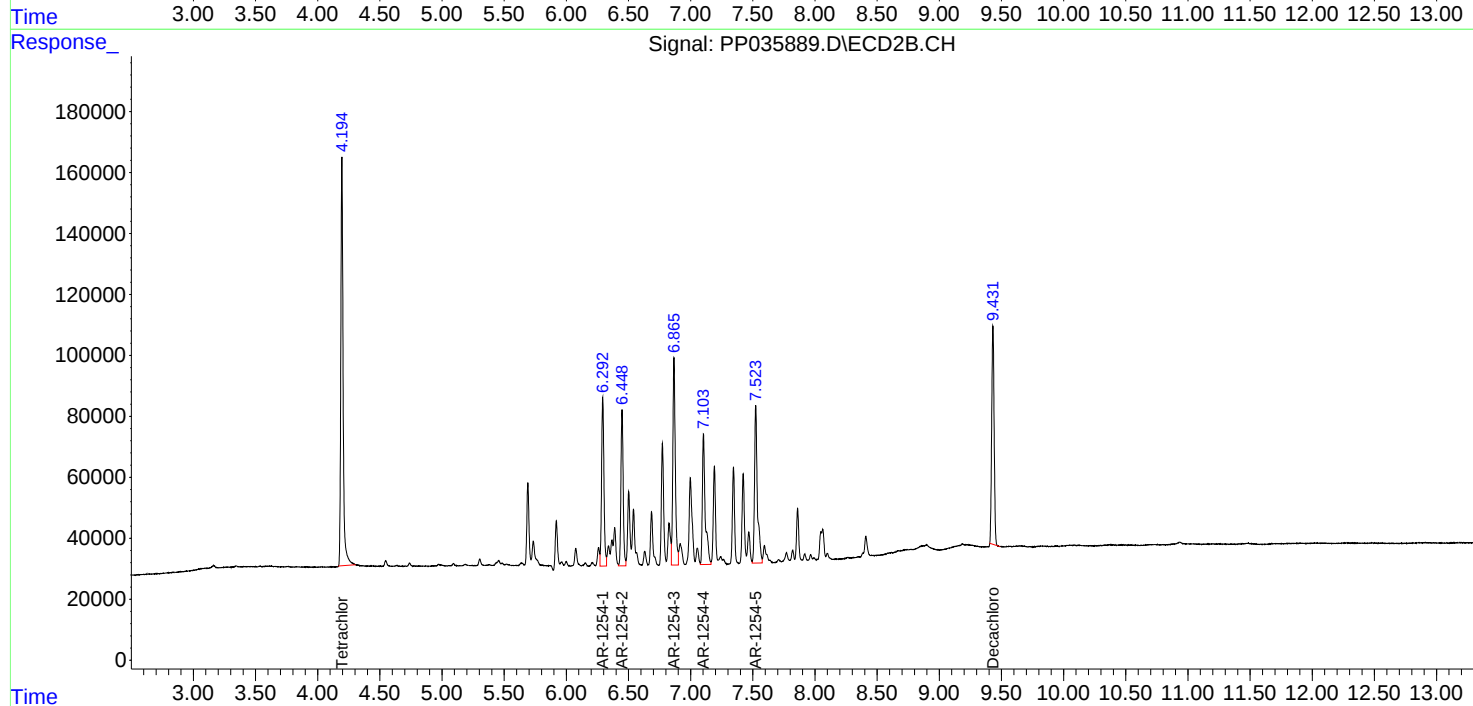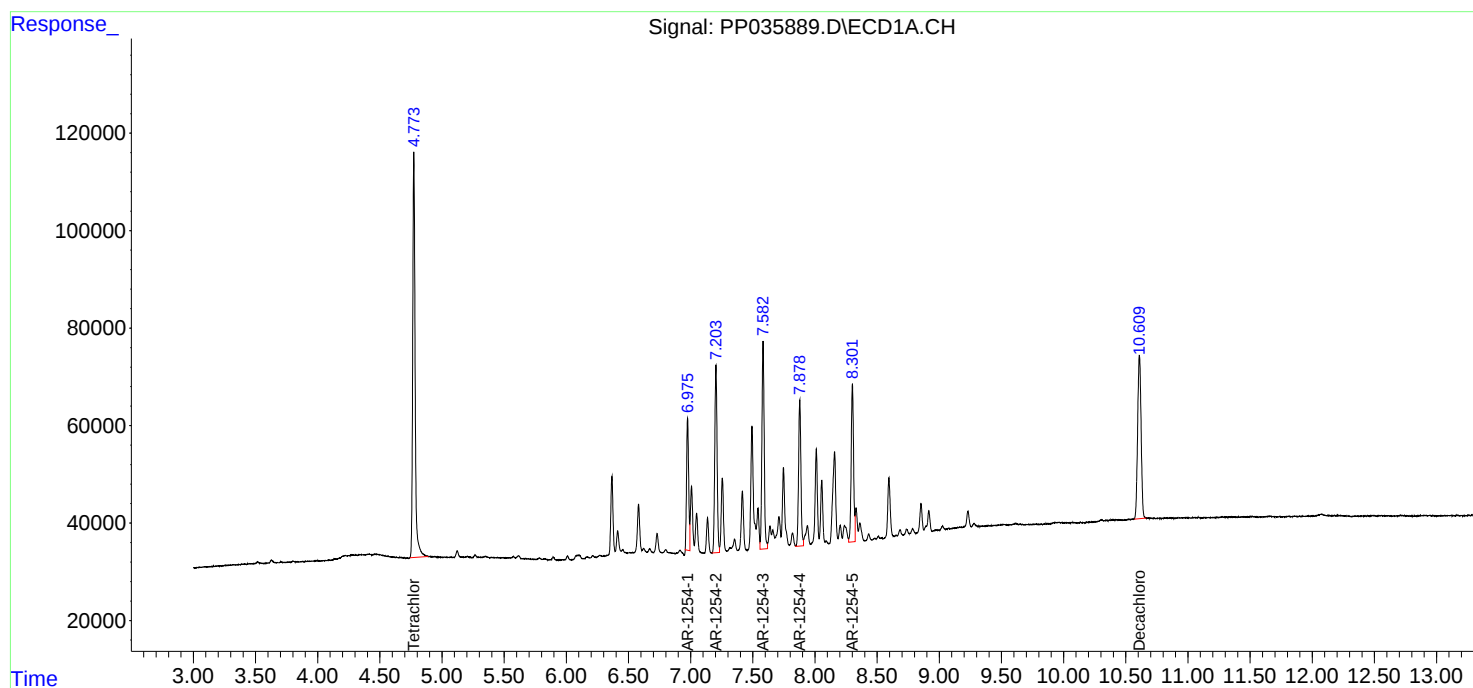

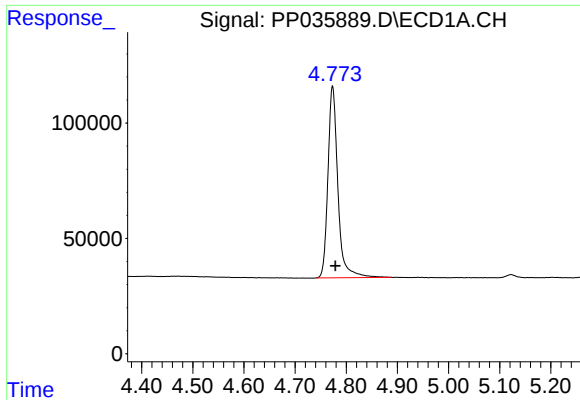


#1 Tetrachloro-m-xylene

R.T.: 4.773 min
Delta R.T.: -0.006 min
Response: 1123639
Conc: 47.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/14/2021 2:10:27 PM

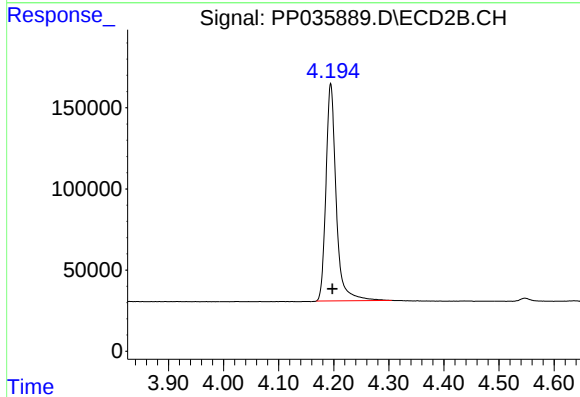


#1 Tetrachloro-m-xylene

R.T.: 4.195 min
Delta R.T.: -0.003 min
Response: 1731935
Conc: 50.95 ng/ml

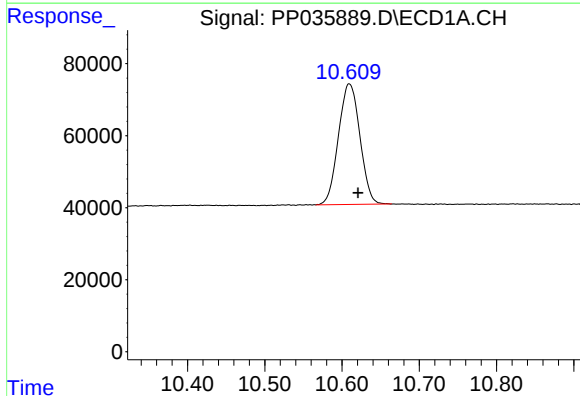


#2 Decachlorobiphenyl

R.T.: 10.609 min
Delta R.T.: -0.012 min
Response: 647033
Conc: 57.48 ng/ml m

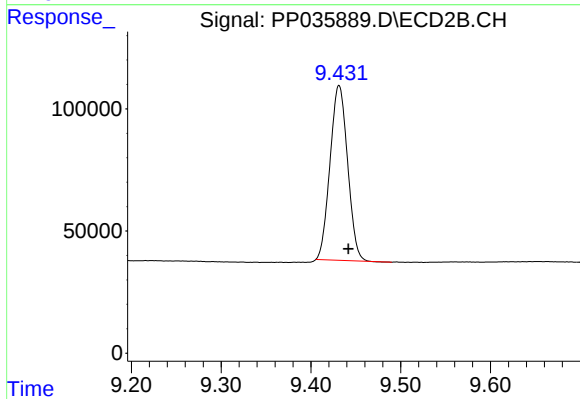

#2 Decachlorobiphenyl

R.T.: 9.431 min
Delta R.T.: -0.010 min
Response: 973089
Conc: 46.01 ng/ml

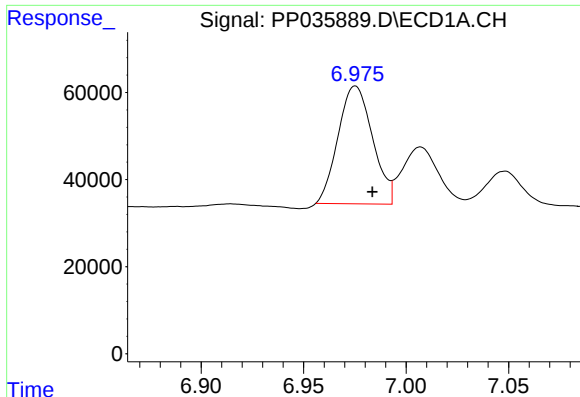


#26 AR-1254-1

R.T.: 6.975 min
Delta R.T.: -0.008 min
Response: 317045
Conc: 452.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/14/2021 2:10:27 PM

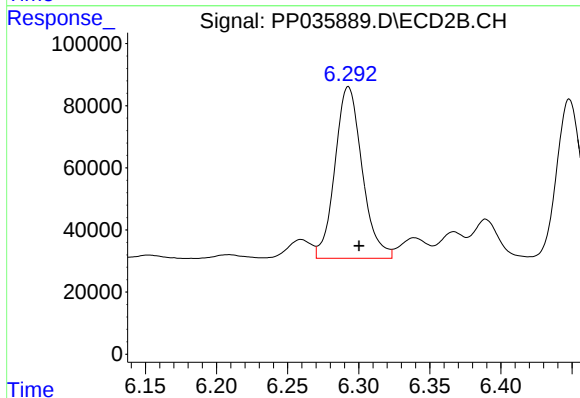


#26 AR-1254-1

R.T.: 6.293 min
Delta R.T.: -0.007 min
Response: 735417
Conc: 450.99 ng/ml

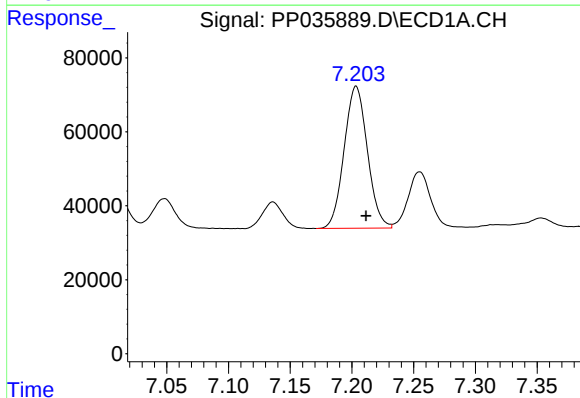


#27 AR-1254-2

R.T.: 7.203 min
Delta R.T.: -0.008 min
Response: 503745
Conc: 457.72 ng/ml

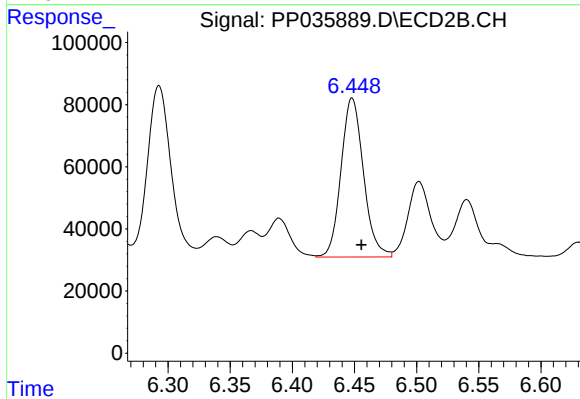

#27 AR-1254-2

R.T.: 6.448 min
Delta R.T.: -0.008 min
Response: 643694
Conc: 468.18 ng/ml

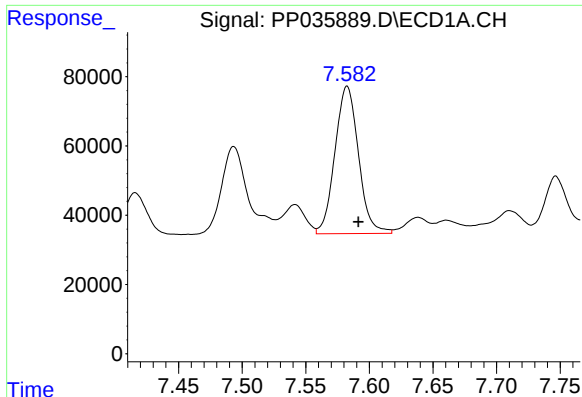


#28 AR-1254-3

R.T.: 7.583 min
Delta R.T.: -0.009 min
Response: 548745
Conc: 463.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
5/14/2021 2:10:27 PM

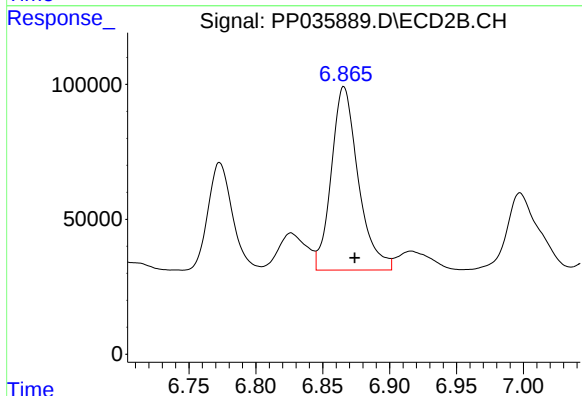


#28 AR-1254-3

R.T.: 6.866 min
Delta R.T.: -0.008 min
Response: 952208
Conc: 458.78 ng/ml

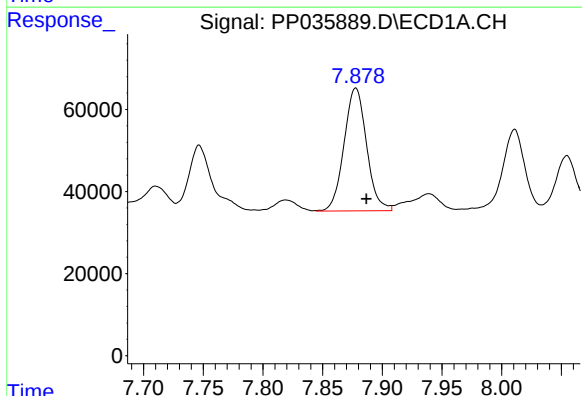


#29 AR-1254-4

R.T.: 7.878 min
Delta R.T.: -0.009 min
Response: 393688
Conc: 493.78 ng/ml

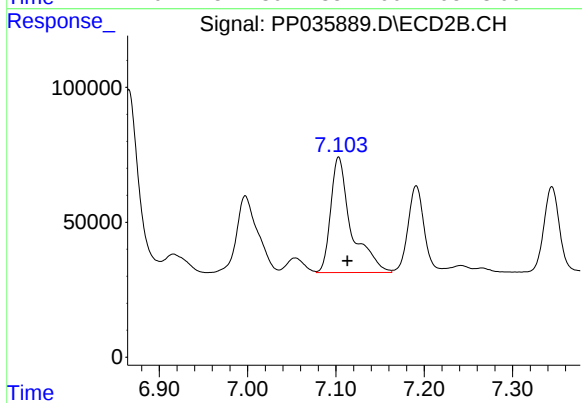

#29 AR-1254-4

R.T.: 7.103 min
Delta R.T.: -0.010 min
Response: 694638
Conc: 477.93 ng/ml

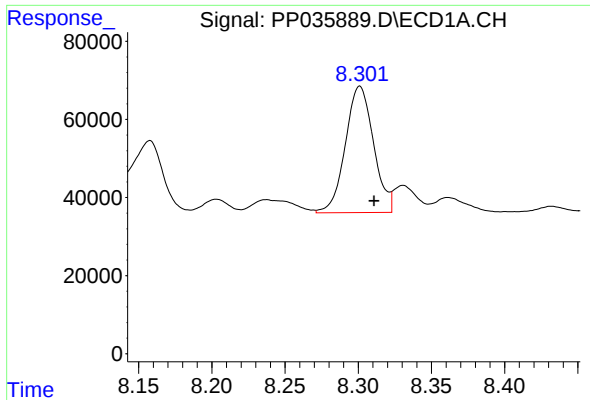


#30 AR-1254-5

R.T.: 8.301 min
Delta R.T.: -0.010 min
Response: 433954
Conc: 459.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
5/14/2021 2:10:27 PM

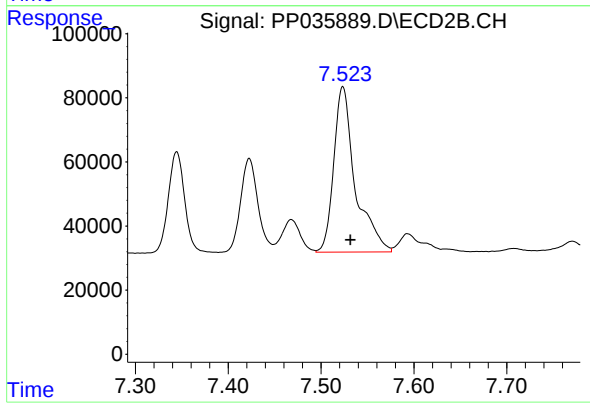

#30 AR-1254-5

R.T.: 7.524 min
Delta R.T.: -0.008 min
Response: 831167
Conc: 433.21 ng/ml