

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
 Data File : PP035891.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 May 2021 7:11
 Operator : DD\AJ
 Sample : PB136387BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB136387BL

Manual Integrations
 APPROVED

Ankita
 5/14/2021 3:50:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 13:01:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.774	4.195	460281	688059	19.644	20.241
2) SA Decachlor...	10.608	9.430	285296	449165	25.346m	21.240m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
Data File : PP035891.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 May 2021 7:11
Operator : DD\AJ
Sample : PB136387BL
Misc :
ALS Vial : 55 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB136387BL


Manual Integrations
APPROVED

Ankita
5/14/2021 3:50:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 13:01:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

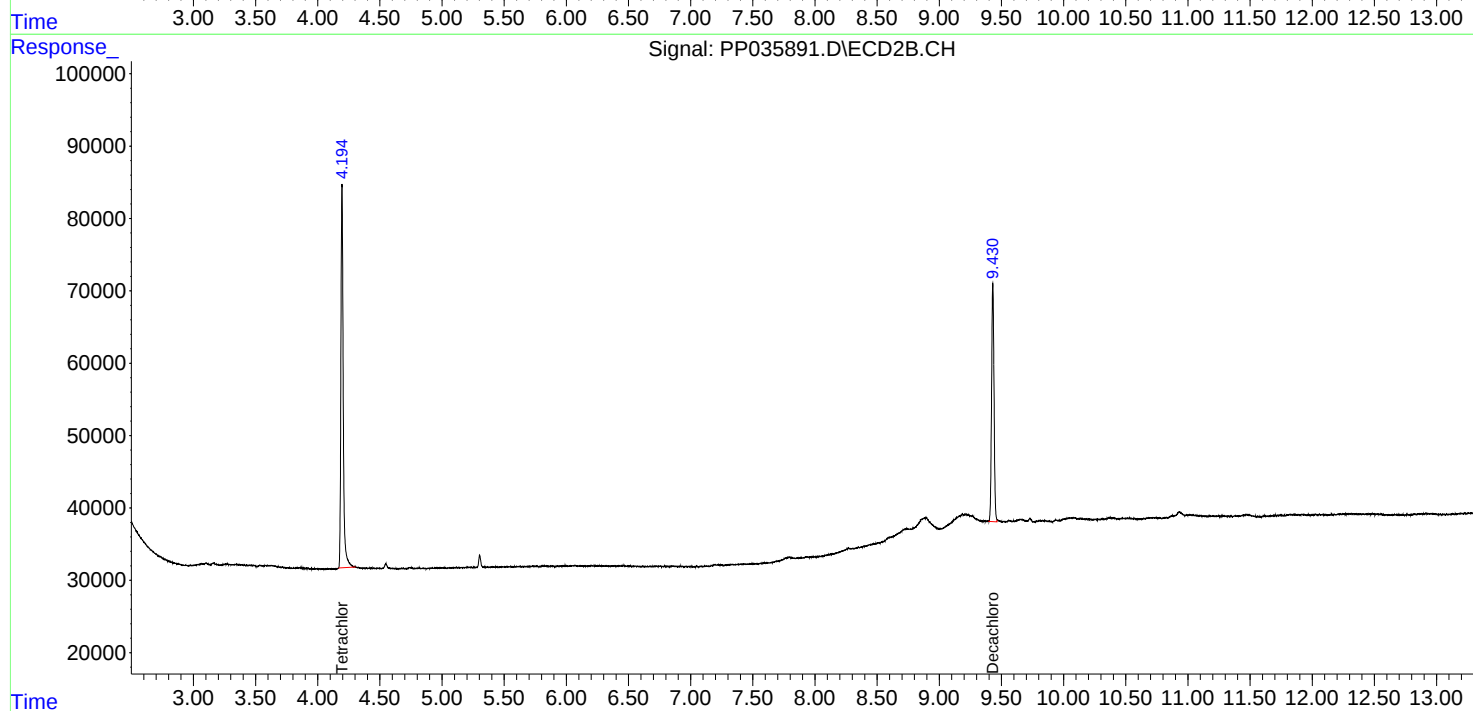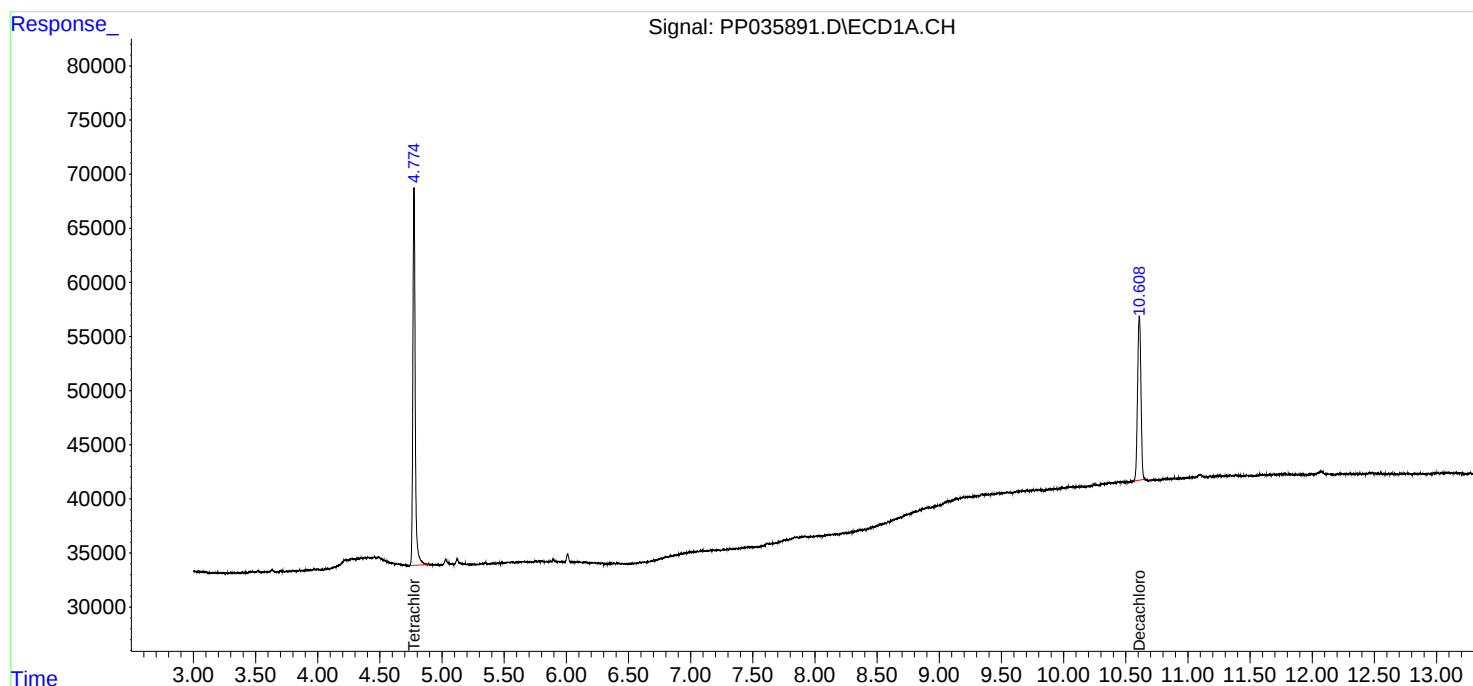

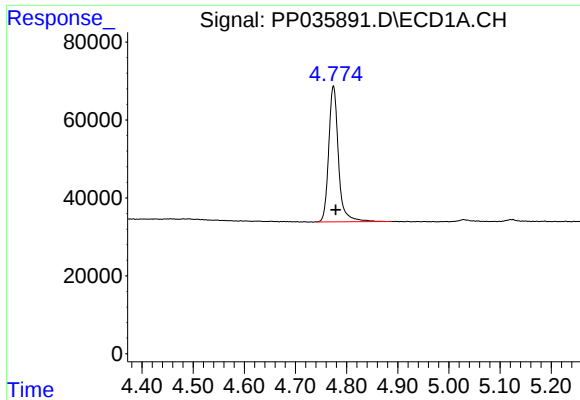


#1 Tetrachloro-m-xylene

R.T.: 4.774 min
Delta R.T.: -0.005 min
Response: 460281
Conc: 19.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB136387BL


Manual Integrations
APPROVED

Ankita
5/14/2021 3:50:00 PM

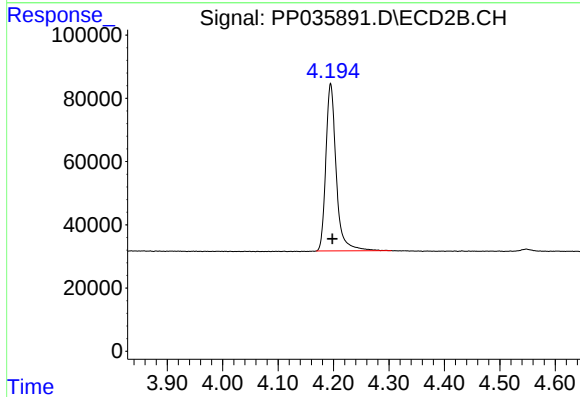


#1 Tetrachloro-m-xylene

R.T.: 4.195 min
Delta R.T.: -0.003 min
Response: 688059
Conc: 20.24 ng/ml

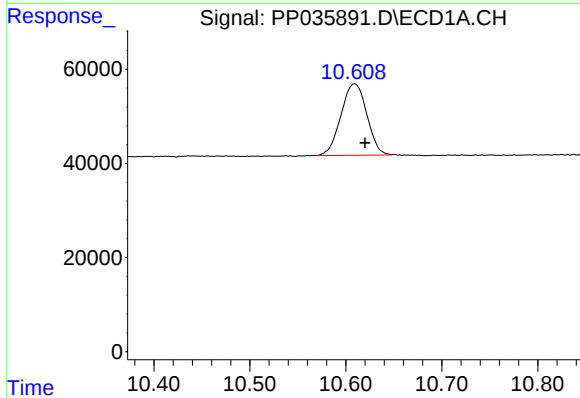

#2 Decachlorobiphenyl

R.T.: 10.608 min
Delta R.T.: -0.012 min
Response: 285296
Conc: 25.35 ng/ml m

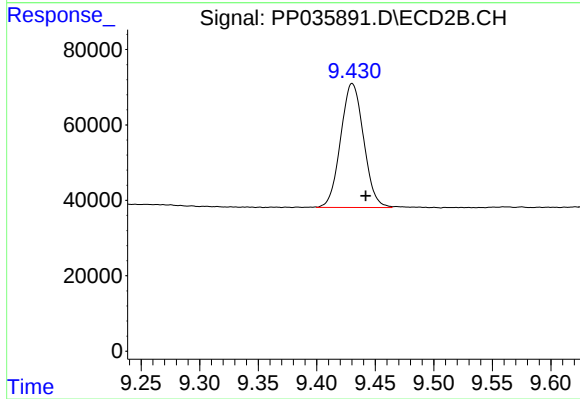

#2 Decachlorobiphenyl

R.T.: 9.430 min
Delta R.T.: -0.012 min
Response: 449165
Conc: 21.24 ng/ml m