

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
 Data File : PP035893.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 May 2021 7:45
 Operator : DD\AJ
 Sample : M2390-01 5X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 01-A-01-B-01-C

Manual Integrations
 APPROVED

Ankita
 5/14/2021 3:50:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 13:02:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.773	4.194	115499	164135	4.929m	4.829
2) SA Decachlor...	10.611	9.449	183346	95783	16.289	4.529m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
Data File : PP035893.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 May 2021 7:45
Operator : DD\AJ
Sample : M2390-01 5X
Misc :
ALS Vial : 57 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
01-A-01-B-01-C


Manual Integrations
APPROVED

Ankita
5/14/2021 3:50:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 13:02:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

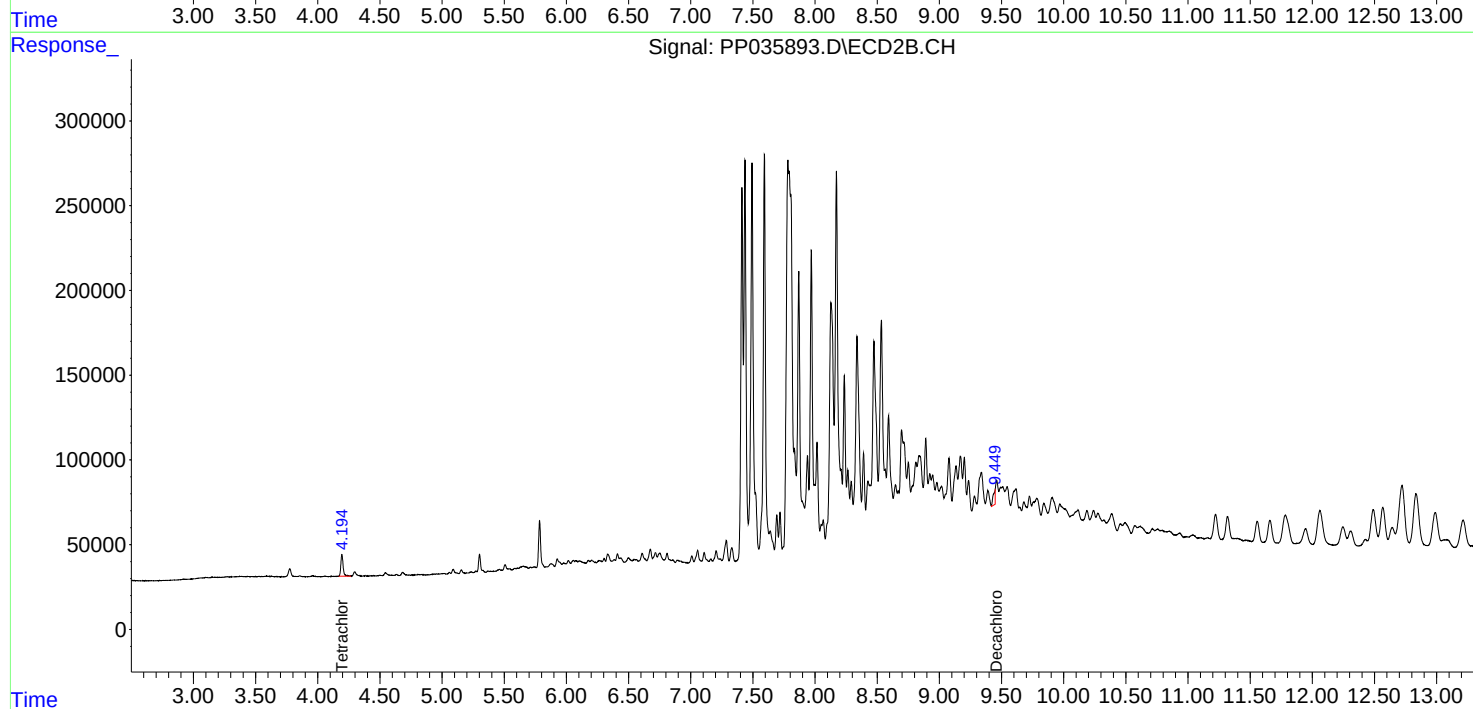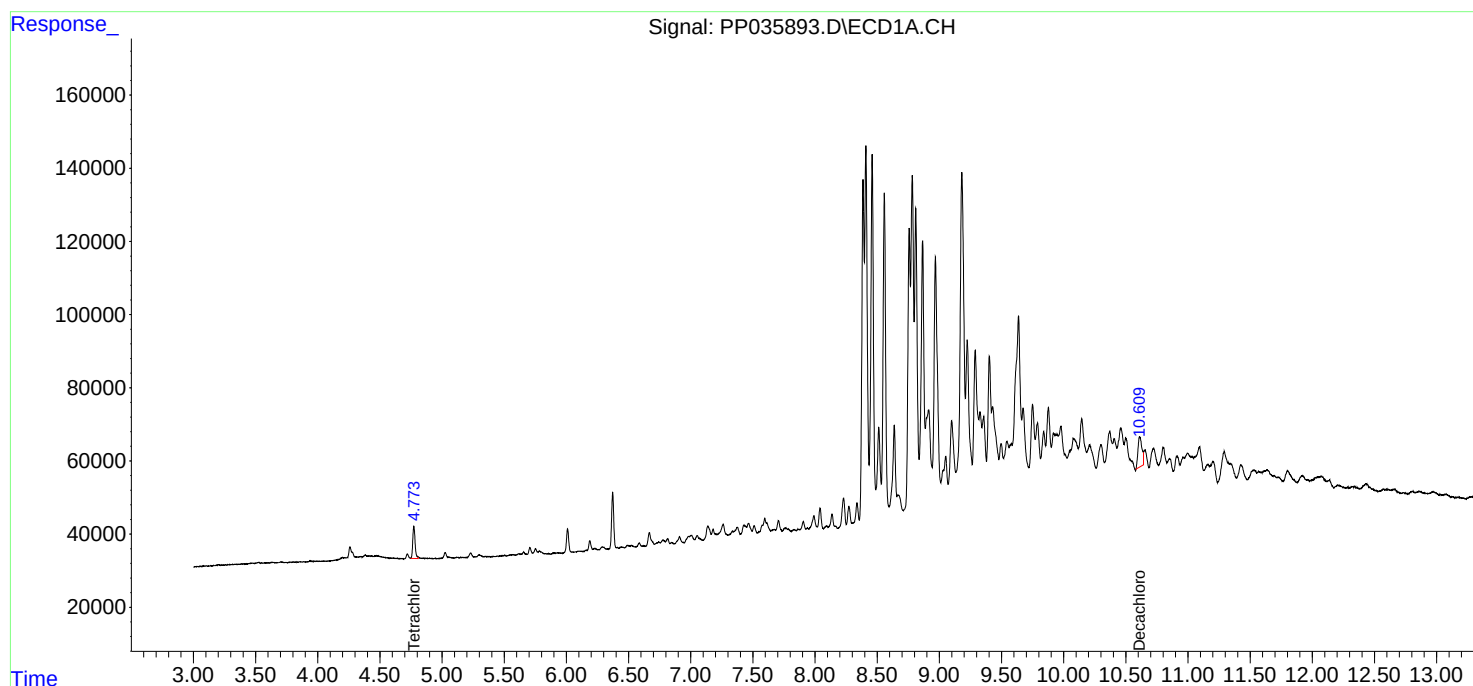

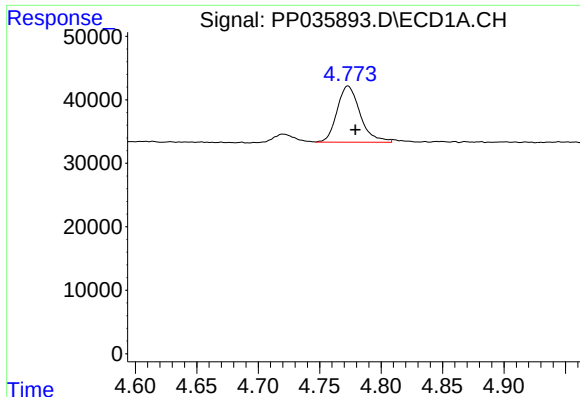


#1 Tetrachloro-m-xylene

R.T.: 4.773 min
Delta R.T.: -0.006 min
Response: 115499
Conc: 4.93 ng/ml m

Instrument :
ECD_P
ClientSampleId :
01-A-01-B-01-C


Manual Integrations
APPROVED

Ankita
5/14/2021 3:50:04 PM

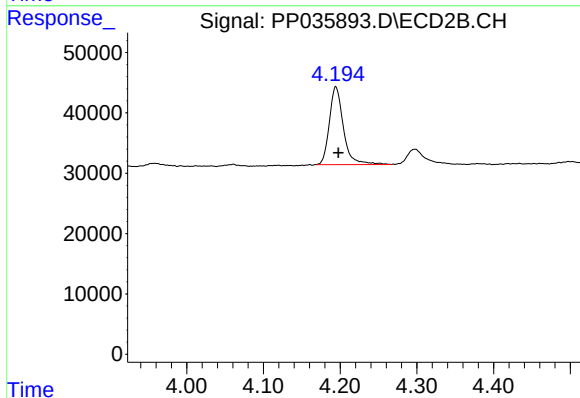


#1 Tetrachloro-m-xylene

R.T.: 4.194 min
Delta R.T.: -0.004 min
Response: 164135
Conc: 4.83 ng/ml

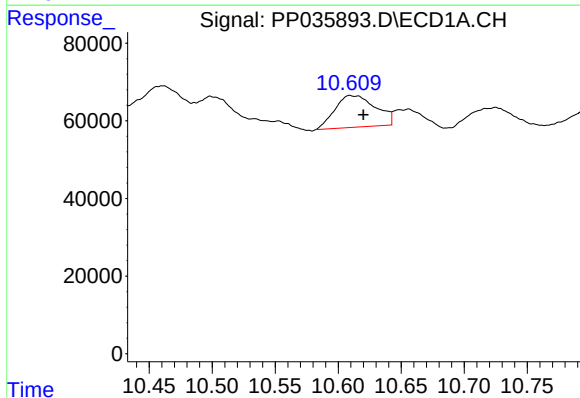

#2 Decachlorobiphenyl

R.T.: 10.611 min
Delta R.T.: -0.009 min
Response: 183346
Conc: 16.29 ng/ml

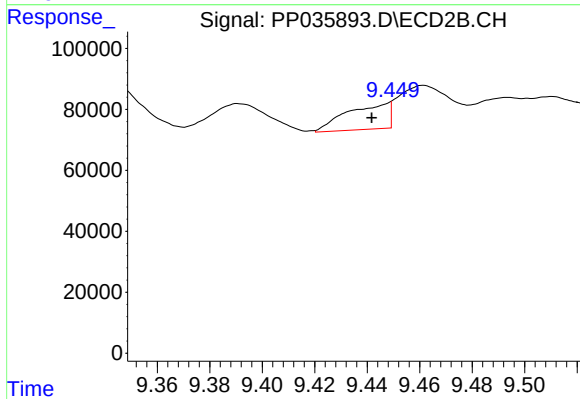

#2 Decachlorobiphenyl

R.T.: 9.449 min
Delta R.T.: 0.007 min
Response: 95783
Conc: 4.53 ng/ml m