

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
 Data File : PP035895.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 May 2021 8:18
 Operator : DD\AJ
 Sample : M2390-03 5X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 03-A-03-B-03-C

Manual Integrations
 APPROVED

Ankita
 5/14/2021 3:50:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 13:05:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.773	4.194	110252	176011	4.705	5.178
2) SA Decachlor...	10.609	9.430	55678	114566	4.947	5.417m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051321\
Data File : PP035895.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 May 2021 8:18
Operator : DD\AJ
Sample : M2390-03 5X
Misc :
ALS Vial : 59 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
5/14/2021 3:50:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 13:05:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

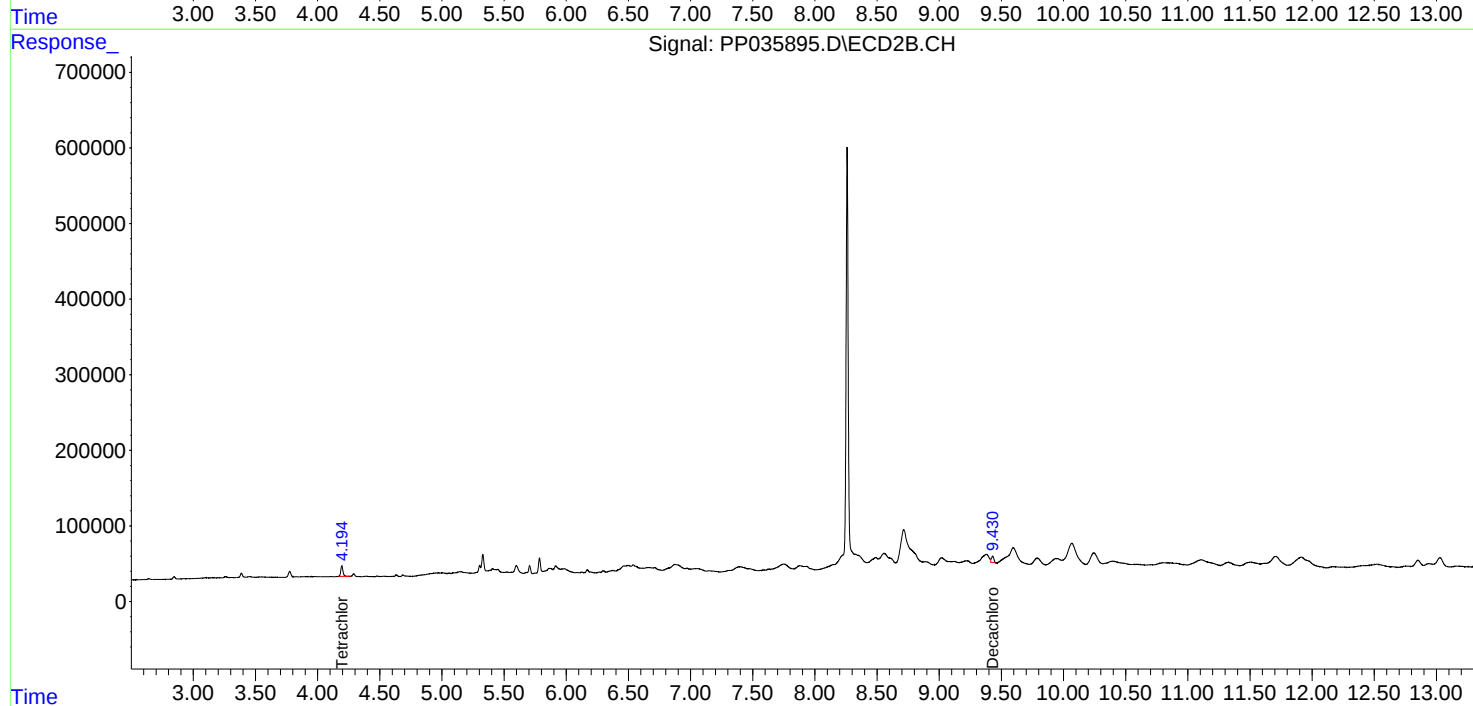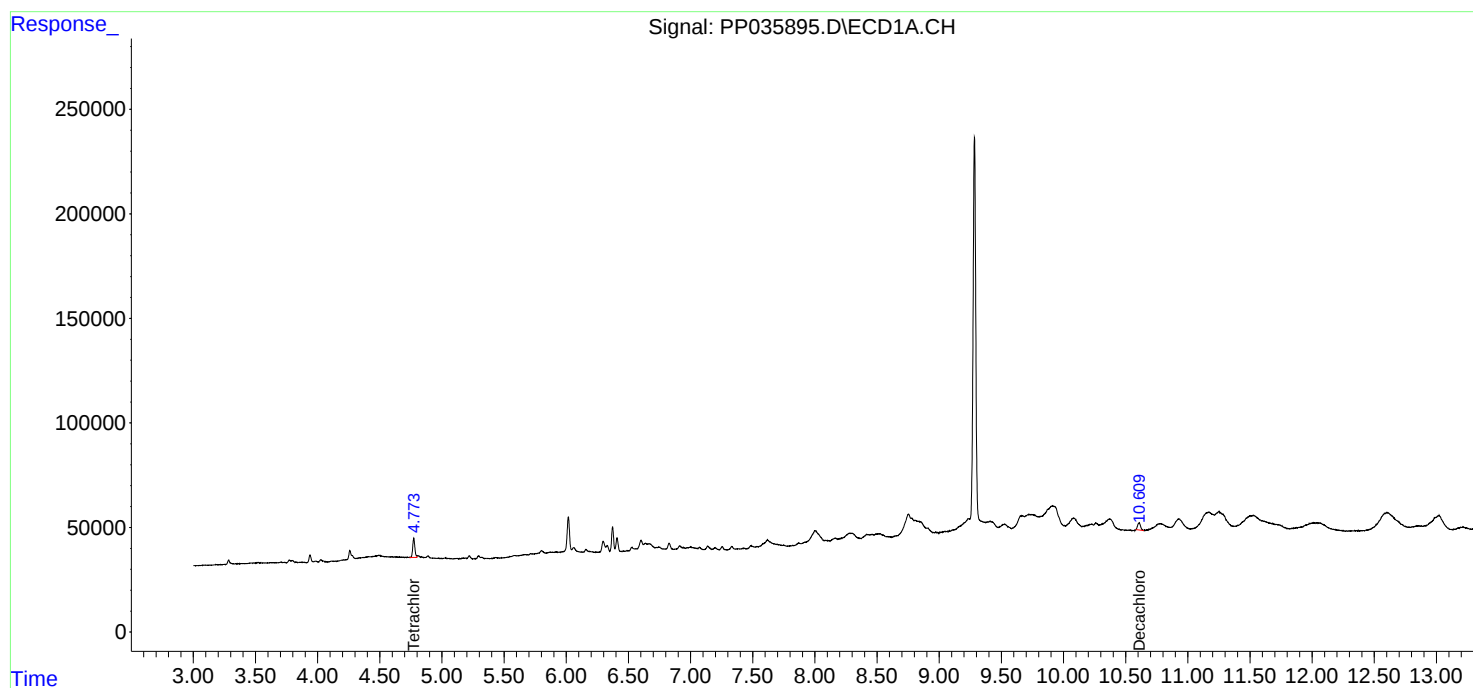

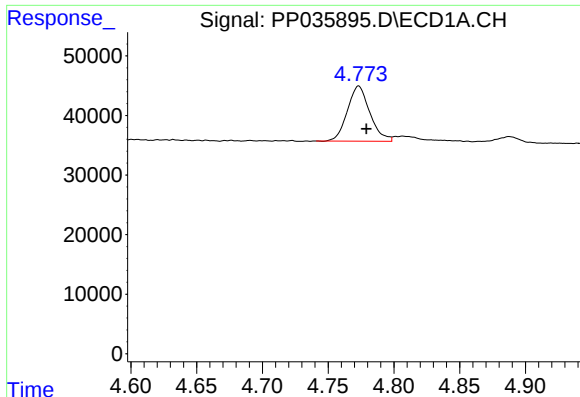


#1 Tetrachloro-m-xylene

R.T.: 4.773 min
Delta R.T.: -0.006 min
Response: 110252
Conc: 4.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
5/14/2021 3:50:07 PM

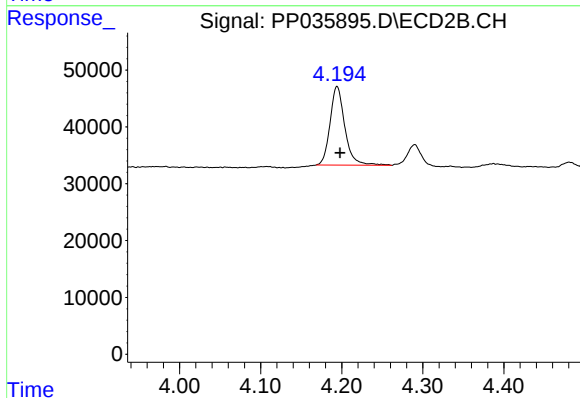


#1 Tetrachloro-m-xylene

R.T.: 4.194 min
Delta R.T.: -0.004 min
Response: 176011
Conc: 5.18 ng/ml

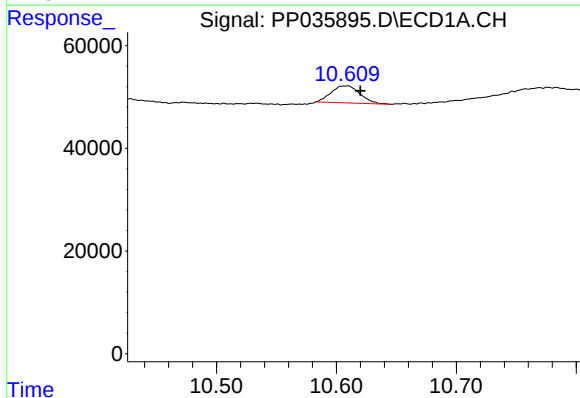

#2 Decachlorobiphenyl

R.T.: 10.609 min
Delta R.T.: -0.011 min
Response: 55678
Conc: 4.95 ng/ml

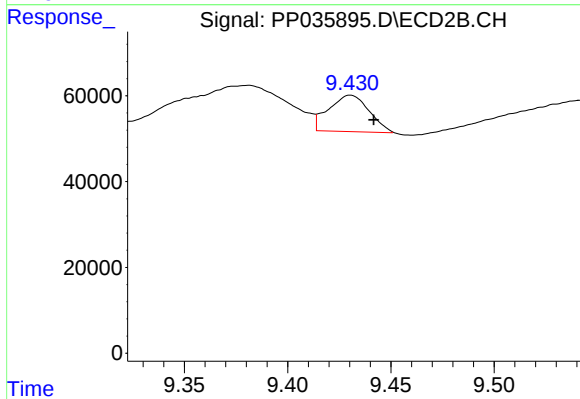

#2 Decachlorobiphenyl

R.T.: 9.430 min
Delta R.T.: -0.012 min
Response: 114566
Conc: 5.42 ng/ml m