

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051325\
 Data File : PP072016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2025 14:56
 Operator : YP\AJ
 Sample : Q2001-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-A1-05-C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/14/2025
 Supervised By :mohammad ahmed 05/16/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 22:54:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042225.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 23 05:02:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.500	3.802	44643383	25223650	22.517m	17.906m
2) SA Decachlor...	10.216	8.825	17217723	15547686	11.891	17.727m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051325\
Data File : PP072016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2025 14:56
Operator : YP\AJ
Sample : Q2001-06
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WC-A1-05-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/14/2025
Supervised By :mohammad ahmed 05/16/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 22:54:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042225.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 23 05:02:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

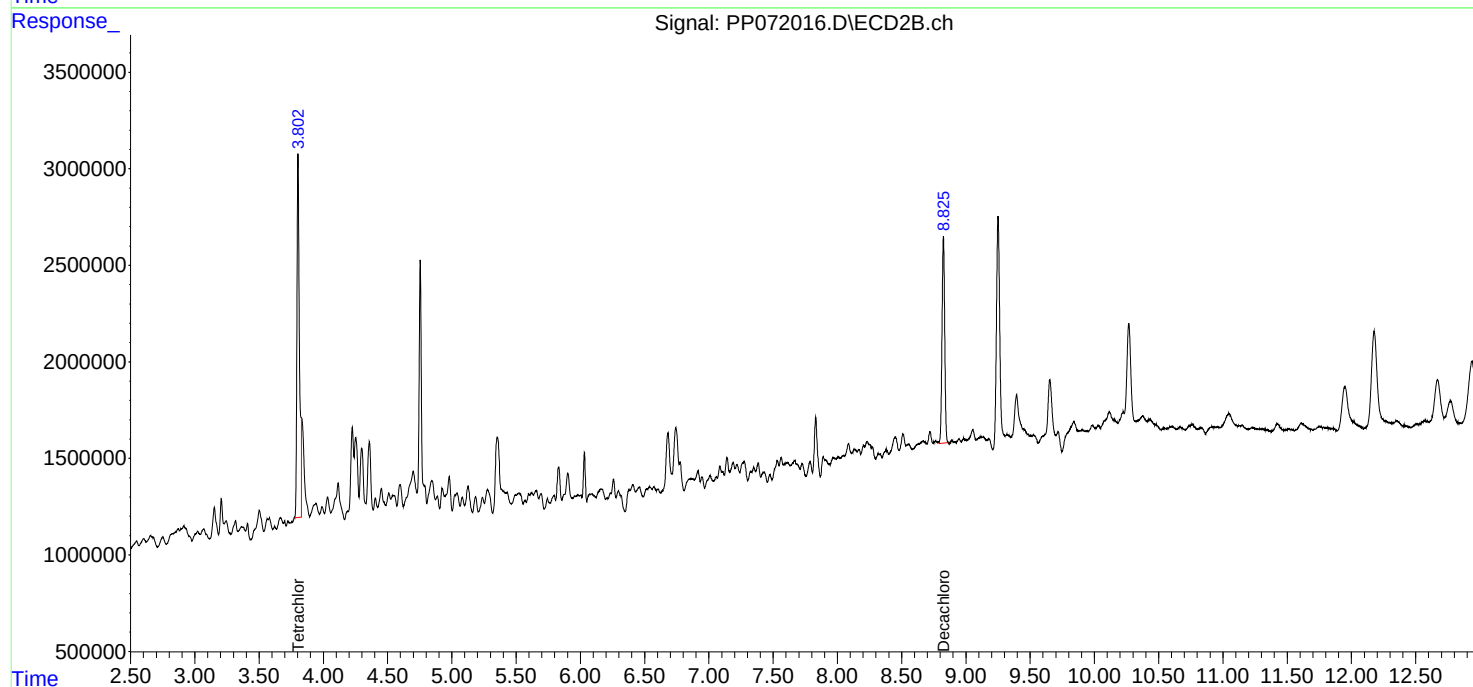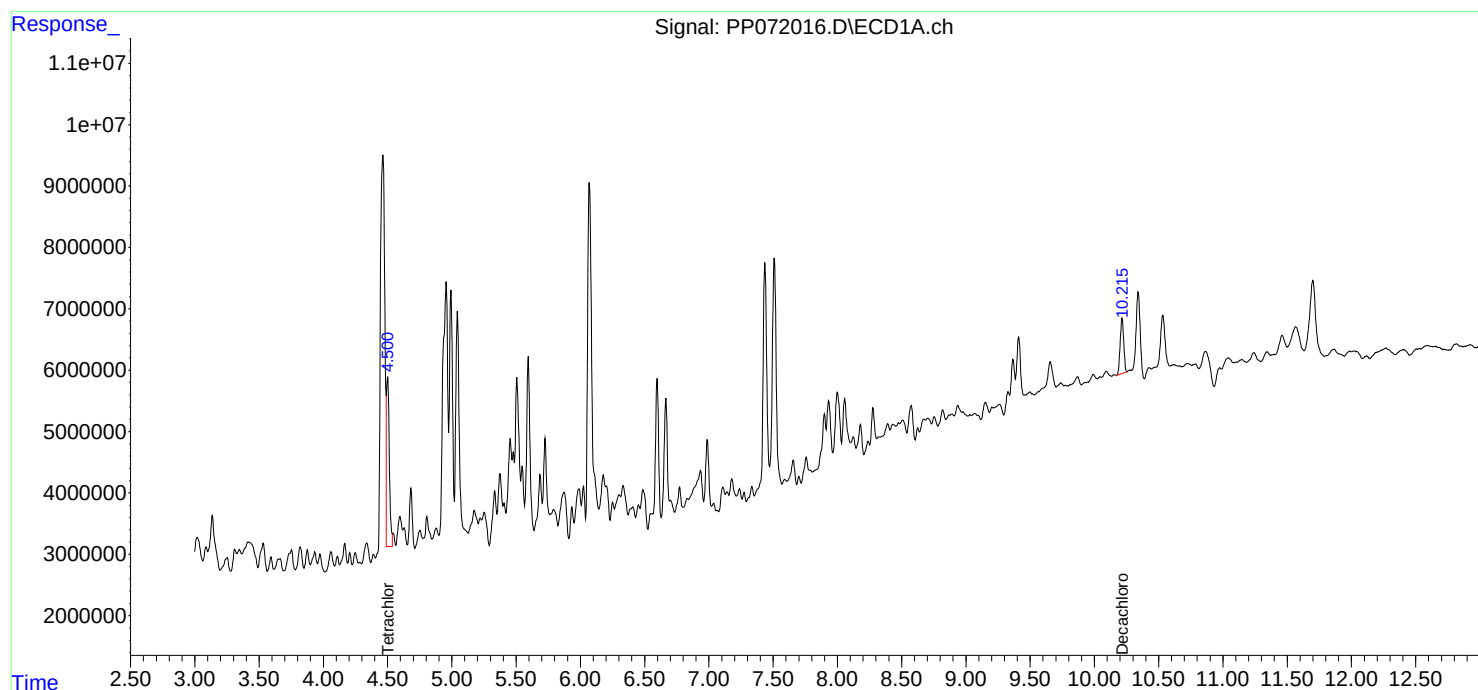

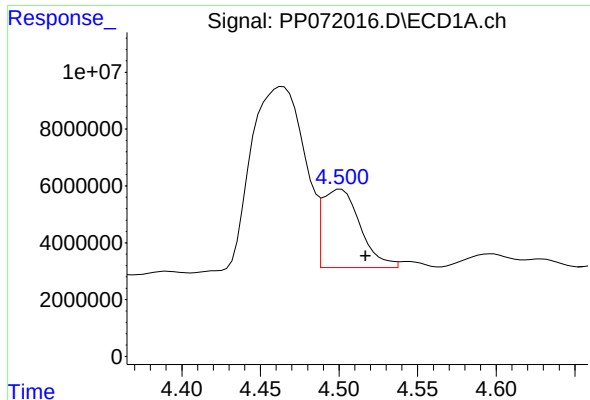

#1 Tetrachloro-m-xylene

R.T.: 4.500 min
Delta R.T.: -0.017 min
Response: 44643383
Conc: 22.52 ng/ml

Instrument :


ECD_P

ClientSampleId :

WC-A1-05-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/14/2025
Supervised By :mohammad ahmed 05/16/2025

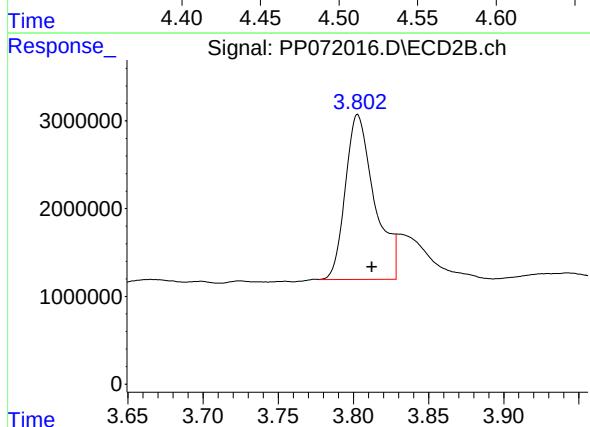


#1 Tetrachloro-m-xylene

R.T.: 3.802 min
Delta R.T.: -0.010 min
Response: 25223650
Conc: 17.91 ng/ml

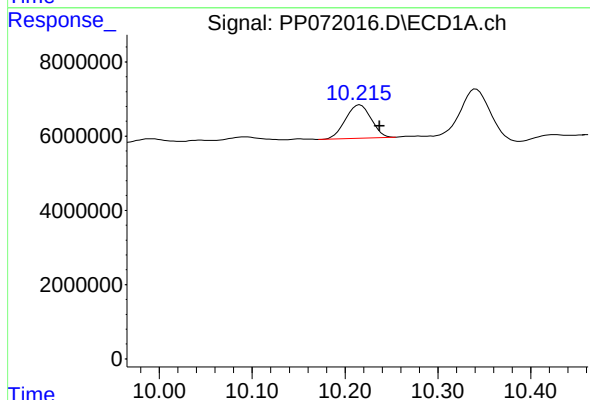

#2 Decachlorobiphenyl

R.T.: 10.216 min
Delta R.T.: -0.021 min
Response: 17217723
Conc: 11.89 ng/ml

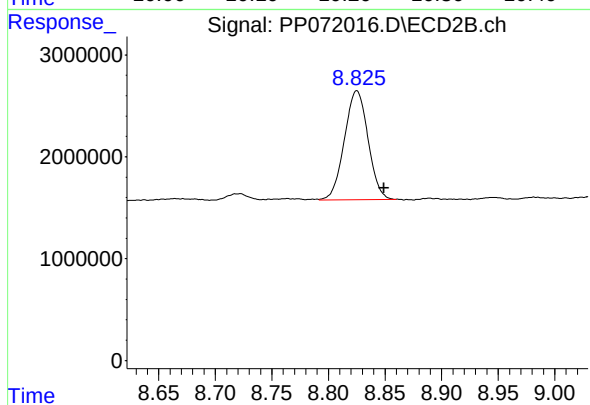

#2 Decachlorobiphenyl

R.T.: 8.825 min
Delta R.T.: -0.024 min
Response: 15547686
Conc: 17.73 ng/ml