

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051421\
 Data File : PP035911.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 May 2021 16:03
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 01:30:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.777	4.194	469617	679074	20.043	19.977
2)	SA Decachlor...	10.612	9.431	264318	408703	23.483	19.326
Target Compounds							
9)	L2 AR-1221-2	5.124	0.000	7077	0	31.536	N.D. #
24)	L5 AR-1248-4	7.010	0.000	5183	0	7.718	N.D. #
26)	L6 AR-1254-1	6.982	0.000	8572	0	12.239	N.D. #
28)	L6 AR-1254-3	7.615f	0.000	16064	0	13.575	N.D. #
29)	L6 AR-1254-4	7.875	0.000	8792	0	11.027	N.D. #
32)	L7 AR-1260-2	8.012	0.000	7058	0	7.245	N.D. #
40)	L8 AR-1262-5	0.000	8.895	0	10133	N.D.	9.711 #
44)	L9 AR-1268-4	0.000	8.895f	0	10133	N.D.	8.701 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051421\
Data File : PP035911.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 May 2021 16:03
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 01:30:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

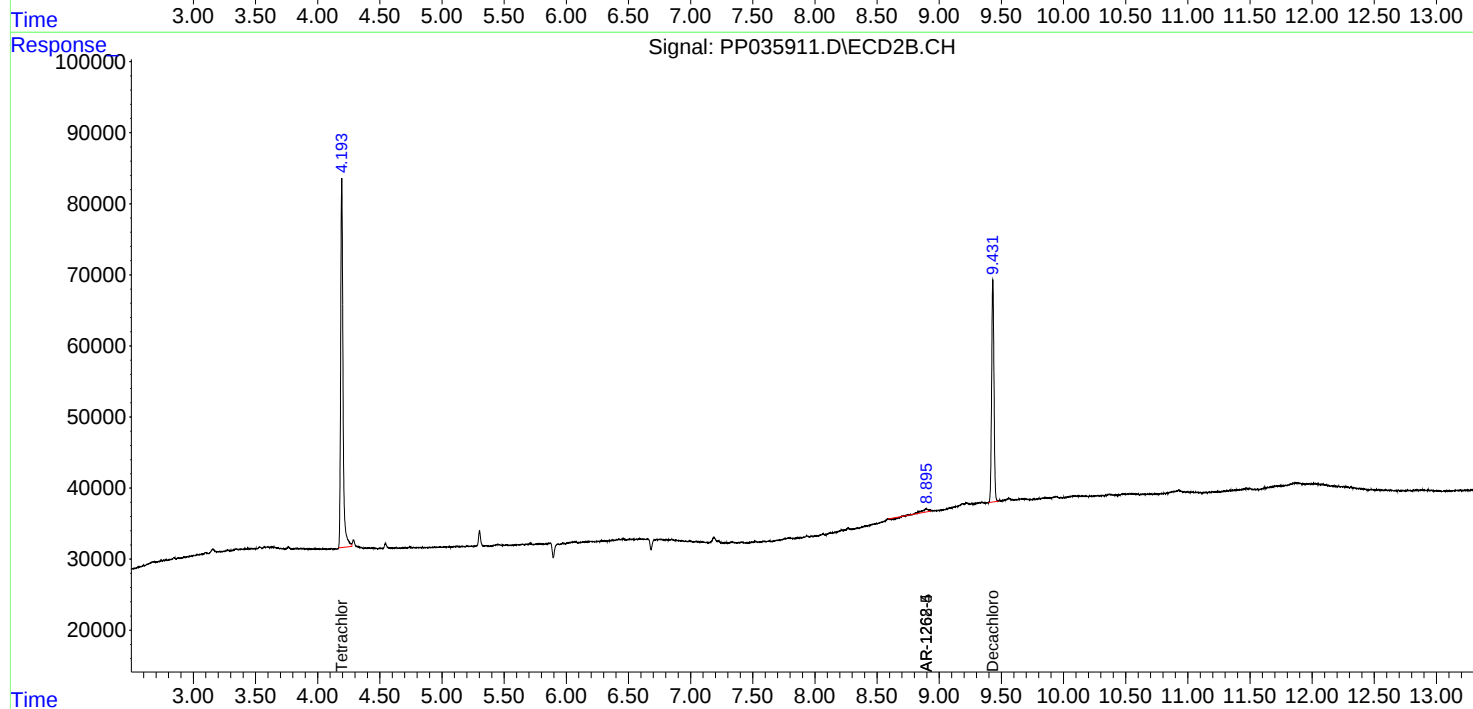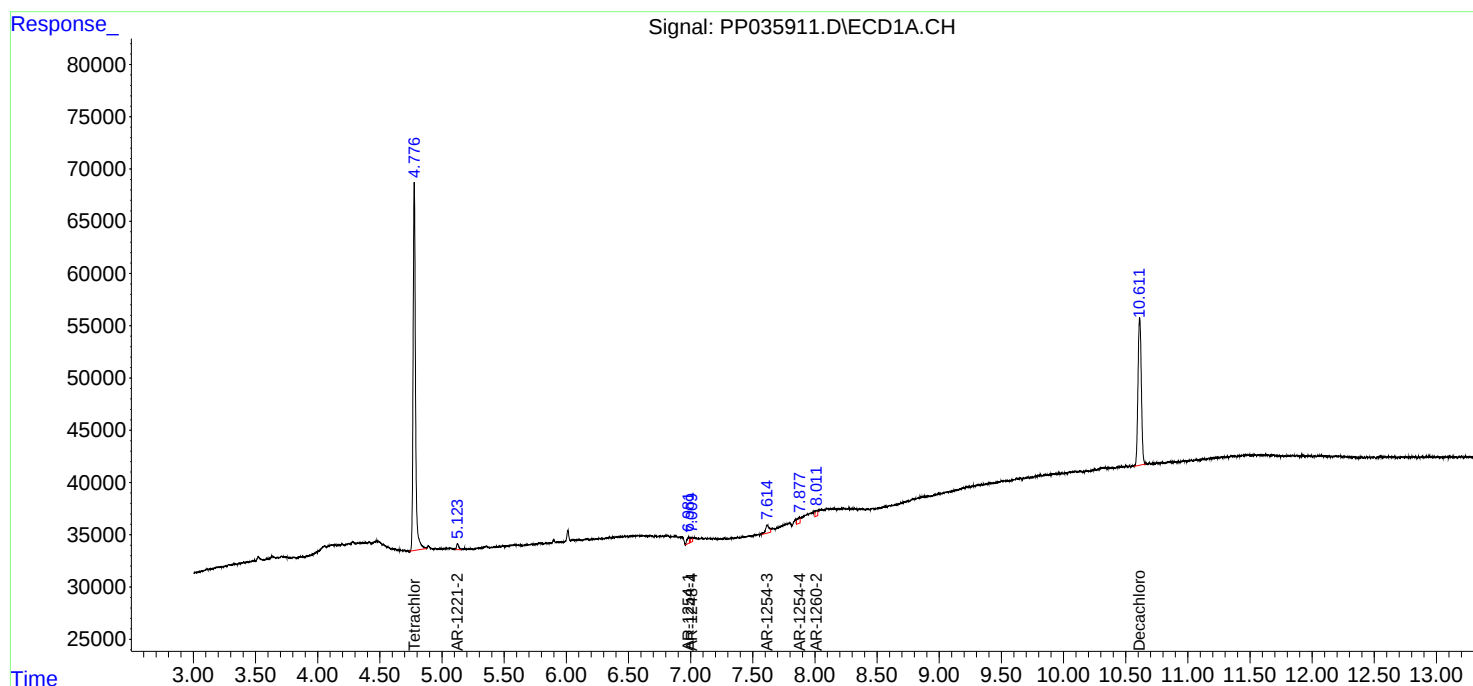


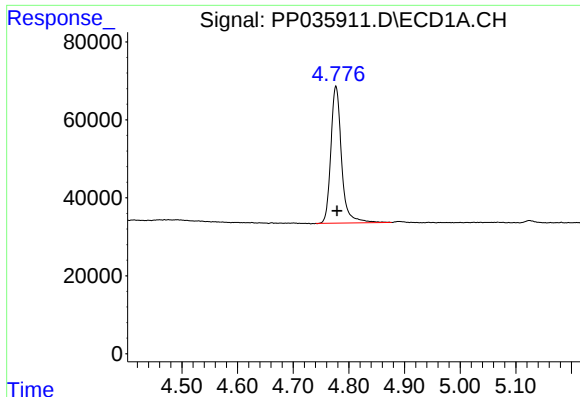

#1 Tetrachloro-m-xylene


R.T.: 4.777 min
Delta R.T.: -0.002 min
Response: 469617
Conc: 20.04 ng/ml

Instrument :
ECD_P
ClientSampleId :

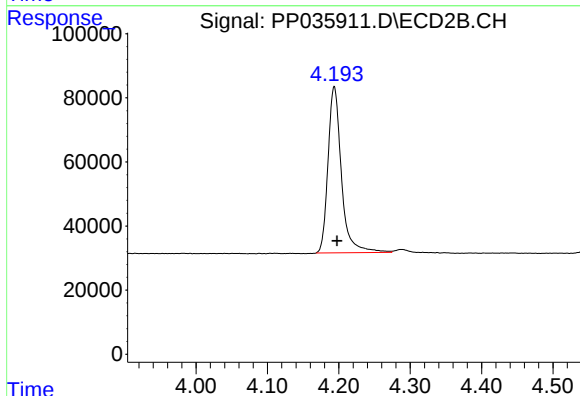


#1 Tetrachloro-m-xylene

R.T.: 4.194 min
Delta R.T.: -0.004 min
Response: 679074
Conc: 19.98 ng/ml

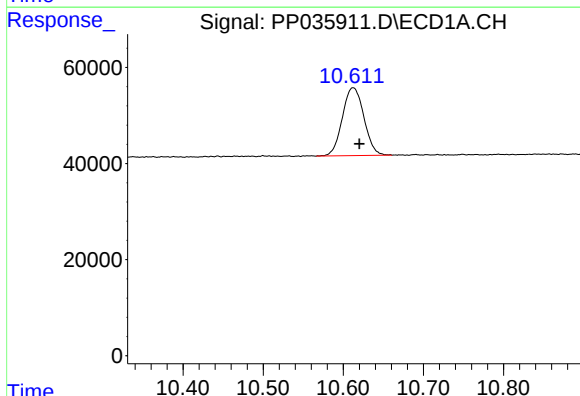


#2 Decachlorobiphenyl

R.T.: 10.612 min
Delta R.T.: -0.008 min
Response: 264318
Conc: 23.48 ng/ml

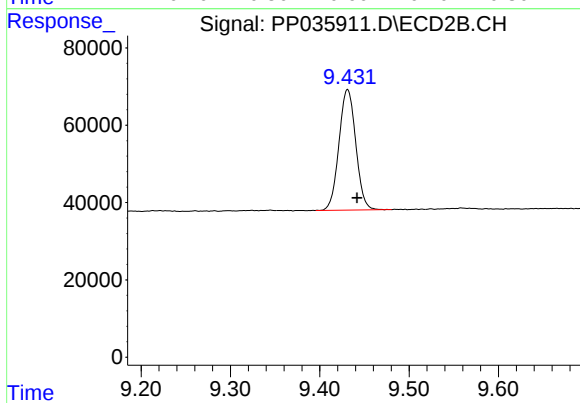

#2 Decachlorobiphenyl


R.T.: 9.431 min
Delta R.T.: -0.011 min
Response: 408703
Conc: 19.33 ng/ml

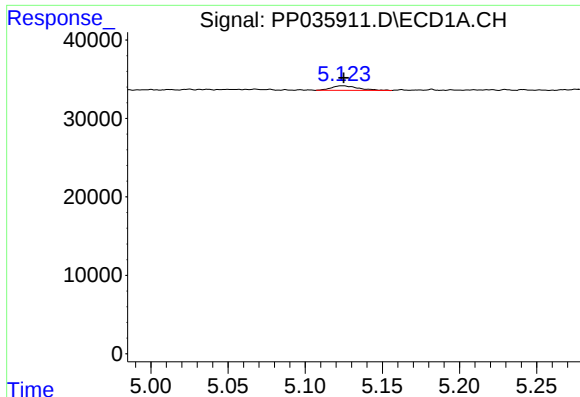

#9 AR-1221-2


R.T.: 5.124 min
Delta R.T.: 0.000 min
Response: 7077
Conc: 31.54 ng/ml

Instrument :
ECD_P
ClientSampleId :

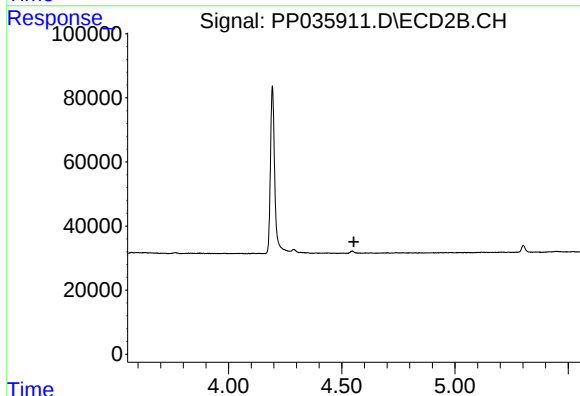


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.554 min
Response: 0
Conc: N.D.

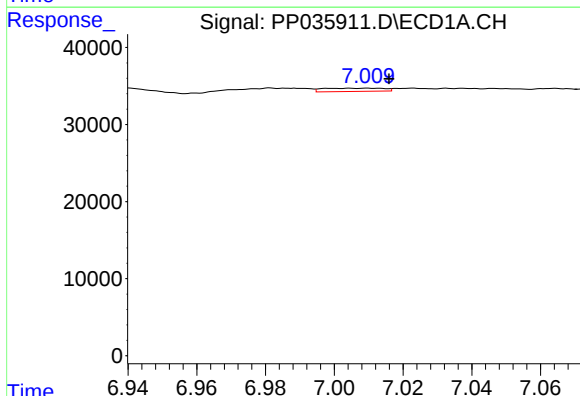


#24 AR-1248-4

R.T.: 7.010 min
Delta R.T.: -0.006 min
Response: 5183
Conc: 7.72 ng/ml

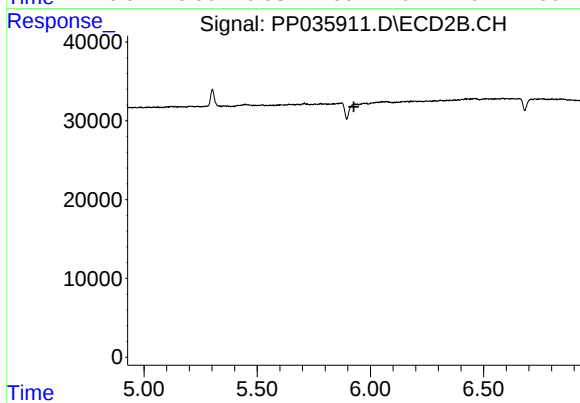

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.927 min
Response: 0
Conc: N.D.

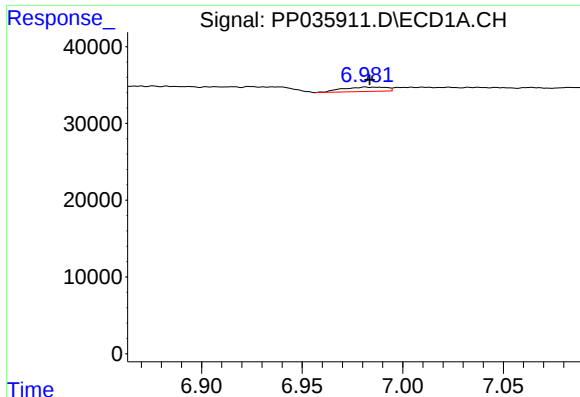

#26 AR-1254-1


R.T.: 6.982 min
Delta R.T.: -0.002 min
Response: 8572
Conc: 12.24 ng/ml

Instrument :
ECD_P
ClientSampleId :

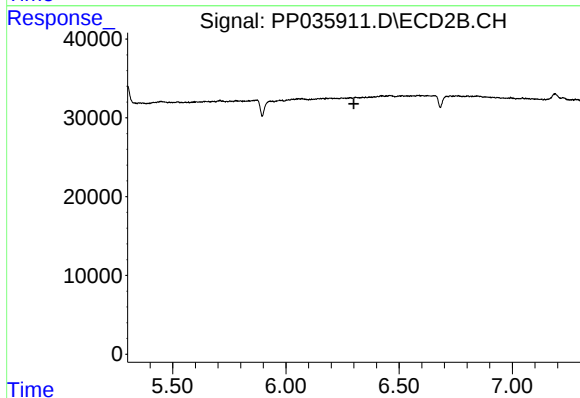


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.300 min
Response: 0
Conc: N.D.

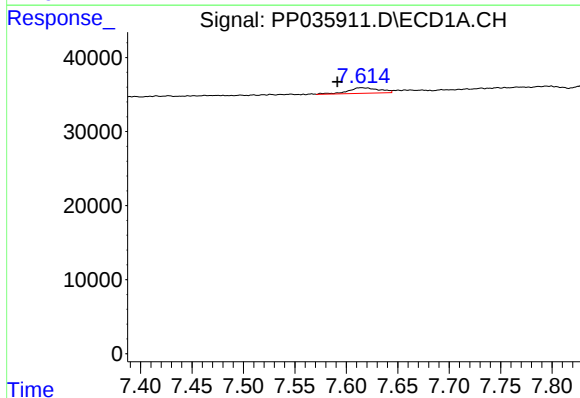


#28 AR-1254-3

R.T.: 7.615 min
Delta R.T.: 0.023 min
Response: 16064
Conc: 13.58 ng/ml

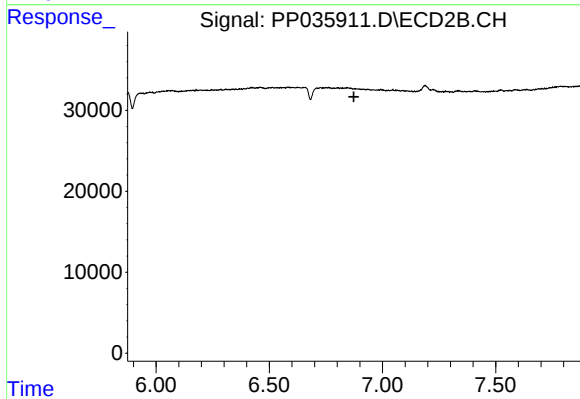

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.874 min
Response: 0
Conc: N.D.

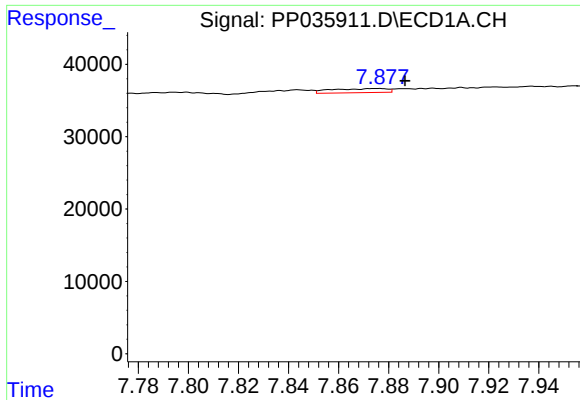

#29 AR-1254-4


R.T.: 7.875 min
Delta R.T.: -0.011 min
Response: 8792
Conc: 11.03 ng/ml

Instrument :
ECD_P
ClientSampleId :

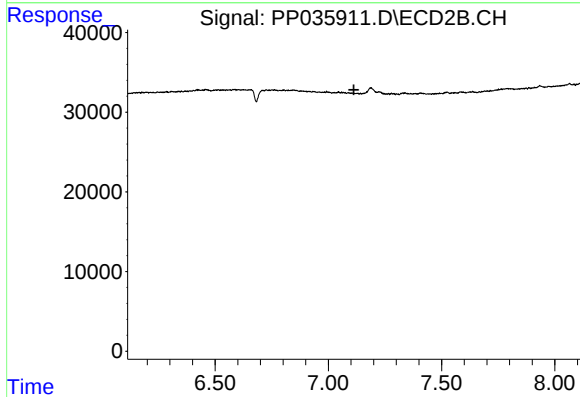


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.113 min
Response: 0
Conc: N.D.

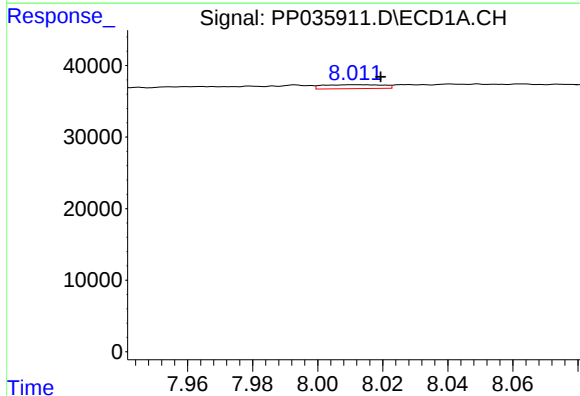


#32 AR-1260-2

R.T.: 8.012 min
Delta R.T.: -0.008 min
Response: 7058
Conc: 7.25 ng/ml

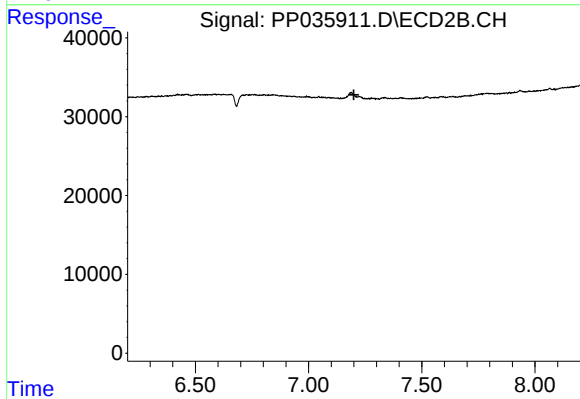

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.200 min
Response: 0
Conc: N.D.

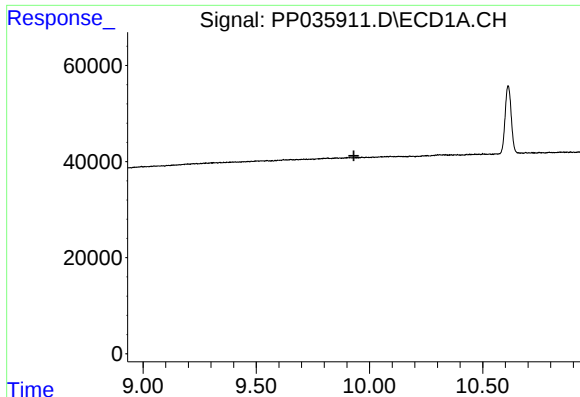

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 9.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

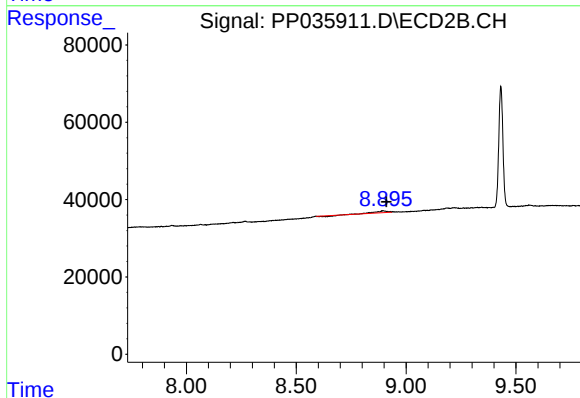


#40 AR-1262-5

R.T.: 8.895 min
Delta R.T.: -0.015 min
Response: 10133
Conc: 9.71 ng/ml

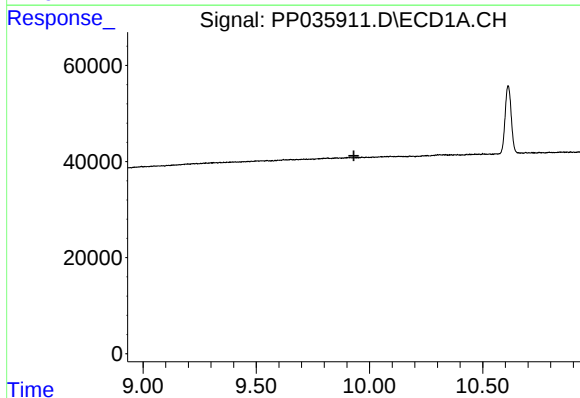

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.931 min
Response: 0
Conc: N.D.

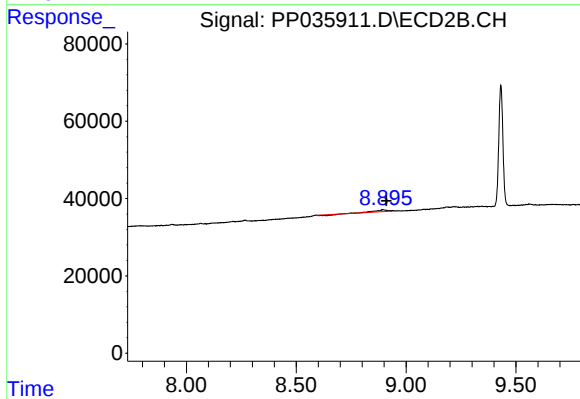

#44 AR-1268-4

R.T.: 8.895 min
Delta R.T.: -0.015 min
Response: 10133
Conc: 8.70 ng/ml