

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051421\
 Data File : PP035907.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 May 2021 13:00
 Operator : DD\AJ
 Sample : M2372-05DL 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CHRT-26598DL

Manual Integrations
 APPROVED

Ankita
 5/19/2021 3:11:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 01:28:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.774	4.194	53269	70203	2.273	2.065
2) SA Decachlor...	10.611	9.432	48209	62646	4.283m	2.962 #
Target Compounds						
31) L7 AR-1260-1	7.748	6.997	410945	656045	455.815	457.590
32) L7 AR-1260-2	8.013	7.192	939401	722738	964.349	418.688 #
33) L7 AR-1260-3	8.376	7.345	410478	685912	613.438	425.095 #
34) L7 AR-1260-4	8.602	7.821	512854	605191	654.445	524.609
35) L7 AR-1260-5	8.918	8.065	781393	1322298	592.420	515.339

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051421\
Data File : PP035907.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 May 2021 13:00
Operator : DD\AJ
Sample : M2372-05DL 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
CHRT-26598DL


Manual Integrations
APPROVED

Ankita
5/19/2021 3:11:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 01:28:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

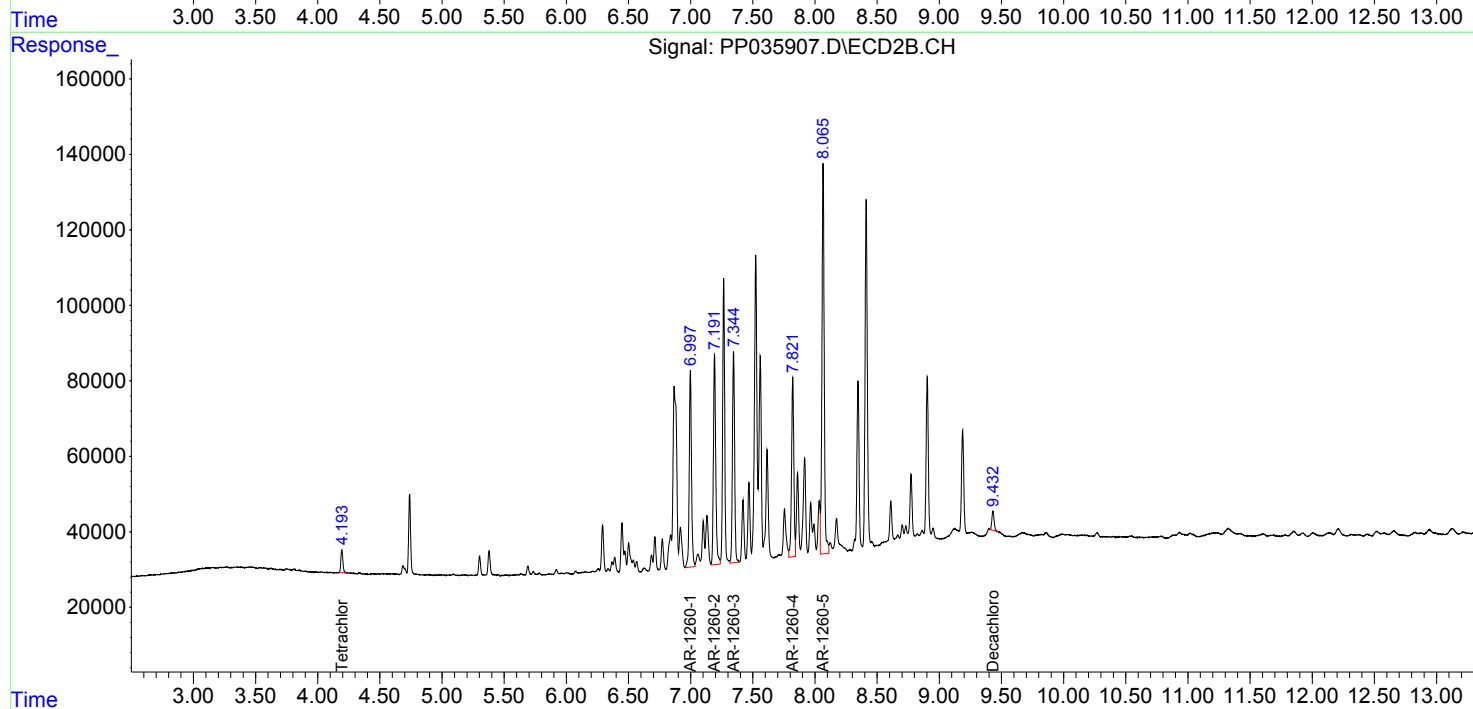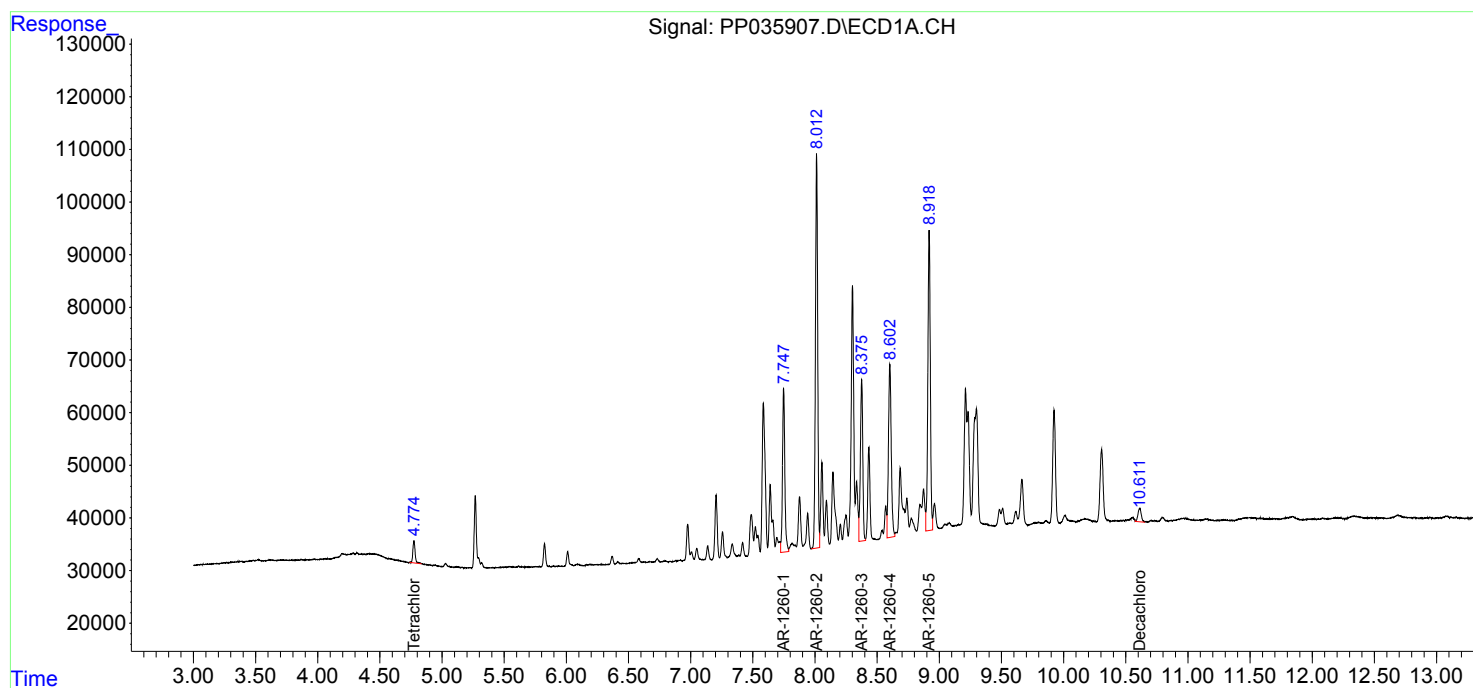

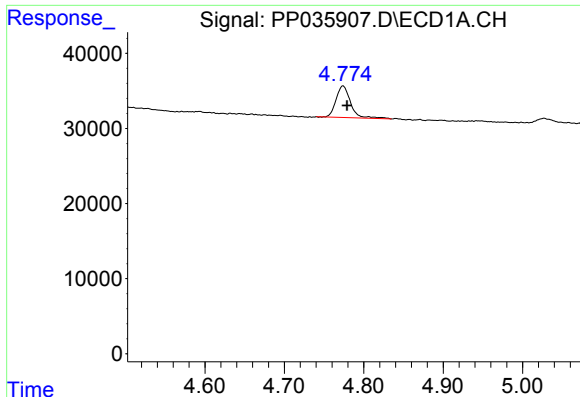


#1 Tetrachloro-m-xylene

R.T.: 4.774 min
Delta R.T.: -0.005 min
Response: 53269
Conc: 2.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-26598DL


Manual Integrations
APPROVED

Ankita
5/19/2021 3:11:54 PM

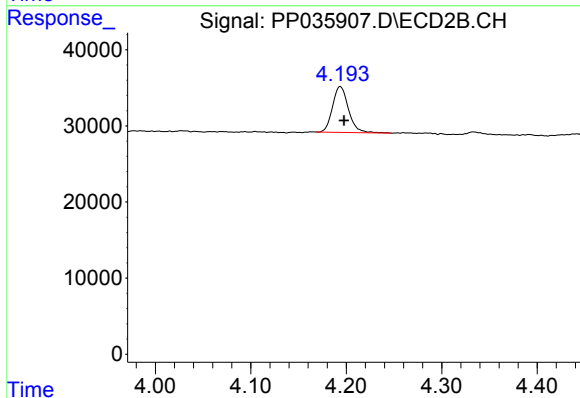


#1 Tetrachloro-m-xylene

R.T.: 4.194 min
Delta R.T.: -0.004 min
Response: 70203
Conc: 2.07 ng/ml

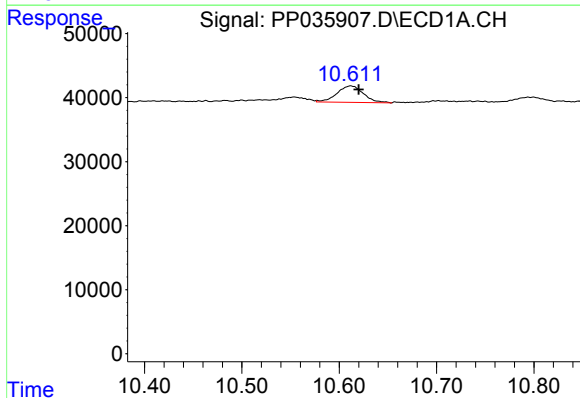


#2 Decachlorobiphenyl

R.T.: 10.611 min
Delta R.T.: -0.009 min
Response: 48209
Conc: 4.28 ng/ml m

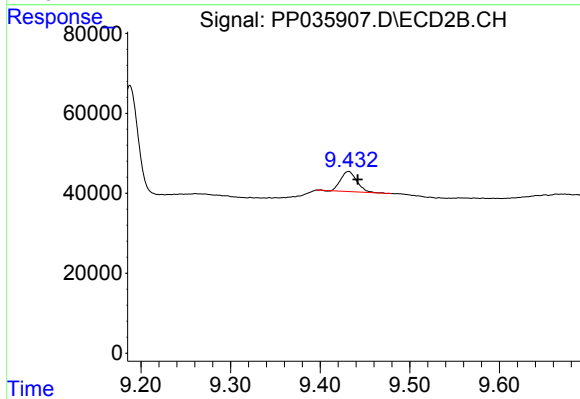

#2 Decachlorobiphenyl

R.T.: 9.432 min
Delta R.T.: -0.010 min
Response: 62646
Conc: 2.96 ng/ml

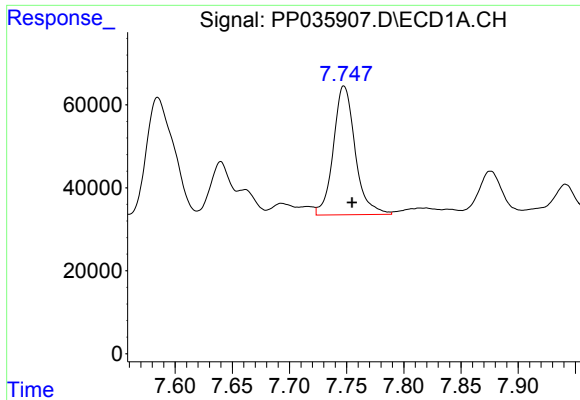


#31 AR-1260-1

R.T.: 7.748 min
Delta R.T.: -0.007 min
Response: 410945
Conc: 455.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-26598DL


Manual Integrations
APPROVED

Ankita
5/19/2021 3:11:54 PM

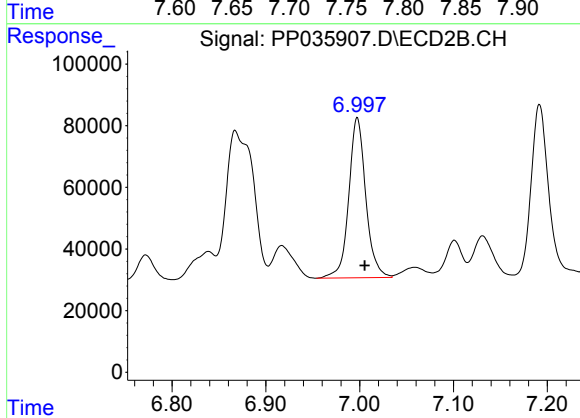


#31 AR-1260-1

R.T.: 6.997 min
Delta R.T.: -0.008 min
Response: 656045
Conc: 457.59 ng/ml

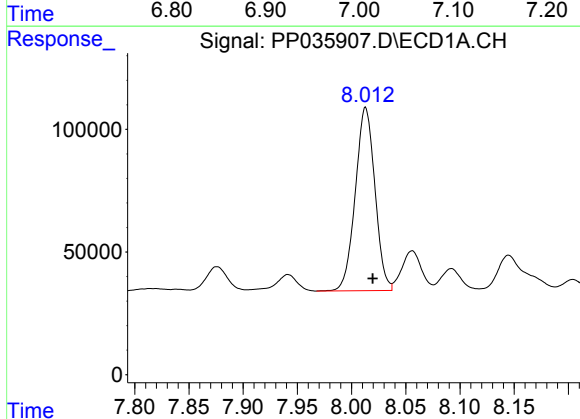


#32 AR-1260-2

R.T.: 8.013 min
Delta R.T.: -0.006 min
Response: 939401
Conc: 964.35 ng/ml

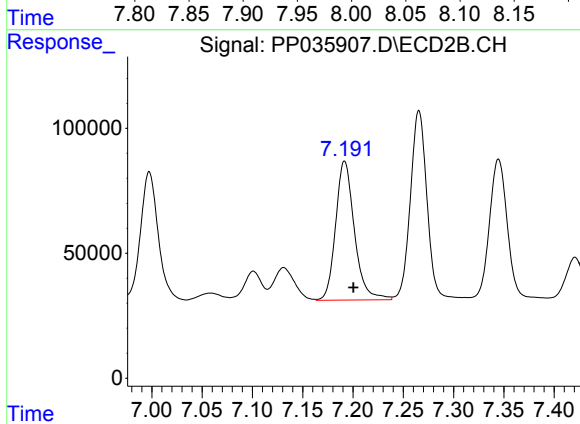

#32 AR-1260-2

R.T.: 7.192 min
Delta R.T.: -0.009 min
Response: 722738
Conc: 418.69 ng/ml

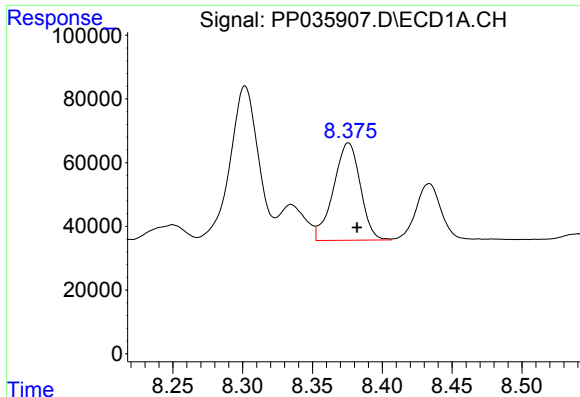


#33 AR-1260-3

R.T.: 8.376 min
Delta R.T.: -0.006 min
Response: 410478
Conc: 613.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-26598DL


Manual Integrations
APPROVED

Ankita
5/19/2021 3:11:54 PM

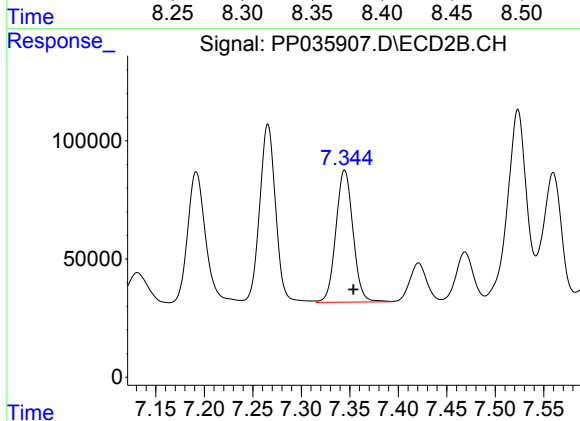


#33 AR-1260-3

R.T.: 7.345 min
Delta R.T.: -0.009 min
Response: 685912
Conc: 425.09 ng/ml

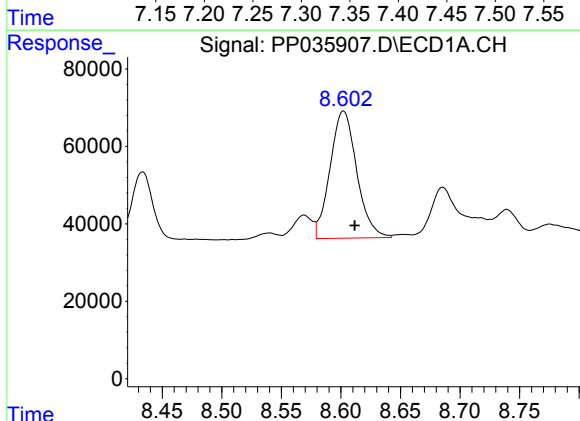


#34 AR-1260-4

R.T.: 8.602 min
Delta R.T.: -0.009 min
Response: 512854
Conc: 654.45 ng/ml

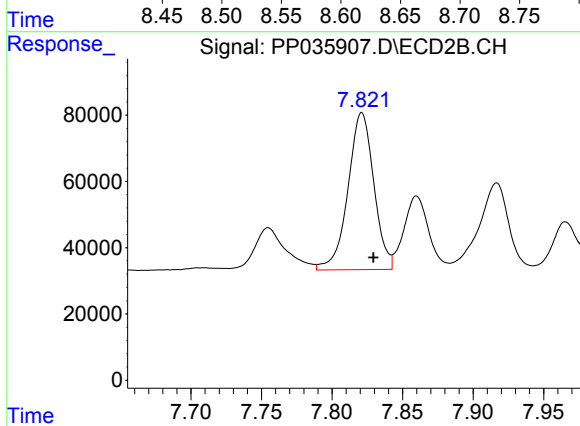

#34 AR-1260-4

R.T.: 7.821 min
Delta R.T.: -0.008 min
Response: 605191
Conc: 524.61 ng/ml

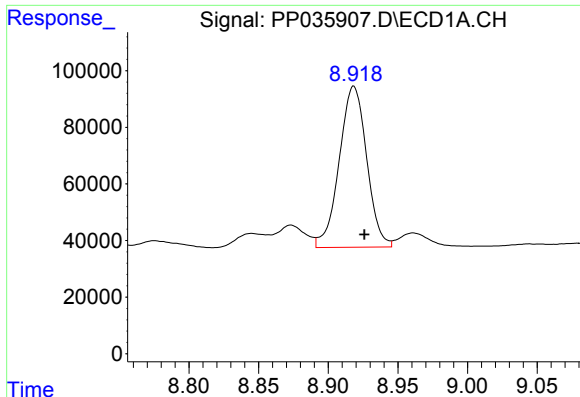


#35 AR-1260-5

R.T.: 8.918 min
Delta R.T.: -0.008 min
Response: 781393
Conc: 592.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-26598DL

Manual Integrations
APPROVED

Ankita
5/19/2021 3:11:54 PM

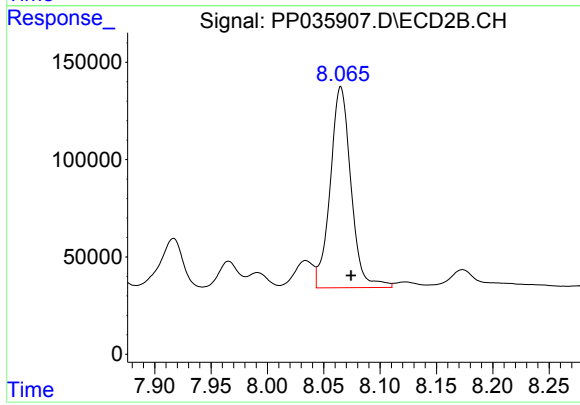

#35 AR-1260-5

R.T.: 8.065 min
Delta R.T.: -0.009 min
Response: 1322298
Conc: 515.34 ng/ml