

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051421\
 Data File : PP035918.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 May 2021 18:19
 Operator : DD\AJ
 Sample : M2388-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 41786-DARK

Manual Integrations
 APPROVED

Ankita
 5/19/2021 3:11:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 01:34:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.772	4.193	454842	662339	19.412m	19.485m
2) SA Decachlor...	10.609	9.430	315104	491906	27.995	23.261

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051421\
Data File : PP035918.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 May 2021 18:19
Operator : DD\AJ
Sample : M2388-07
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
41786-DARK


Manual Integrations
APPROVED

Ankita
5/19/2021 3:11:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 01:34:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

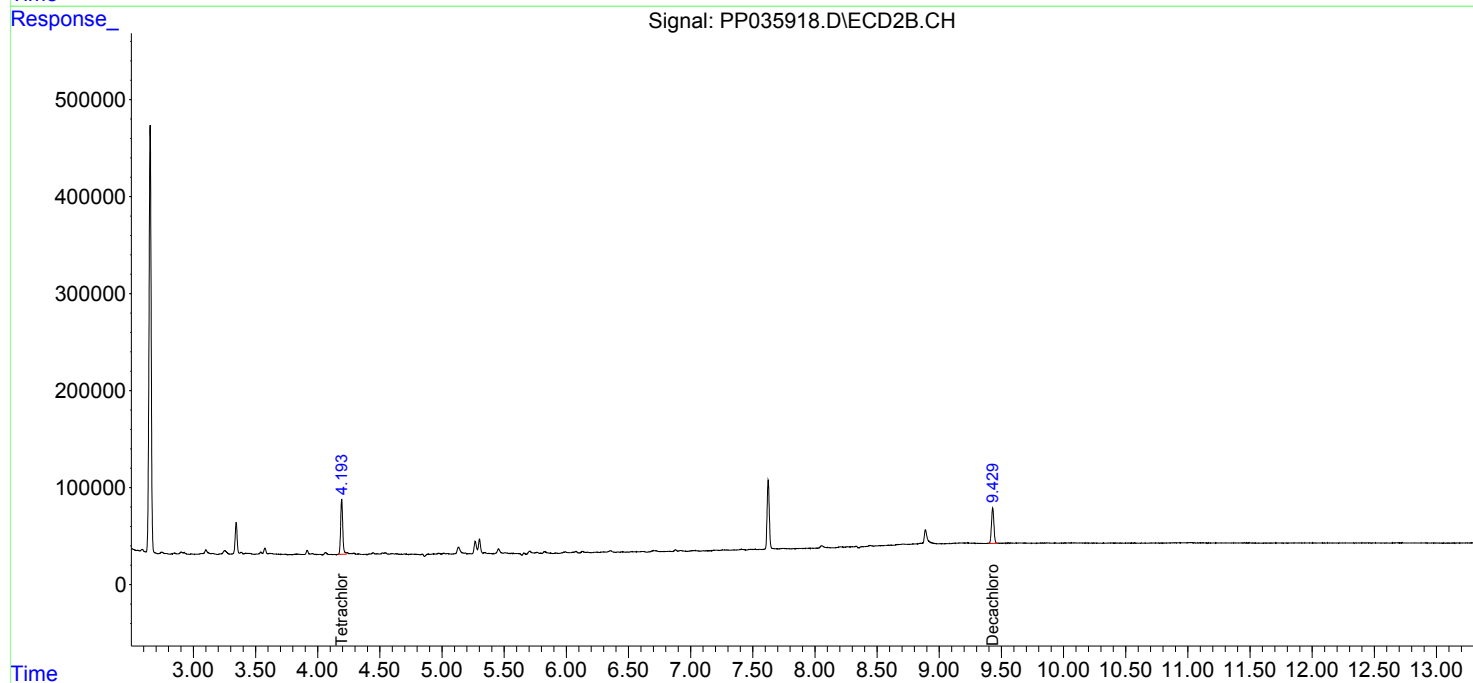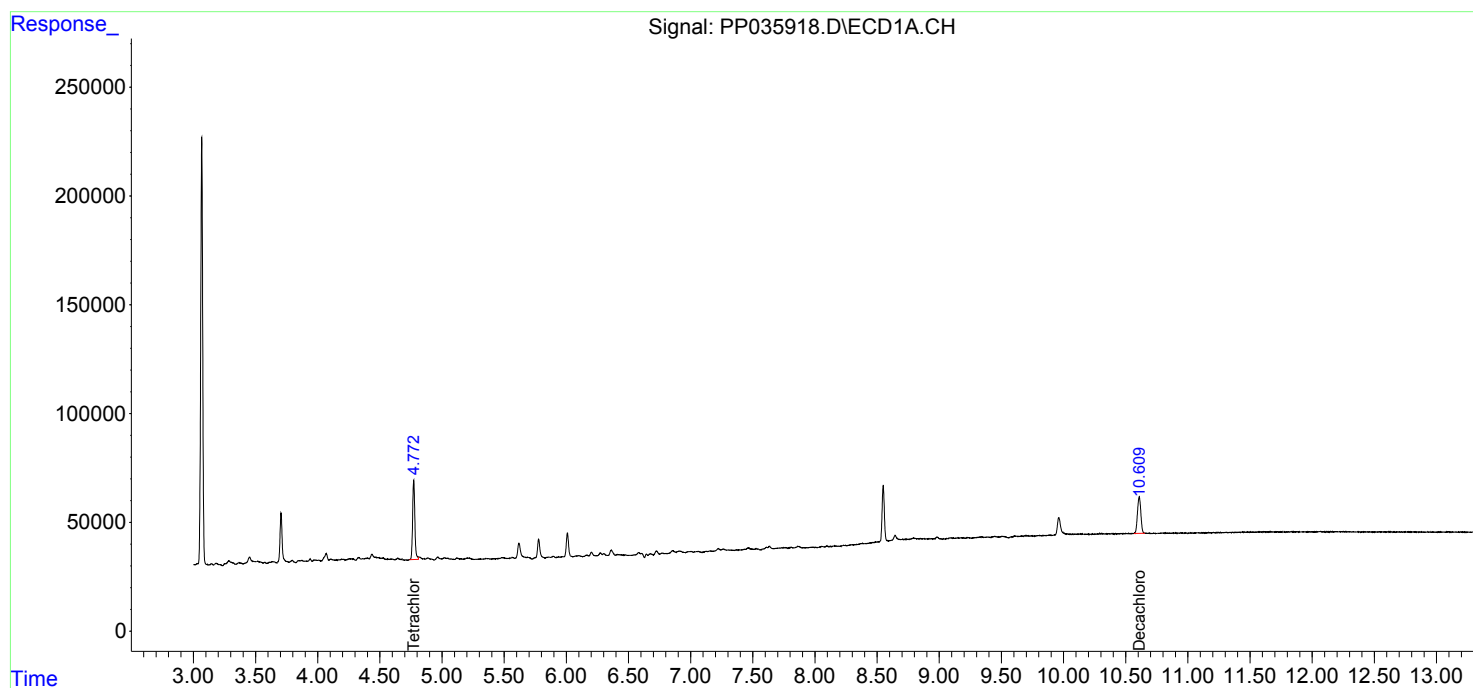

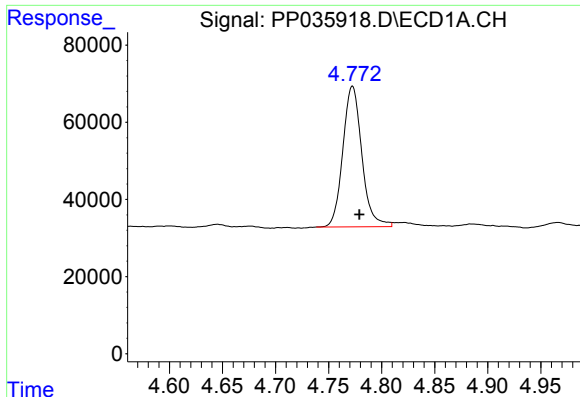


#1 Tetrachloro-m-xylene

R.T.: 4.772 min
Delta R.T.: -0.007 min
Response: 454842
Conc: 19.41 ng/ml m

Instrument :
ECD_P
ClientSampleId :
41786-DARK


Manual Integrations
APPROVED

Ankita
5/19/2021 3:11:56 PM

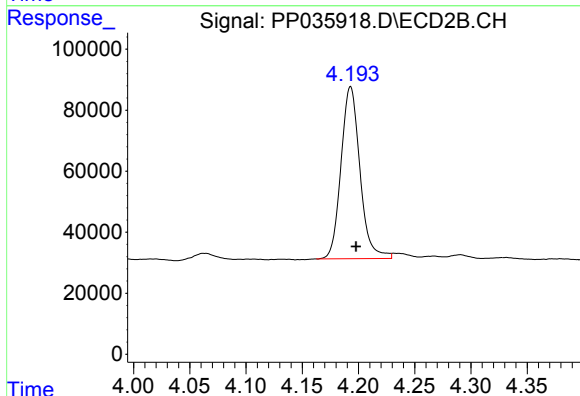


#1 Tetrachloro-m-xylene

R.T.: 4.193 min
Delta R.T.: -0.005 min
Response: 662339
Conc: 19.48 ng/ml m

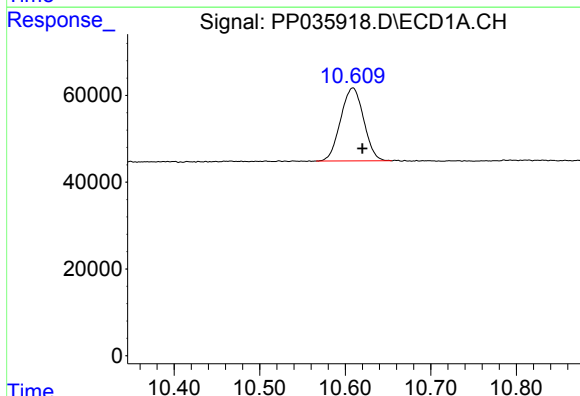

#2 Decachlorobiphenyl

R.T.: 10.609 min
Delta R.T.: -0.011 min
Response: 315104
Conc: 27.99 ng/ml

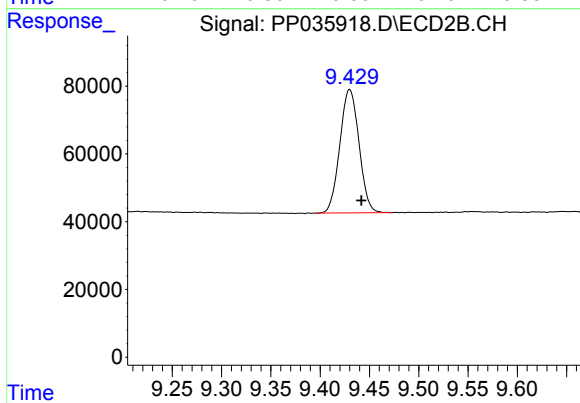

#2 Decachlorobiphenyl

R.T.: 9.430 min
Delta R.T.: -0.012 min
Response: 491906
Conc: 23.26 ng/ml