

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051421\
 Data File : PP035919.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 May 2021 18:36
 Operator : DD\AJ
 Sample : M2389-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BURNETT-AVE-1-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 01:35:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.773	4.195	512939	747441	21.892	21.988
2) SA Decachlor...	10.608	9.430	273519	443349	24.300	20.965

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051421\
Data File : PP035919.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 May 2021 18:36
Operator : DD\AJ
Sample : M2389-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BURNETT-AVE-1-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 01:35:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

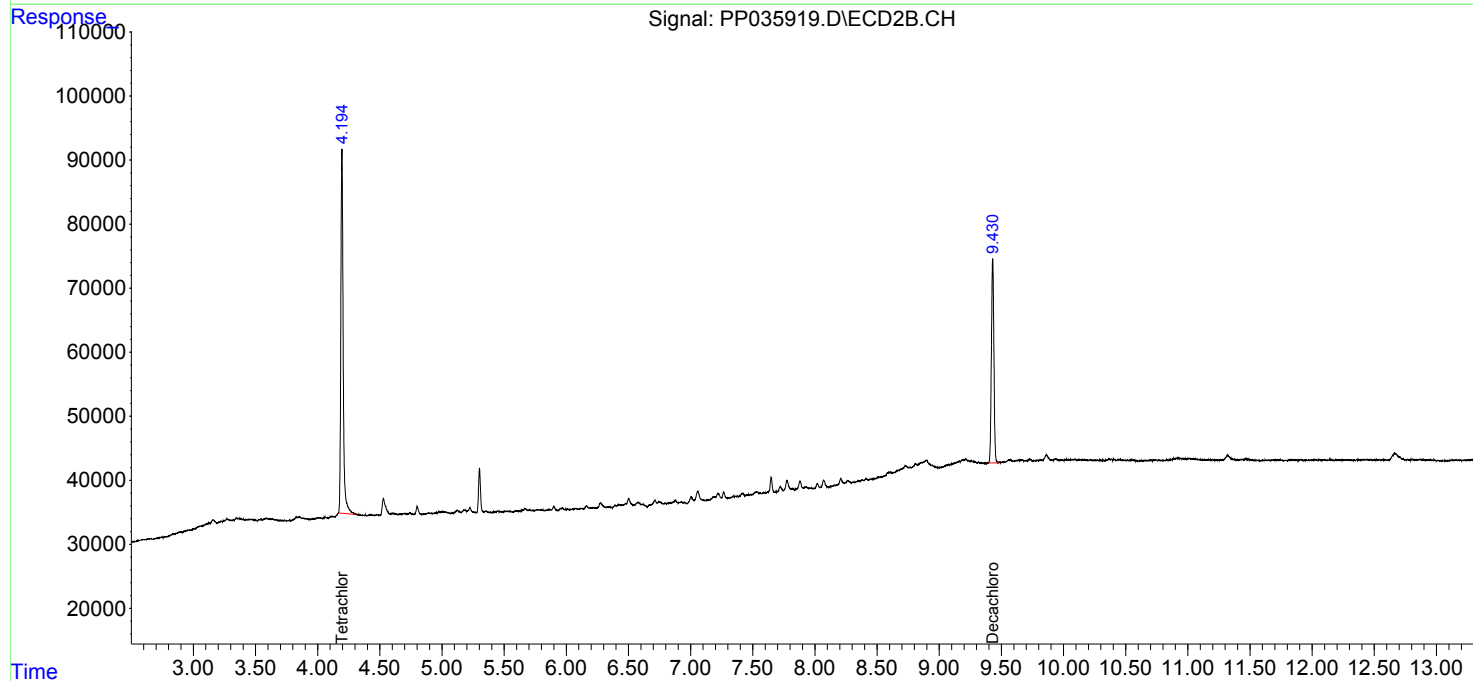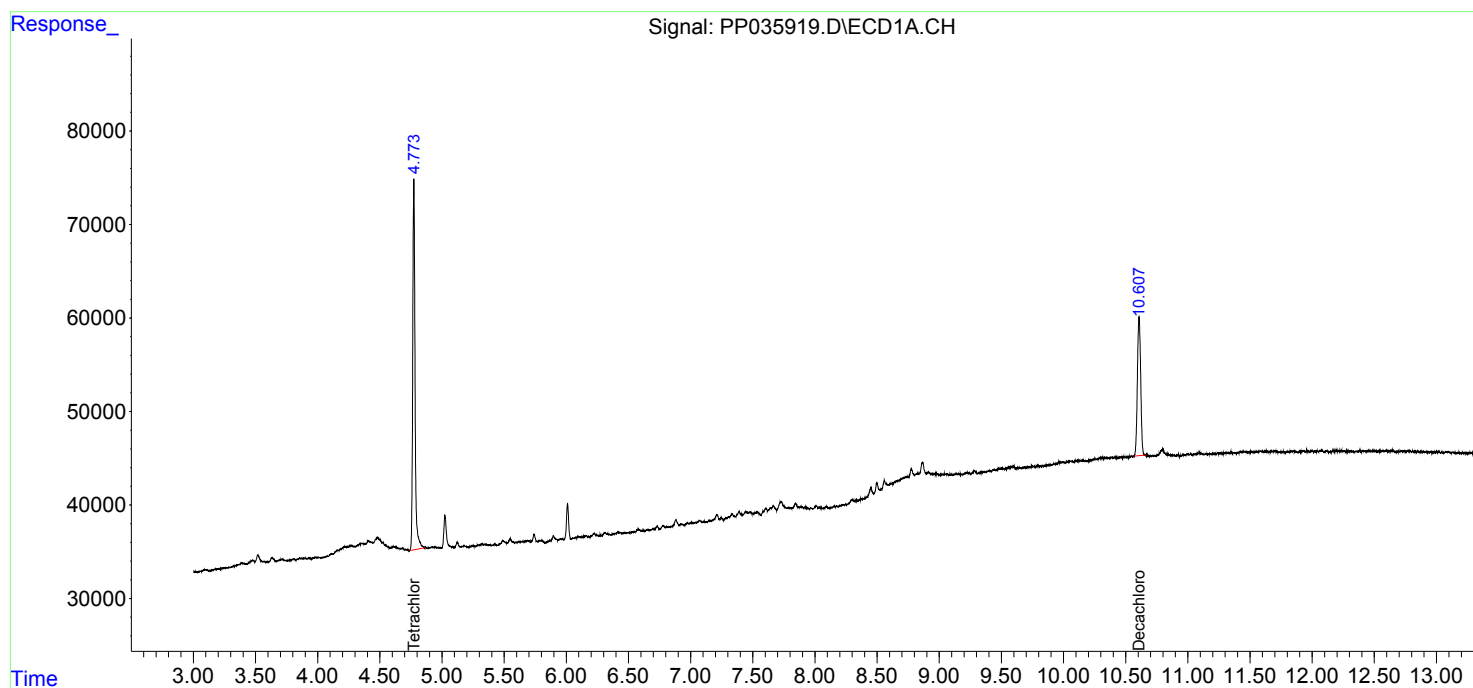


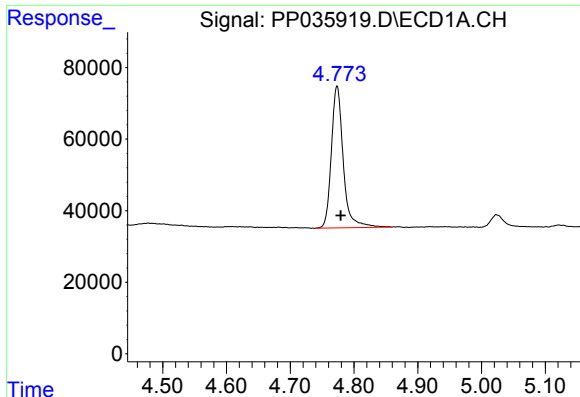

#1 Tetrachloro-m-xylene


R.T.: 4.773 min
Delta R.T.: -0.006 min
Response: 512939
Conc: 21.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
BURNETT-AVE-1-3

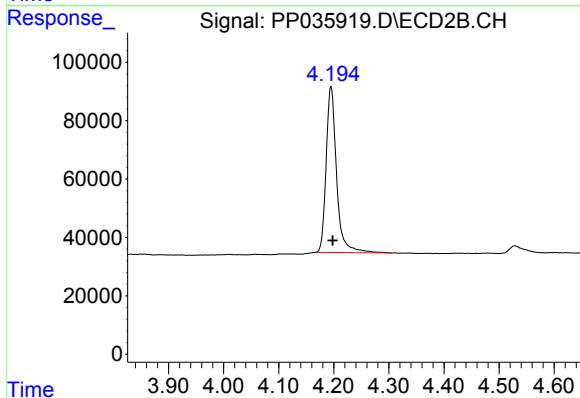


#1 Tetrachloro-m-xylene

R.T.: 4.195 min
Delta R.T.: -0.003 min
Response: 747441
Conc: 21.99 ng/ml

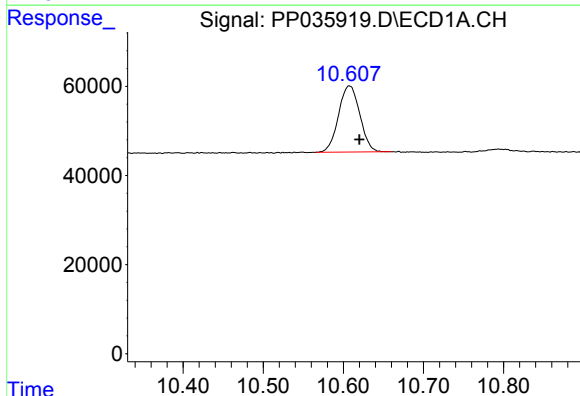

#2 Decachlorobiphenyl

R.T.: 10.608 min
Delta R.T.: -0.012 min
Response: 273519
Conc: 24.30 ng/ml

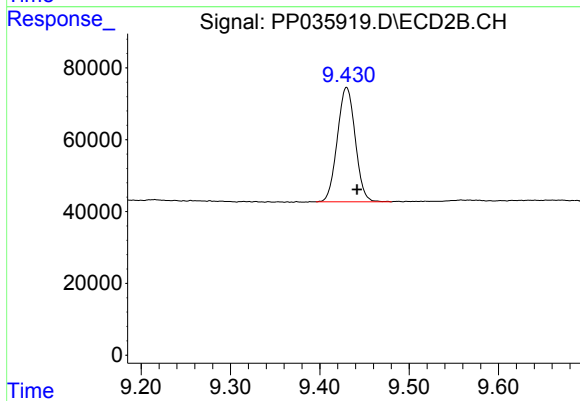

#2 Decachlorobiphenyl

R.T.: 9.430 min
Delta R.T.: -0.012 min
Response: 443349
Conc: 20.96 ng/ml