

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051424\
 Data File : PP064943.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2024 00:49
 Operator : YP\AJ
 Sample : P2403-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 01:55:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 14 06:05:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.259	3.372	38995148	51318363	20.503	22.797
2) SA Decachlor...	9.909	8.266	18518250	42626742	25.790	24.337
Target Compounds						
3) L1 AR-1016-1	5.428	4.430	501276	847792	12.177	11.043
4) L1 AR-1016-2	5.450	4.447	723082	1096545	11.715	10.190
5) L1 AR-1016-3	5.511	4.618	583084	603753	14.867	10.188 #
6) L1 AR-1016-4	5.610	4.662	405020	463654	13.509	9.544 #
7) L1 AR-1016-5	5.906	4.870	216875	620395	7.436	9.809 #
8) L2 AR-1221-1	4.466	3.581	1487422	1250060	62.317	40.114 #
9) L2 AR-1221-2	4.558	3.663	986065	2035450	59.169	87.443 #
10) L2 AR-1221-3	4.630	3.737	2389081	3204430	47.132	47.135
11) L3 AR-1232-1	4.630	3.737	2389081	3204430	58.067	58.506
12) L3 AR-1232-2	5.158	4.447	470758	1096545	23.695	20.875
13) L3 AR-1232-3	5.450	4.618	723082	603753	21.873	20.923
14) L3 AR-1232-4	5.610	4.703	405020	439754	24.477	16.211 #
15) L3 AR-1232-5	5.703	4.870	306909	620395	22.283	21.707
16) L4 AR-1242-1	5.428	4.430	501276	847792	14.327	12.658
17) L4 AR-1242-2	5.450	4.447	723082	1096545	13.705	11.856
18) L4 AR-1242-3	5.511	4.618	583084	603753	17.381	11.780 #
19) L4 AR-1242-4	5.610	4.703	405020	439754	15.322	8.360 #
20) L4 AR-1242-5	0.000	5.217	0	565503	N.D.	9.375 #
21) L5 AR-1248-1	5.428	4.430	501276	847792	19.380	17.152
22) L5 AR-1248-2	5.703	4.662	306909	463654	7.880	6.429
23) L5 AR-1248-3	5.906	4.703	216875	439754	5.388	5.769
24) L5 AR-1248-4	6.285f	4.870	461698	620395	12.063	7.022 #
25) L5 AR-1248-5	0.000	5.241f	0	498444	N.D.	6.050 #
26) L6 AR-1254-1	6.285	5.217	461698	565503	10.773	4.320 #
27) L6 AR-1254-2	0.000	5.364	0	568908	N.D.	5.011 #
28) L6 AR-1254-3	6.869	5.739f	528579	304286	8.344	1.720 #
30) L6 AR-1254-5	7.574	6.400	501511	1295275	11.133	8.625
31) L7 AR-1260-1	7.035	5.889	378746	1285780	7.588	10.703 #
32) L7 AR-1260-2	7.293	6.077	417784	1589900	8.279	11.745 #
33) L7 AR-1260-3	7.652	6.226	354715	1282960	9.151	9.689
34) L7 AR-1260-4	7.877	6.694	479666	838208	10.934	7.876 #
35) L7 AR-1260-5	8.186	6.936	628798	2040176	8.672	8.809
36) L8 AR-1262-1	7.709	6.492	194660	442264	7.551	6.231
37) L8 AR-1262-2	8.186	6.694	628798	838208	7.190	5.885
38) L8 AR-1262-3	8.496	7.215	430802	850380	6.928	8.030
39) L8 AR-1262-4	0.000	7.278	0	1564780	N.D.	8.123 #
40) L8 AR-1262-5	0.000	7.770	0	496688	N.D.	5.604 #
41) L9 AR-1268-1	8.496	7.215	430802	850380	4.046	2.954 #
42) L9 AR-1268-2	0.000	7.278	0	1564780	N.D.	5.913 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051424\
 Data File : PP064943.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2024 00:49
 Operator : YP\AJ
 Sample : P2403-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 01:55:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 14 06:05:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	0.000	7.770	0	496688	N.D.	5.282 #
45) L9	AR-1268-5	0.000	8.037	0	449251	N.D.	0.701 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051424\
Data File : PP064943.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2024 00:49
Operator : YP\AJ
Sample : P2403-07
Misc : AR1660 LOD 40 PPB
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 01:55:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051324.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 14 06:05:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

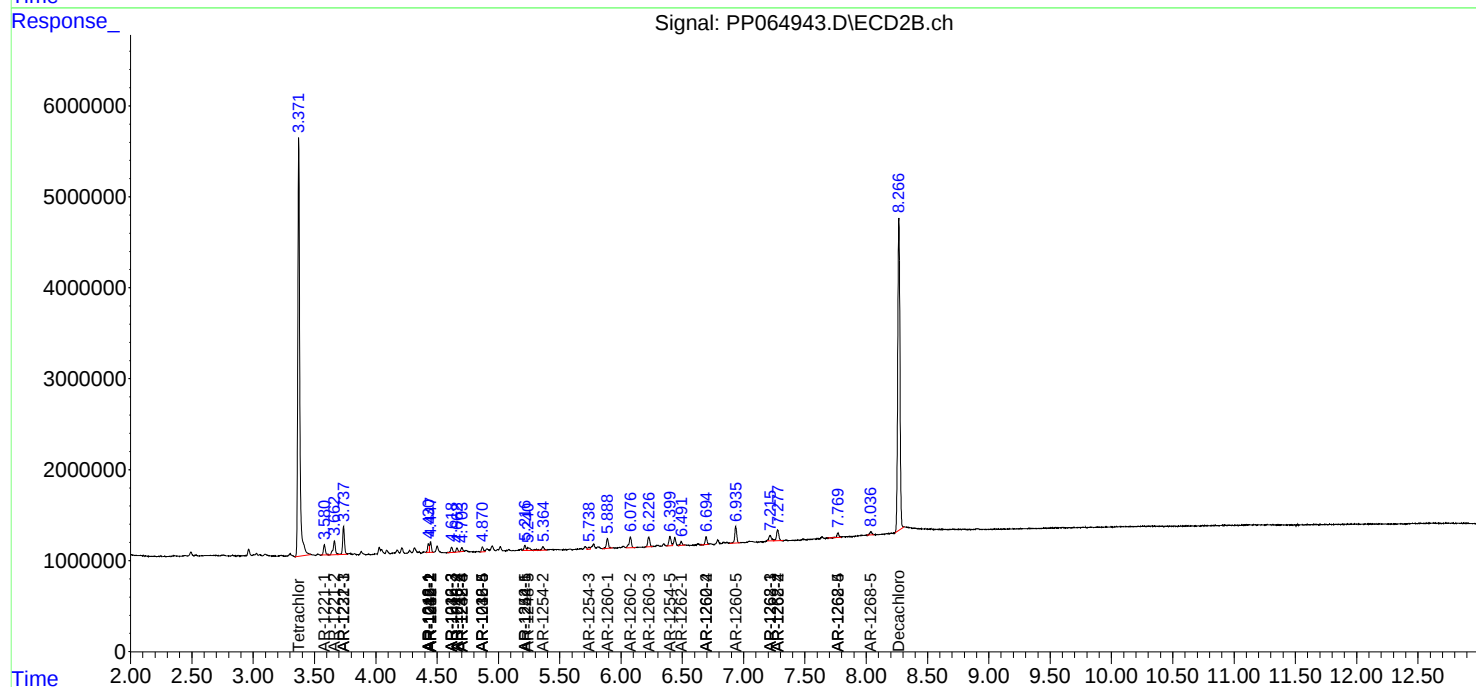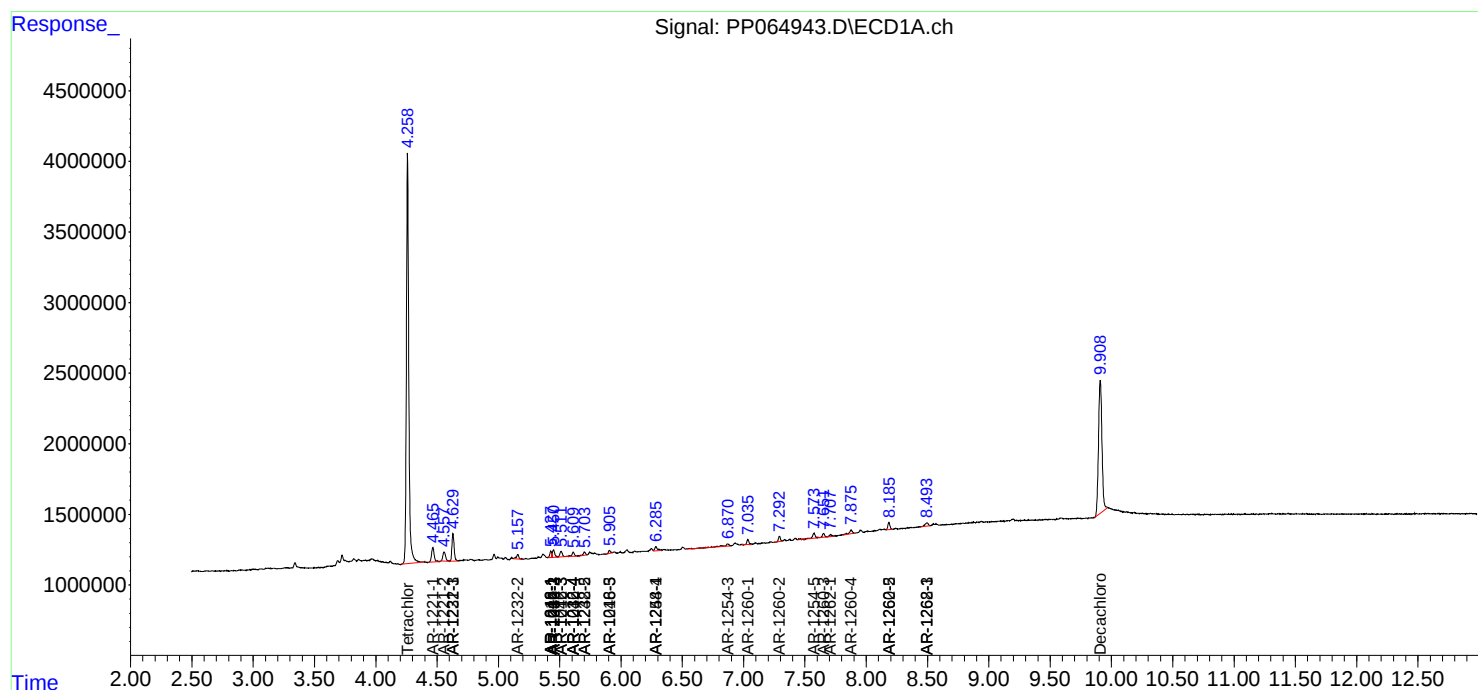


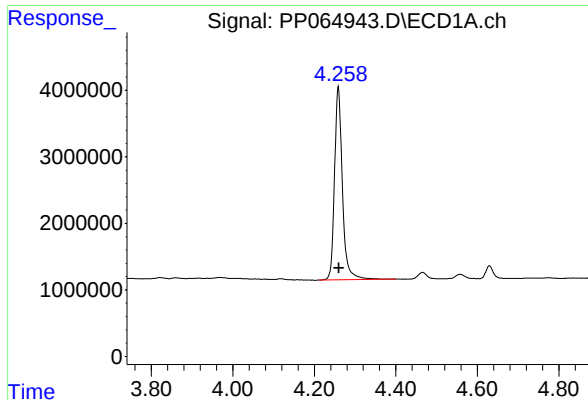

#1 Tetrachloro-m-xylene


R.T.: 4.259 min
Delta R.T.: -0.001 min
Response: 38995148
Conc: 20.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

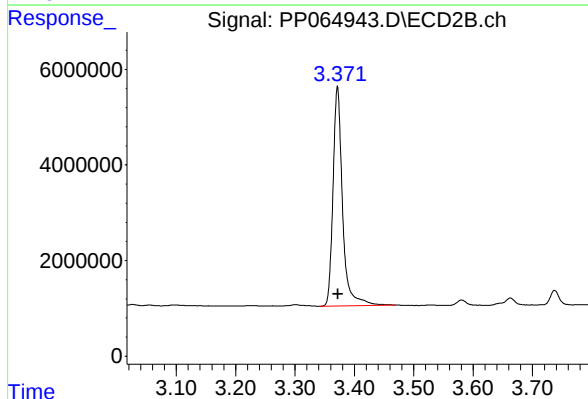


#1 Tetrachloro-m-xylene

R.T.: 3.372 min
Delta R.T.: 0.000 min
Response: 51318363
Conc: 22.80 ng/ml

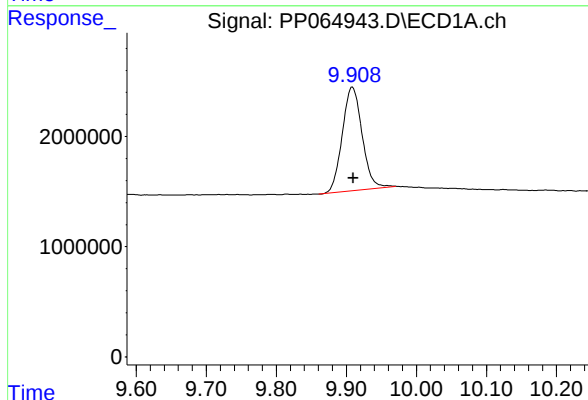


#2 Decachlorobiphenyl

R.T.: 9.909 min
Delta R.T.: -0.001 min
Response: 18518250
Conc: 25.79 ng/ml

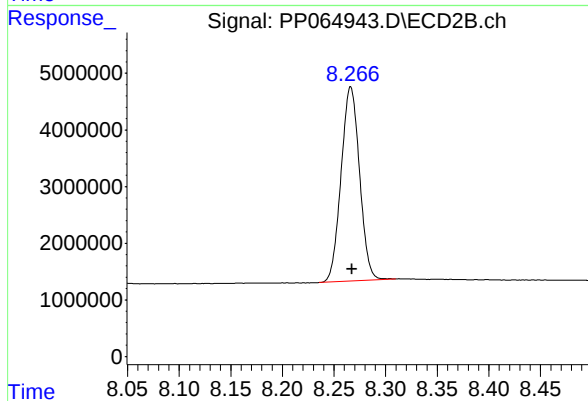

#2 Decachlorobiphenyl


R.T.: 8.266 min
Delta R.T.: -0.001 min
Response: 42626742
Conc: 24.34 ng/ml

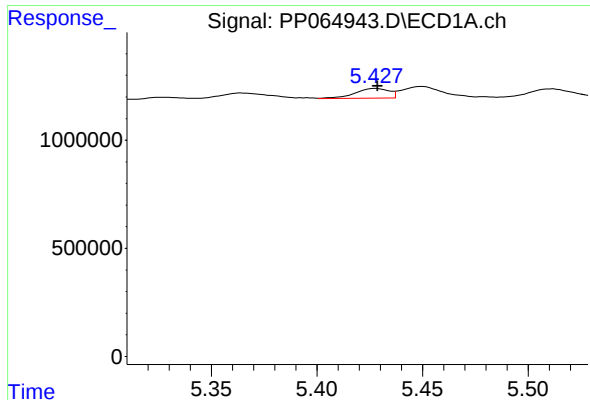

#3 AR-1016-1


R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 501276
Conc: 12.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

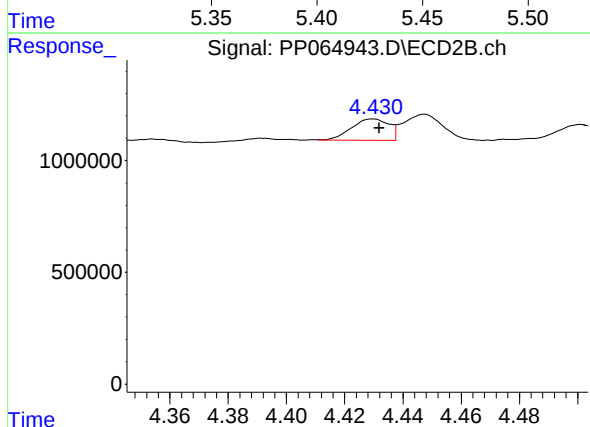


#3 AR-1016-1

R.T.: 4.430 min
Delta R.T.: -0.002 min
Response: 847792
Conc: 11.04 ng/ml

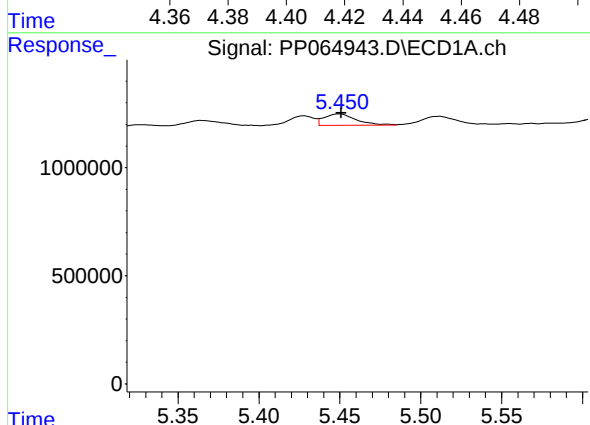


#4 AR-1016-2

R.T.: 5.450 min
Delta R.T.: -0.001 min
Response: 723082
Conc: 11.72 ng/ml

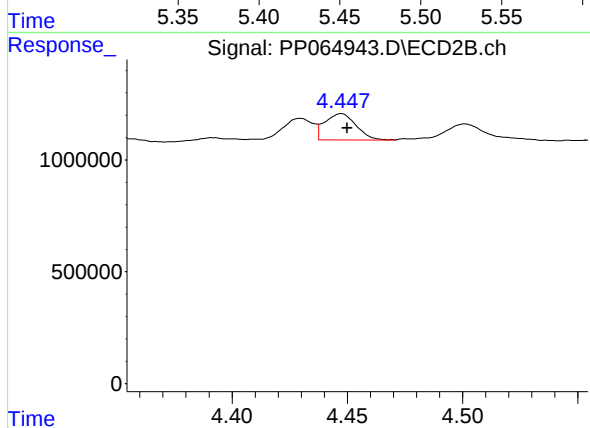

#4 AR-1016-2


R.T.: 4.447 min
Delta R.T.: -0.003 min
Response: 1096545
Conc: 10.19 ng/ml

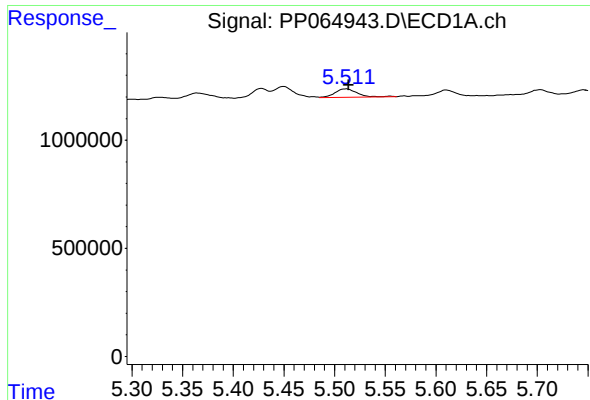

#5 AR-1016-3


R.T.: 5.511 min
Delta R.T.: -0.002 min
Response: 583084
Conc: 14.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

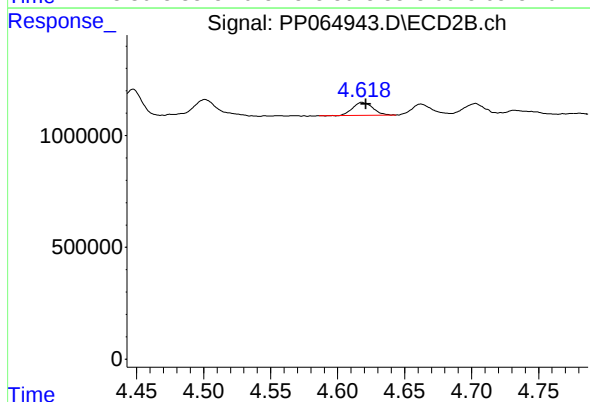


#5 AR-1016-3

R.T.: 4.618 min
Delta R.T.: -0.003 min
Response: 603753
Conc: 10.19 ng/ml

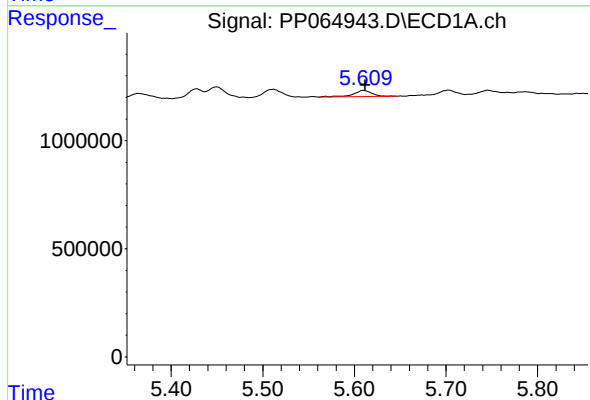


#6 AR-1016-4

R.T.: 5.610 min
Delta R.T.: -0.001 min
Response: 405020
Conc: 13.51 ng/ml

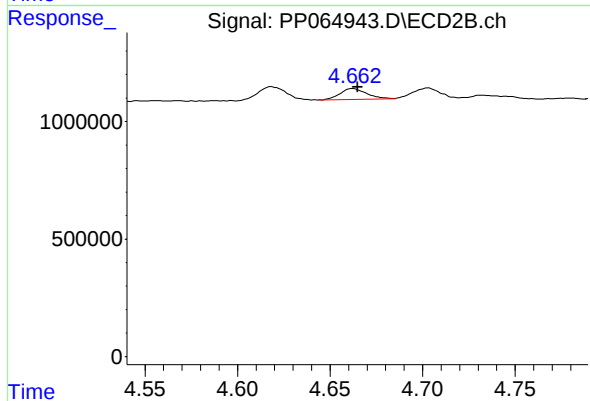

#6 AR-1016-4


R.T.: 4.662 min
Delta R.T.: -0.003 min
Response: 463654
Conc: 9.54 ng/ml

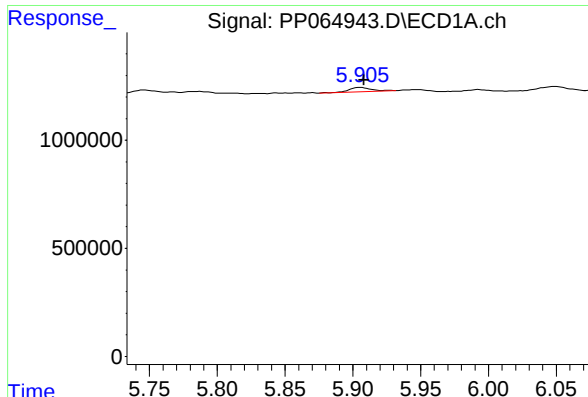

#7 AR-1016-5


R.T.: 5.906 min
Delta R.T.: -0.003 min
Response: 216875
Conc: 7.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

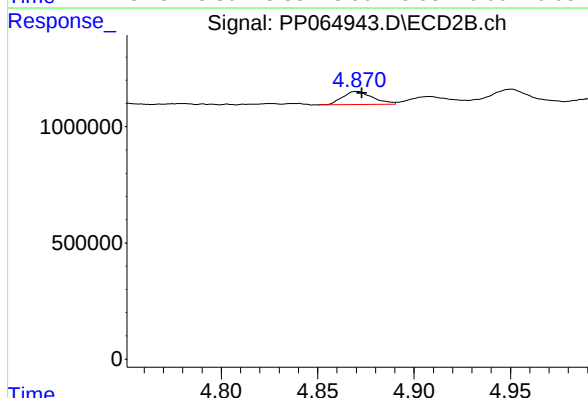


#7 AR-1016-5

R.T.: 4.870 min
Delta R.T.: -0.003 min
Response: 620395
Conc: 9.81 ng/ml

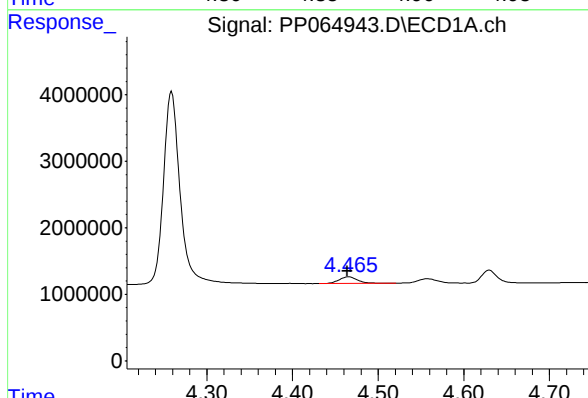


#8 AR-1221-1

R.T.: 4.466 min
Delta R.T.: 0.002 min
Response: 1487422
Conc: 62.32 ng/ml

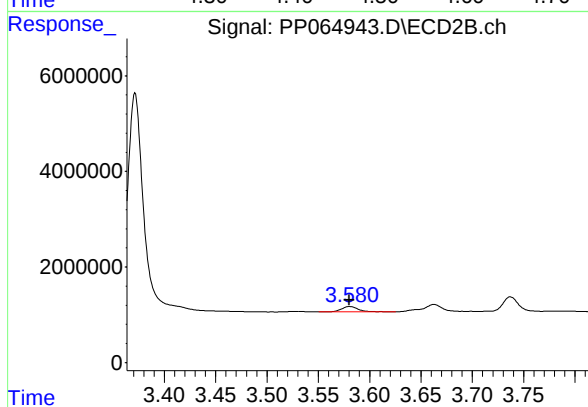

#8 AR-1221-1


R.T.: 3.581 min
Delta R.T.: 0.000 min
Response: 1250060
Conc: 40.11 ng/ml

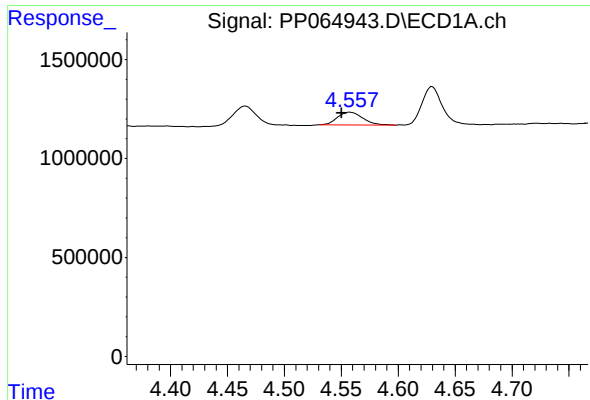

#9 AR-1221-2


R.T.: 4.558 min
Delta R.T.: 0.007 min
Response: 986065
Conc: 59.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

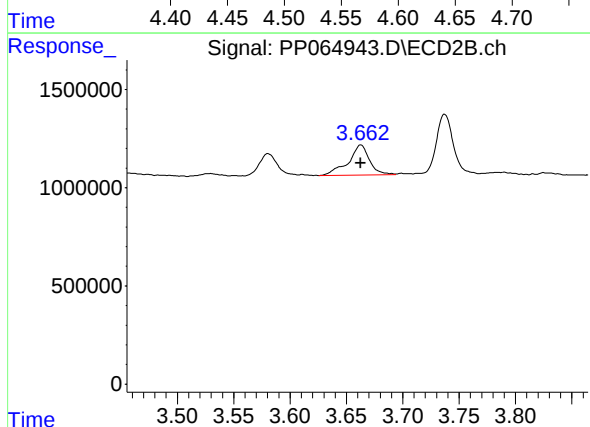


#9 AR-1221-2

R.T.: 3.663 min
Delta R.T.: 0.000 min
Response: 2035450
Conc: 87.44 ng/ml

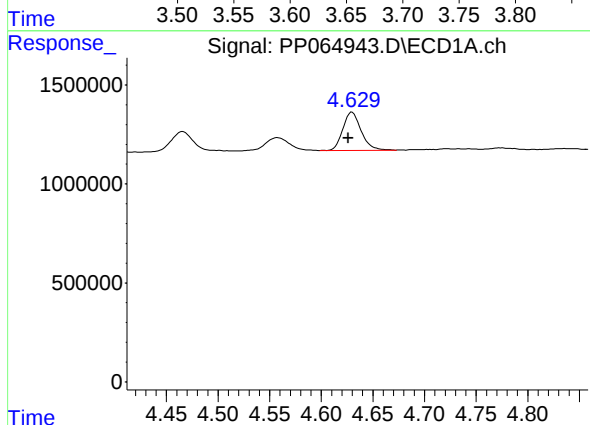


#10 AR-1221-3

R.T.: 4.630 min
Delta R.T.: 0.004 min
Response: 2389081
Conc: 47.13 ng/ml

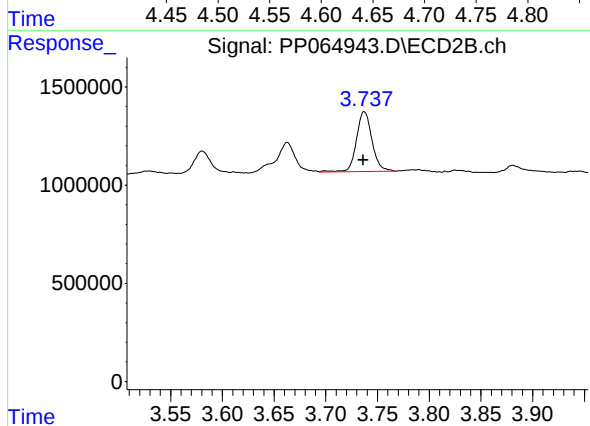

#10 AR-1221-3


R.T.: 3.737 min
Delta R.T.: 0.000 min
Response: 3204430
Conc: 47.13 ng/ml

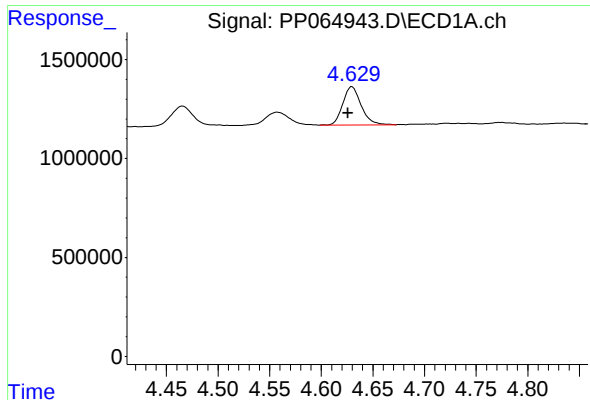

#11 AR-1232-1


R.T.: 4.630 min
Delta R.T.: 0.004 min
Response: 2389081
Conc: 58.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

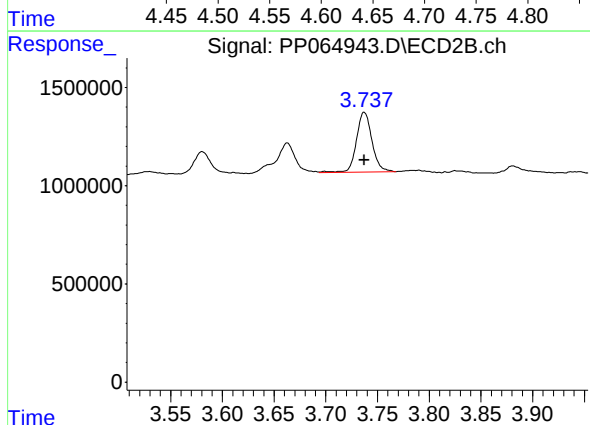


#11 AR-1232-1

R.T.: 3.737 min
Delta R.T.: 0.000 min
Response: 3204430
Conc: 58.51 ng/ml

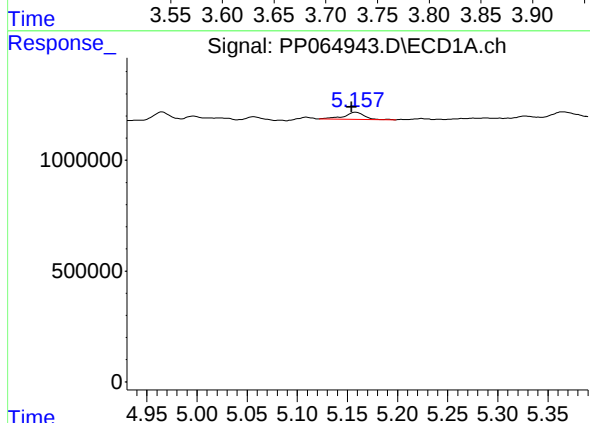


#12 AR-1232-2

R.T.: 5.158 min
Delta R.T.: 0.004 min
Response: 470758
Conc: 23.69 ng/ml

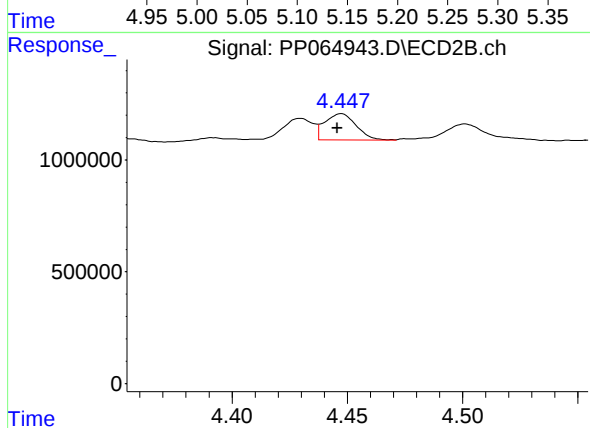

#12 AR-1232-2


R.T.: 4.447 min
Delta R.T.: 0.002 min
Response: 1096545
Conc: 20.88 ng/ml

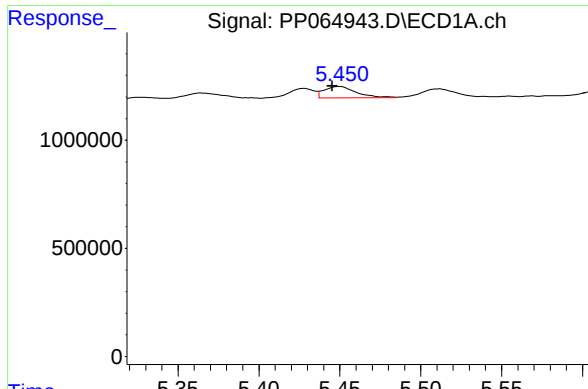

#13 AR-1232-3


R.T.: 5.450 min
Delta R.T.: 0.005 min
Response: 723082
Conc: 21.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

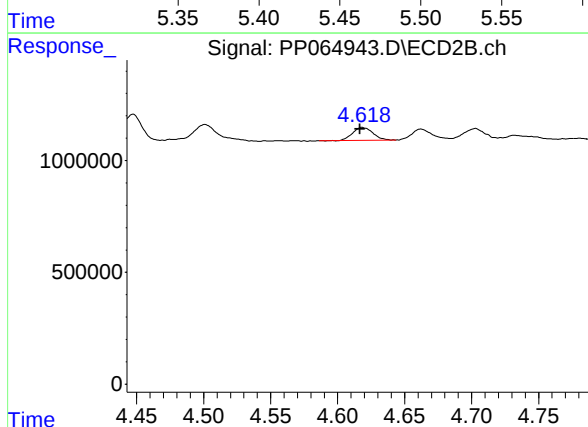


#13 AR-1232-3

R.T.: 4.618 min
Delta R.T.: 0.002 min
Response: 603753
Conc: 20.92 ng/ml

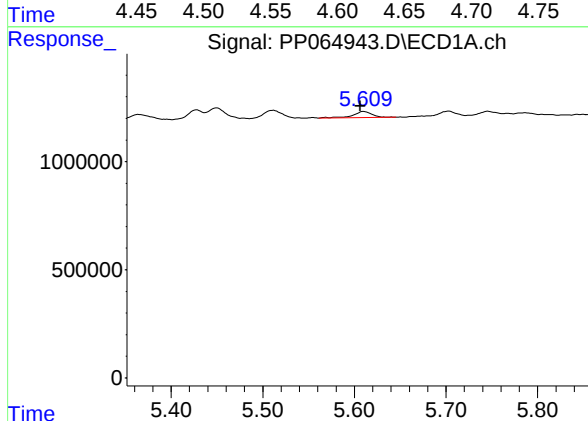


#14 AR-1232-4

R.T.: 5.610 min
Delta R.T.: 0.004 min
Response: 405020
Conc: 24.48 ng/ml

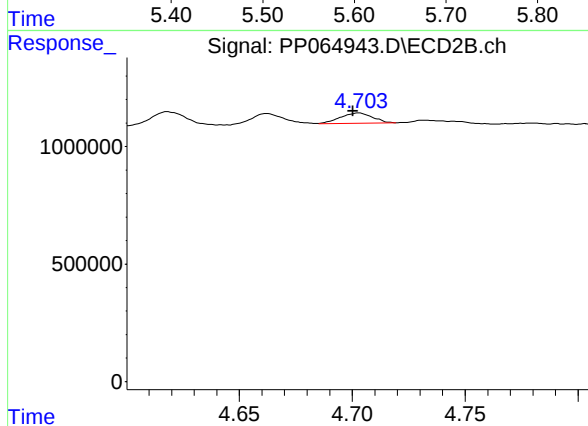

#14 AR-1232-4


R.T.: 4.703 min
Delta R.T.: 0.003 min
Response: 439754
Conc: 16.21 ng/ml

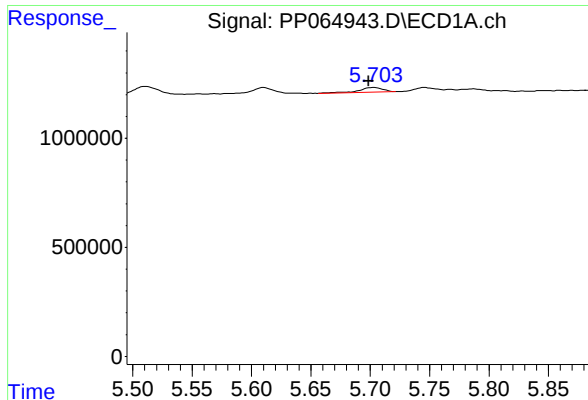

#15 AR-1232-5


R.T.: 5.703 min
Delta R.T.: 0.004 min
Response: 306909
Conc: 22.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

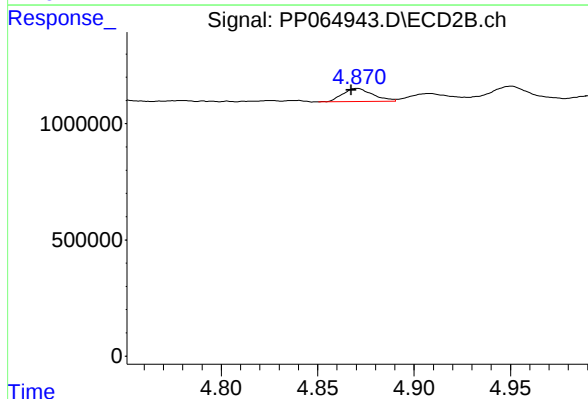


#15 AR-1232-5

R.T.: 4.870 min
Delta R.T.: 0.003 min
Response: 620395
Conc: 21.71 ng/ml

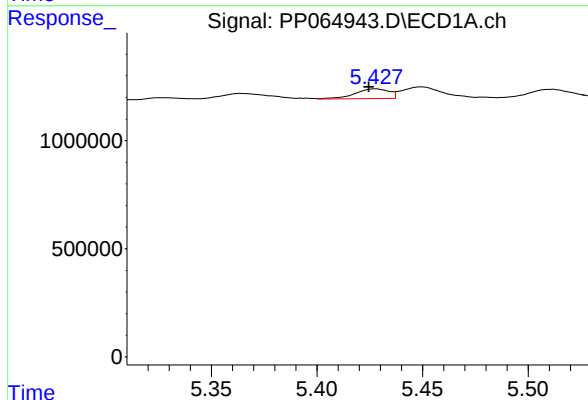


#16 AR-1242-1

R.T.: 5.428 min
Delta R.T.: 0.003 min
Response: 501276
Conc: 14.33 ng/ml

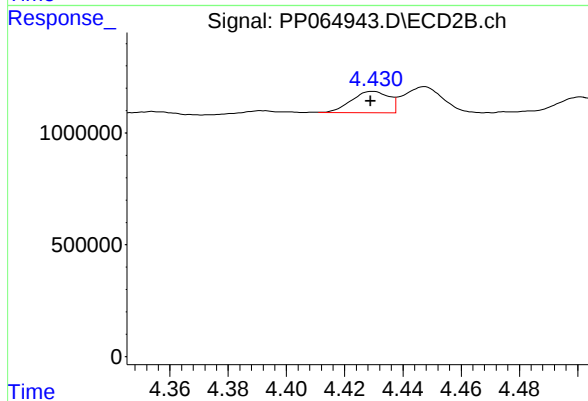

#16 AR-1242-1


R.T.: 4.430 min
Delta R.T.: 0.000 min
Response: 847792
Conc: 12.66 ng/ml

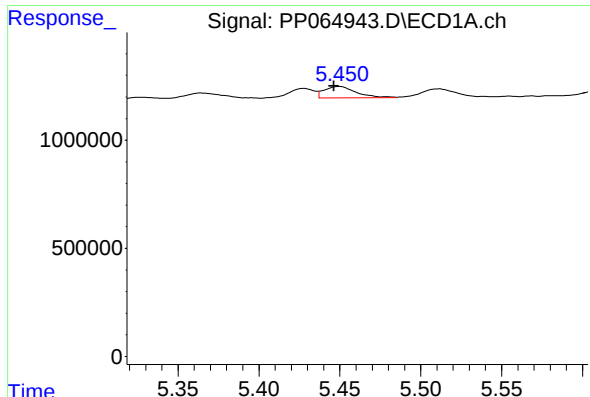

#17 AR-1242-2


R.T.: 5.450 min
Delta R.T.: 0.003 min
Response: 723082
Conc: 13.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

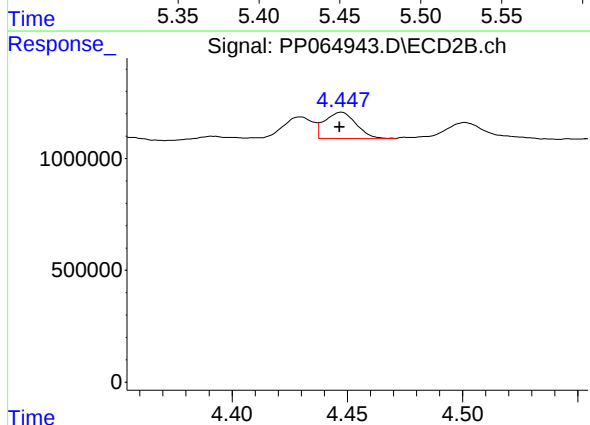


#17 AR-1242-2

R.T.: 4.447 min
Delta R.T.: 0.000 min
Response: 1096545
Conc: 11.86 ng/ml

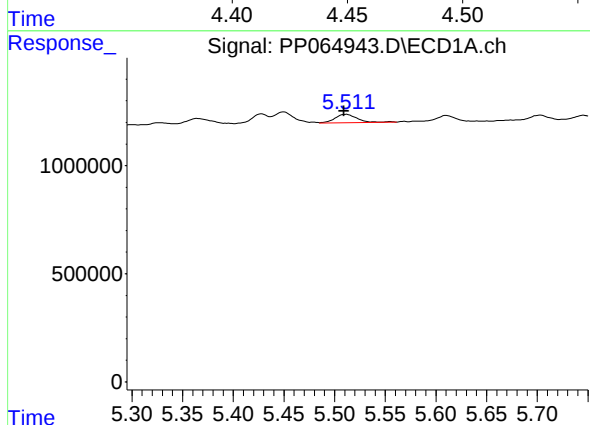


#18 AR-1242-3

R.T.: 5.511 min
Delta R.T.: 0.002 min
Response: 583084
Conc: 17.38 ng/ml

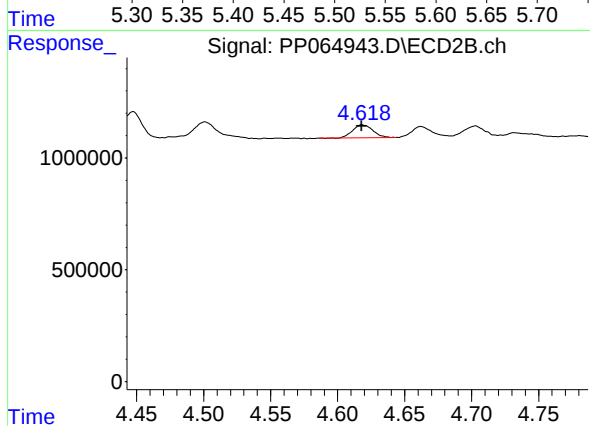

#18 AR-1242-3


R.T.: 4.618 min
Delta R.T.: 0.000 min
Response: 603753
Conc: 11.78 ng/ml

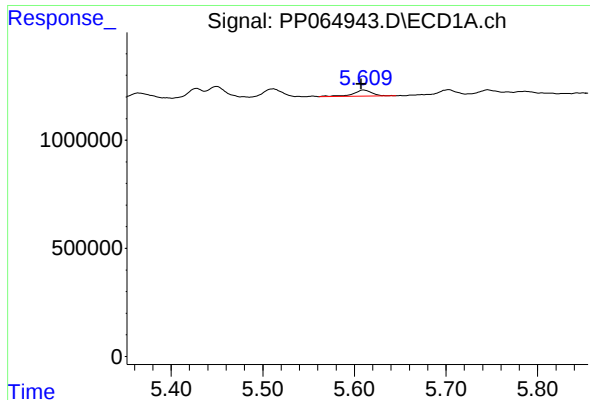

#19 AR-1242-4


R.T.: 5.610 min
Delta R.T.: 0.003 min
Response: 405020
Conc: 15.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

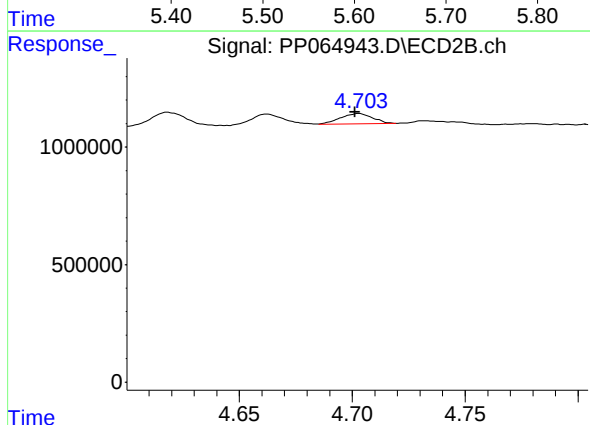


#19 AR-1242-4

R.T.: 4.703 min
Delta R.T.: 0.002 min
Response: 439754
Conc: 8.36 ng/ml

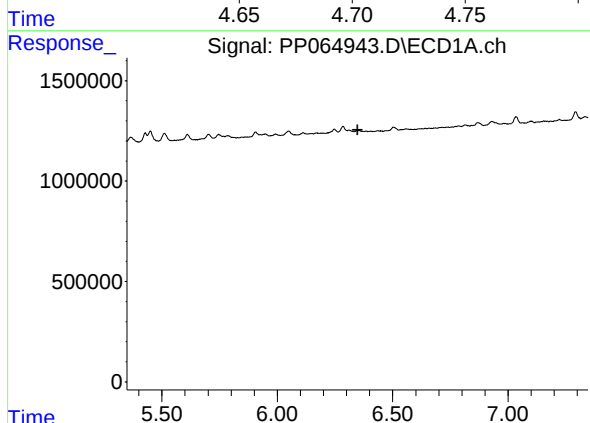


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 6.347 min
Response: 0
Conc: N.D.

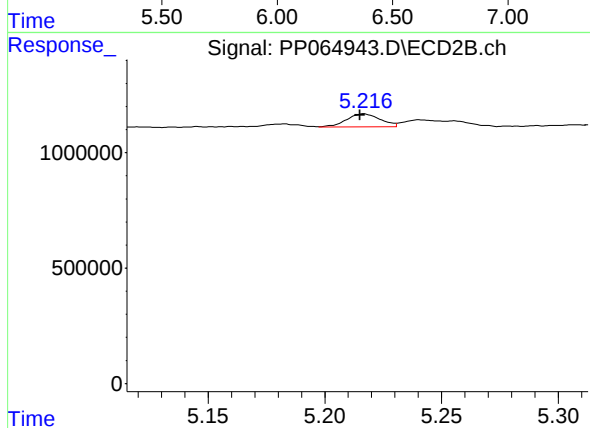

#20 AR-1242-5


R.T.: 5.217 min
Delta R.T.: 0.002 min
Response: 565503
Conc: 9.38 ng/ml

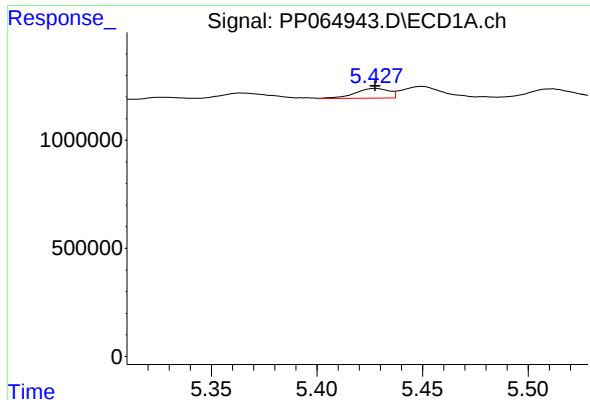

#21 AR-1248-1


R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 501276
Conc: 19.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

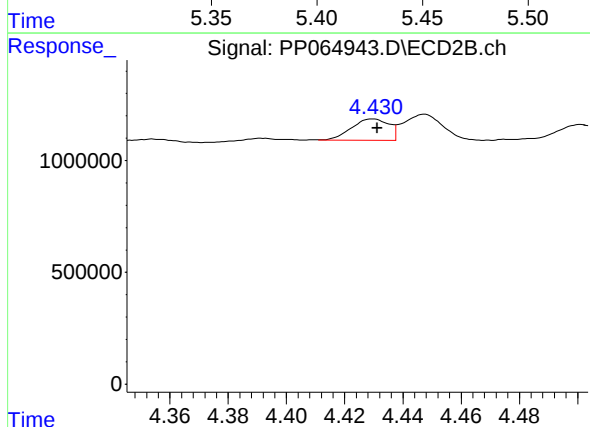


#21 AR-1248-1

R.T.: 4.430 min
Delta R.T.: -0.002 min
Response: 847792
Conc: 17.15 ng/ml

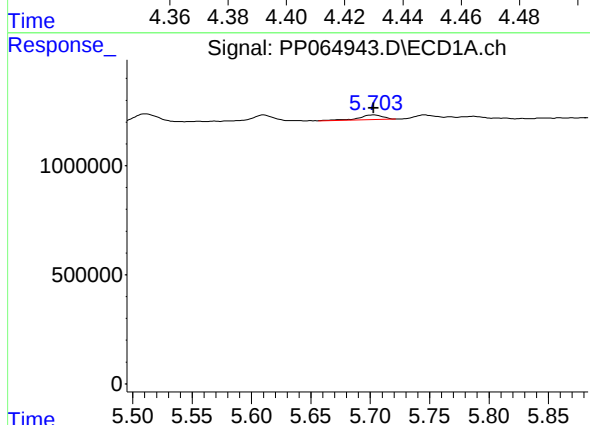


#22 AR-1248-2

R.T.: 5.703 min
Delta R.T.: 0.000 min
Response: 306909
Conc: 7.88 ng/ml

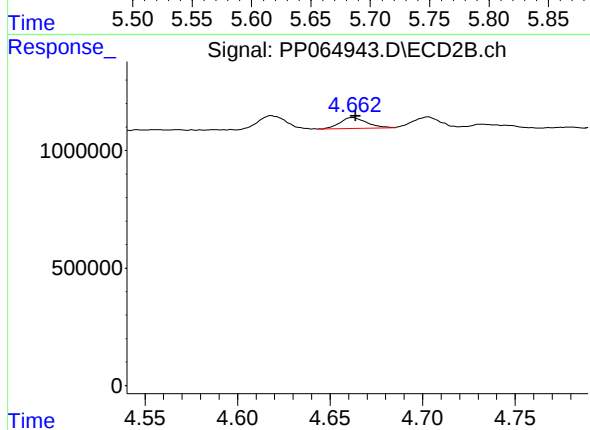

#22 AR-1248-2


R.T.: 4.662 min
Delta R.T.: -0.002 min
Response: 463654
Conc: 6.43 ng/ml

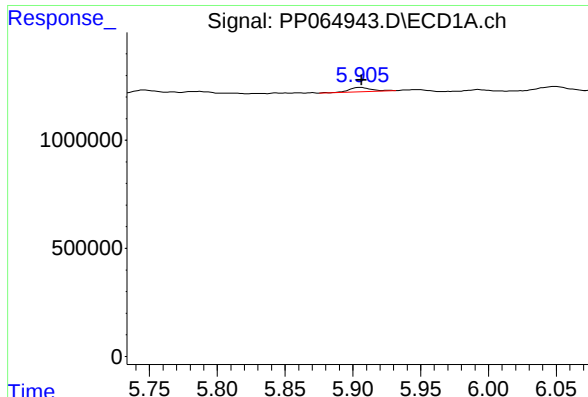

#23 AR-1248-3


R.T.: 5.906 min
Delta R.T.: 0.000 min
Response: 216875
Conc: 5.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

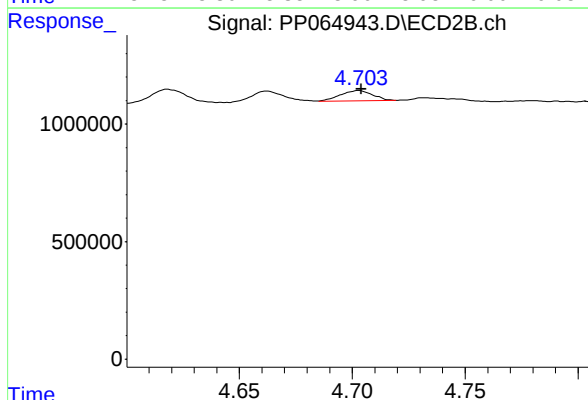


#23 AR-1248-3

R.T.: 4.703 min
Delta R.T.: -0.001 min
Response: 439754
Conc: 5.77 ng/ml

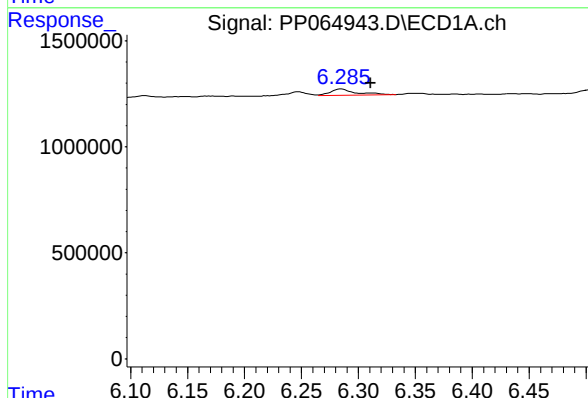


#24 AR-1248-4

R.T.: 6.285 min
Delta R.T.: -0.026 min
Response: 461698
Conc: 12.06 ng/ml

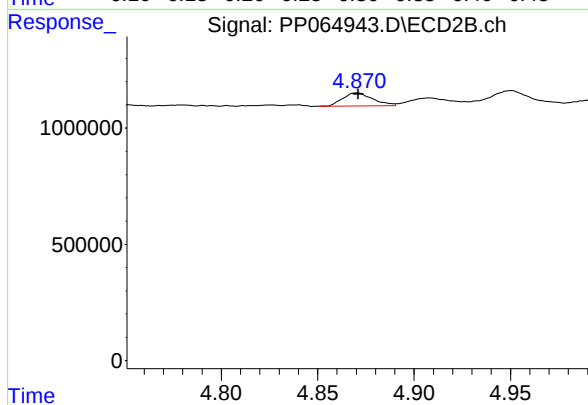

#24 AR-1248-4


R.T.: 4.870 min
Delta R.T.: 0.000 min
Response: 620395
Conc: 7.02 ng/ml

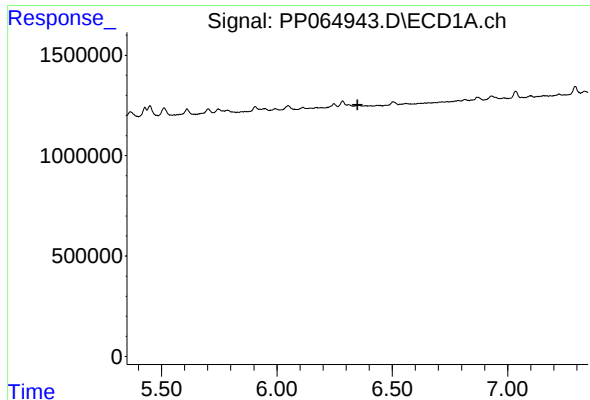

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.349 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

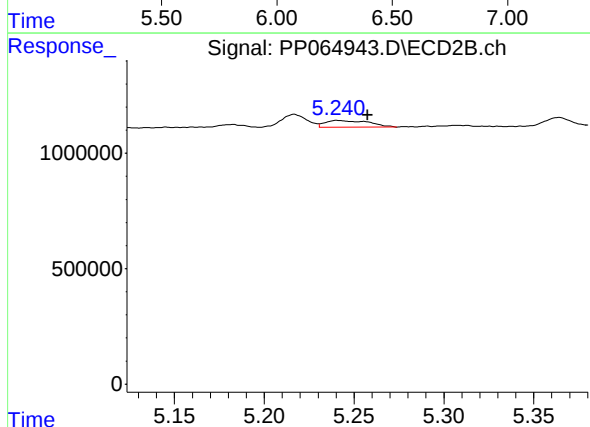


#25 AR-1248-5

R.T.: 5.241 min
Delta R.T.: -0.017 min
Response: 498444
Conc: 6.05 ng/ml

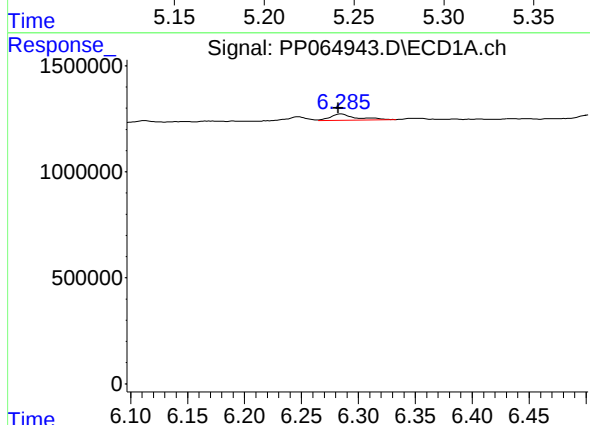


#26 AR-1254-1

R.T.: 6.285 min
Delta R.T.: 0.003 min
Response: 461698
Conc: 10.77 ng/ml

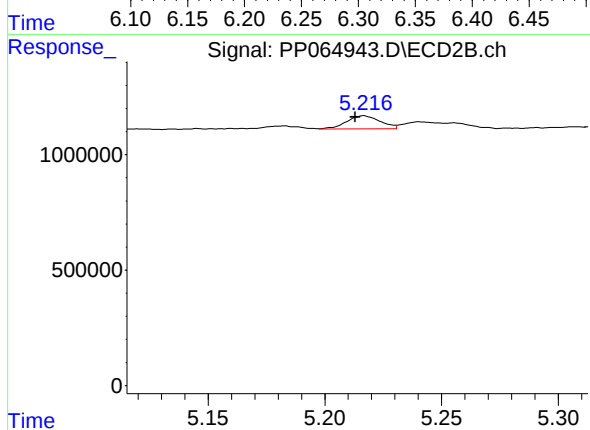

#26 AR-1254-1


R.T.: 5.217 min
Delta R.T.: 0.004 min
Response: 565503
Conc: 4.32 ng/ml

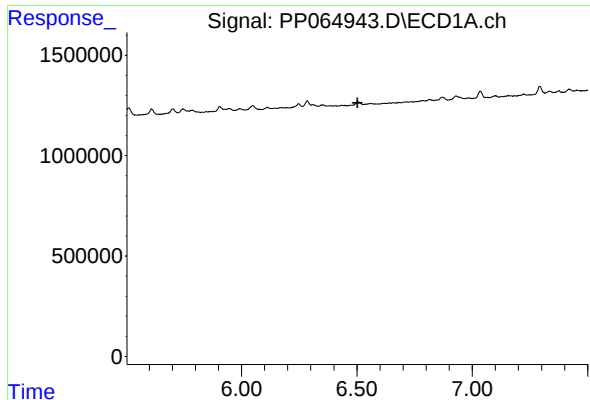

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

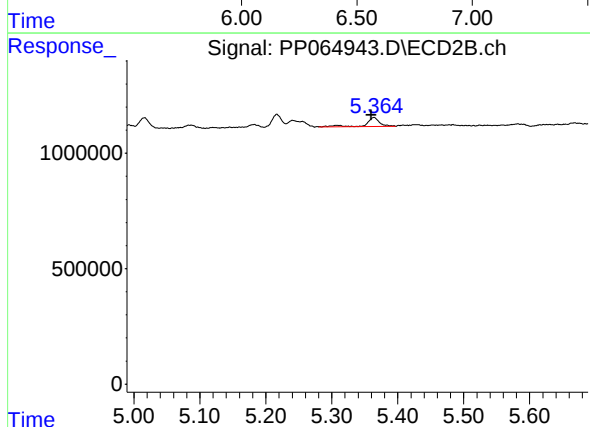


#27 AR-1254-2

R.T.: 5.364 min
Delta R.T.: 0.004 min
Response: 568908
Conc: 5.01 ng/ml

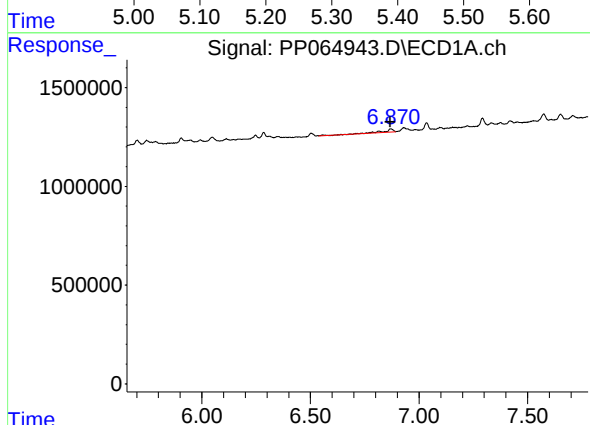


#28 AR-1254-3

R.T.: 6.869 min
Delta R.T.: 0.001 min
Response: 528579
Conc: 8.34 ng/ml

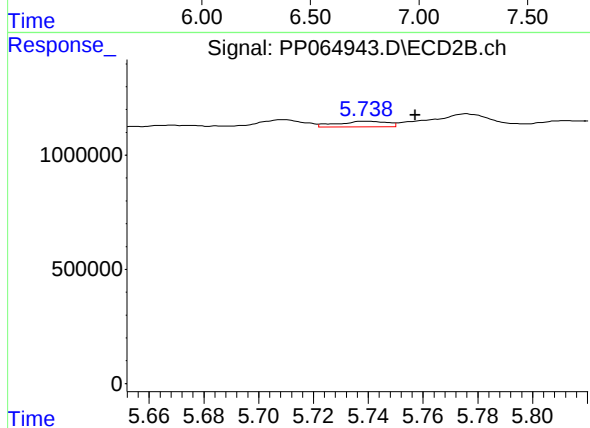

#28 AR-1254-3


R.T.: 5.739 min
Delta R.T.: -0.018 min
Response: 304286
Conc: 1.72 ng/ml

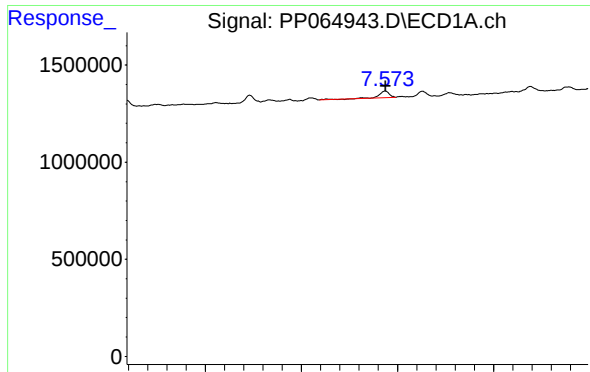

#30 AR-1254-5


R.T.: 7.574 min
Delta R.T.: 0.000 min
Response: 501511
Conc: 11.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

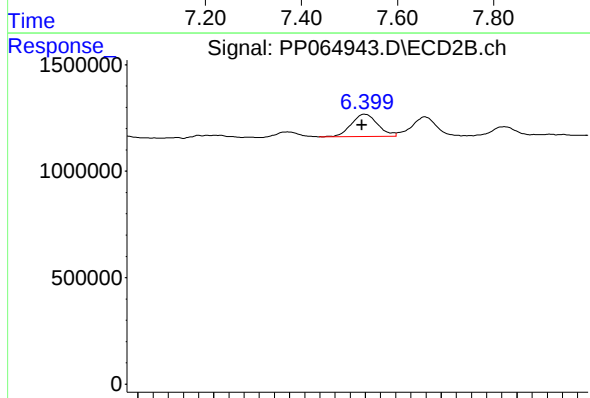


#30 AR-1254-5

R.T.: 6.400 min
Delta R.T.: 0.002 min
Response: 1295275
Conc: 8.62 ng/ml

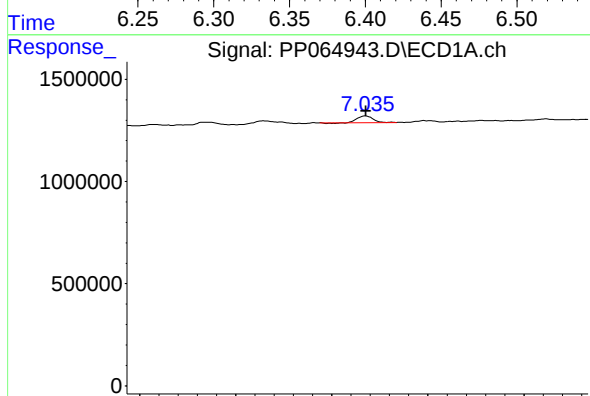


#31 AR-1260-1

R.T.: 7.035 min
Delta R.T.: 0.000 min
Response: 378746
Conc: 7.59 ng/ml

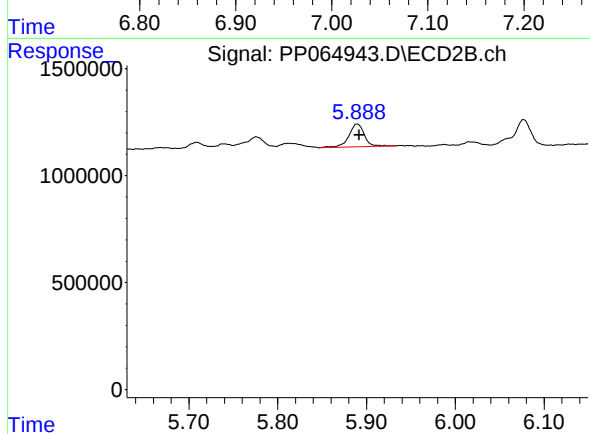

#31 AR-1260-1


R.T.: 5.889 min
Delta R.T.: -0.002 min
Response: 1285780
Conc: 10.70 ng/ml

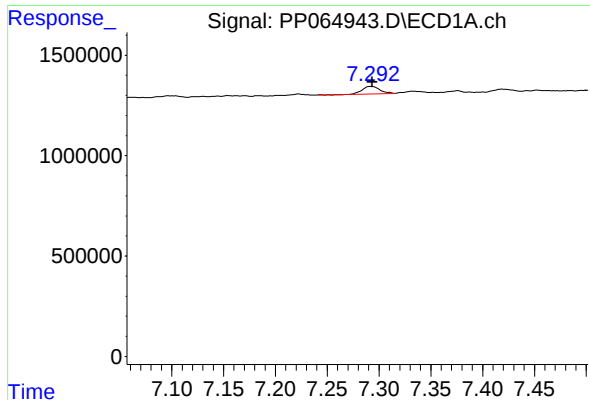

#32 AR-1260-2


R.T.: 7.293 min
Delta R.T.: 0.000 min
Response: 417784
Conc: 8.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

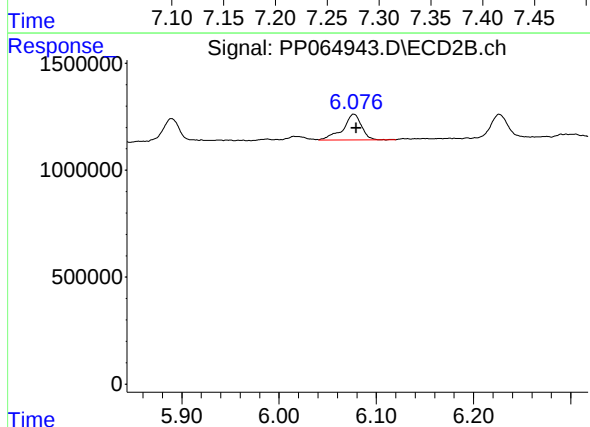


#32 AR-1260-2

R.T.: 6.077 min
Delta R.T.: -0.002 min
Response: 1589900
Conc: 11.75 ng/ml

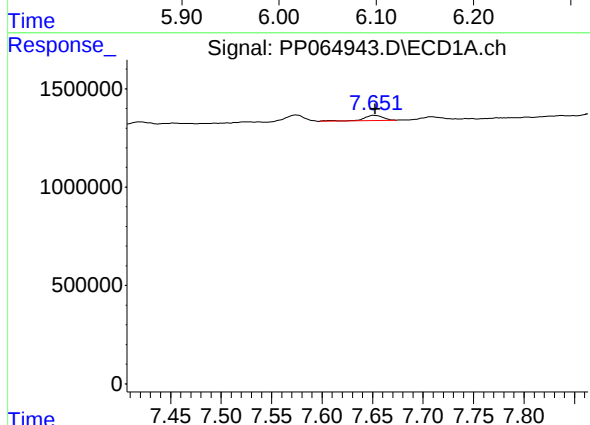


#33 AR-1260-3

R.T.: 7.652 min
Delta R.T.: 0.000 min
Response: 354715
Conc: 9.15 ng/ml

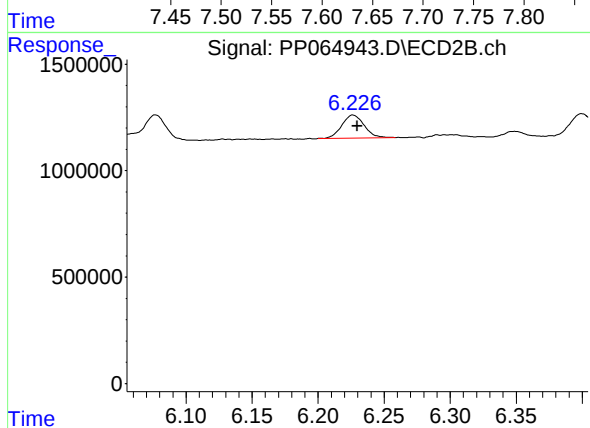

#33 AR-1260-3


R.T.: 6.226 min
Delta R.T.: -0.003 min
Response: 1282960
Conc: 9.69 ng/ml

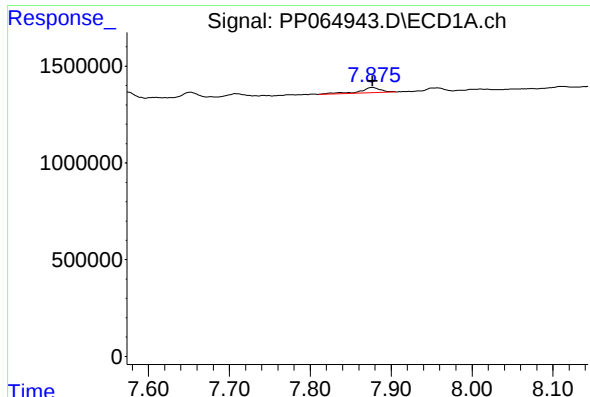

#34 AR-1260-4


R.T.: 7.877 min
Delta R.T.: 0.000 min
Response: 479666
Conc: 10.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

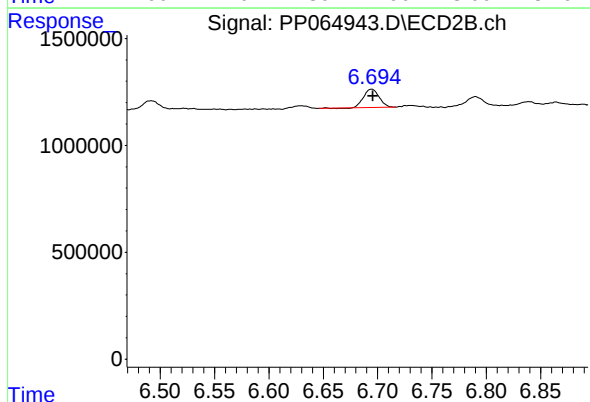


#34 AR-1260-4

R.T.: 6.694 min
Delta R.T.: -0.001 min
Response: 838208
Conc: 7.88 ng/ml

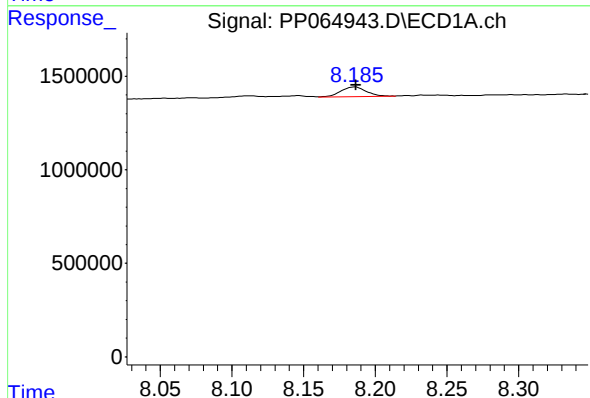


#35 AR-1260-5

R.T.: 8.186 min
Delta R.T.: 0.000 min
Response: 628798
Conc: 8.67 ng/ml

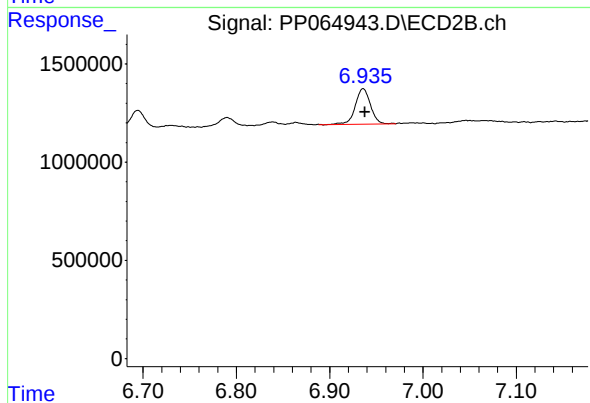

#35 AR-1260-5


R.T.: 6.936 min
Delta R.T.: -0.002 min
Response: 2040176
Conc: 8.81 ng/ml

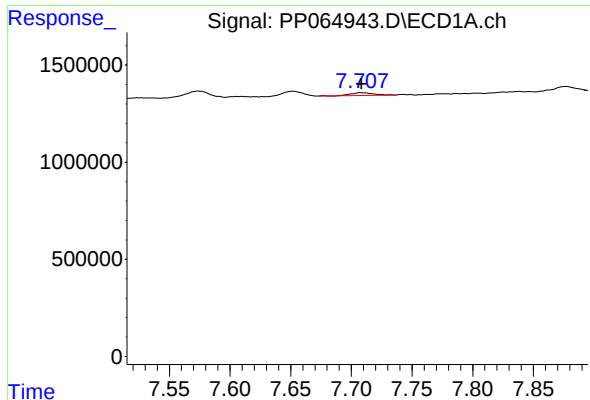

#36 AR-1262-1


R.T.: 7.709 min
Delta R.T.: 0.000 min
Response: 194660
Conc: 7.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

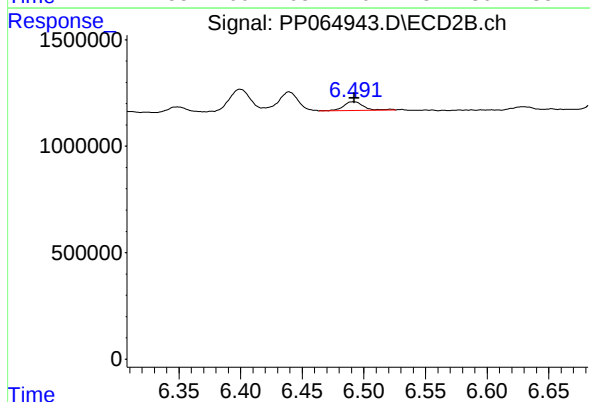


#36 AR-1262-1

R.T.: 6.492 min
Delta R.T.: 0.000 min
Response: 442264
Conc: 6.23 ng/ml

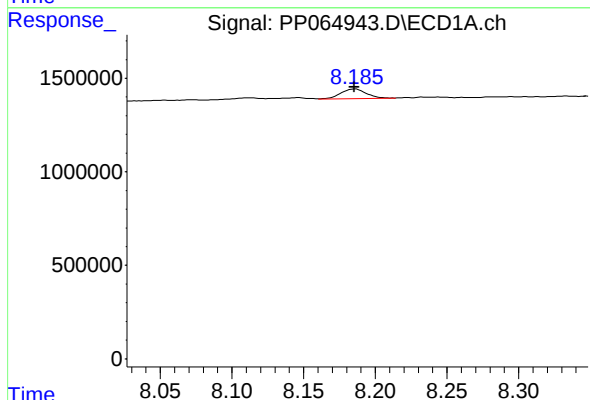


#37 AR-1262-2

R.T.: 8.186 min
Delta R.T.: 0.000 min
Response: 628798
Conc: 7.19 ng/ml

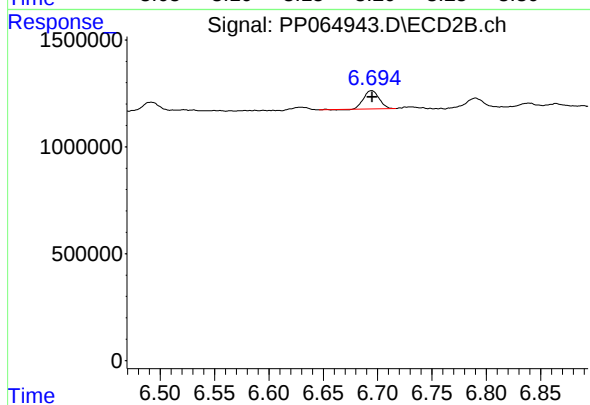

#37 AR-1262-2


R.T.: 6.694 min
Delta R.T.: 0.000 min
Response: 838208
Conc: 5.88 ng/ml

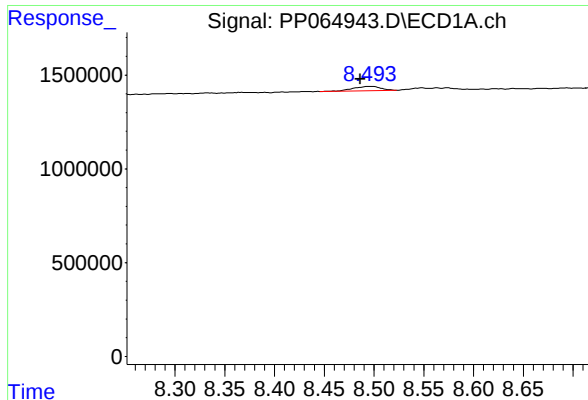

#38 AR-1262-3


R.T.: 8.496 min
Delta R.T.: 0.010 min
Response: 430802
Conc: 6.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

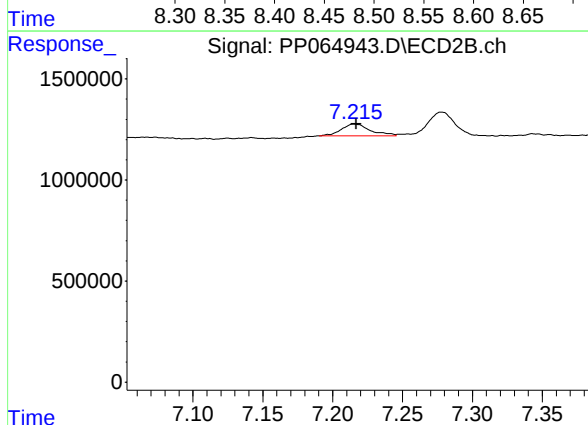


#38 AR-1262-3

R.T.: 7.215 min
Delta R.T.: -0.002 min
Response: 850380
Conc: 8.03 ng/ml

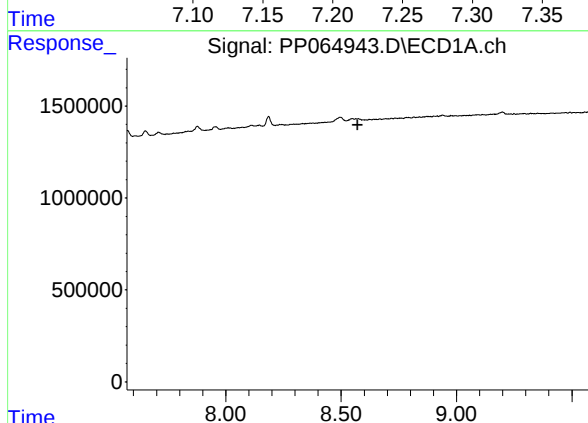


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.570 min
Response: 0
Conc: N.D.

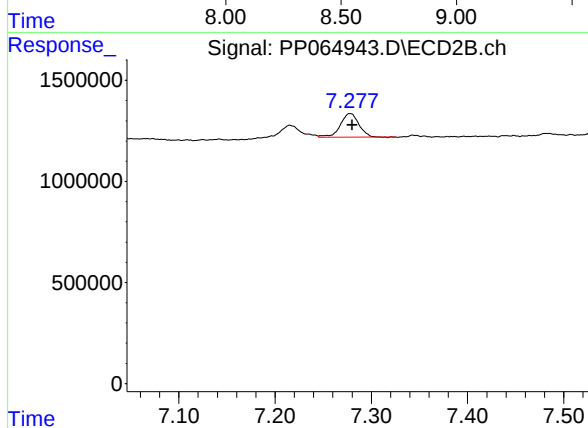

#39 AR-1262-4


R.T.: 7.278 min
Delta R.T.: -0.002 min
Response: 1564780
Conc: 8.12 ng/ml

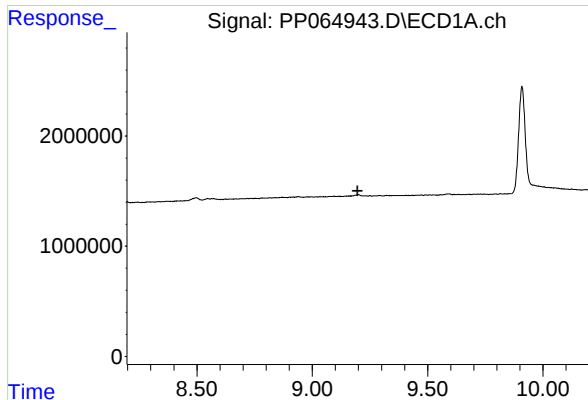

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 9.196 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

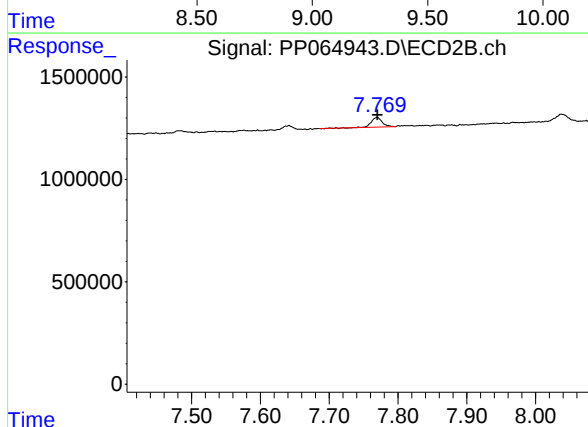


#40 AR-1262-5

R.T.: 7.770 min
Delta R.T.: 0.000 min
Response: 496688
Conc: 5.60 ng/ml

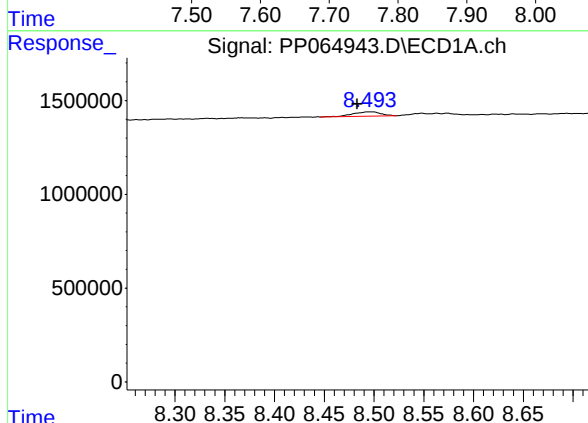


#41 AR-1268-1

R.T.: 8.496 min
Delta R.T.: 0.013 min
Response: 430802
Conc: 4.05 ng/ml

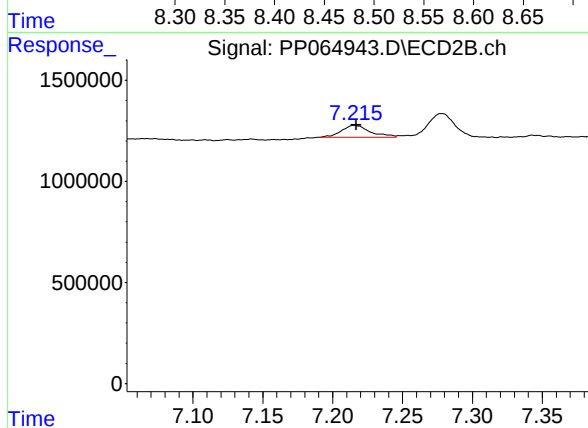

#41 AR-1268-1


R.T.: 7.215 min
Delta R.T.: -0.002 min
Response: 850380
Conc: 2.95 ng/ml

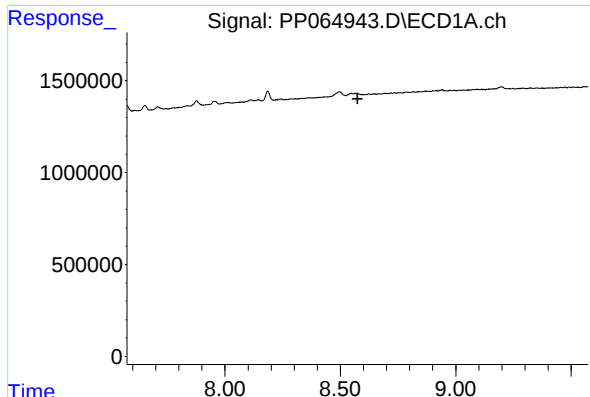

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 8.574 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

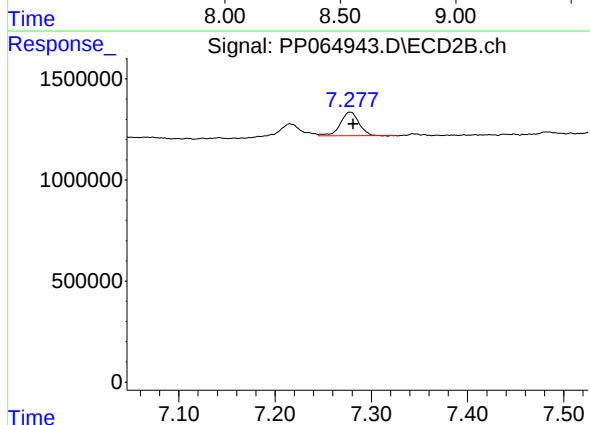


#42 AR-1268-2

R.T.: 7.278 min
Delta R.T.: -0.003 min
Response: 1564780
Conc: 5.91 ng/ml

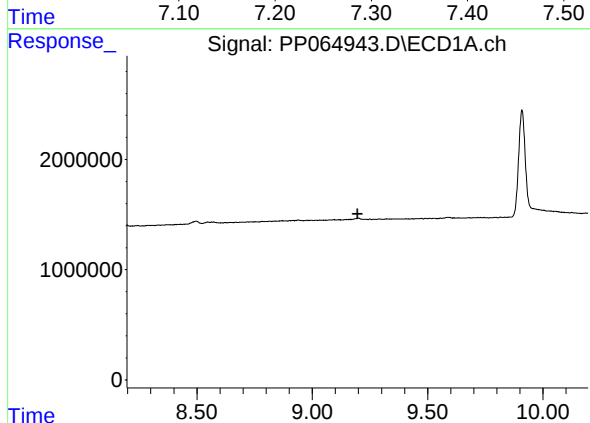


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.196 min
Response: 0
Conc: N.D.

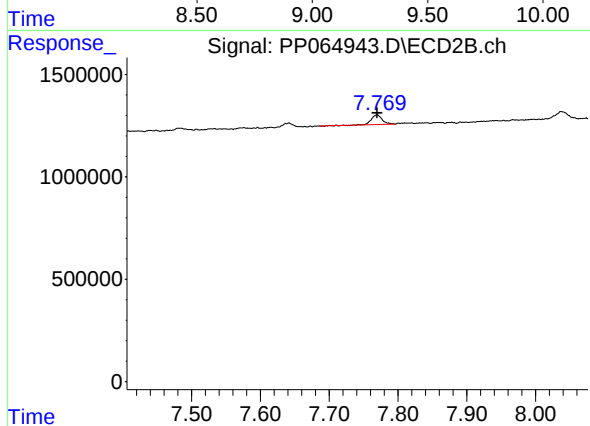

#44 AR-1268-4


R.T.: 7.770 min
Delta R.T.: 0.000 min
Response: 496688
Conc: 5.28 ng/ml

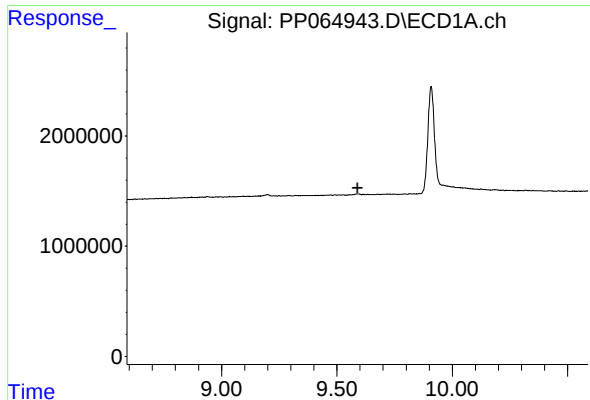

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.589 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT2-2024

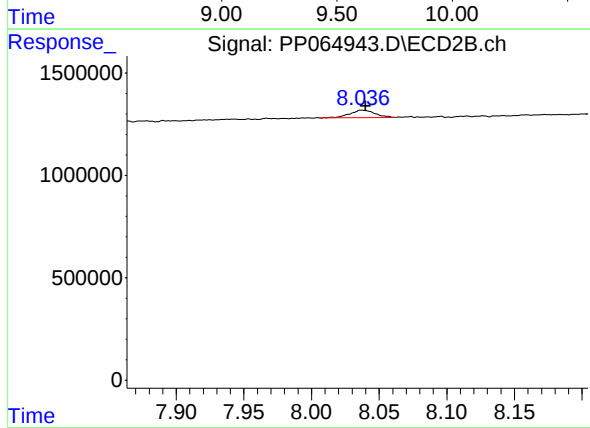

#45 AR-1268-5

R.T.: 8.037 min
Delta R.T.: -0.002 min
Response: 449251
Conc: 0.70 ng/ml