

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051524\
 Data File : PP064965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2024 15:56
 Operator : YP\AJ
 Sample : P2403-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT2-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 01:34:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 14 06:05:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.259	3.372	32179520	42670984	16.920	18.955
2) SA Decachlor...	9.911	8.265	16424621	39741613	22.874	22.690
Target Compounds						
9) L2 AR-1221-2	4.564	3.662	359426	641476	21.567	27.558 #
33) L7 AR-1260-3	7.653	0.000	1337194	0	34.498	N.D. #
34) L7 AR-1260-4	7.898f	6.691	784372	2112900	17.879	19.852
35) L7 AR-1260-5	8.188	6.935	409980	823019	5.655	3.554 #
37) L8 AR-1262-2	8.188	6.691	409980	2112900	4.688	14.834 #
38) L8 AR-1262-3	8.486	7.215	3094410	8428745	49.764	79.595 #
39) L8 AR-1262-4	8.575	7.280	2678164	7505884	55.009	38.963 #
40) L8 AR-1262-5	9.198	7.769	920287	2726738	29.486	30.764
41) L9 AR-1268-1	8.486	7.215	3094410	8428745	29.059	29.278
42) L9 AR-1268-2	8.575	7.280	2678164	7505884	28.675	28.363
43) L9 AR-1268-3	8.794	7.483	2442654	6748020	28.485	28.737
44) L9 AR-1268-4	9.198	7.769	920287	2726738	27.765	28.998
45) L9 AR-1268-5	9.591	8.039	6820513	18228440	31.019	28.461



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051524\
Data File : PP064965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2024 15:56
Operator : YP\AJ
Sample : P2403-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 01:34:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051324.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 14 06:05:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

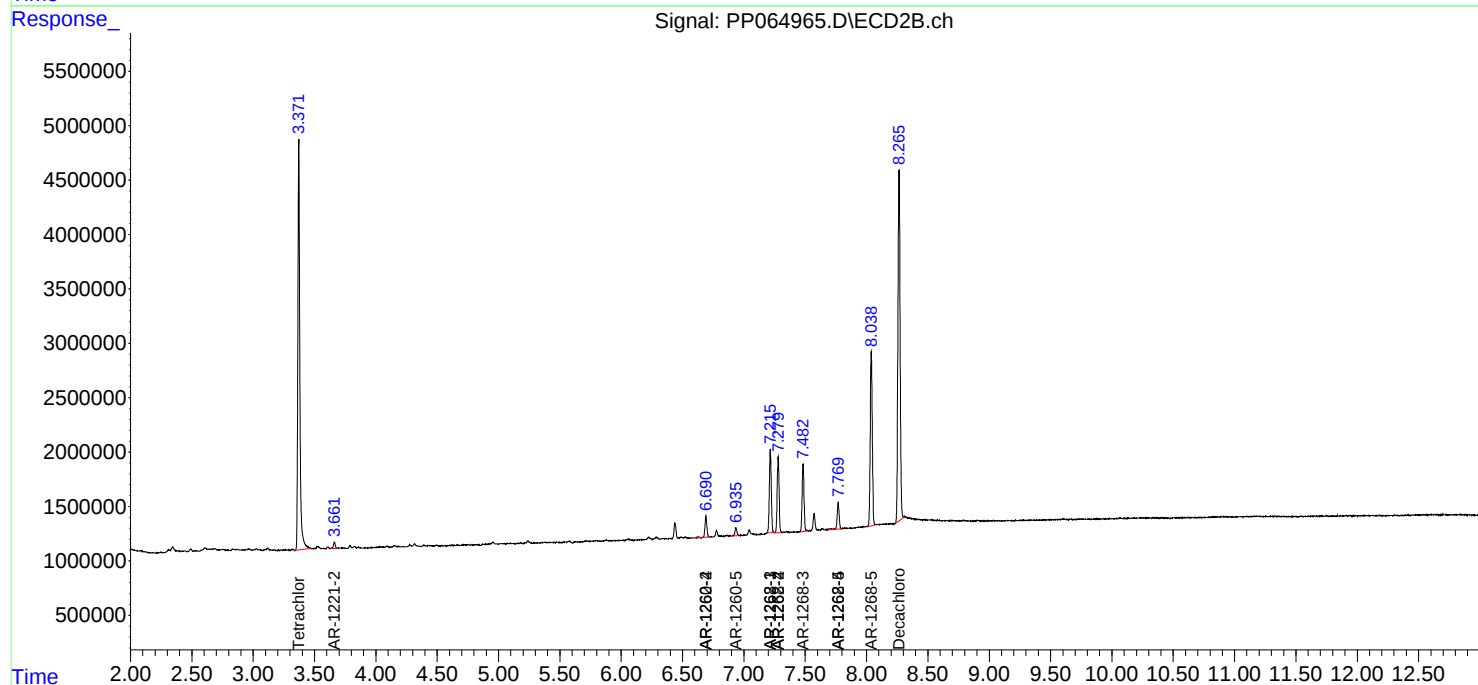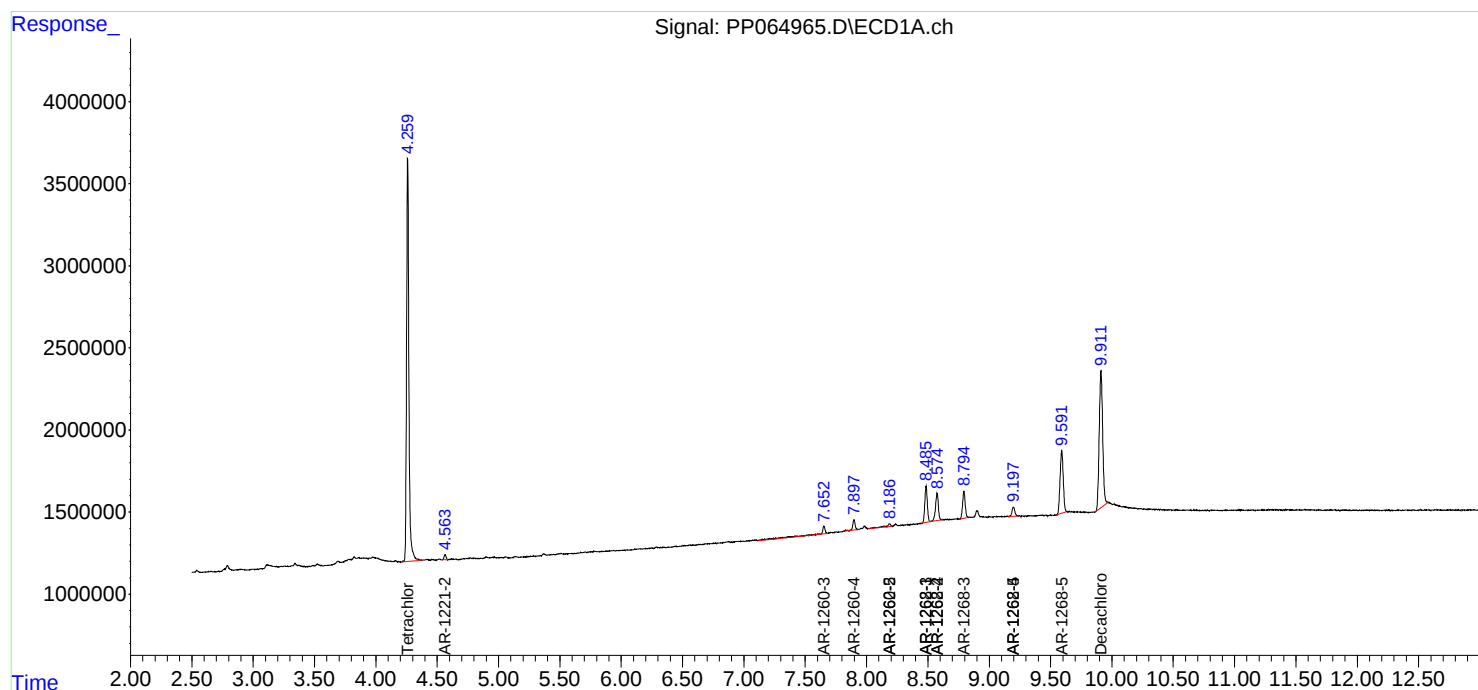


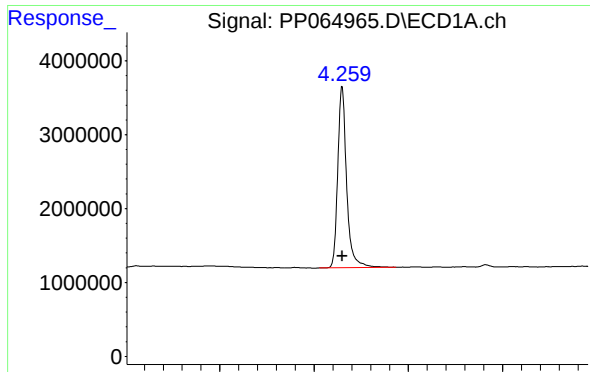

#1 Tetrachloro-m-xylene


R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 32179520
Conc: 16.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2024

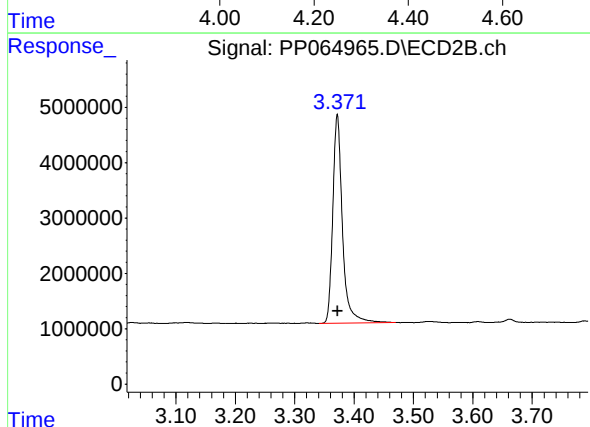


#1 Tetrachloro-m-xylene

R.T.: 3.372 min
Delta R.T.: 0.000 min
Response: 42670984
Conc: 18.96 ng/ml

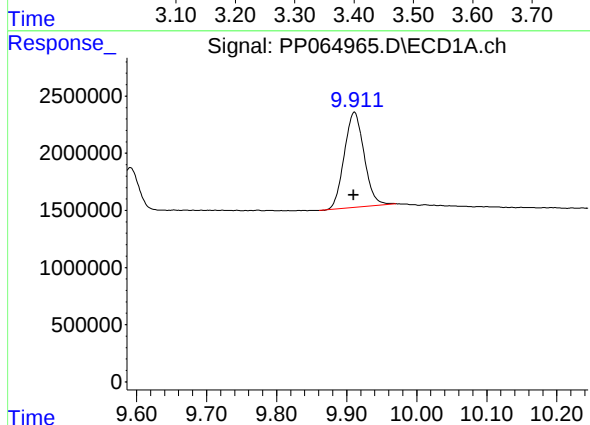


#2 Decachlorobiphenyl

R.T.: 9.911 min
Delta R.T.: 0.001 min
Response: 16424621
Conc: 22.87 ng/ml

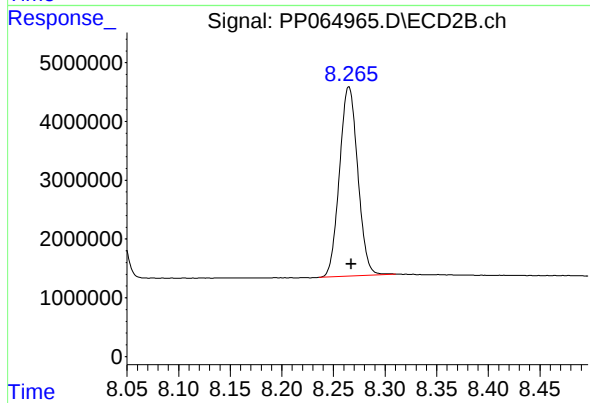

#2 Decachlorobiphenyl


R.T.: 8.265 min
Delta R.T.: -0.002 min
Response: 39741613
Conc: 22.69 ng/ml

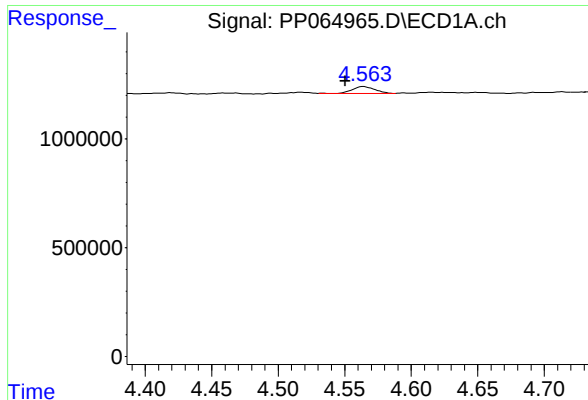

#9 AR-1221-2


R.T.: 4.564 min
Delta R.T.: 0.014 min
Response: 359426
Conc: 21.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2024

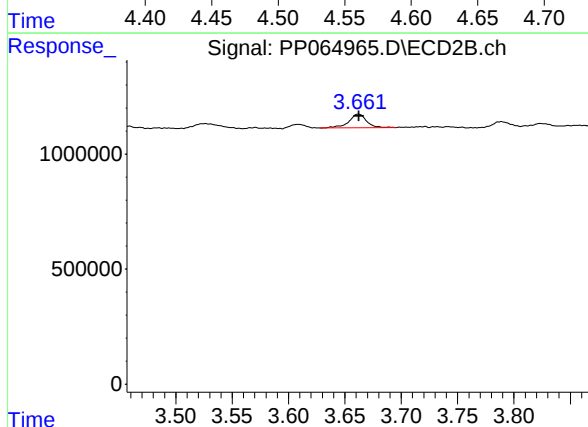


#9 AR-1221-2

R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 641476
Conc: 27.56 ng/ml

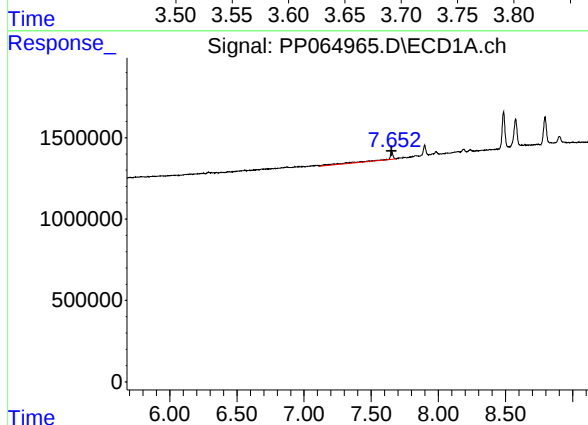


#33 AR-1260-3

R.T.: 7.653 min
Delta R.T.: 0.000 min
Response: 1337194
Conc: 34.50 ng/ml

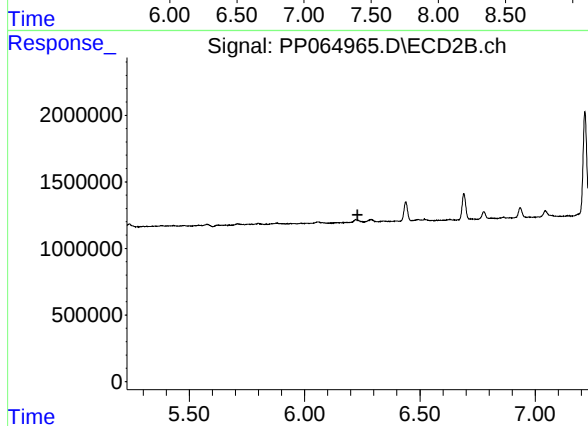

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 6.230 min
Response: 0
Conc: N.D.

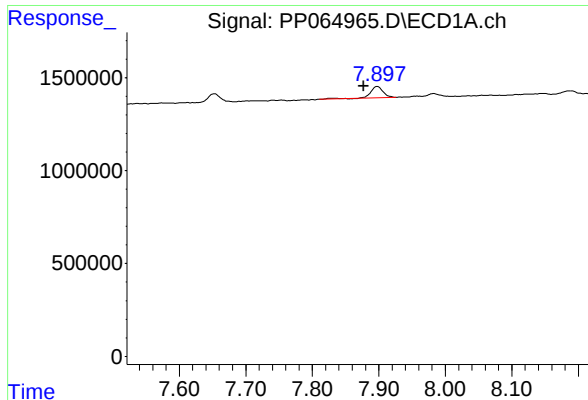

#34 AR-1260-4


R.T.: 7.898 min
Delta R.T.: 0.021 min
Response: 784372
Conc: 17.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2024

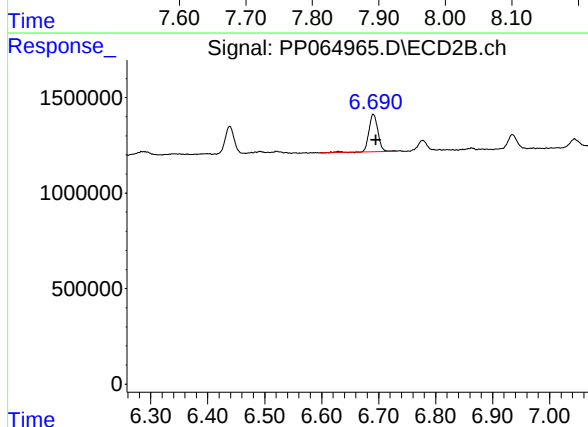


#34 AR-1260-4

R.T.: 6.691 min
Delta R.T.: -0.005 min
Response: 2112900
Conc: 19.85 ng/ml

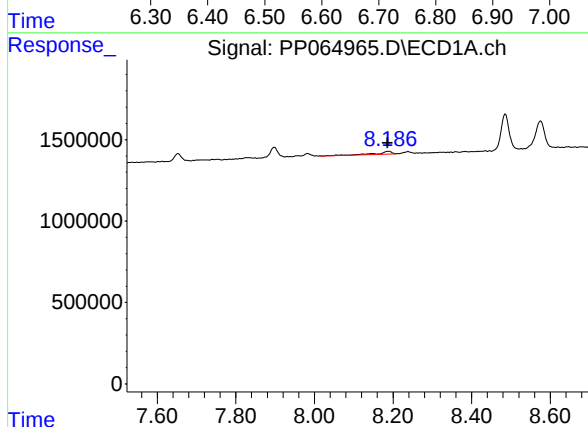


#35 AR-1260-5

R.T.: 8.188 min
Delta R.T.: 0.001 min
Response: 409980
Conc: 5.65 ng/ml

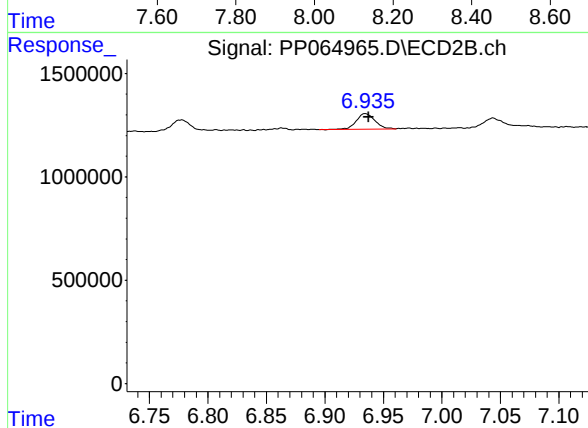

#35 AR-1260-5


R.T.: 6.935 min
Delta R.T.: -0.003 min
Response: 823019
Conc: 3.55 ng/ml

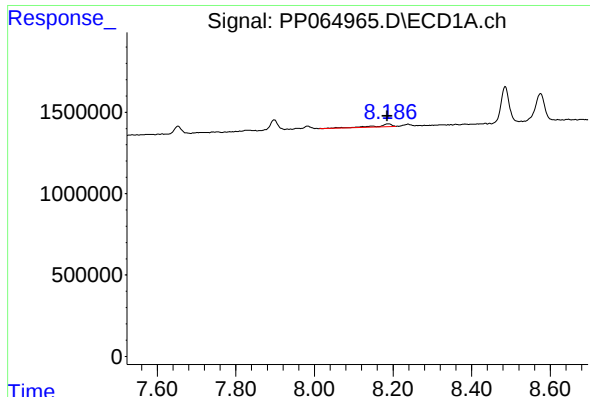

#37 AR-1262-2


R.T.: 8.188 min
Delta R.T.: 0.002 min
Response: 409980
Conc: 4.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2024

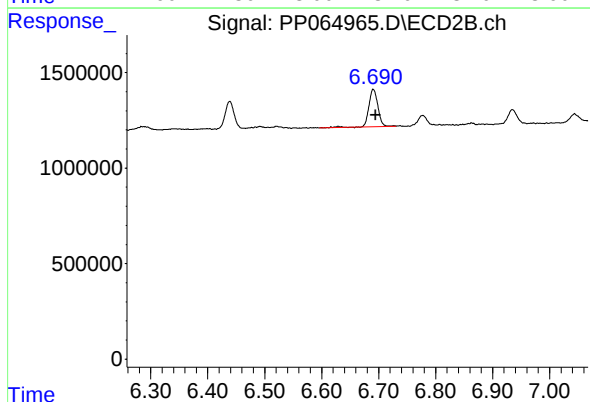


#37 AR-1262-2

R.T.: 6.691 min
Delta R.T.: -0.004 min
Response: 2112900
Conc: 14.83 ng/ml

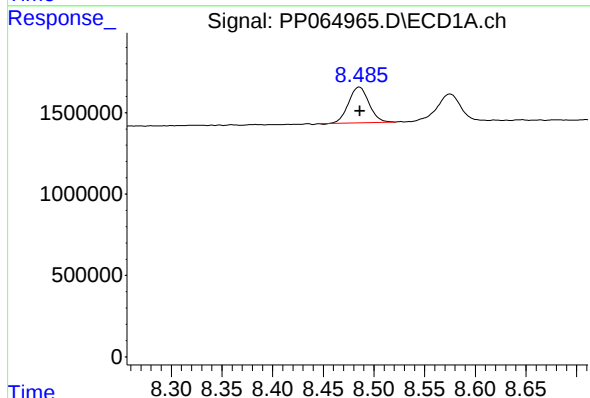


#38 AR-1262-3

R.T.: 8.486 min
Delta R.T.: 0.000 min
Response: 3094410
Conc: 49.76 ng/ml

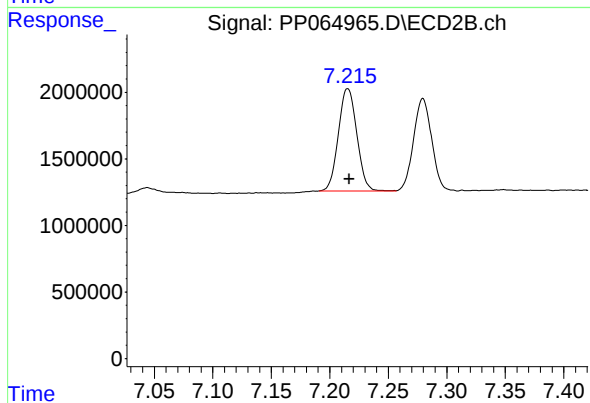

#38 AR-1262-3


R.T.: 7.215 min
Delta R.T.: -0.001 min
Response: 8428745
Conc: 79.60 ng/ml

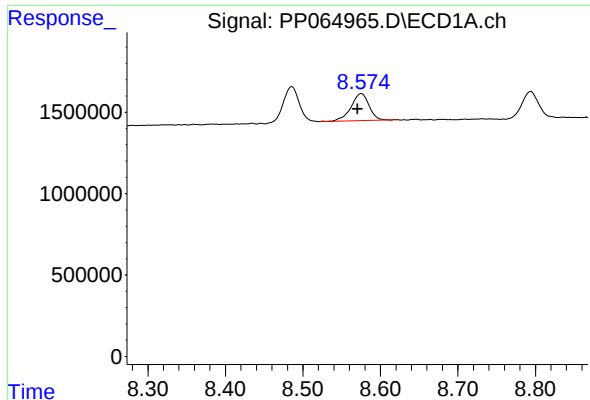

#39 AR-1262-4


R.T.: 8.575 min
Delta R.T.: 0.005 min
Response: 2678164
Conc: 55.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2024

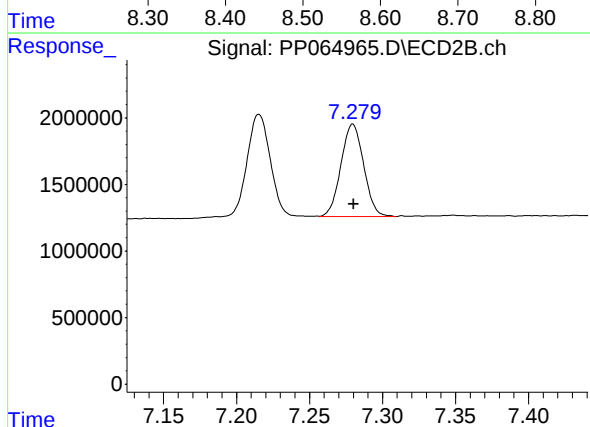


#39 AR-1262-4

R.T.: 7.280 min
Delta R.T.: 0.000 min
Response: 7505884
Conc: 38.96 ng/ml

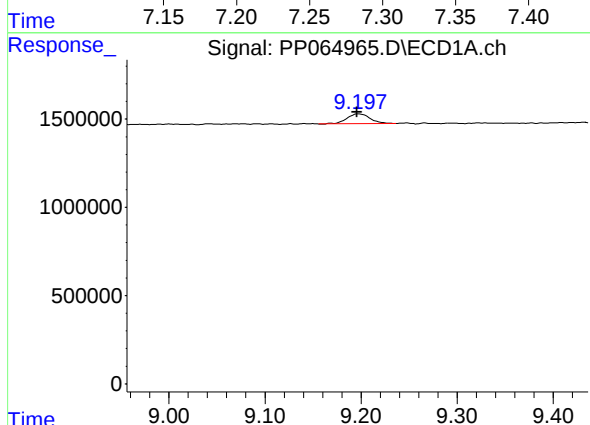


#40 AR-1262-5

R.T.: 9.198 min
Delta R.T.: 0.002 min
Response: 920287
Conc: 29.49 ng/ml

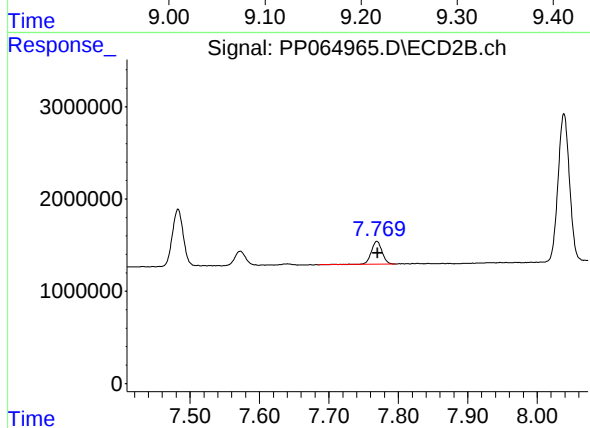

#40 AR-1262-5


R.T.: 7.769 min
Delta R.T.: -0.001 min
Response: 2726738
Conc: 30.76 ng/ml

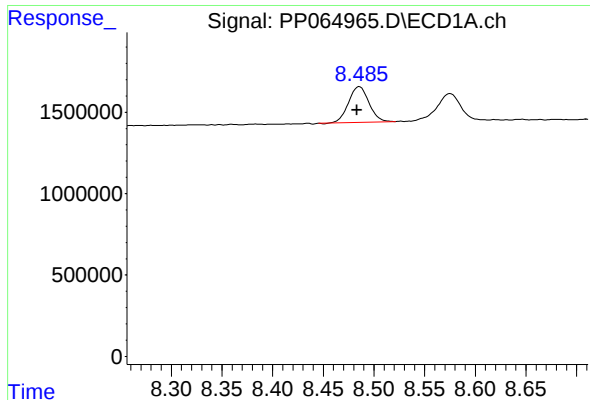

#41 AR-1268-1


R.T.: 8.486 min
Delta R.T.: 0.002 min
Response: 3094410
Conc: 29.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2024

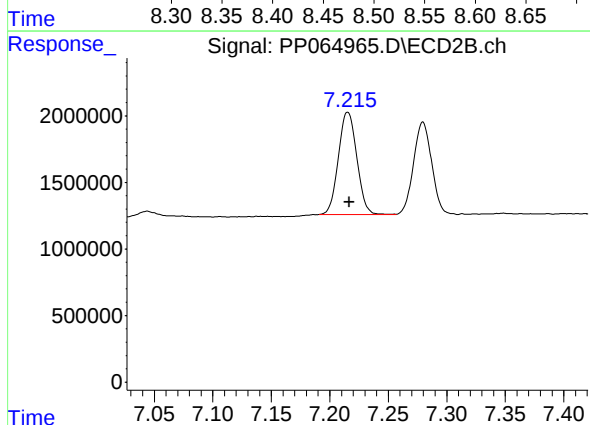


#41 AR-1268-1

R.T.: 7.215 min
Delta R.T.: -0.001 min
Response: 8428745
Conc: 29.28 ng/ml

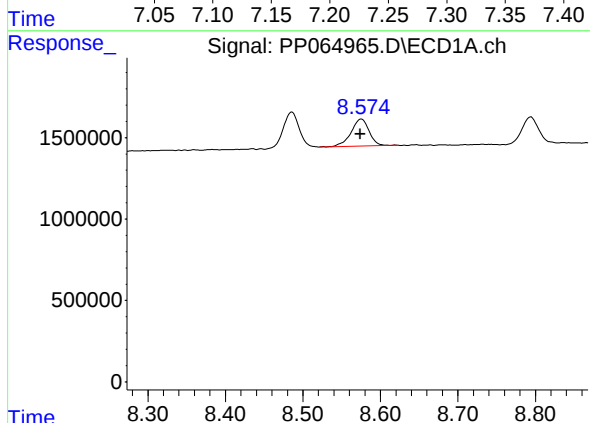


#42 AR-1268-2

R.T.: 8.575 min
Delta R.T.: 0.001 min
Response: 2678164
Conc: 28.67 ng/ml

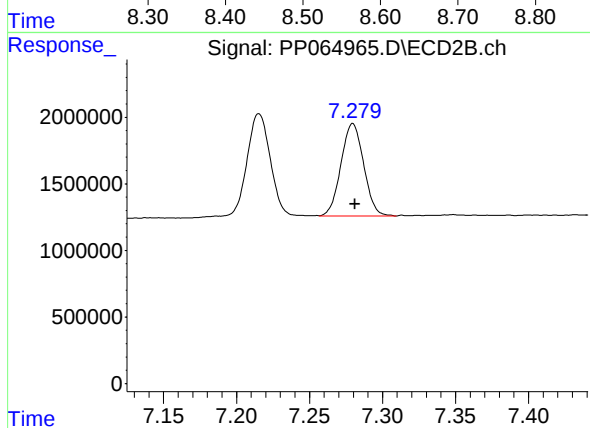

#42 AR-1268-2


R.T.: 7.280 min
Delta R.T.: -0.002 min
Response: 7505884
Conc: 28.36 ng/ml

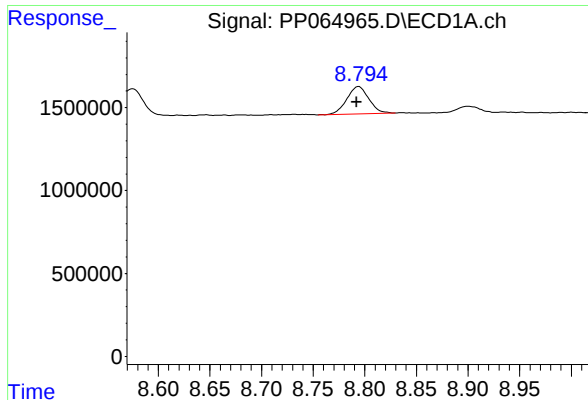

#43 AR-1268-3


R.T.: 8.794 min
Delta R.T.: 0.002 min
Response: 2442654
Conc: 28.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2024

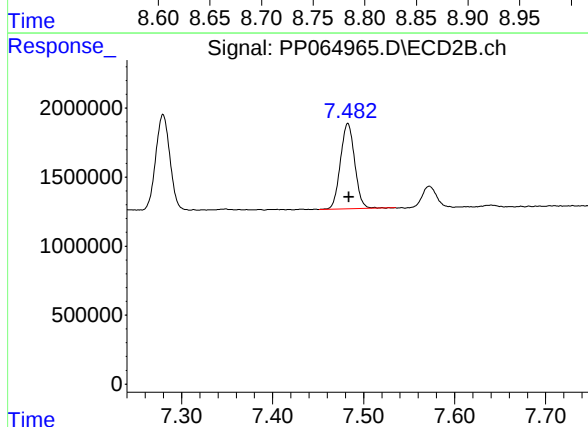


#43 AR-1268-3

R.T.: 7.483 min
Delta R.T.: -0.001 min
Response: 6748020
Conc: 28.74 ng/ml

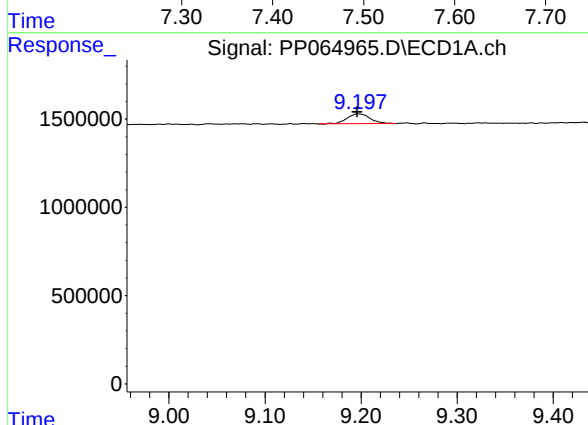


#44 AR-1268-4

R.T.: 9.198 min
Delta R.T.: 0.002 min
Response: 920287
Conc: 27.77 ng/ml

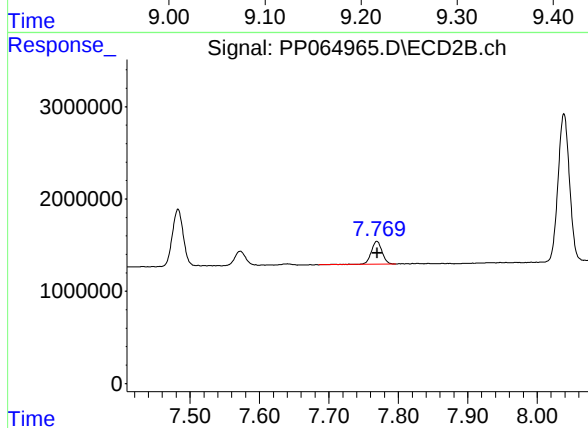

#44 AR-1268-4


R.T.: 7.769 min
Delta R.T.: 0.000 min
Response: 2726738
Conc: 29.00 ng/ml

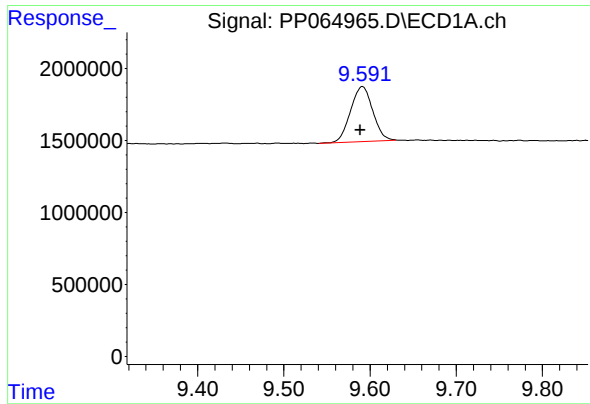

#45 AR-1268-5

R.T.: 9.591 min
Delta R.T.: 0.002 min
Response: 6820513
Conc: 31.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2024

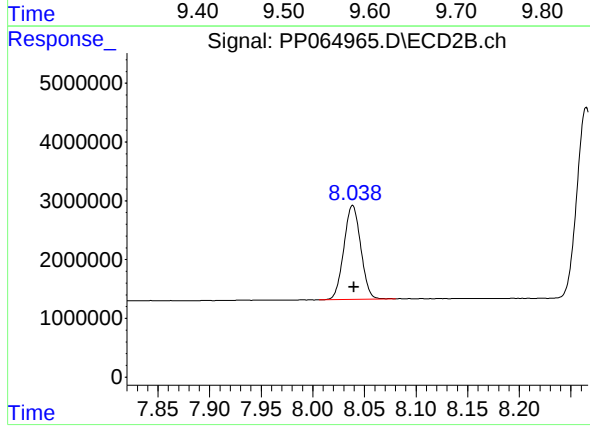

#45 AR-1268-5

R.T.: 8.039 min
Delta R.T.: -0.001 min
Response: 18228440
Conc: 28.46 ng/ml