

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051524\
 Data File : PP064980.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2024 21:22
 Operator : YP\AJ
 Sample : P2475-01 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KHB046K-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/16/2024
 Supervised By :Ankita Jodhani 05/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 01:40:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 14 06:05:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.265	3.375	3447138	4708952	1.812	2.092
2) SA Decachlor...	9.911	8.267	2374039	4032398	3.306m	2.302 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051524\
Data File : PP064980.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2024 21:22
Operator : YP\AJ
Sample : P2475-01 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KHB046K-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/16/2024
Supervised By :Ankita Jodhani 05/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 01:40:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051324.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 14 06:05:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

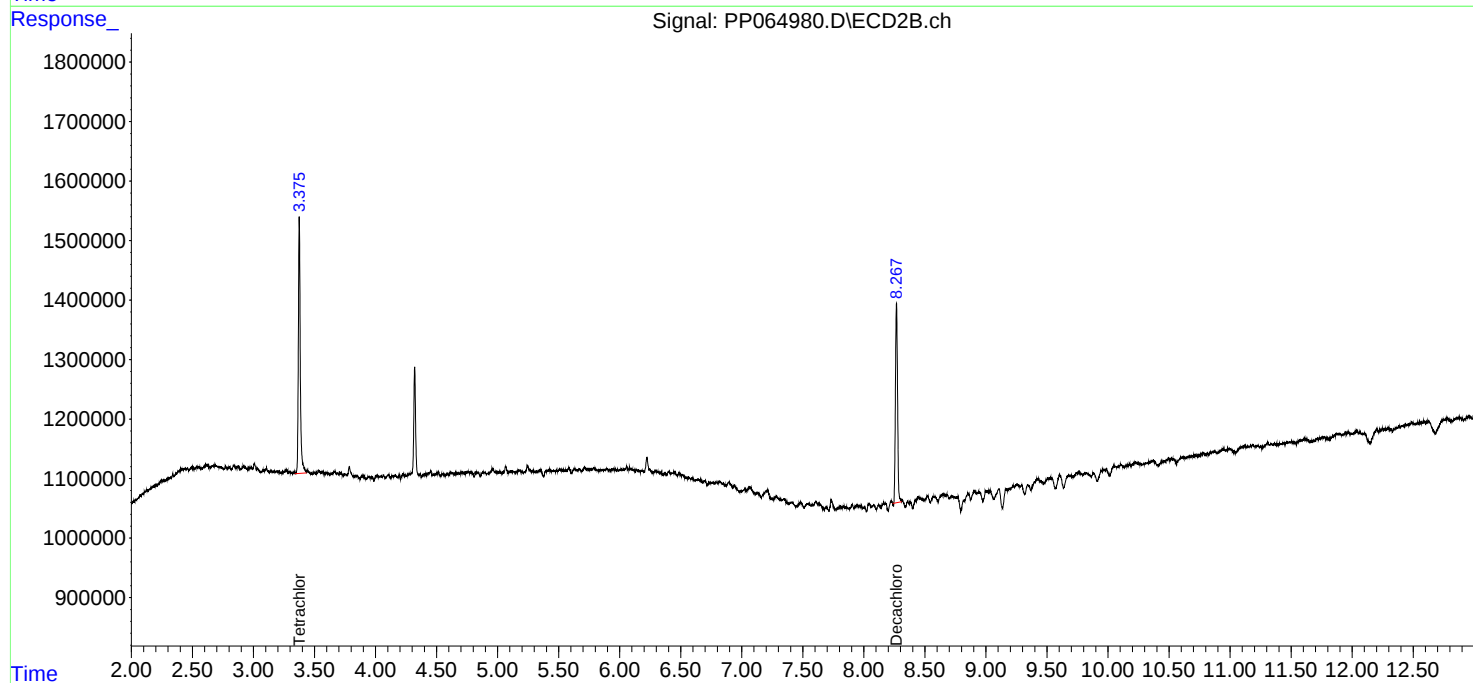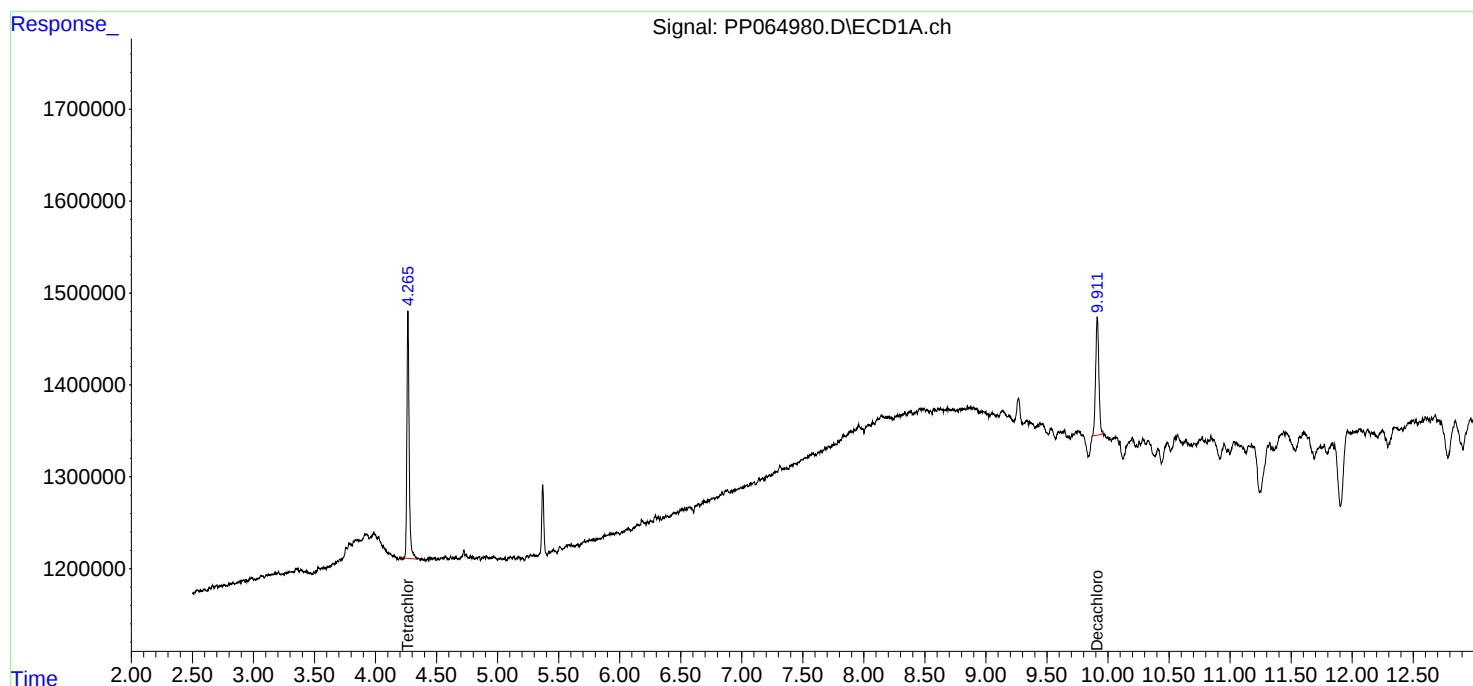

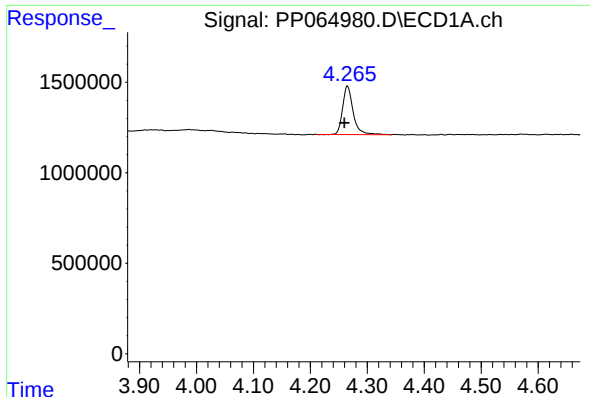


#1 Tetrachloro-m-xylene

R.T.: 4.265 min
Delta R.T.: 0.005 min
Response: 3447138
Conc: 1.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
KHB046K-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/16/2024
Supervised By :Ankita Jodhani 05/16/2024

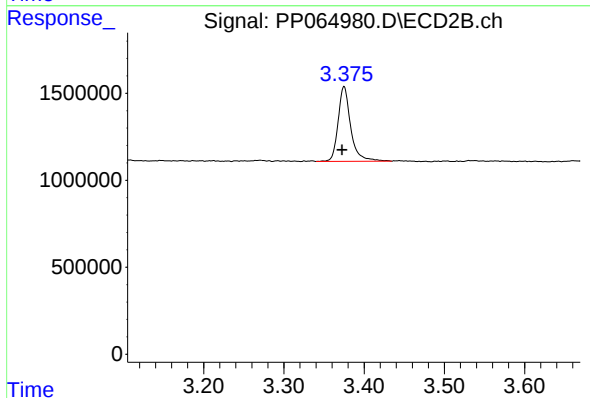


#1 Tetrachloro-m-xylene

R.T.: 3.375 min
Delta R.T.: 0.003 min
Response: 4708952
Conc: 2.09 ng/ml

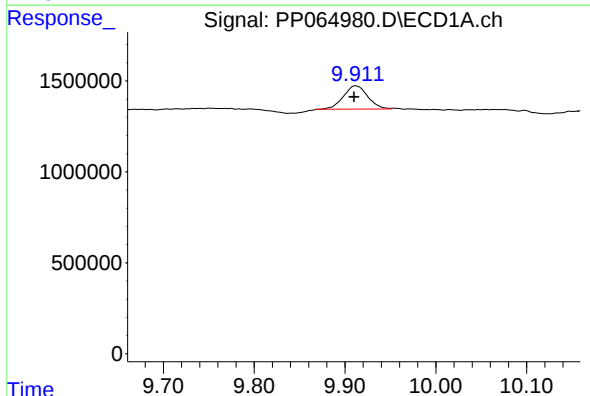

#2 Decachlorobiphenyl

R.T.: 9.911 min
Delta R.T.: 0.001 min
Response: 2374039
Conc: 3.31 ng/ml m

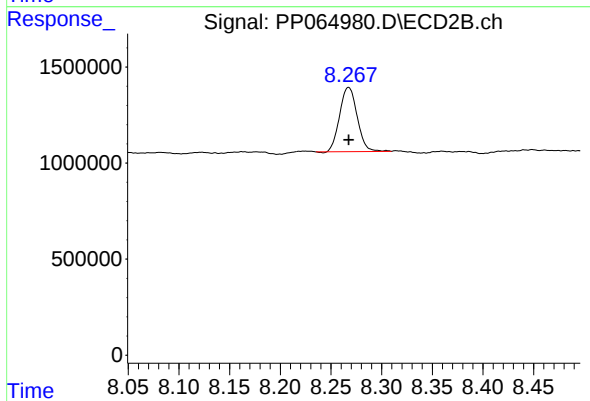

#2 Decachlorobiphenyl

R.T.: 8.267 min
Delta R.T.: 0.000 min
Response: 4032398
Conc: 2.30 ng/ml