

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051524\
 Data File : PP064981.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2024 21:39
 Operator : YP\AJ
 Sample : P2475-02 10X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KHB046K-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/16/2024
 Supervised By :Ankita Jodhani 05/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 01:40:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 14 06:05:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.265	3.374	3017594	4258056	1.587	1.892
2) SA Decachlor...	9.911	8.267	1991546	3619554	2.774m	2.067 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051524\
Data File : PP064981.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2024 21:39
Operator : YP\AJ
Sample : P2475-02 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KHB046K-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/16/2024
Supervised By :Ankita Jodhani 05/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 01:40:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051324.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 14 06:05:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

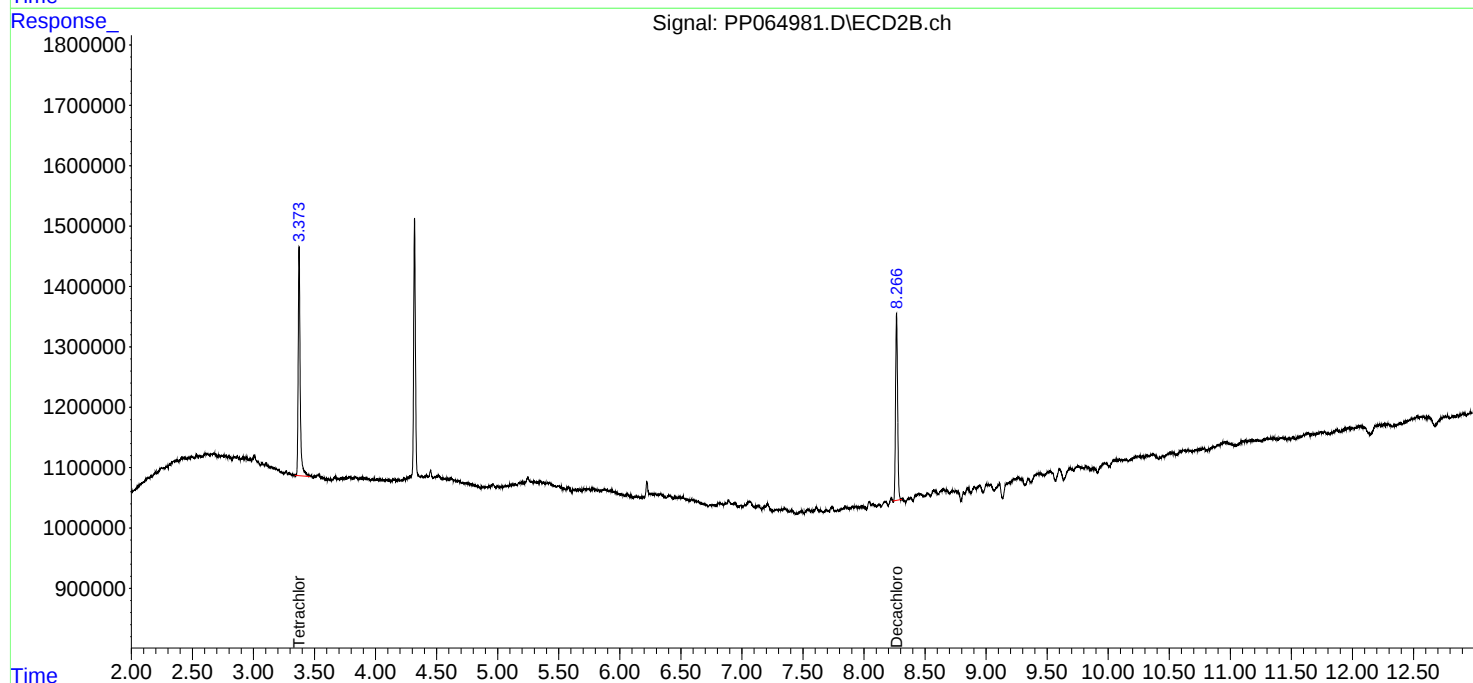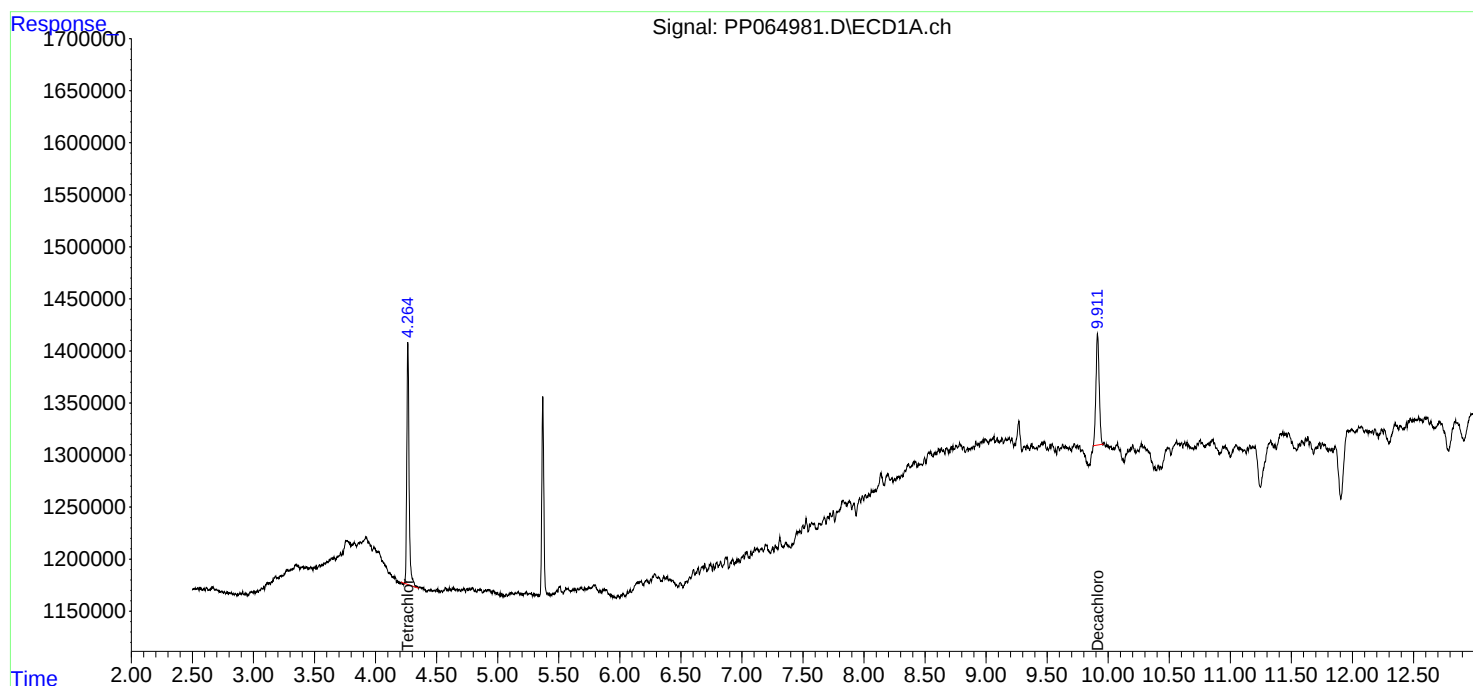

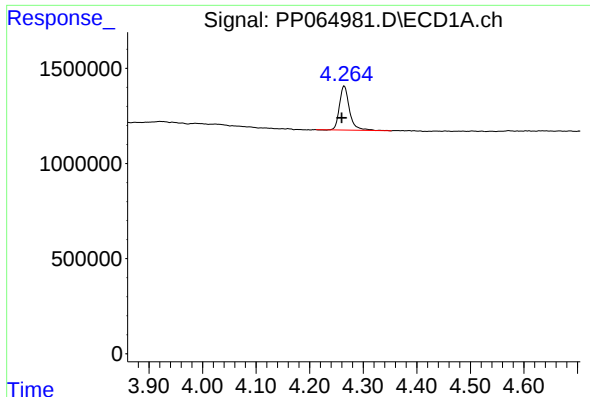


#1 Tetrachloro-m-xylene

R.T.: 4.265 min
Delta R.T.: 0.005 min
Response: 3017594
Conc: 1.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
KHB046K-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/16/2024
Supervised By :Ankita Jodhani 05/16/2024

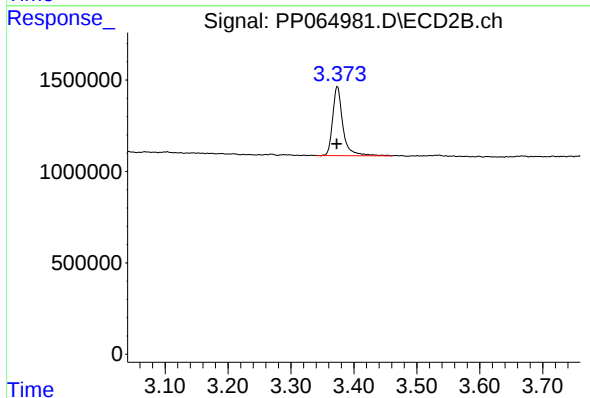


#1 Tetrachloro-m-xylene

R.T.: 3.374 min
Delta R.T.: 0.001 min
Response: 4258056
Conc: 1.89 ng/ml

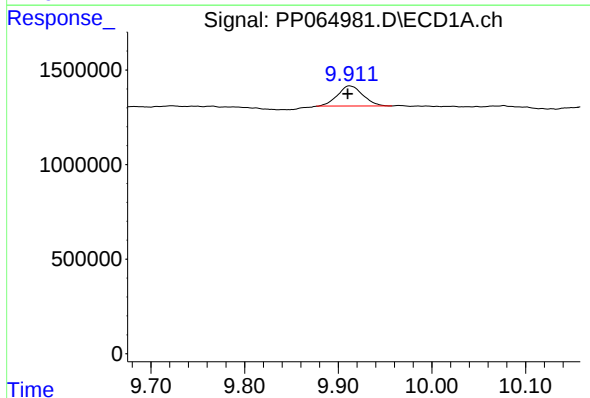

#2 Decachlorobiphenyl

R.T.: 9.911 min
Delta R.T.: 0.001 min
Response: 1991546
Conc: 2.77 ng/ml m

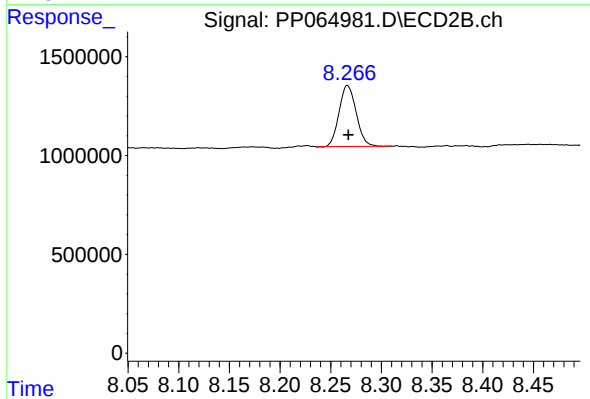

#2 Decachlorobiphenyl

R.T.: 8.267 min
Delta R.T.: 0.000 min
Response: 3619554
Conc: 2.07 ng/ml