

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051524\
 Data File : PP064985.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2024 22:44
 Operator : YP\AJ
 Sample : P2475-06 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 JEH578G-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/16/2024
 Supervised By :Ankita Jodhani 05/16/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 01:41:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 14 06:05:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.264	3.374	3428917	4646143	1.803m	2.064
2) SA Decachlor...	9.914	8.267	3230496	3898194	4.499	2.226 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051524\
Data File : PP064985.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2024 22:44
Operator : YP\AJ
Sample : P2475-06 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
JEH578G-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/16/2024
Supervised By :Ankita Jodhani 05/16/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 01:41:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051324.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 14 06:05:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

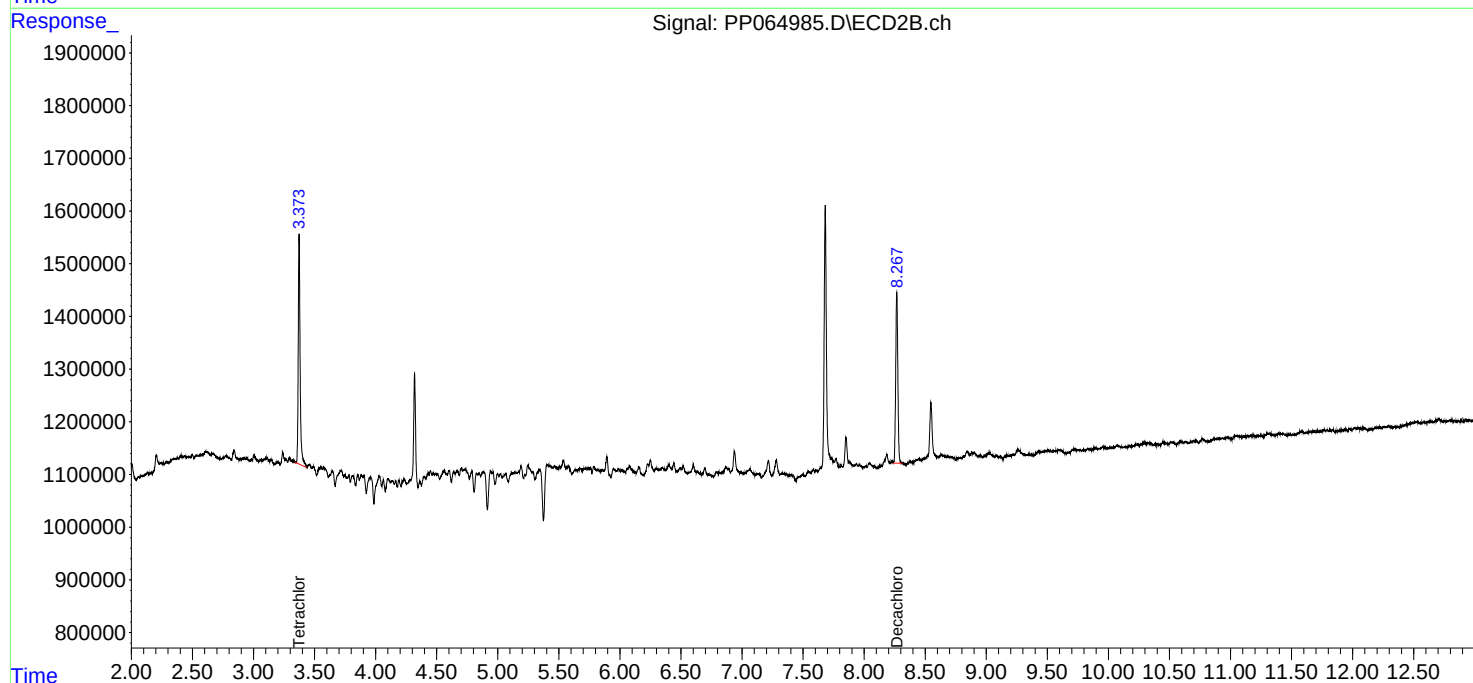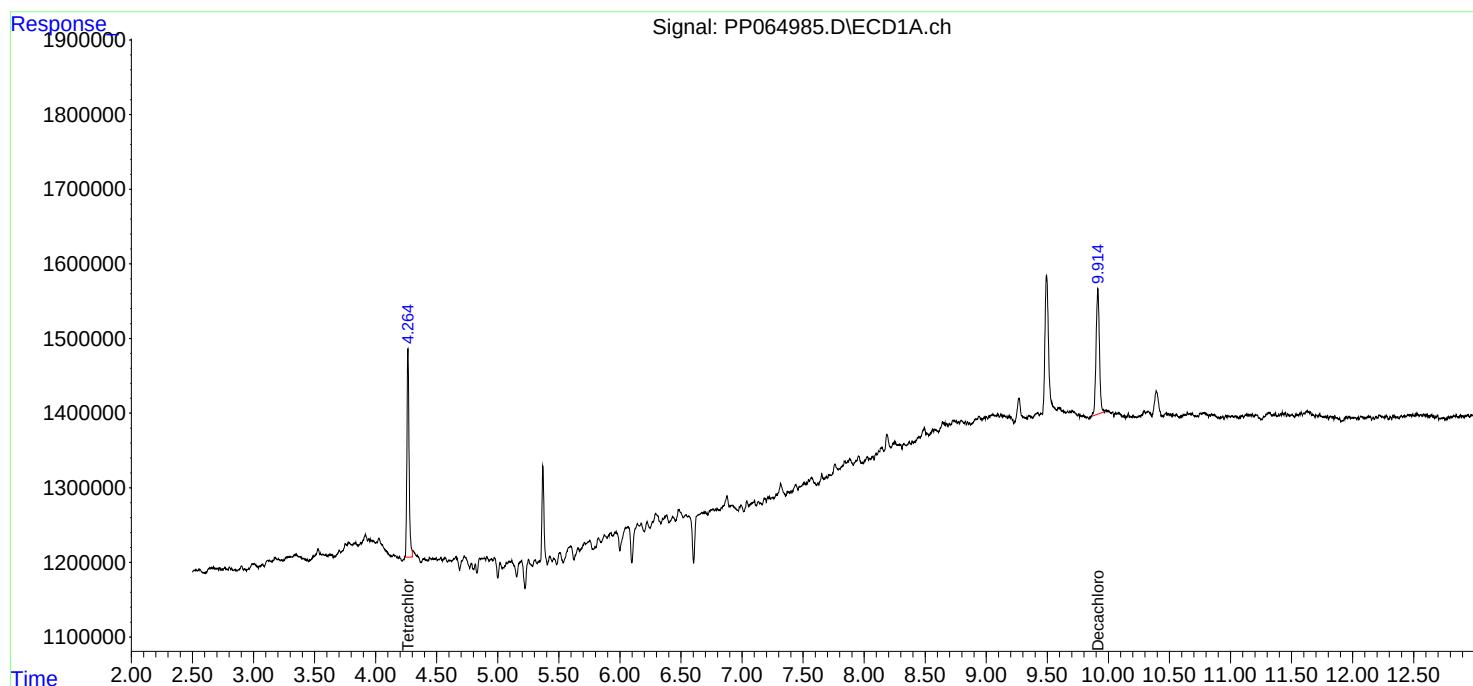

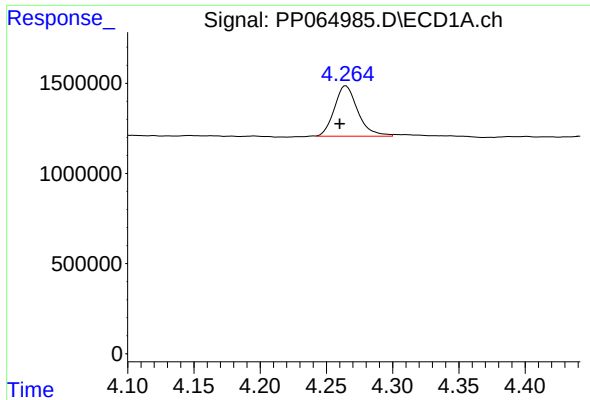


#1 Tetrachloro-m-xylene

R.T.: 4.264 min
Delta R.T.: 0.004 min
Response: 3428917
Conc: 1.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
JEH578G-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/16/2024
Supervised By :Ankita Jodhani 05/16/2024

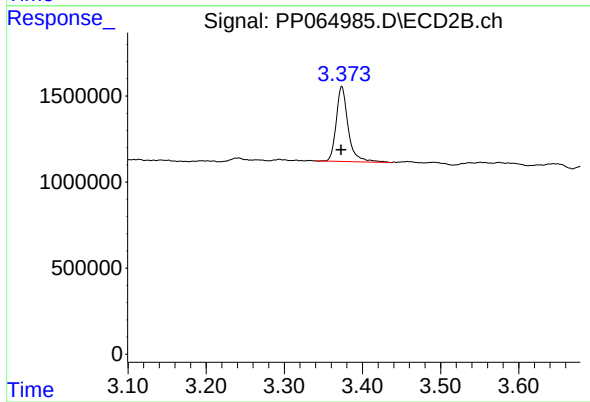


#1 Tetrachloro-m-xylene

R.T.: 3.374 min
Delta R.T.: 0.001 min
Response: 4646143
Conc: 2.06 ng/ml

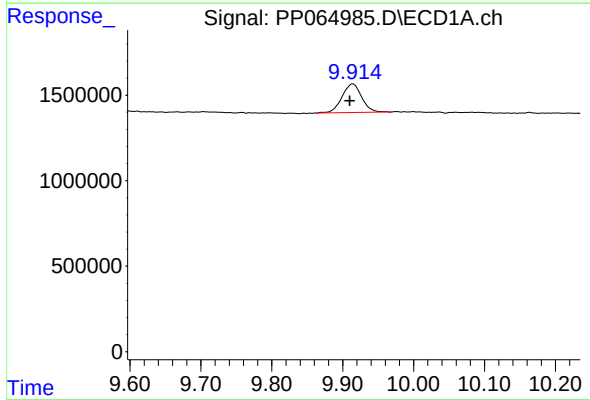

#2 Decachlorobiphenyl

R.T.: 9.914 min
Delta R.T.: 0.004 min
Response: 3230496
Conc: 4.50 ng/ml

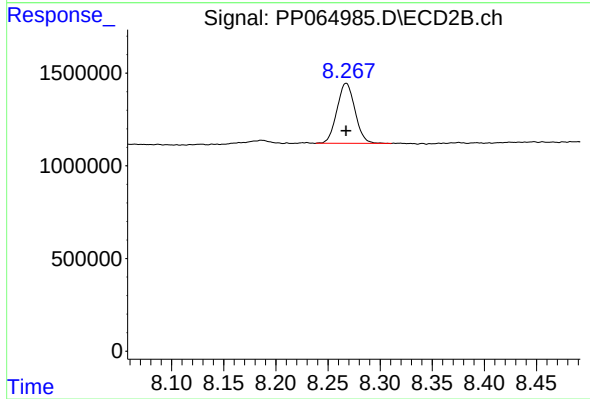

#2 Decachlorobiphenyl

R.T.: 8.267 min
Delta R.T.: 0.000 min
Response: 3898194
Conc: 2.23 ng/ml