

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051525\
 Data File : PP072117.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2025 18:21
 Operator : YP\AJ
 Sample : Q2048-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 L2-WC-3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/16/2025
 Supervised By :mohammad ahmed 05/19/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 03:05:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042225.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 23 05:02:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.507	3.801	36229988	29768088	18.274	21.132m
2) SA Decachlor...	10.216	8.824	23168398	16794569	16.000	19.149m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051525\
Data File : PP072117.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2025 18:21
Operator : YP\AJ
Sample : Q2048-09
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
L2-WC-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/16/2025
Supervised By :mohammad ahmed 05/19/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 03:05:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042225.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 23 05:02:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

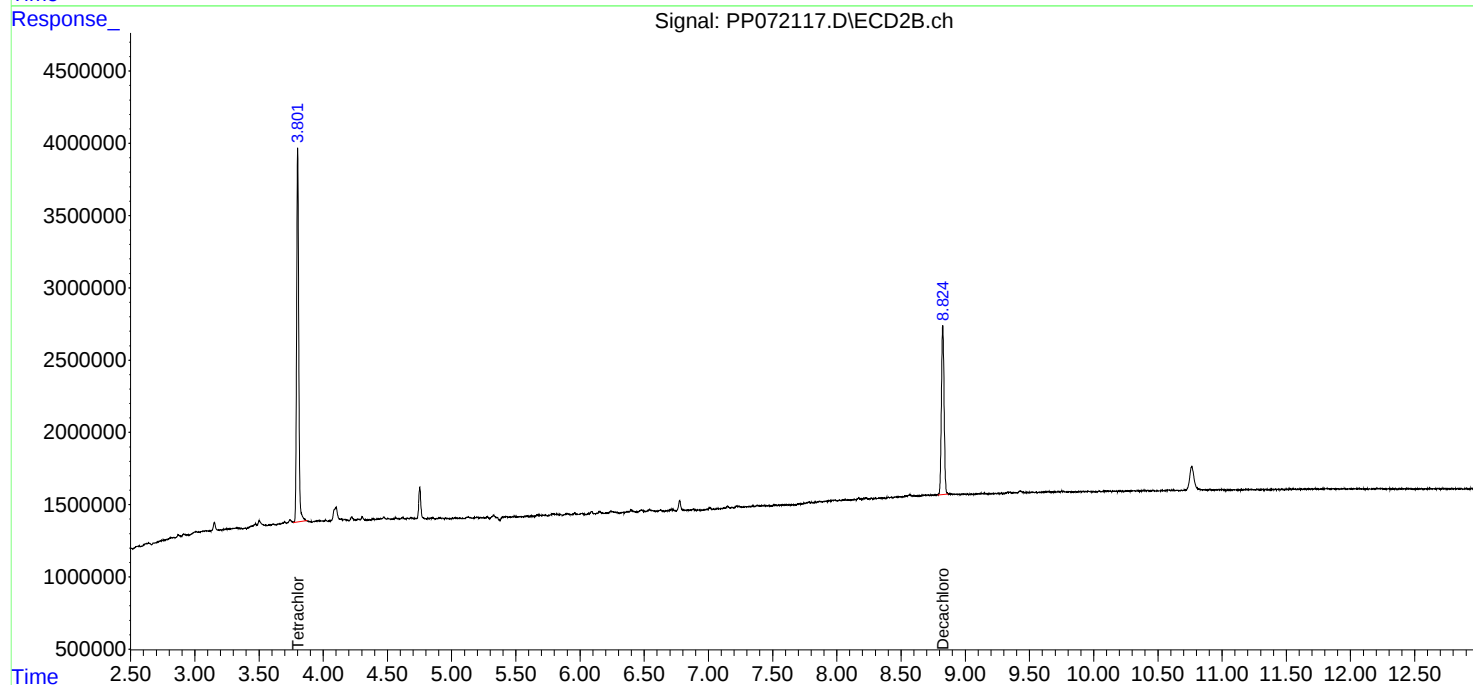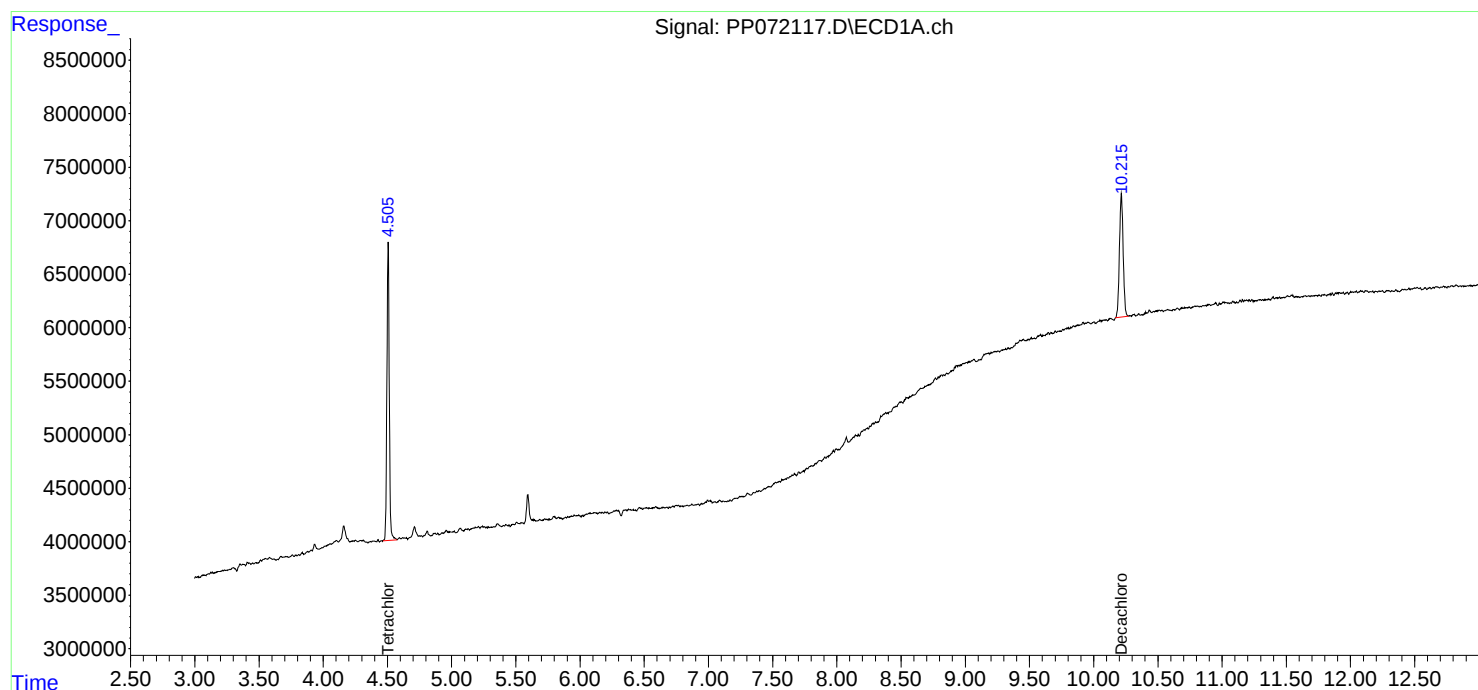

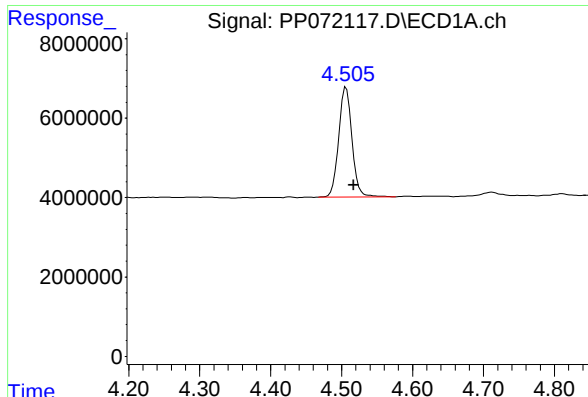


#1 Tetrachloro-m-xylene

R.T.: 4.507 min
Delta R.T.: -0.011 min
Response: 36229988
Conc: 18.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
L2-WC-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/16/2025
Supervised By :mohammad ahmed 05/19/2025

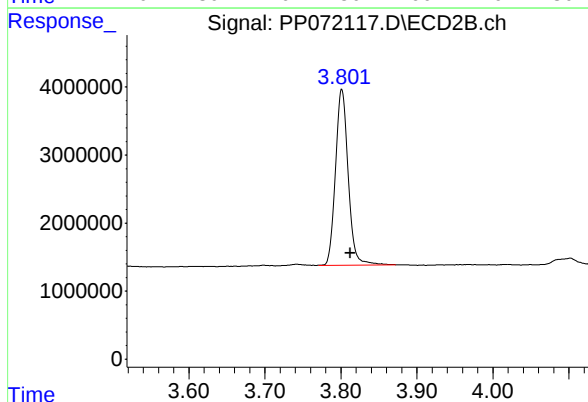


#1 Tetrachloro-m-xylene

R.T.: 3.801 min
Delta R.T.: -0.012 min
Response: 29768088
Conc: 21.13 ng/ml

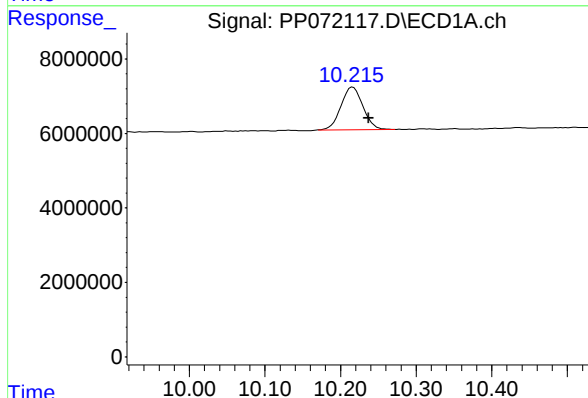

#2 Decachlorobiphenyl

R.T.: 10.216 min
Delta R.T.: -0.021 min
Response: 23168398
Conc: 16.00 ng/ml

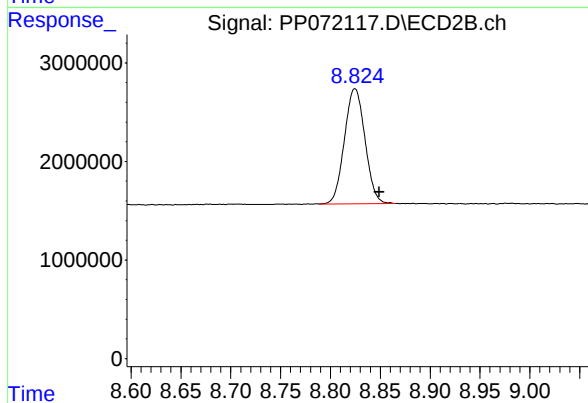

#2 Decachlorobiphenyl

R.T.: 8.824 min
Delta R.T.: -0.025 min
Response: 16794569
Conc: 19.15 ng/ml