

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051622\
 Data File : PP047598.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2022 12:47
 Operator : YP\AJ
 Sample : N2809-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-14A-TP-5R

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/16/2022
 Supervised By :mohammad ahmed 05/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 13:11:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 11 13:10:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.845	3.114	34488950	38396598	13.566m	11.662m
2) SA Decachlor...	9.922	8.429	29432617	37786916	20.574	13.882 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051622\
Data File : PP047598.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2022 12:47
Operator : YP\AJ
Sample : N2809-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WC-14A-TP-5R


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/16/2022
Supervised By :mohammad ahmed 05/17/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 13:11:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 11 13:10:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

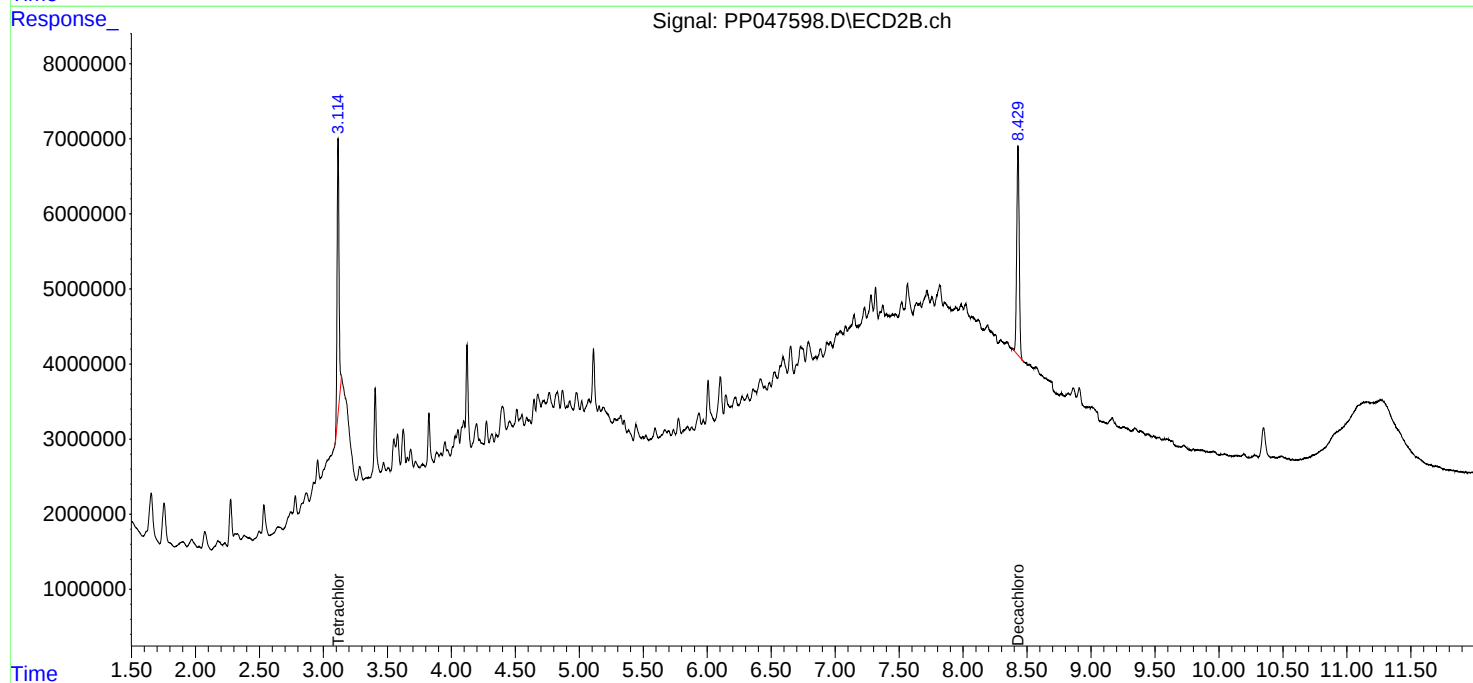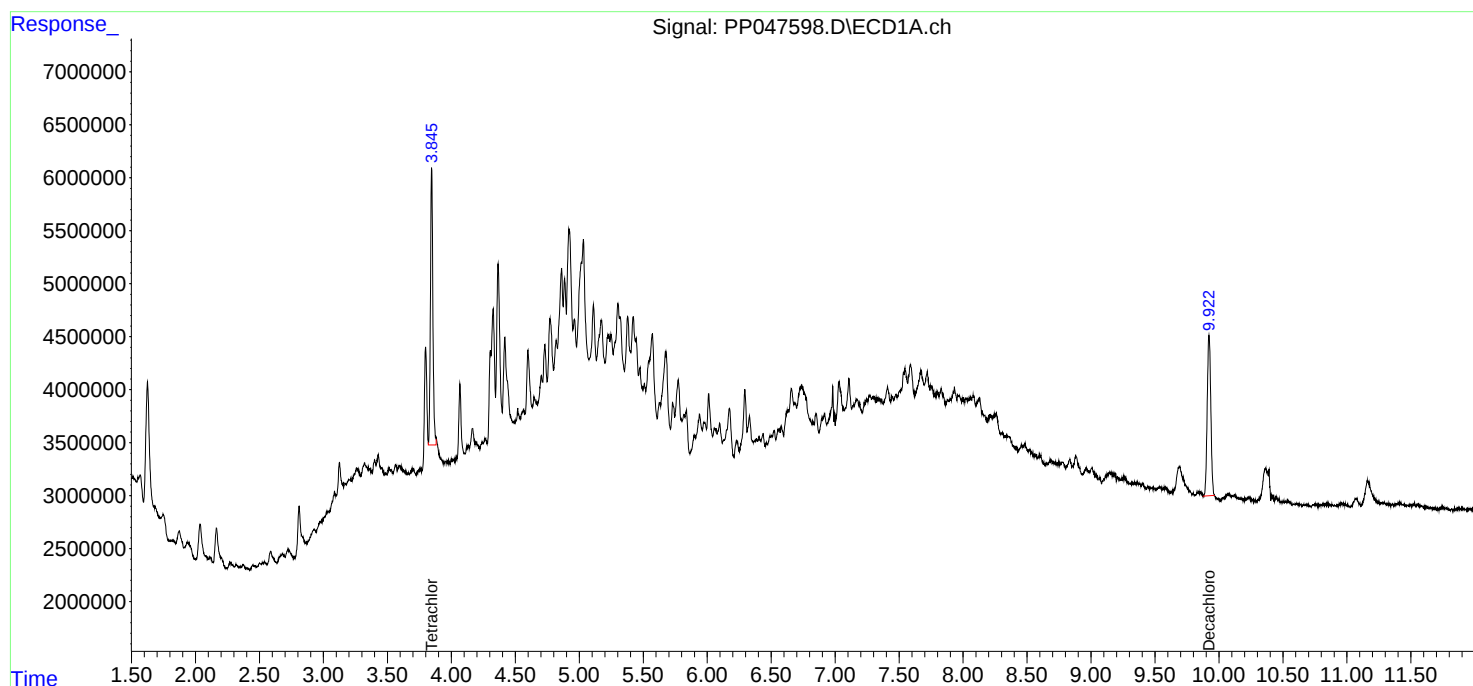

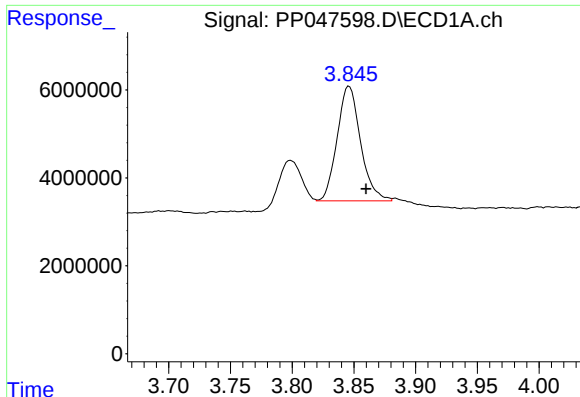


#1 Tetrachloro-m-xylene

R.T.: 3.845 min
Delta R.T.: -0.015 min
Response: 34488950
Conc: 13.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-14A-TP-5R


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/16/2022
Supervised By :mohammad ahmed 05/17/2022

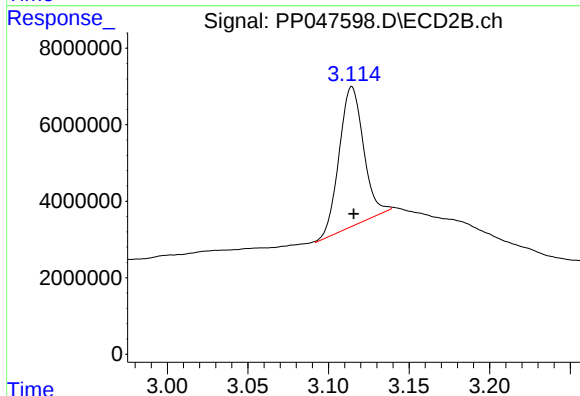


#1 Tetrachloro-m-xylene

R.T.: 3.114 min
Delta R.T.: -0.002 min
Response: 38396598
Conc: 11.66 ng/ml m

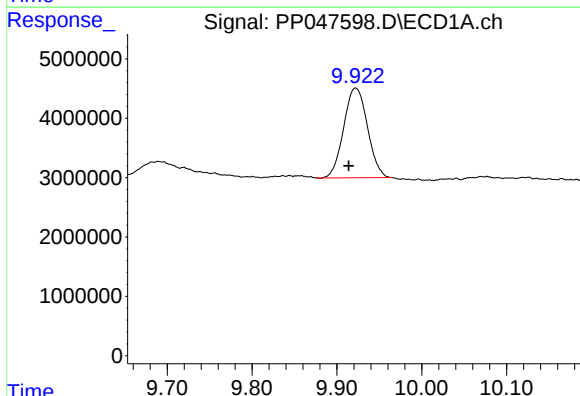

#2 Decachlorobiphenyl

R.T.: 9.922 min
Delta R.T.: 0.008 min
Response: 29432617
Conc: 20.57 ng/ml

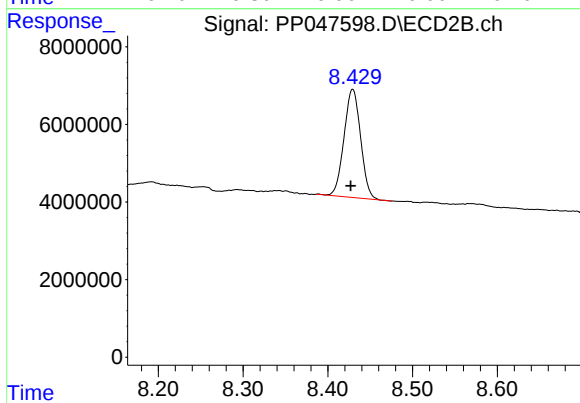

#2 Decachlorobiphenyl

R.T.: 8.429 min
Delta R.T.: 0.002 min
Response: 37786916
Conc: 13.88 ng/ml