

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051625\
 Data File : PP072138.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2025 13:31
 Operator : YP\AJ
 Sample : Q2055-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 OR-02-051525

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/19/2025
 Supervised By :mohammad ahmed 05/20/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 14:27:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042225.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 23 05:02:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.505	3.800	29680715	26635800	14.970m	18.909m#
2) SA Decachlor...	10.216	8.823	17736853	12755687	12.249	14.544m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051625\
Data File : PP072138.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2025 13:31
Operator : YP\AJ
Sample : Q2055-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleID :
OR-02-051525


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/19/2025
Supervised By :mohammad ahmed 05/20/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 14:27:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042225.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 23 05:02:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

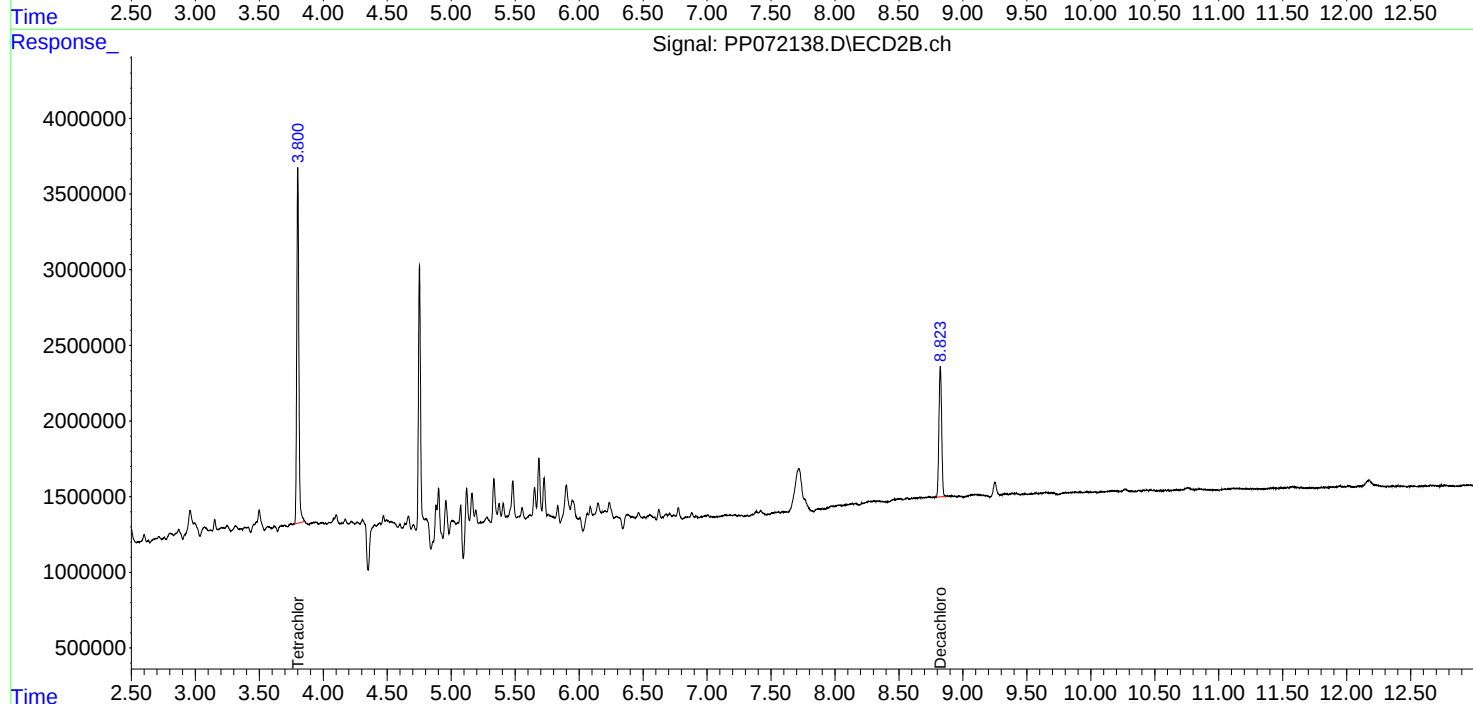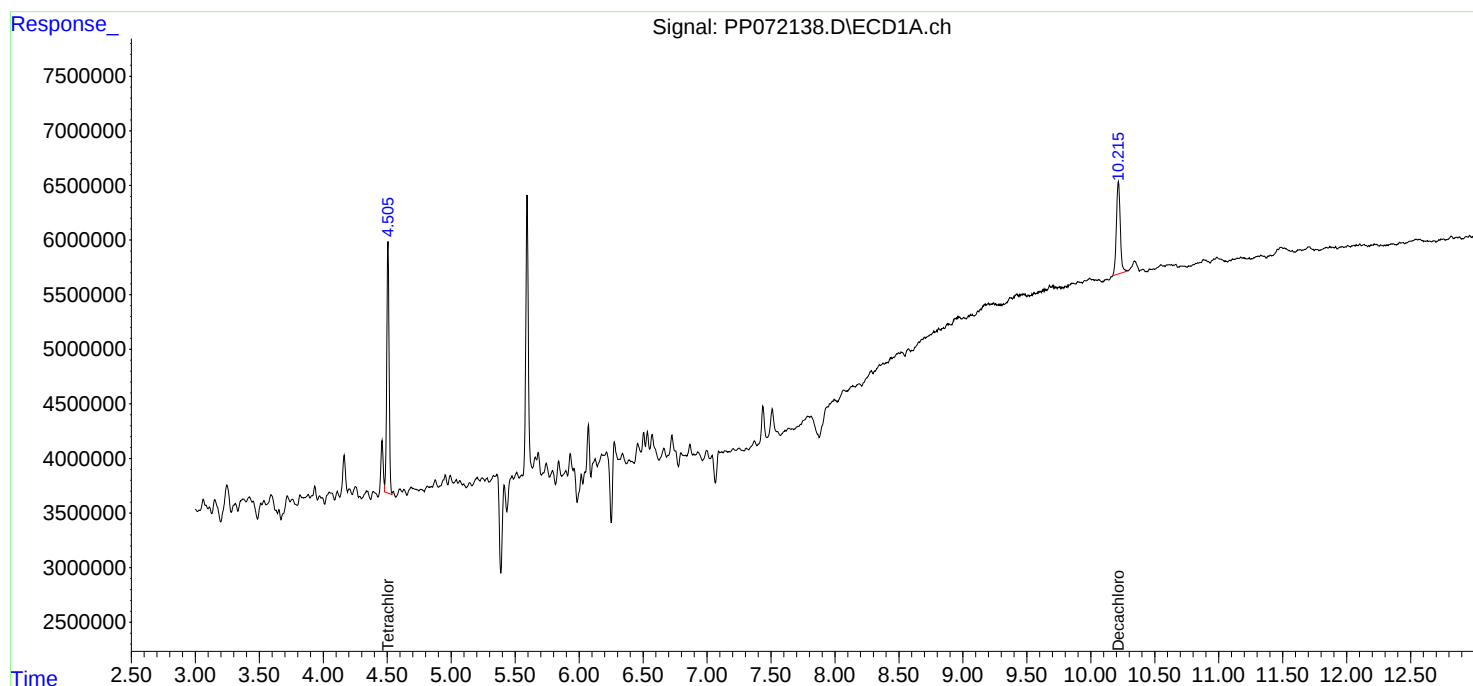

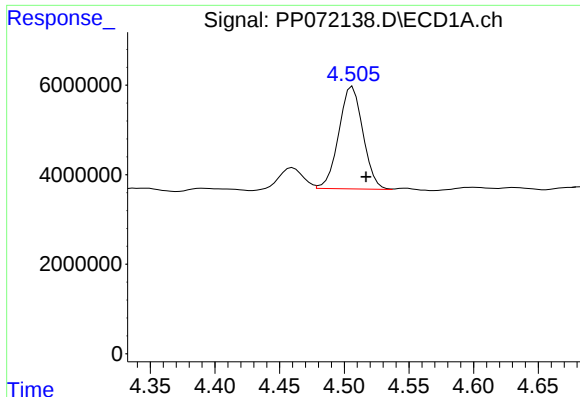


#1 Tetrachloro-m-xylene

R.T.: 4.505 min
Delta R.T.: -0.012 min
Response: 29680715
Conc: 14.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
OR-02-051525


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/19/2025
Supervised By :mohammad ahmed 05/20/2025

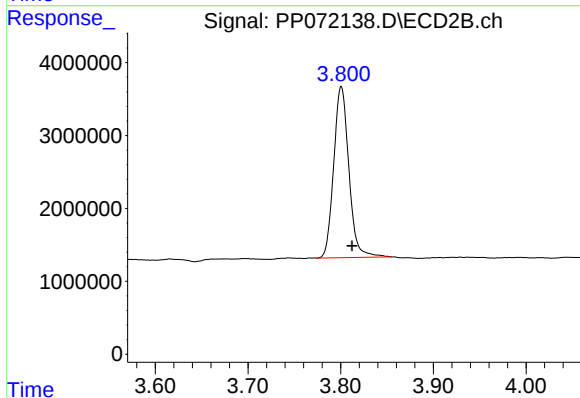


#1 Tetrachloro-m-xylene

R.T.: 3.800 min
Delta R.T.: -0.012 min
Response: 26635800
Conc: 18.91 ng/ml m

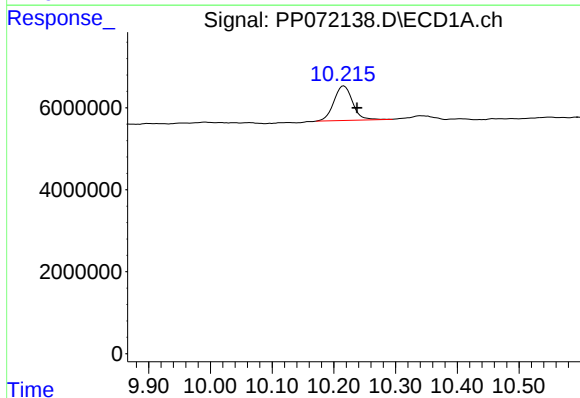

#2 Decachlorobiphenyl

R.T.: 10.216 min
Delta R.T.: -0.021 min
Response: 17736853
Conc: 12.25 ng/ml

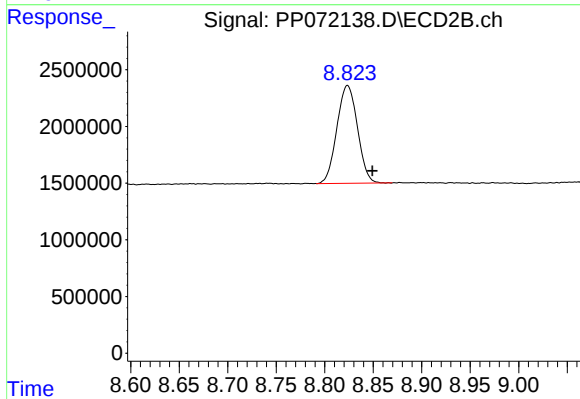

#2 Decachlorobiphenyl

R.T.: 8.823 min
Delta R.T.: -0.026 min
Response: 12755687
Conc: 14.54 ng/ml m