

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051721\
 Data File : PP035946.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 May 2021 12:21
 Operator : DD\AJ
 Sample : M2391-01 2X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEF239Y-2-1

Manual Integrations
 APPROVED

Ankita
 5/18/2021 4:22:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 12:59:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 06:42:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.772	4.193	181463	245913	7.745m	7.234m
2) SA Decachlor...	10.612	9.437	111052	177109	9.866	8.375

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051721\
Data File : PP035946.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 May 2021 12:21
Operator : DD\AJ
Sample : M2391-01 2X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HEF239Y-2-1


Manual Integrations
APPROVED

Ankita
5/18/2021 4:22:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 12:59:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 06:42:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

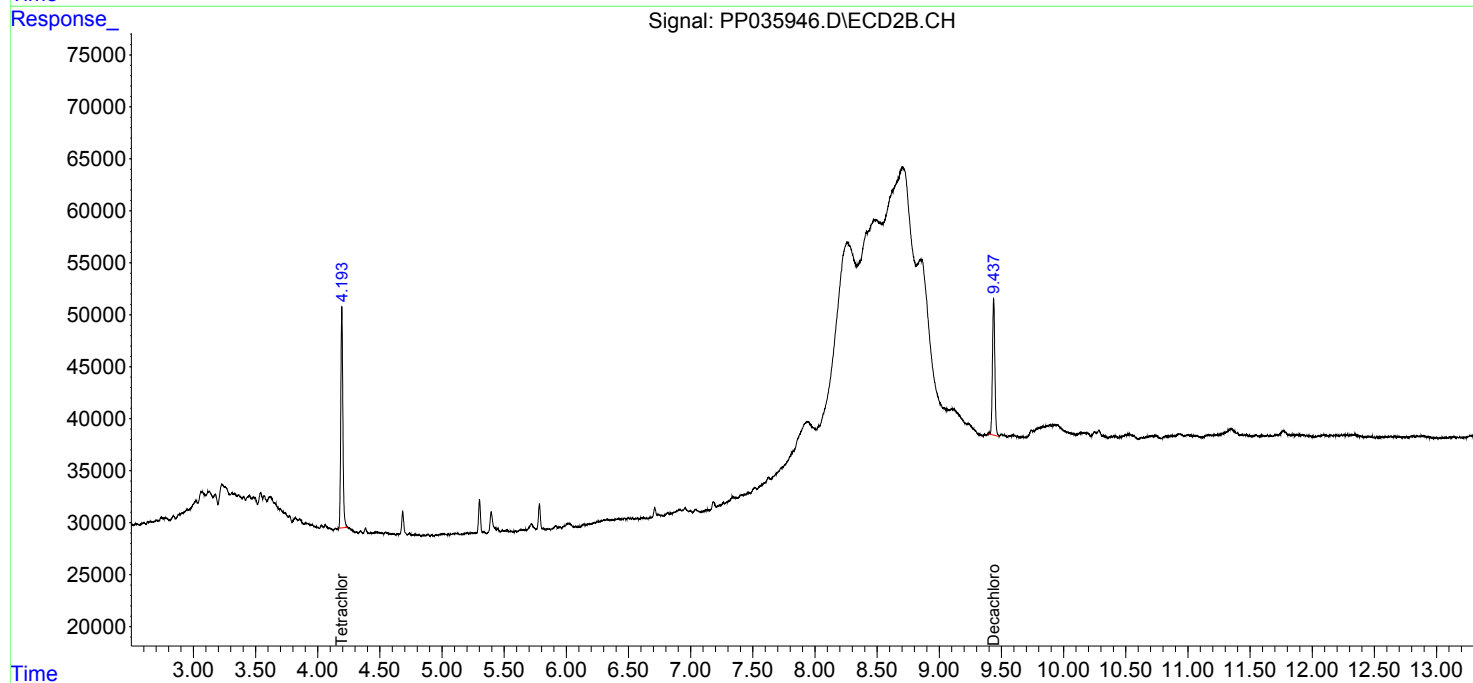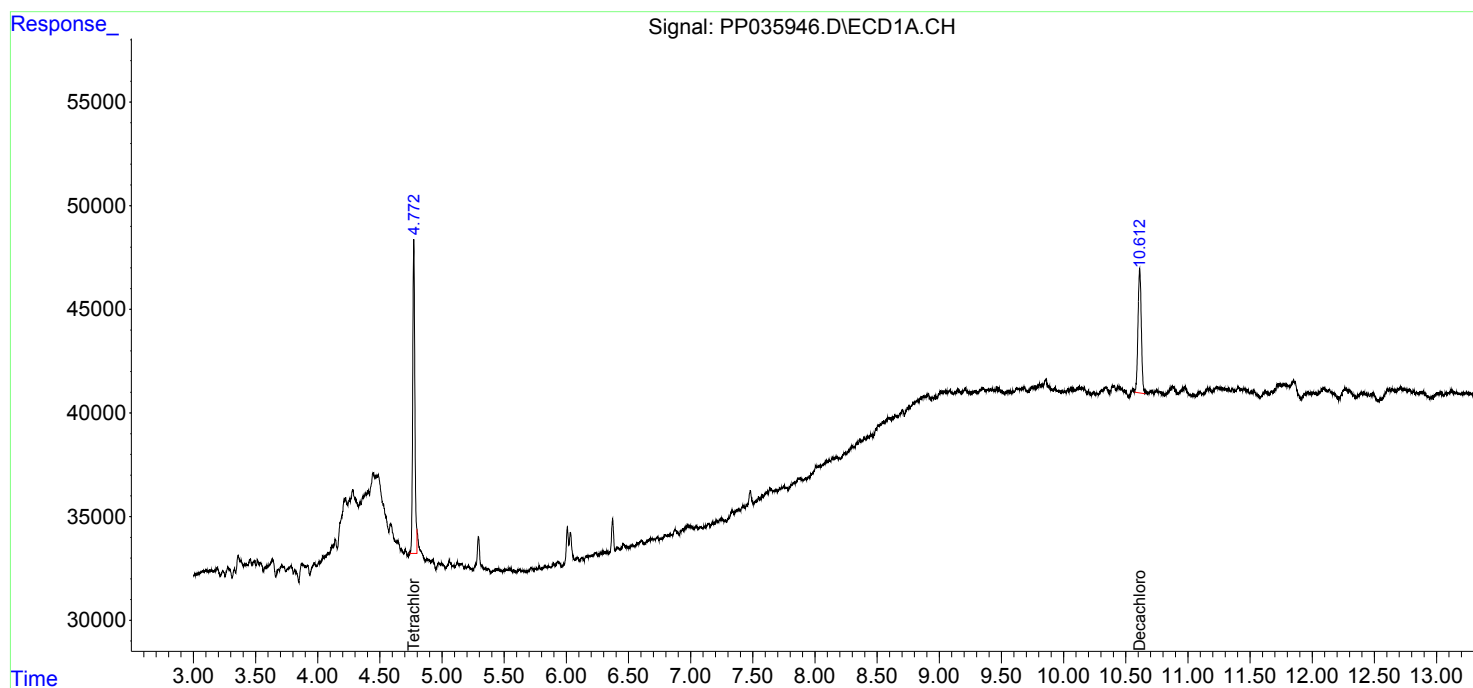

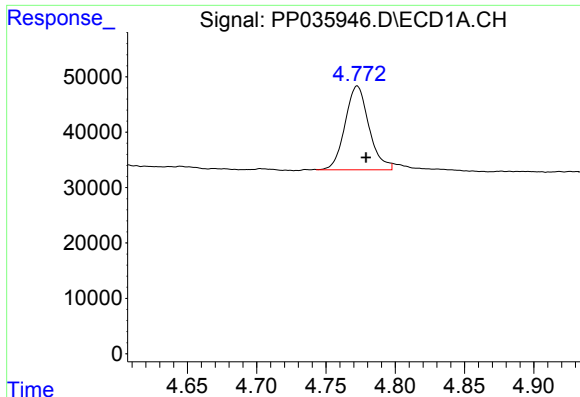


#1 Tetrachloro-m-xylene

R.T.: 4.772 min
Delta R.T.: -0.007 min
Response: 181463
Conc: 7.74 ng/ml m

Instrument :
ECD_P
ClientSampleId :
HEF239Y-2-1


Manual Integrations
APPROVED

Ankita
5/18/2021 4:22:05 PM

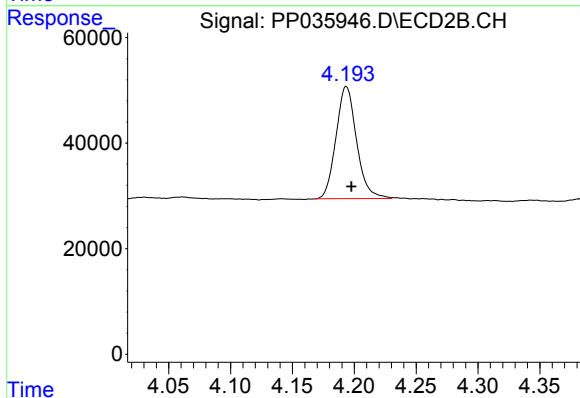


#1 Tetrachloro-m-xylene

R.T.: 4.193 min
Delta R.T.: -0.005 min
Response: 245913
Conc: 7.23 ng/ml m

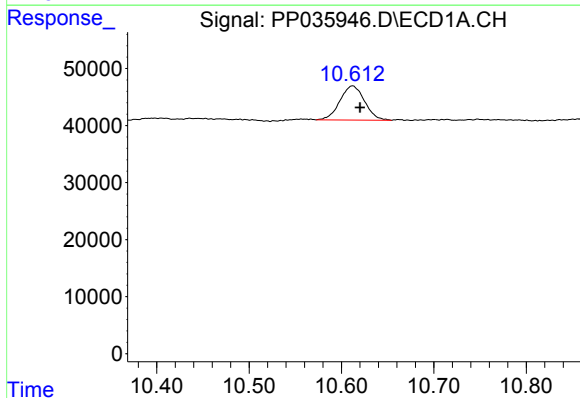

#2 Decachlorobiphenyl

R.T.: 10.612 min
Delta R.T.: -0.008 min
Response: 111052
Conc: 9.87 ng/ml

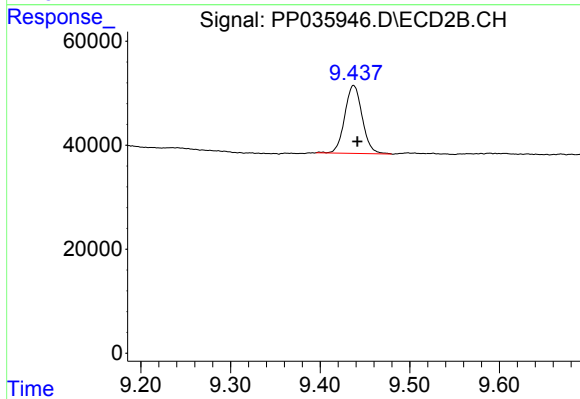

#2 Decachlorobiphenyl

R.T.: 9.437 min
Delta R.T.: -0.004 min
Response: 177109
Conc: 8.37 ng/ml