

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051723\
 Data File : PP057649.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 May 2023 09:57
 Operator : YP\AJ
 Sample : 02783-02 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KMH4447Y-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/18/2023
 Supervised By :Ankita Jodhani 05/18/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 21:06:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 08 19:18:05 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.387	3.624	3335340	3420790	1.520m	1.508
2) SA Decachlor...	10.218	8.687	7653302	2904056	6.753	1.850 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051723\
Data File : PP057649.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2023 09:57
Operator : YP\AJ
Sample : 02783-02 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KMH4447Y-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/18/2023
Supervised By :Ankita Jodhani 05/18/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 21:06:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050823.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 08 19:18:05 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

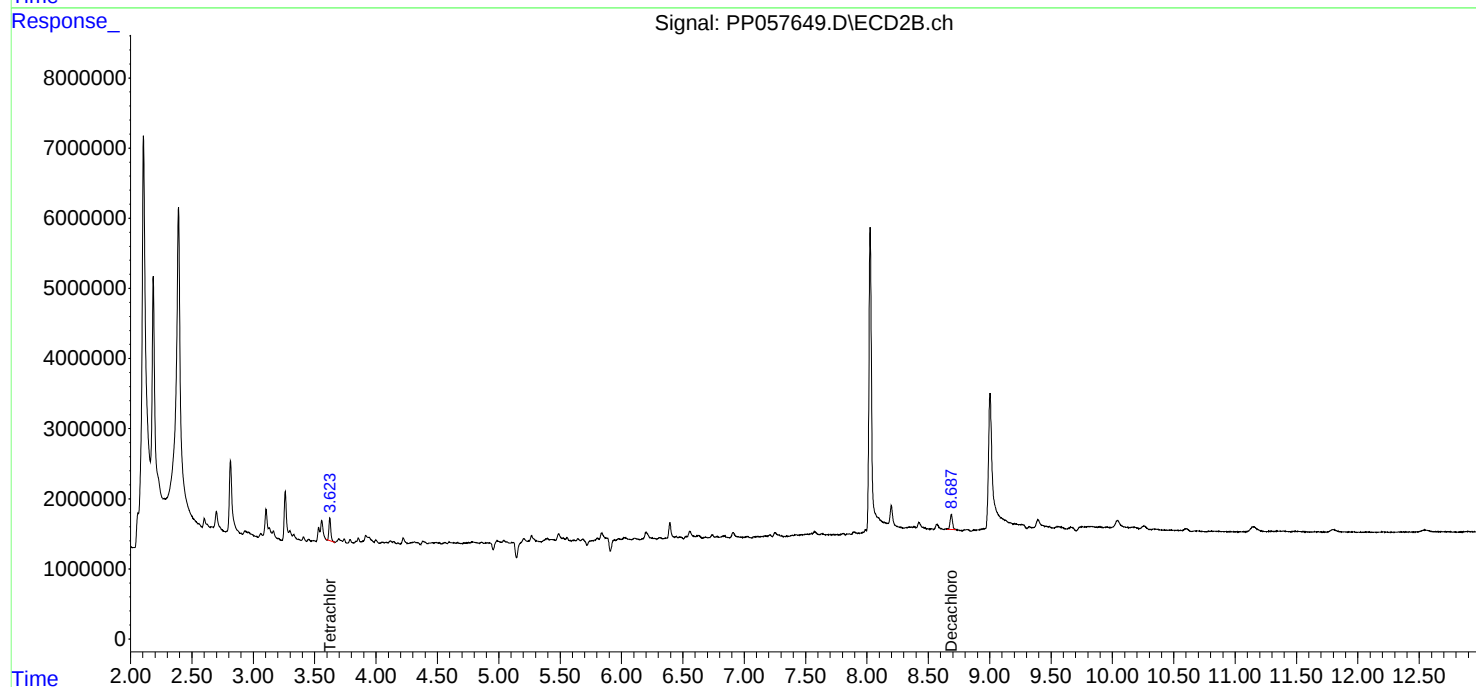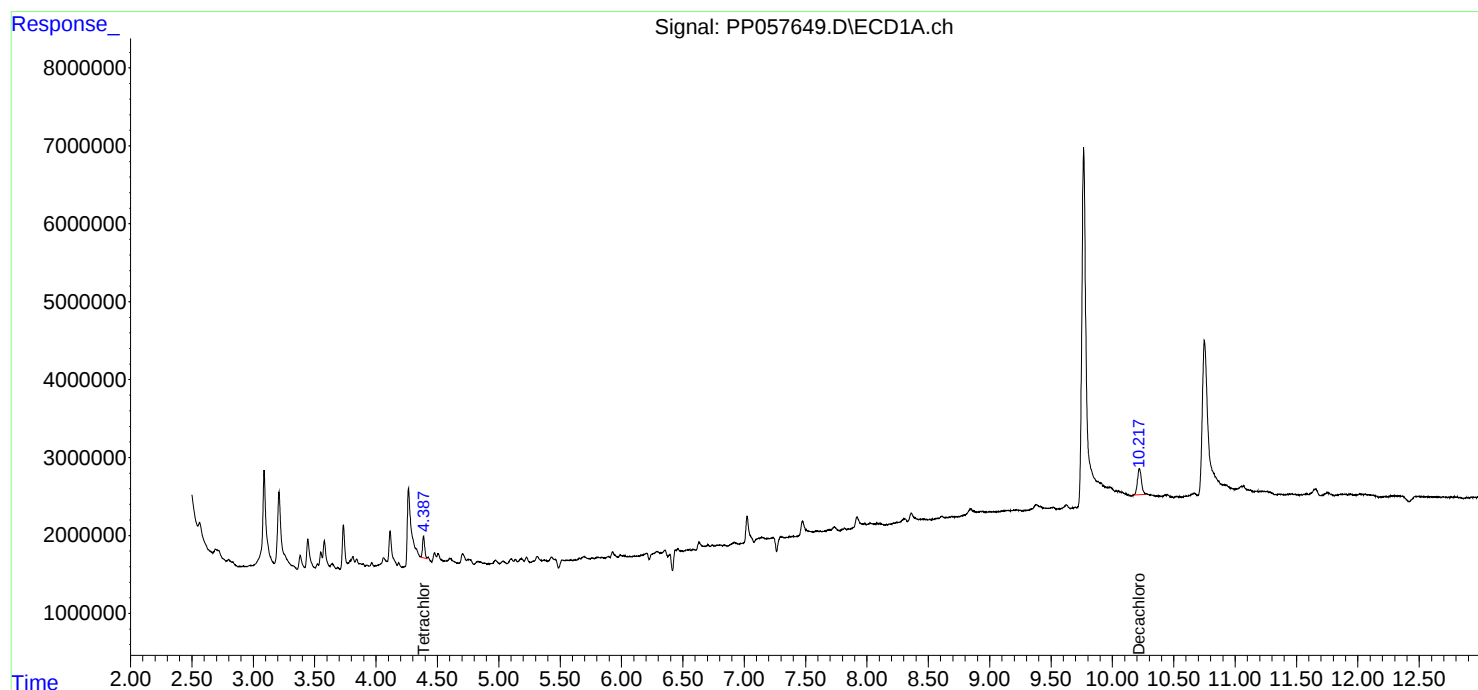

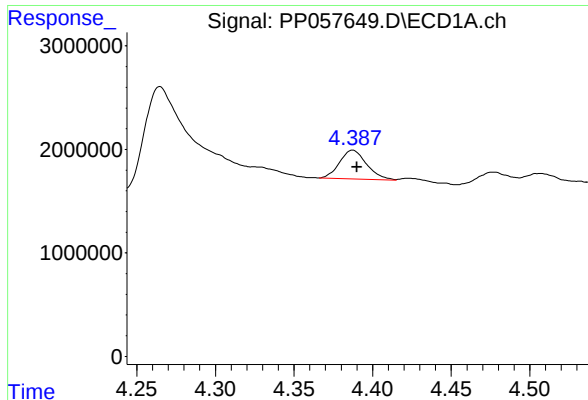

#1 Tetrachloro-m-xylene

R.T.: 4.387 min
Delta R.T.: -0.003 min
Response: 3335340
Conc: 1.52 ng/ml

Instrument :

ECD_P


ClientSampleId :

KMH4447Y-1-2

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 05/18/2023
Supervised By :Ankita Jodhani 05/18/2023

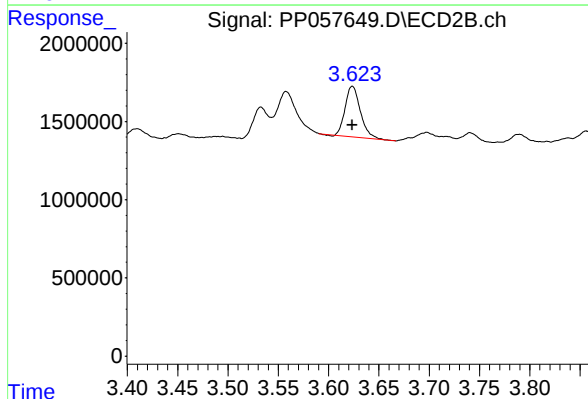


#1 Tetrachloro-m-xylene

R.T.: 3.624 min
Delta R.T.: 0.000 min
Response: 3420790
Conc: 1.51 ng/ml

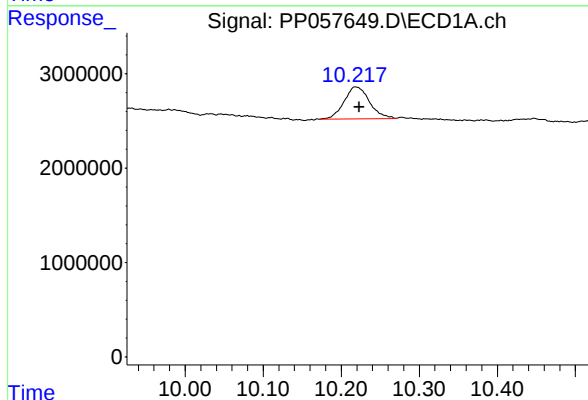

#2 Decachlorobiphenyl

R.T.: 10.218 min
Delta R.T.: -0.005 min
Response: 7653302
Conc: 6.75 ng/ml

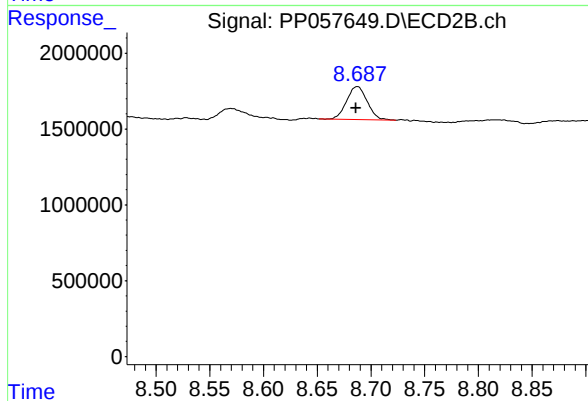

#2 Decachlorobiphenyl

R.T.: 8.687 min
Delta R.T.: 0.001 min
Response: 2904056
Conc: 1.85 ng/ml