

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051821\
 Data File : PP036022.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 May 2021 13:47
 Operator : DD\AJ
 Sample : M2409-01RE
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BACKFILL-ASHCROFT-REAR-06RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 18:03:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 18 06:25:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.775	4.191	520121	762014	24.078	23.840
2)	SA Decachlor...	10.603	9.421	349214	512223	25.800	25.941
Target Compounds							
8)	L2 AR-1221-1	5.031	0.000	23642	0	96.119	N.D. #
9)	L2 AR-1221-2	5.123	4.543	7542	8537	41.478	32.103
27)	L6 AR-1254-2	7.209	0.000	2199	0	2.135	N.D. #
28)	L6 AR-1254-3	7.606f	0.000	3695	0	3.325	N.D. #
32)	L7 AR-1260-2	8.039f	0.000	1334	0	1.530	N.D. #
33)	L7 AR-1260-3	8.350f	0.000	883	0	1.314	N.D. #
36)	L8 AR-1262-1	8.350f	0.000	883	0	0.841	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051821\
Data File : PP036022.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 May 2021 13:47
Operator : DD\AJ
Sample : M2409-01RE
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BACKFILL-ASHCROFT-REAR-06RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 18:03:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 18 06:25:23 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

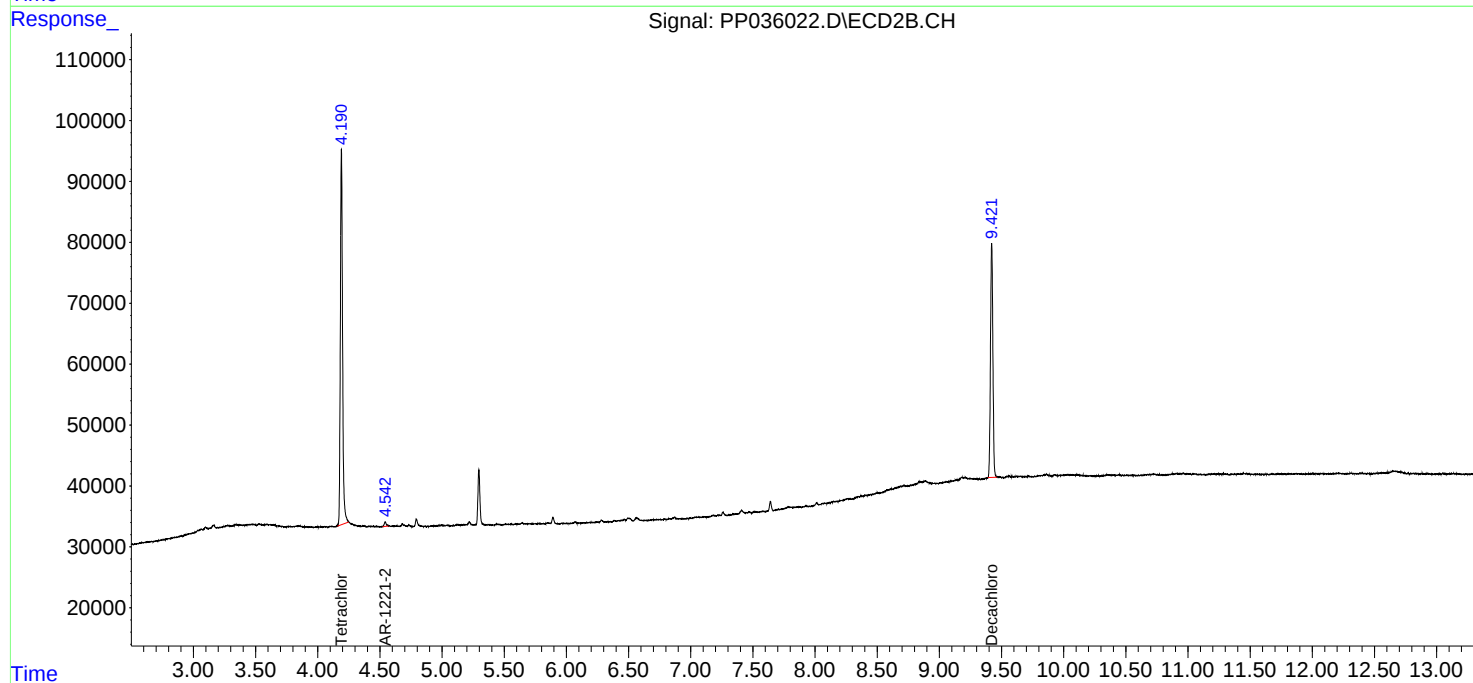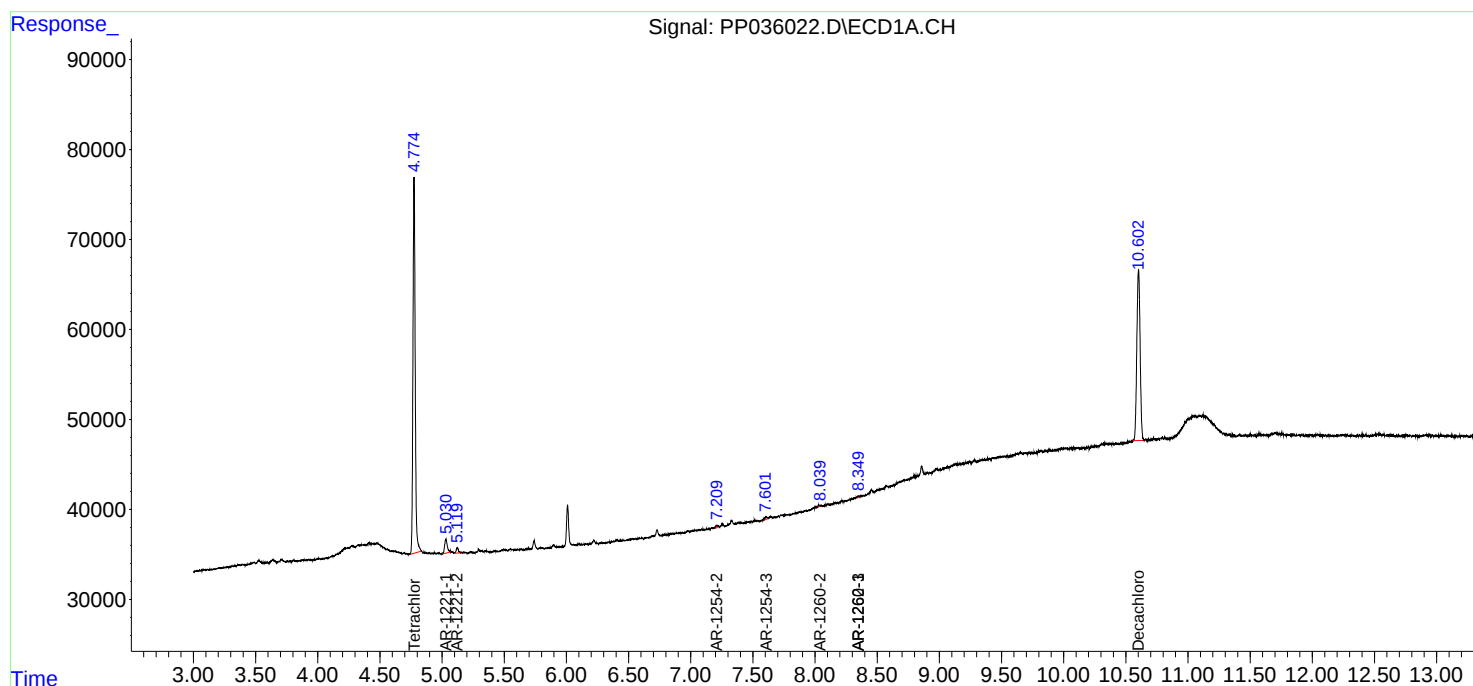


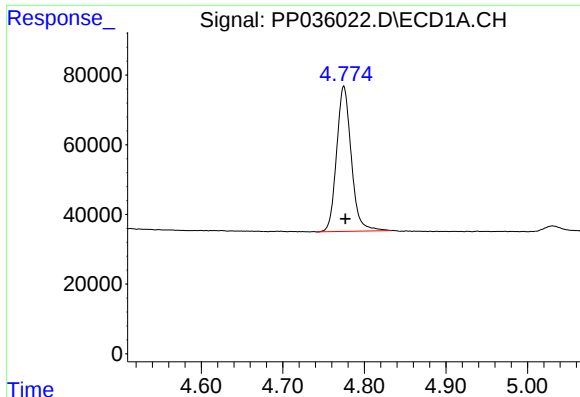

#1 Tetrachloro-m-xylene


R.T.: 4.775 min
Delta R.T.: -0.002 min
Response: 520121
Conc: 24.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
BACKFILL-ASHCROFT-REAR-06RE

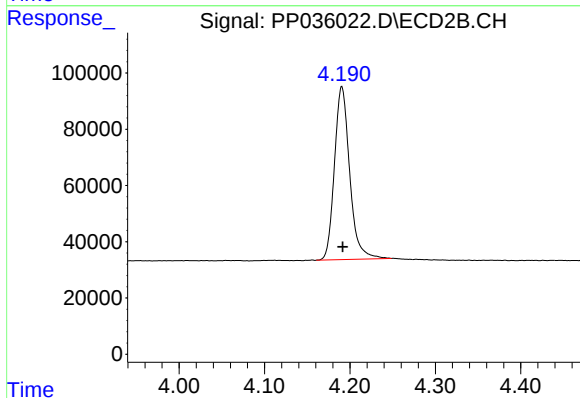


#1 Tetrachloro-m-xylene

R.T.: 4.191 min
Delta R.T.: -0.001 min
Response: 762014
Conc: 23.84 ng/ml

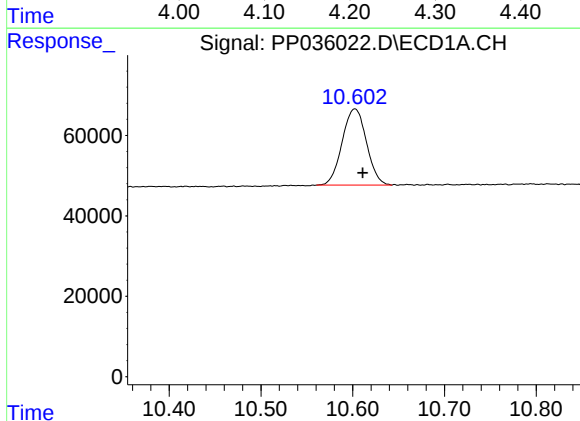


#2 Decachlorobiphenyl

R.T.: 10.603 min
Delta R.T.: -0.009 min
Response: 349214
Conc: 25.80 ng/ml

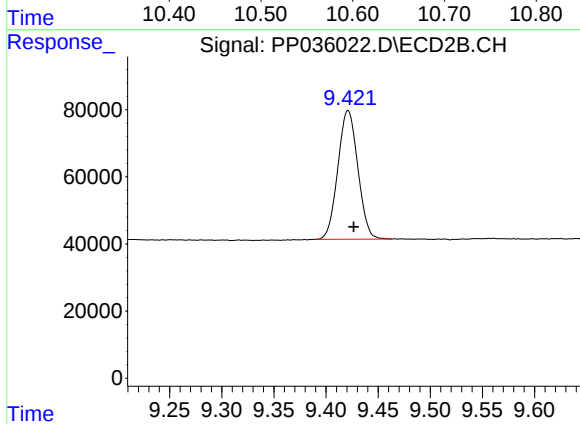

#2 Decachlorobiphenyl


R.T.: 9.421 min
Delta R.T.: -0.005 min
Response: 512223
Conc: 25.94 ng/ml

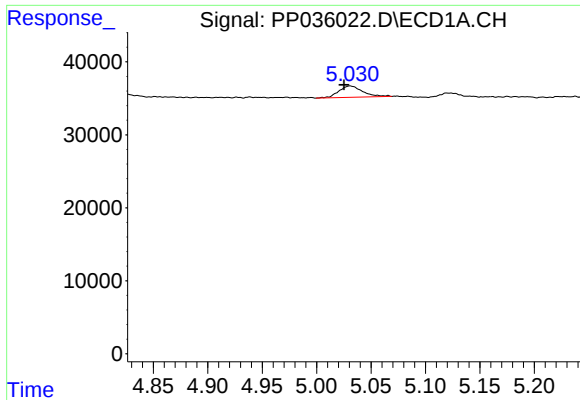

#8 AR-1221-1


R.T.: 5.031 min
Delta R.T.: 0.006 min
Response: 23642
Conc: 96.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
BACKFILL-ASHCROFT-REAR-06RE

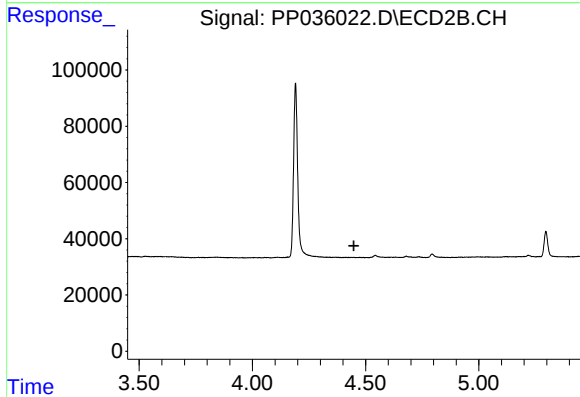


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.448 min
Response: 0
Conc: N.D.

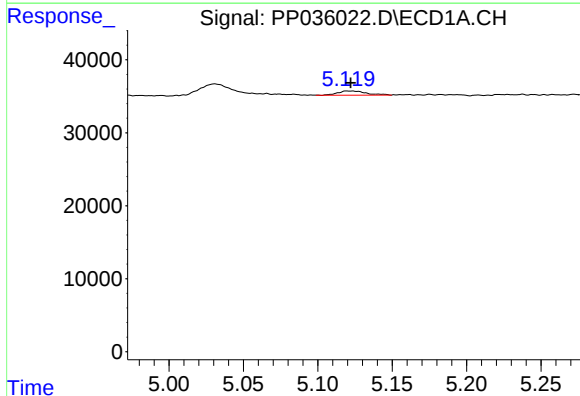


#9 AR-1221-2

R.T.: 5.123 min
Delta R.T.: 0.001 min
Response: 7542
Conc: 41.48 ng/ml

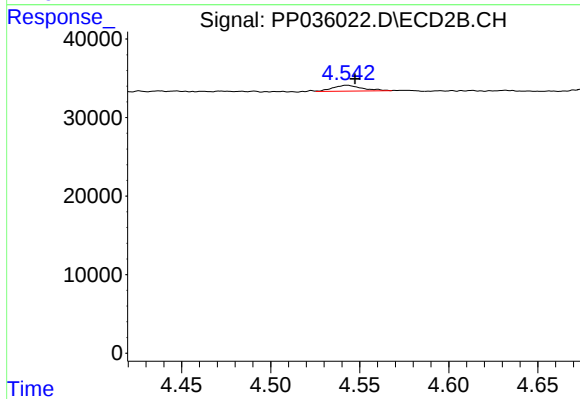

#9 AR-1221-2


R.T.: 4.543 min
Delta R.T.: -0.005 min
Response: 8537
Conc: 32.10 ng/ml

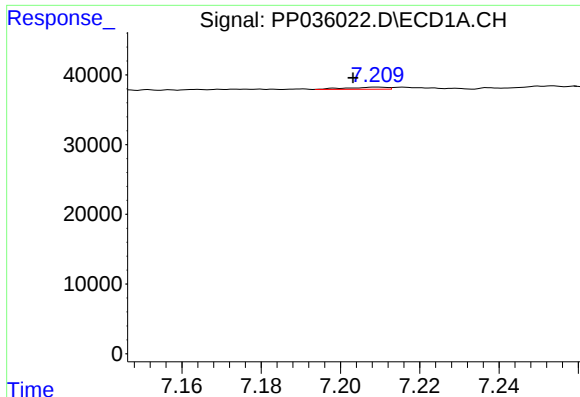

#27 AR-1254-2


R.T.: 7.209 min
Delta R.T.: 0.006 min
Response: 2199
Conc: 2.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
BACKFILL-ASHCROFT-REAR-06RE

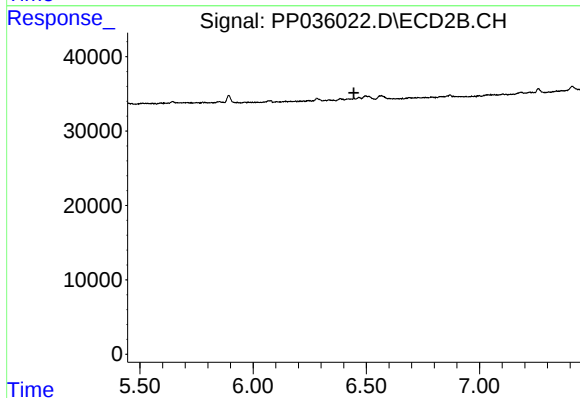


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.445 min
Response: 0
Conc: N.D.

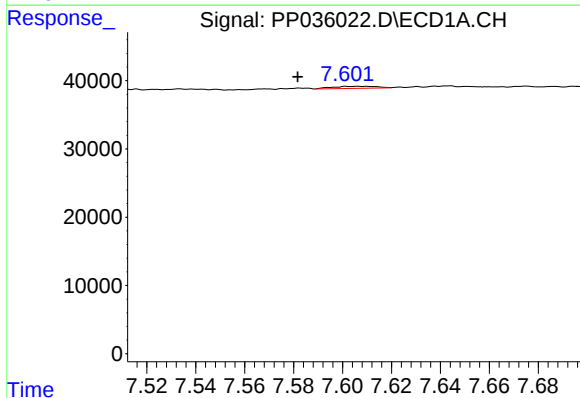


#28 AR-1254-3

R.T.: 7.606 min
Delta R.T.: 0.025 min
Response: 3695
Conc: 3.33 ng/ml

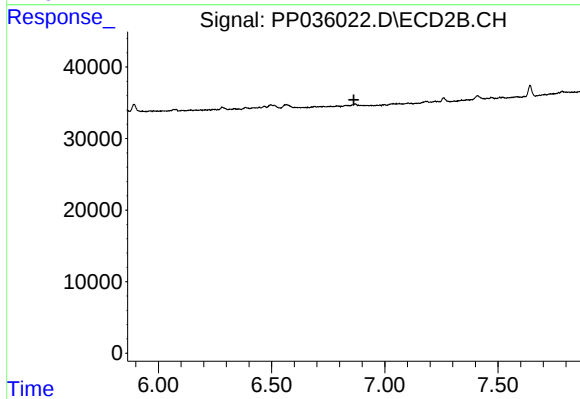

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.863 min
Response: 0
Conc: N.D.

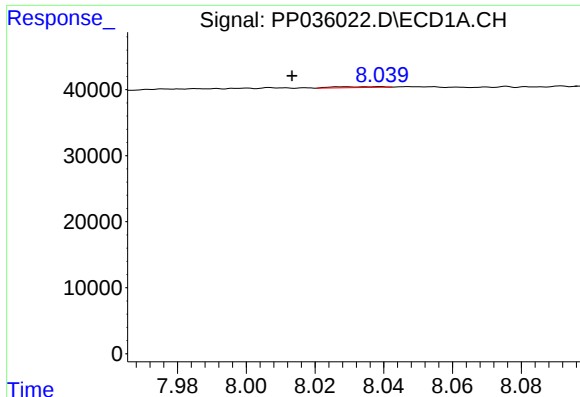

#32 AR-1260-2


R.T.: 8.039 min
Delta R.T.: 0.026 min
Response: 1334
Conc: 1.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
BACKFILL-ASHCROFT-REAR-06RE

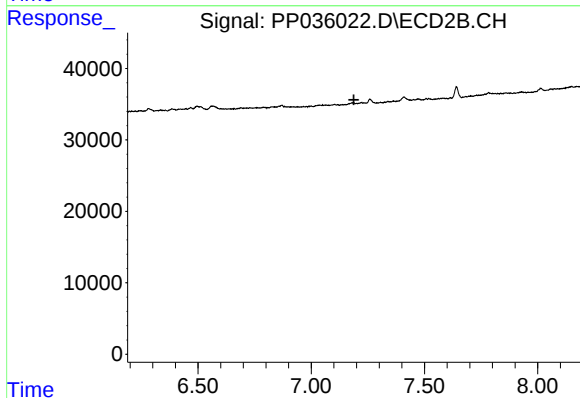


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

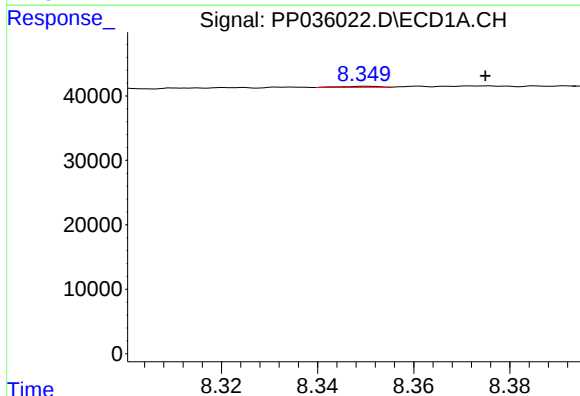


#33 AR-1260-3

R.T.: 8.350 min
Delta R.T.: -0.025 min
Response: 883
Conc: 1.31 ng/ml

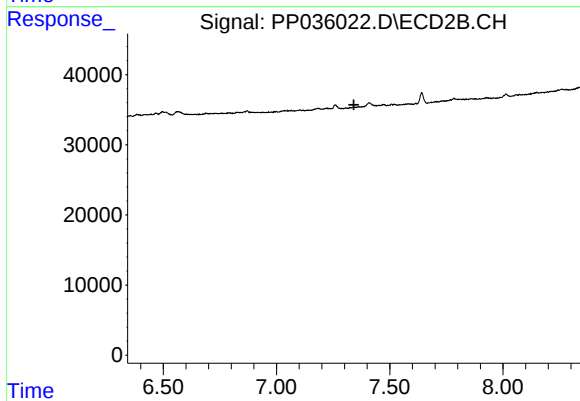

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.342 min
Response: 0
Conc: N.D.

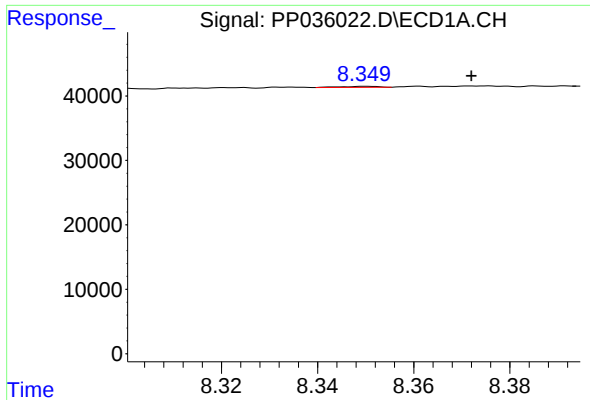

#36 AR-1262-1

R.T.: 8.350 min
Delta R.T.: -0.022 min
Response: 883
Conc: 0.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
BACKFILL-ASHCROFT-REAR-06RE

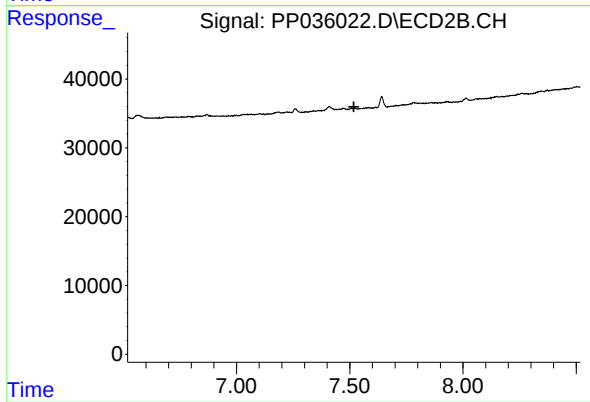

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.518 min
Response: 0
Conc: N.D.