

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051821\
 Data File : PP036028.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 May 2021 16:10
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 18:07:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 18 06:25:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.777	4.189	431449	633950	19.973	19.833
2)	SA Decachlor...	10.605	9.422	297756	449193	21.998	22.749
Target Compounds							
9)	L2 AR-1221-2	5.127	0.000	5217	0	28.692	N.D. #
20)	L4 AR-1242-5	7.041	0.000	15655	0	40.382	N.D. #
24)	L5 AR-1248-4	7.015	0.000	92779	0	145.442	N.D. #
25)	L5 AR-1248-5	7.041	0.000	15655	0	23.365	N.D. #
29)	L6 AR-1254-4	7.874	0.000	19742	0	26.840	N.D. #
32)	L7 AR-1260-2	0.000	7.188	0	7537	N.D.	4.917 #
35)	L7 AR-1260-5	8.907	0.000	2608	0	1.702	N.D. #
37)	L8 AR-1262-2	8.907	0.000	2608	0	1.422	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051821\
Data File : PP036028.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 May 2021 16:10
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 18:07:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 18 06:25:23 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

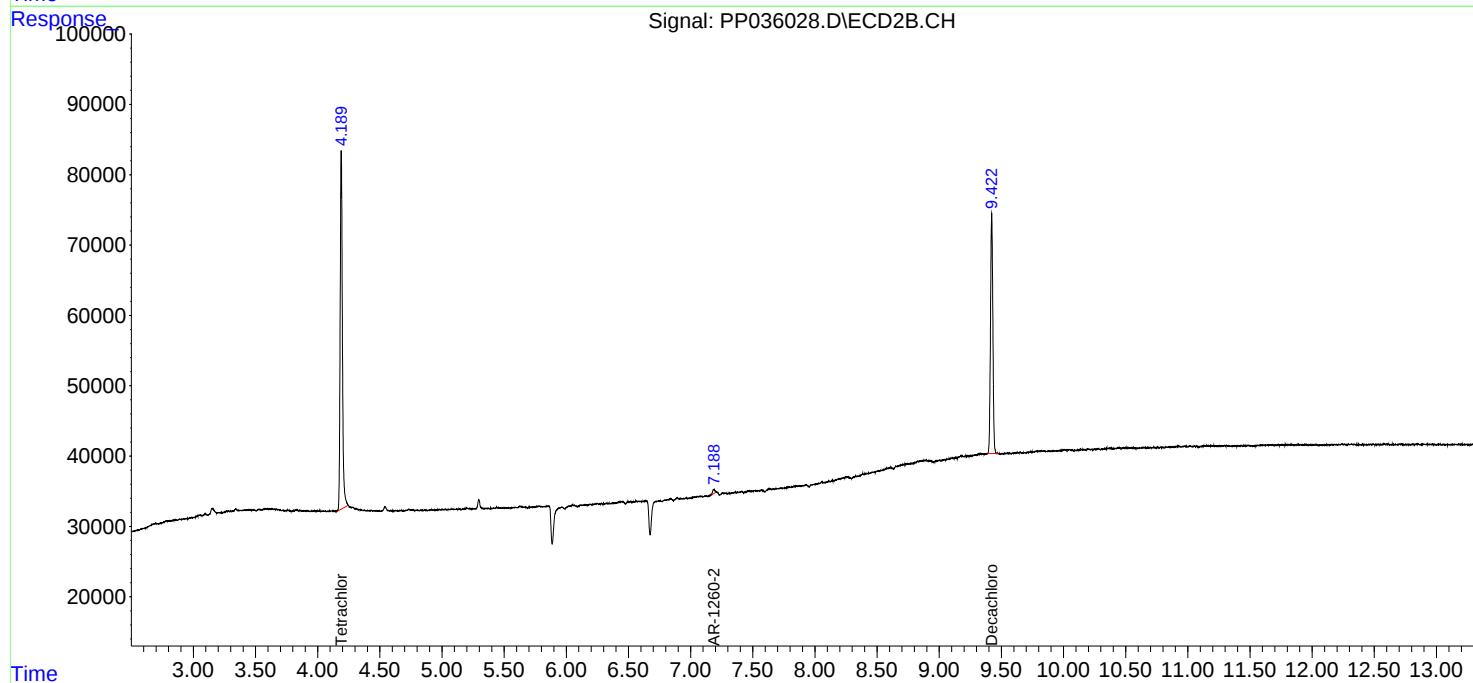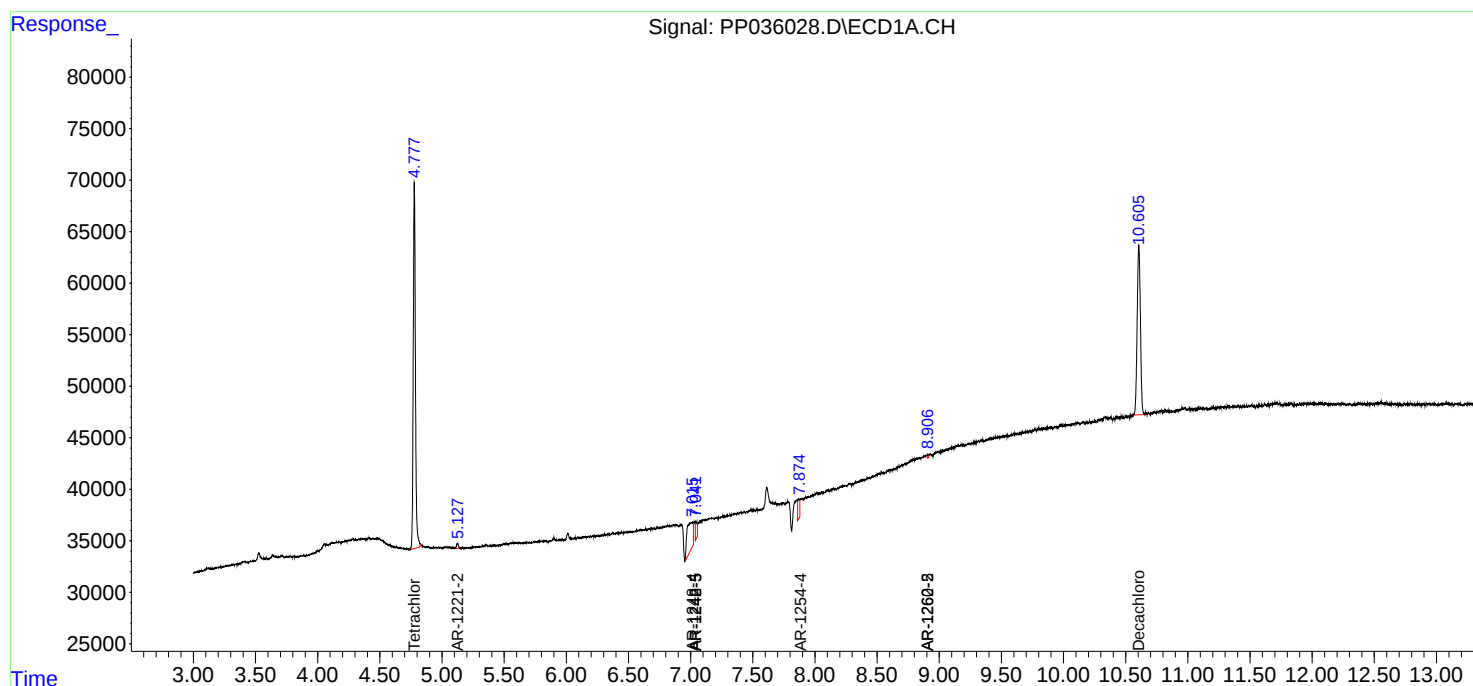


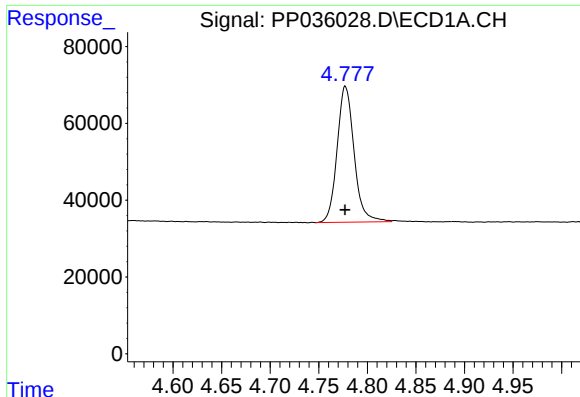

#1 Tetrachloro-m-xylene


R.T.: 4.777 min
Delta R.T.: 0.000 min
Response: 431449
Conc: 19.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

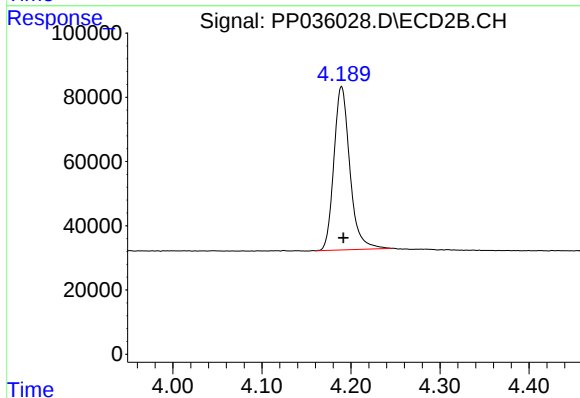


#1 Tetrachloro-m-xylene

R.T.: 4.189 min
Delta R.T.: -0.002 min
Response: 633950
Conc: 19.83 ng/ml

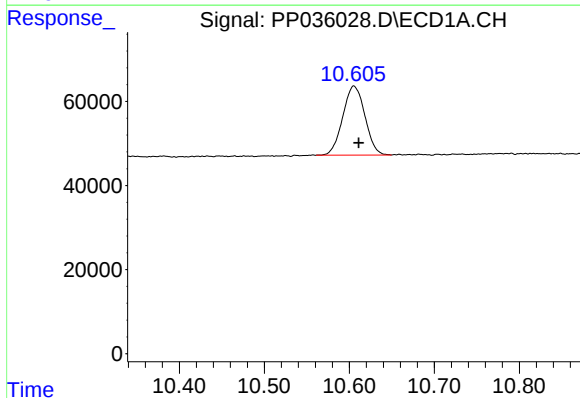


#2 Decachlorobiphenyl

R.T.: 10.605 min
Delta R.T.: -0.006 min
Response: 297756
Conc: 22.00 ng/ml

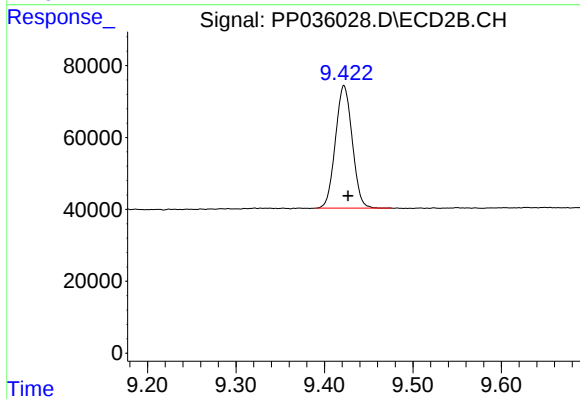

#2 Decachlorobiphenyl


R.T.: 9.422 min
Delta R.T.: -0.004 min
Response: 449193
Conc: 22.75 ng/ml

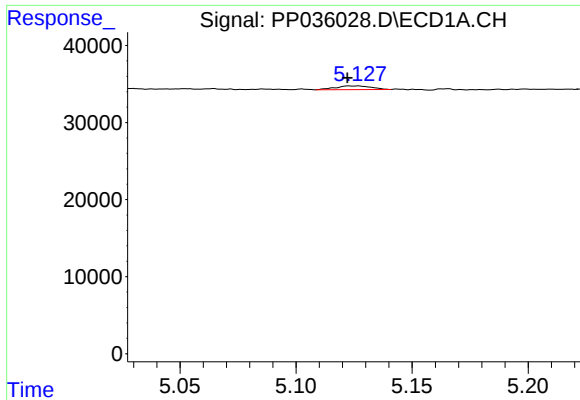

#9 AR-1221-2


R.T.: 5.127 min
Delta R.T.: 0.005 min
Response: 5217
Conc: 28.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

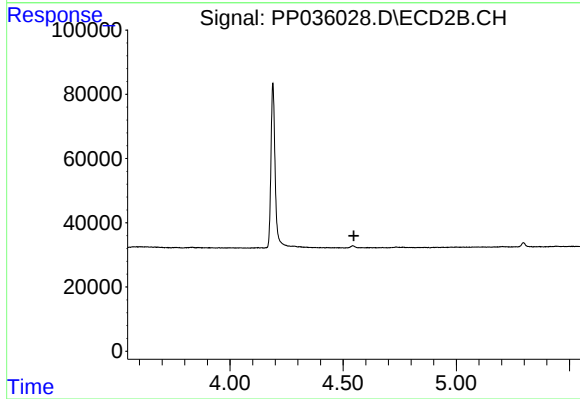


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.547 min
Response: 0
Conc: N.D.

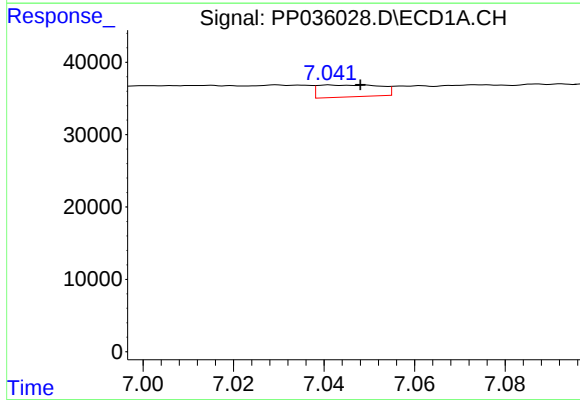


#20 AR-1242-5

R.T.: 7.041 min
Delta R.T.: -0.007 min
Response: 15655
Conc: 40.38 ng/ml

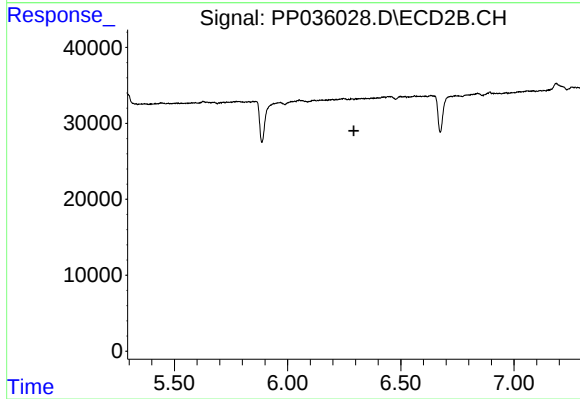

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 6.293 min
Response: 0
Conc: N.D.

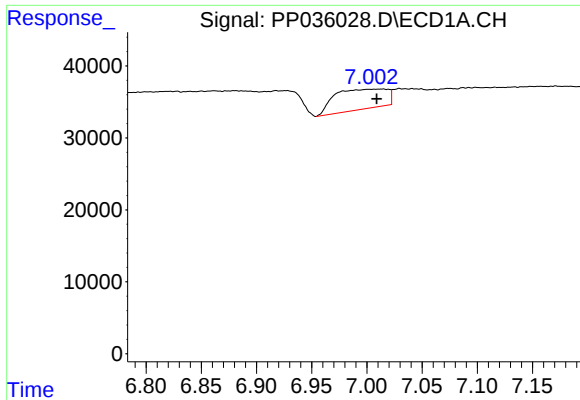

#24 AR-1248-4


R.T.: 7.015 min
Delta R.T.: 0.006 min
Response: 92779
Conc: 145.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

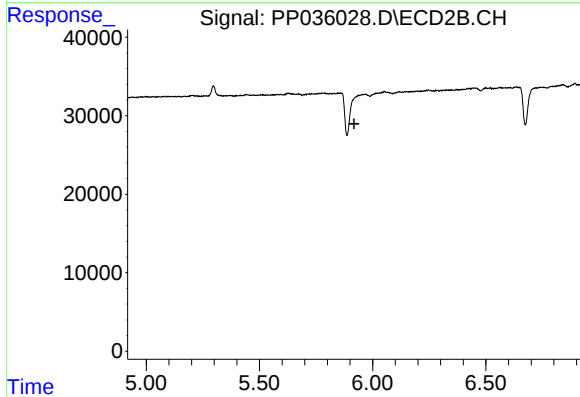


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.917 min
Response: 0
Conc: N.D.

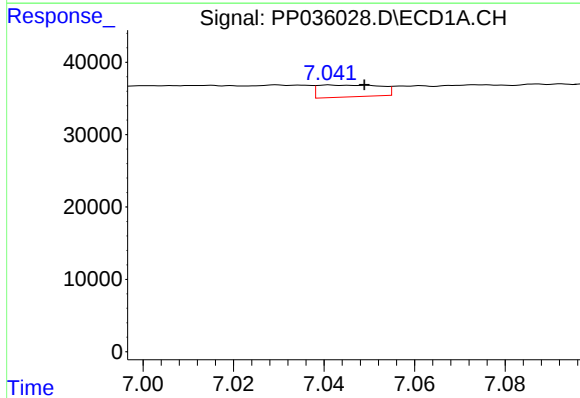


#25 AR-1248-5

R.T.: 7.041 min
Delta R.T.: -0.008 min
Response: 15655
Conc: 23.37 ng/ml

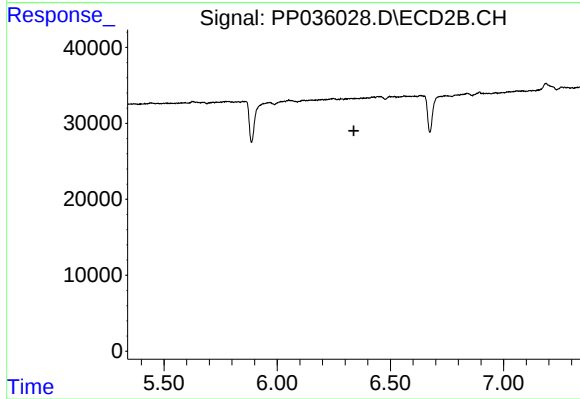

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.339 min
Response: 0
Conc: N.D.

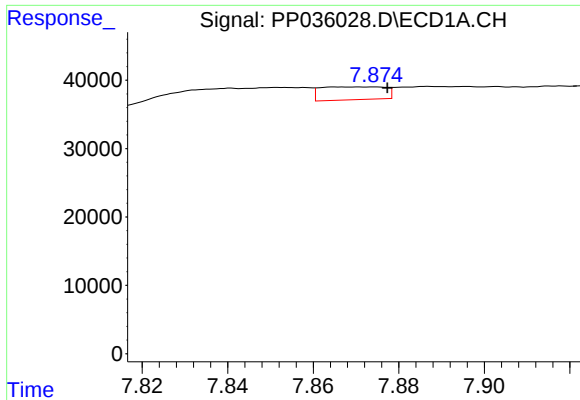

#29 AR-1254-4


R.T.: 7.874 min
Delta R.T.: -0.003 min
Response: 19742
Conc: 26.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

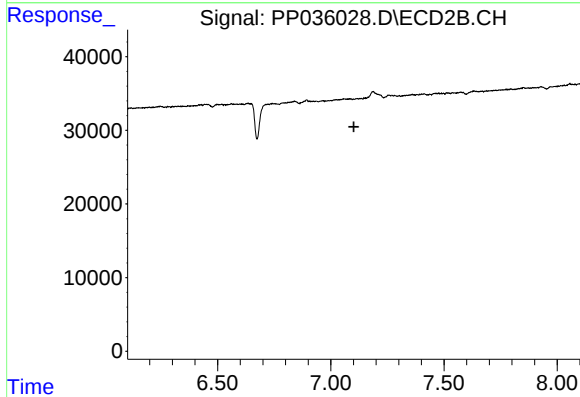


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.102 min
Response: 0
Conc: N.D.

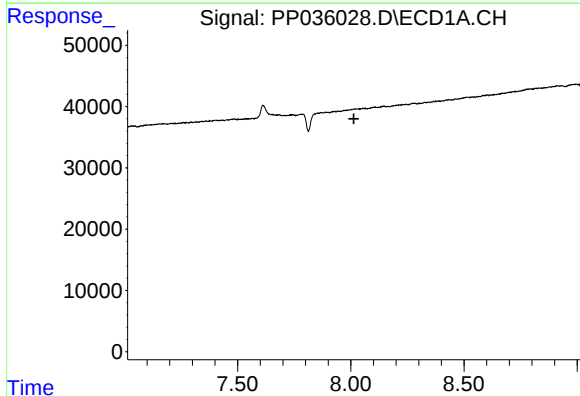


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.013 min
Response: 0
Conc: N.D.

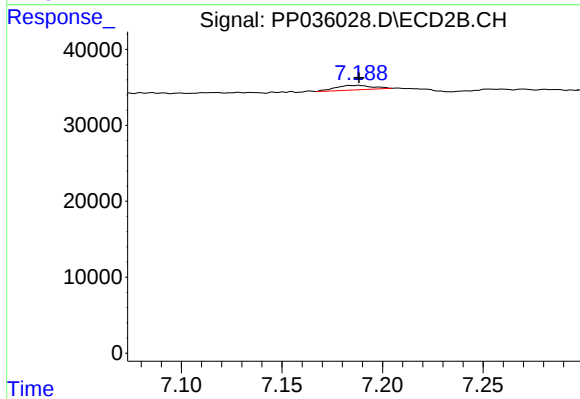

#32 AR-1260-2


R.T.: 7.188 min
Delta R.T.: 0.000 min
Response: 7537
Conc: 4.92 ng/ml

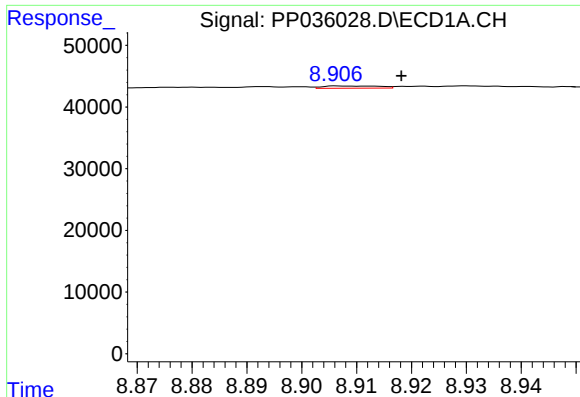

#35 AR-1260-5


R.T.: 8.907 min
Delta R.T.: -0.012 min
Response: 2608
Conc: 1.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

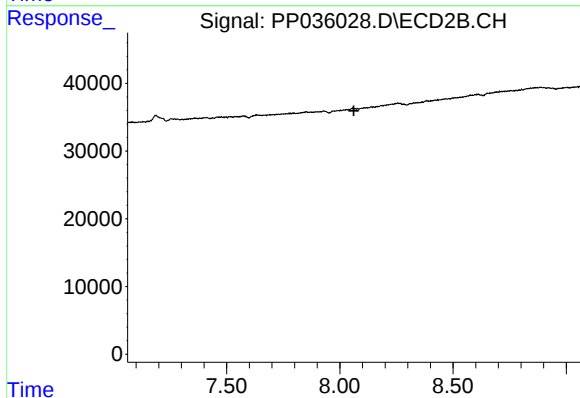


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 8.062 min
Response: 0
Conc: N.D.

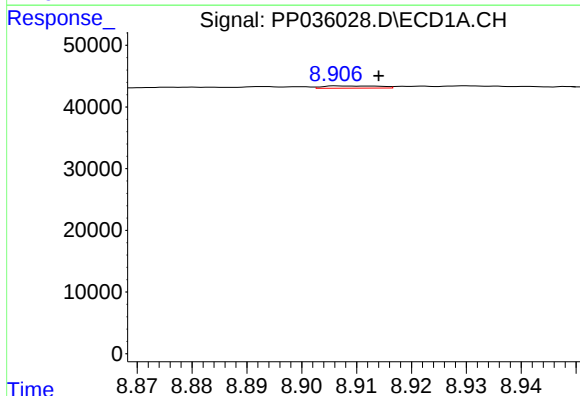

#37 AR-1262-2

R.T.: 8.907 min
Delta R.T.: -0.007 min
Response: 2608
Conc: 1.42 ng/ml

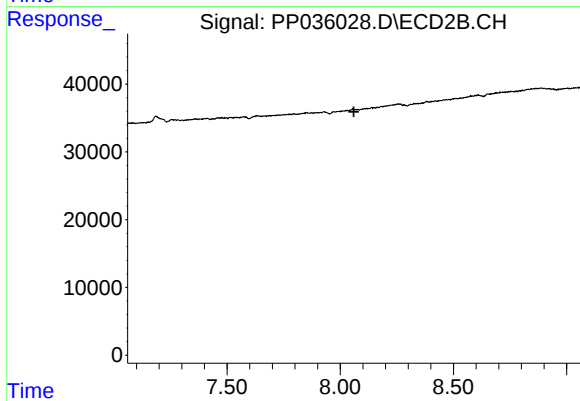

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.060 min
Response: 0
Conc: N.D.