

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051821\
 Data File : PP036034.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 May 2021 17:51
 Operator : DD\AJ
 Sample : M2435-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VAN-REIPEN-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 18:13:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 18 06:25:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.774	4.190	514648	751526	23.825	23.512
2)	SA Decachlor...	10.602	9.422	268047	389597	19.803	19.731
Target Compounds							
9)	L2 AR-1221-2	5.123	0.000	8912	0	49.014	N.D. #
24)	L5 AR-1248-4	6.998	0.000	19672	0	30.839	N.D. #
26)	L6 AR-1254-1	6.998f	0.000	19672	0	29.159	N.D. #
27)	L6 AR-1254-2	7.211	0.000	8659	0	8.407	N.D. #
28)	L6 AR-1254-3	7.581	0.000	4413	0	3.972	N.D. #
30)	L6 AR-1254-5	8.298	7.516	9135	29566	9.842	16.529 #
31)	L7 AR-1260-1	7.737	0.000	2383	0	3.034	N.D. #
32)	L7 AR-1260-2	8.004	7.187	12126	8754	13.905	5.711 #
33)	L7 AR-1260-3	8.358f	0.000	391	0	0.582	N.D. #
34)	L7 AR-1260-4	8.595	0.000	6312	0	7.286	N.D. #
35)	L7 AR-1260-5	8.914	0.000	6093	0	3.976	N.D. #
36)	L8 AR-1262-1	8.358	7.516	391	29566	0.372	33.442 #
37)	L8 AR-1262-2	8.914	0.000	6093	0	3.322	N.D. #
39)	L8 AR-1262-4	9.278f	8.404	3685	5993	3.704	2.615 #
42)	L9 AR-1268-2	9.278f	8.404	3685	5993	1.899	1.900



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051821\
Data File : PP036034.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 May 2021 17:51
Operator : DD\AJ
Sample : M2435-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
VAN-REIPEN-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 18:13:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 18 06:25:23 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

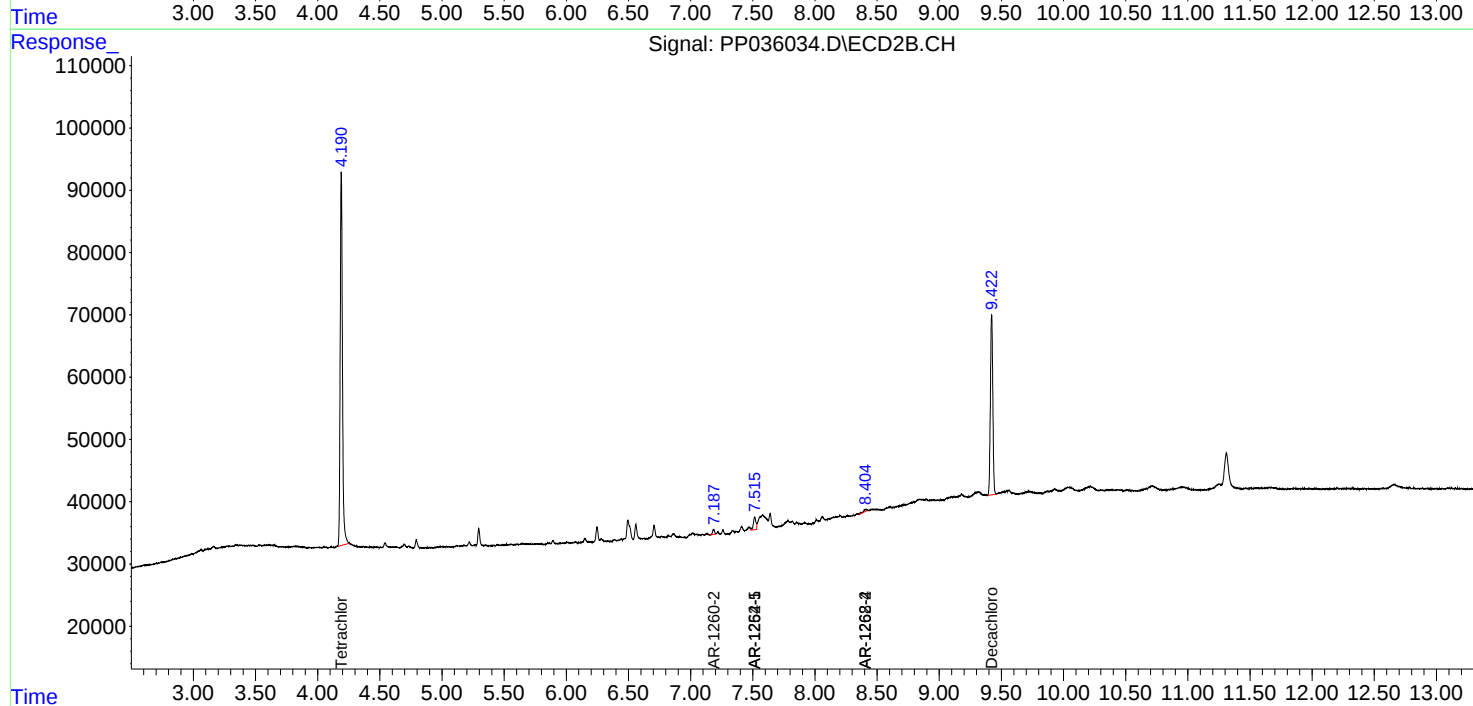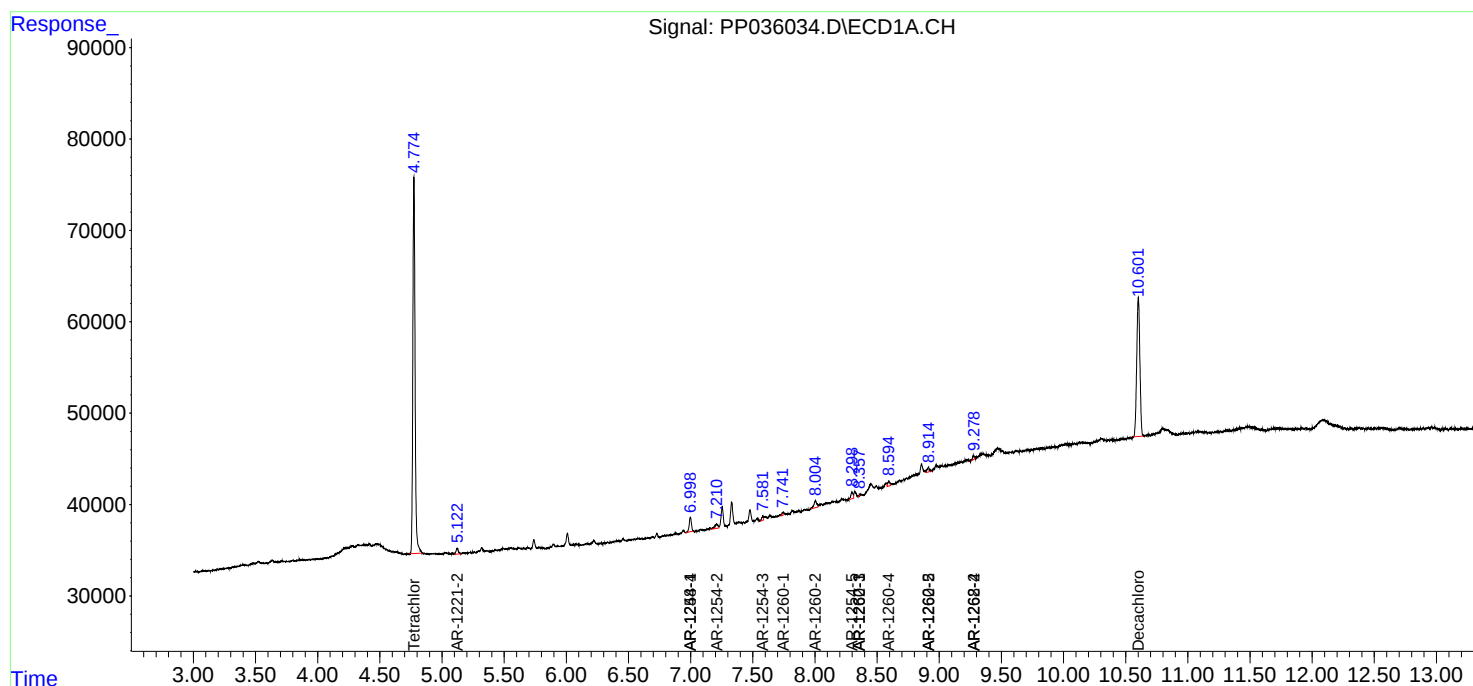


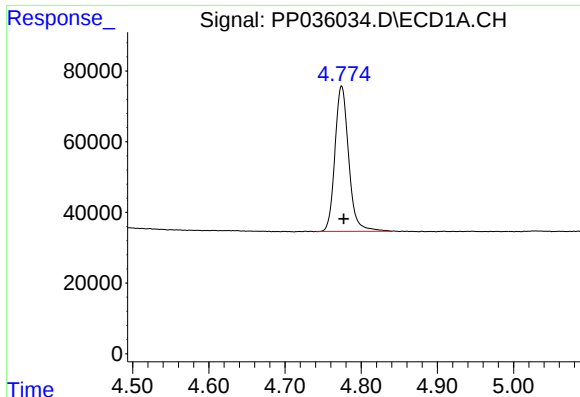

#1 Tetrachloro-m-xylene


R.T.: 4.774 min
Delta R.T.: -0.003 min
Response: 514648
Conc: 23.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
VAN-REIPEN-A

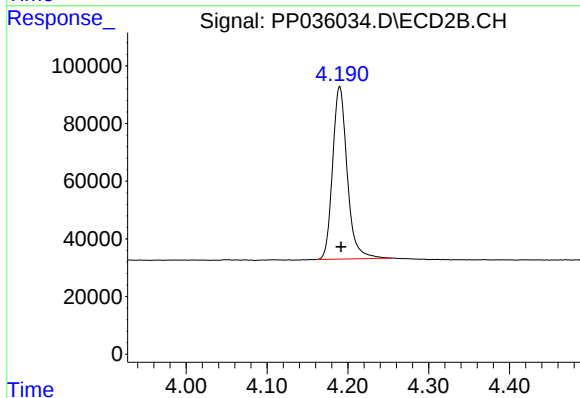


#1 Tetrachloro-m-xylene

R.T.: 4.190 min
Delta R.T.: -0.002 min
Response: 751526
Conc: 23.51 ng/ml

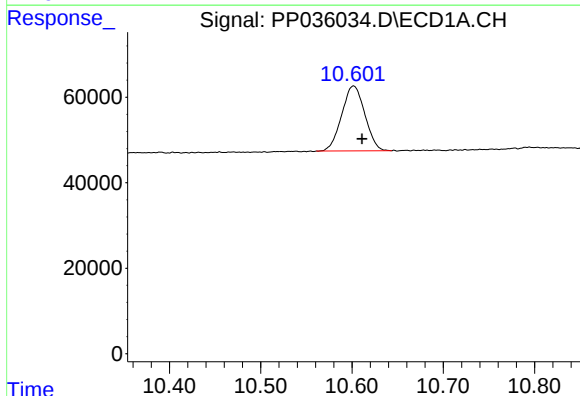


#2 Decachlorobiphenyl

R.T.: 10.602 min
Delta R.T.: -0.009 min
Response: 268047
Conc: 19.80 ng/ml

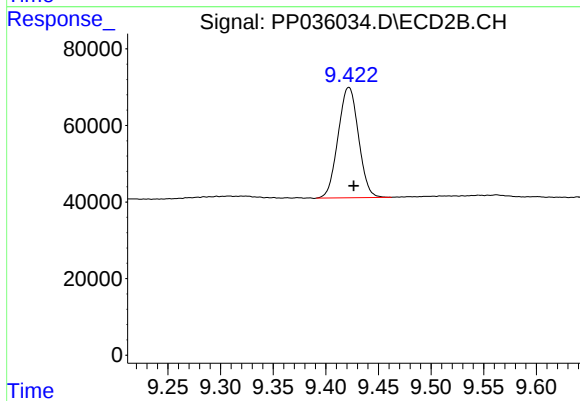

#2 Decachlorobiphenyl


R.T.: 9.422 min
Delta R.T.: -0.005 min
Response: 389597
Conc: 19.73 ng/ml

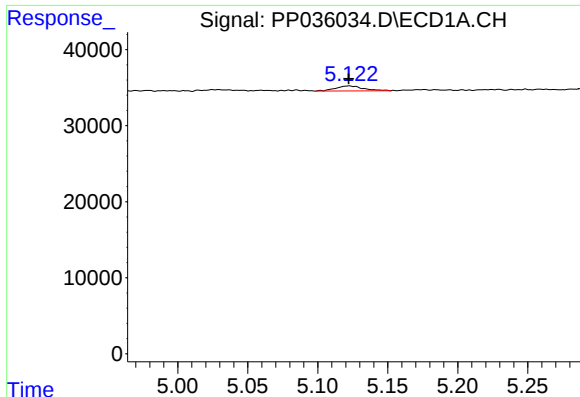

#9 AR-1221-2


R.T.: 5.123 min
Delta R.T.: 0.000 min
Response: 8912
Conc: 49.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
VAN-REIPEN-A

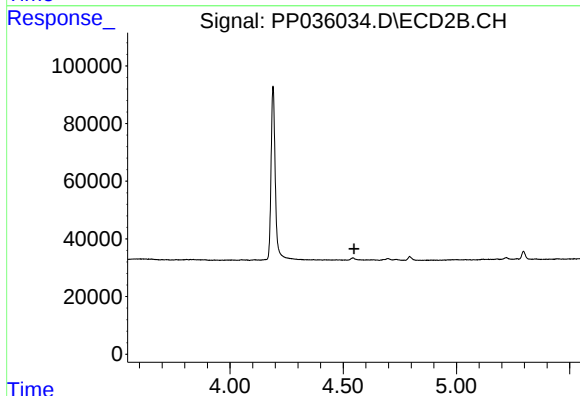


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.547 min
Response: 0
Conc: N.D.

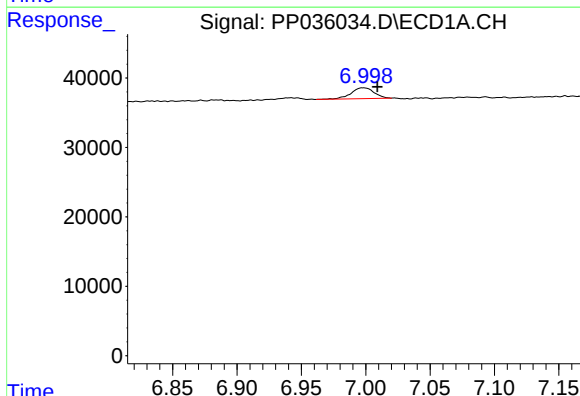


#24 AR-1248-4

R.T.: 6.998 min
Delta R.T.: -0.011 min
Response: 19672
Conc: 30.84 ng/ml

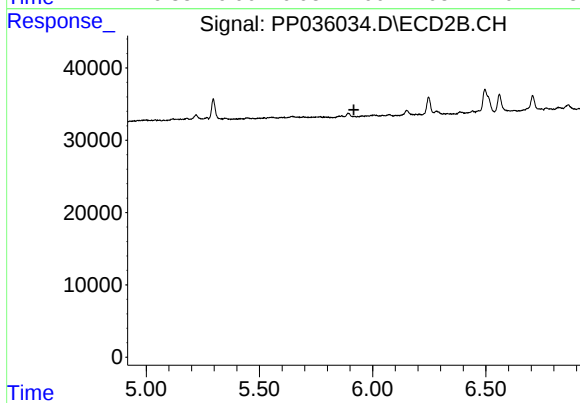

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.917 min
Response: 0
Conc: N.D.

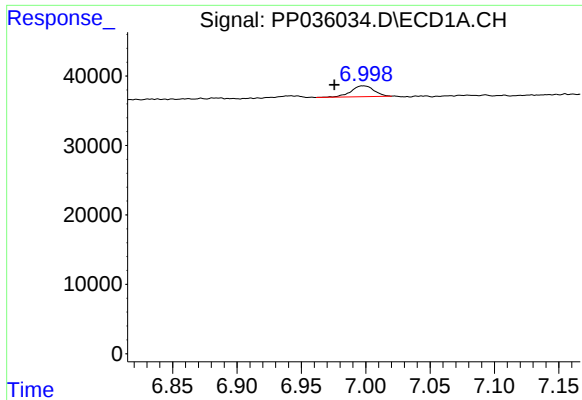

#26 AR-1254-1


R.T.: 6.998 min
Delta R.T.: 0.022 min
Response: 19672
Conc: 29.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
VAN-REIPEN-A

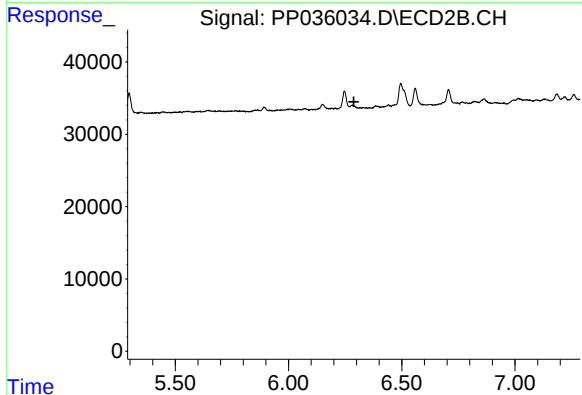


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.289 min
Response: 0
Conc: N.D.

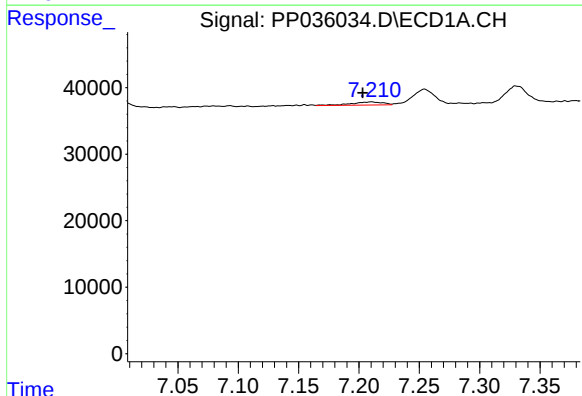


#27 AR-1254-2

R.T.: 7.211 min
Delta R.T.: 0.008 min
Response: 8659
Conc: 8.41 ng/ml

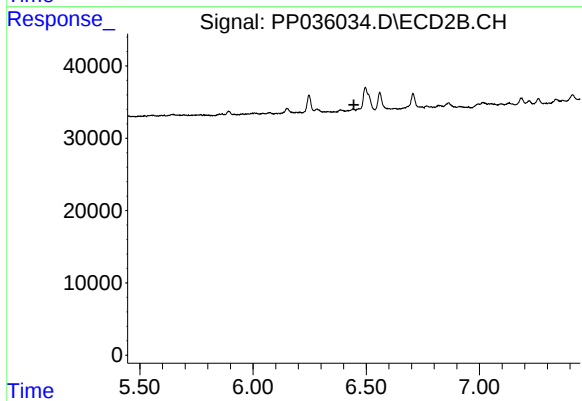

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 6.445 min
Response: 0
Conc: N.D.

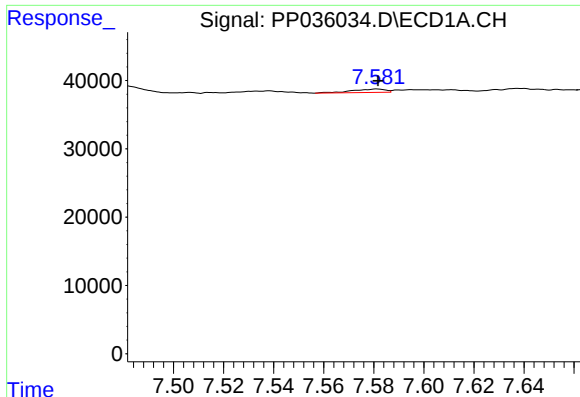

#28 AR-1254-3


R.T.: 7.581 min
Delta R.T.: 0.000 min
Response: 4413
Conc: 3.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
VAN-REIPEN-A

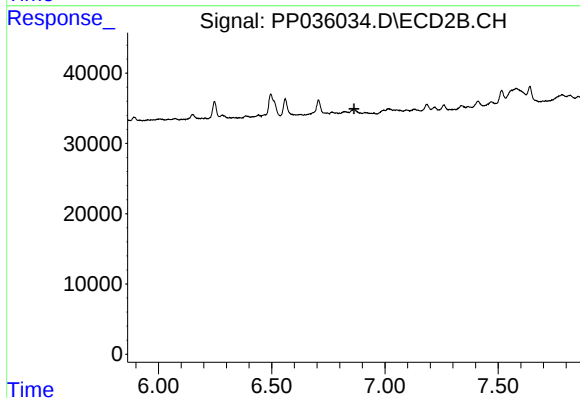


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.863 min
Response: 0
Conc: N.D.

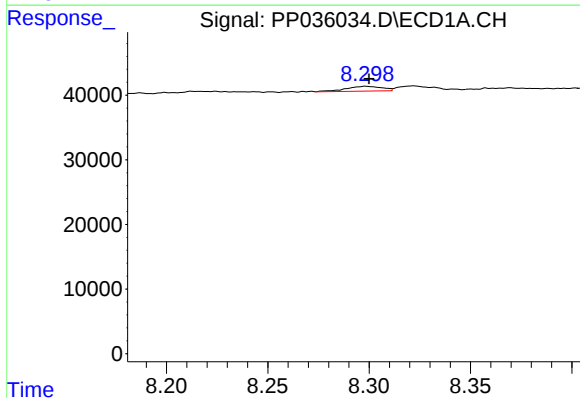


#30 AR-1254-5

R.T.: 8.298 min
Delta R.T.: -0.002 min
Response: 9135
Conc: 9.84 ng/ml

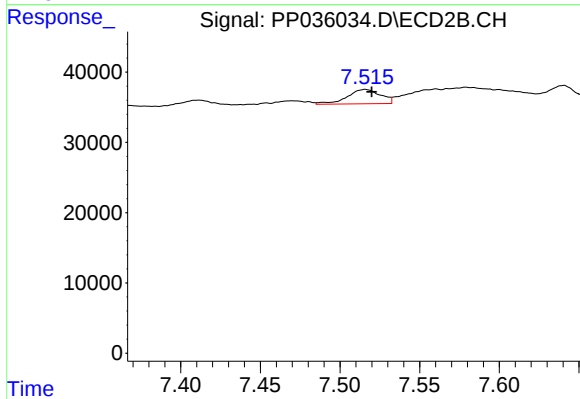

#30 AR-1254-5


R.T.: 7.516 min
Delta R.T.: -0.004 min
Response: 29566
Conc: 16.53 ng/ml

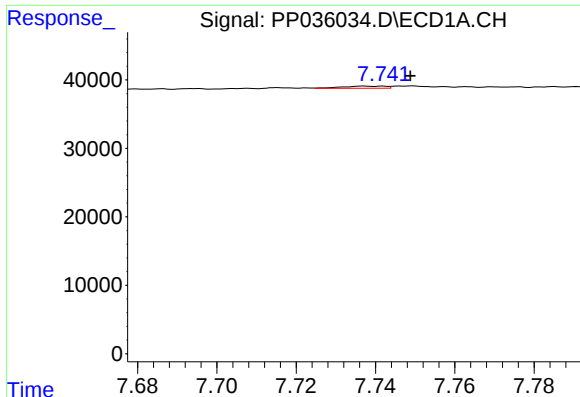

#31 AR-1260-1


R.T.: 7.737 min
Delta R.T.: -0.012 min
Response: 2383
Conc: 3.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
VAN-REIPEN-A

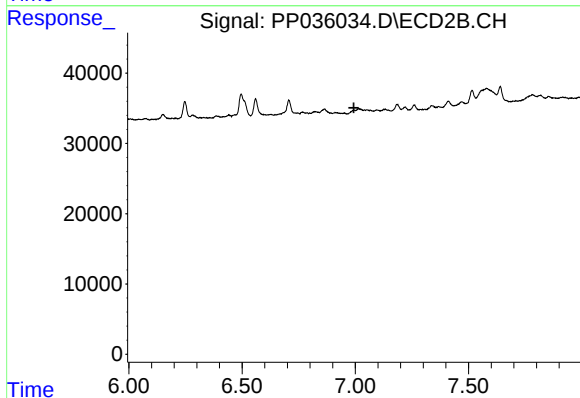


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.994 min
Response: 0
Conc: N.D.

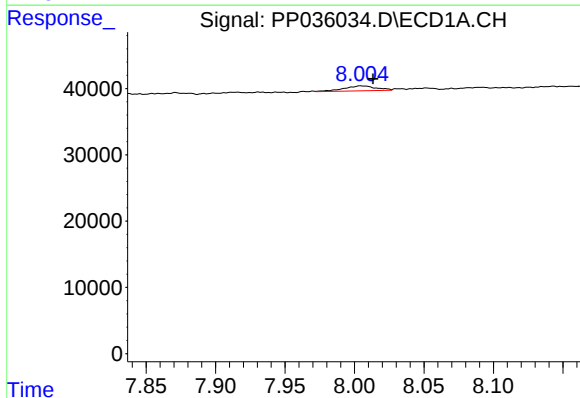


#32 AR-1260-2

R.T.: 8.004 min
Delta R.T.: -0.009 min
Response: 12126
Conc: 13.90 ng/ml

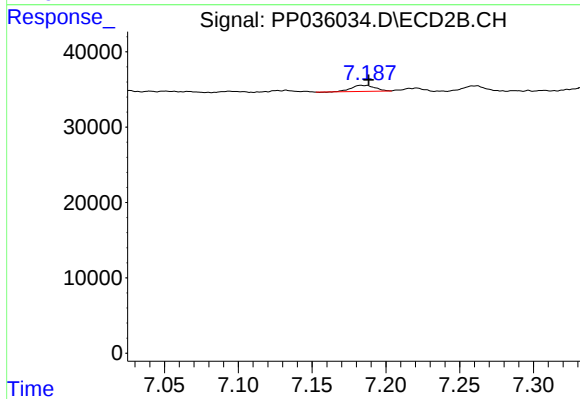

#32 AR-1260-2


R.T.: 7.187 min
Delta R.T.: 0.000 min
Response: 8754
Conc: 5.71 ng/ml

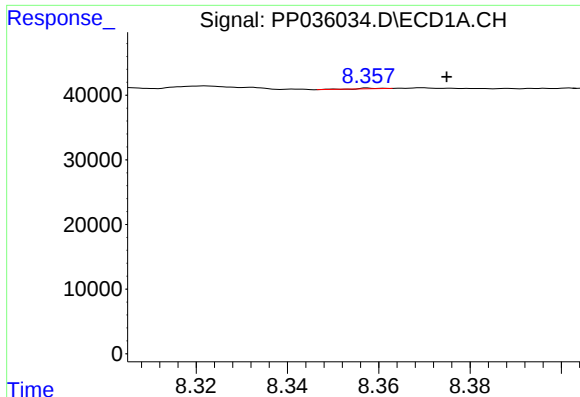

#33 AR-1260-3


R.T.: 8.358 min
Delta R.T.: -0.017 min
Response: 391
Conc: 0.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
VAN-REIPEN-A

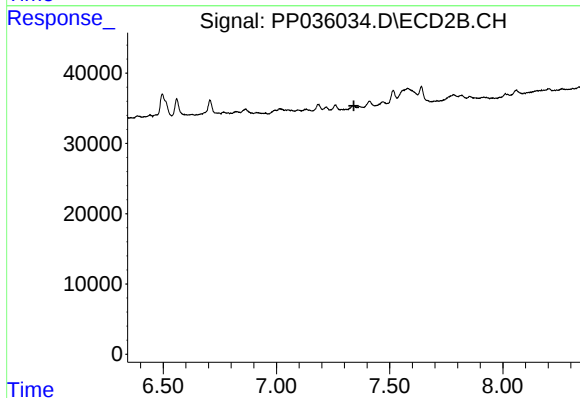


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.342 min
Response: 0
Conc: N.D.

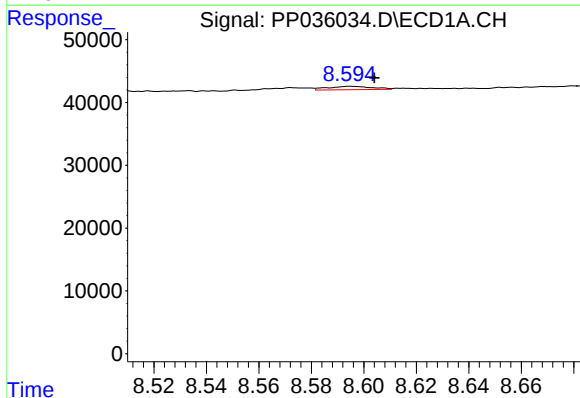


#34 AR-1260-4

R.T.: 8.595 min
Delta R.T.: -0.010 min
Response: 6312
Conc: 7.29 ng/ml

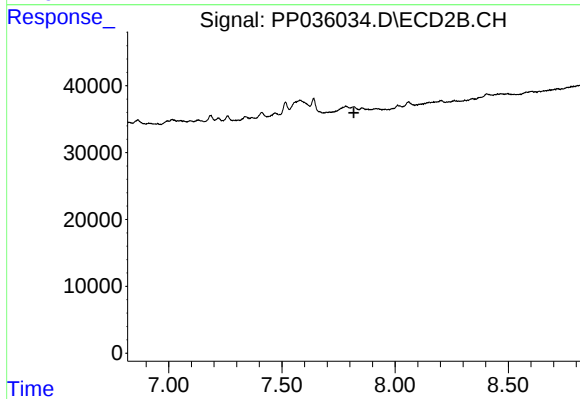

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.818 min
Response: 0
Conc: N.D.

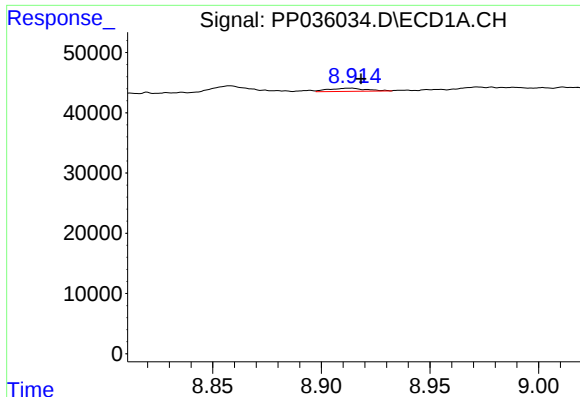

#35 AR-1260-5


R.T.: 8.914 min
Delta R.T.: -0.004 min
Response: 6093
Conc: 3.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
VAN-REIPEN-A

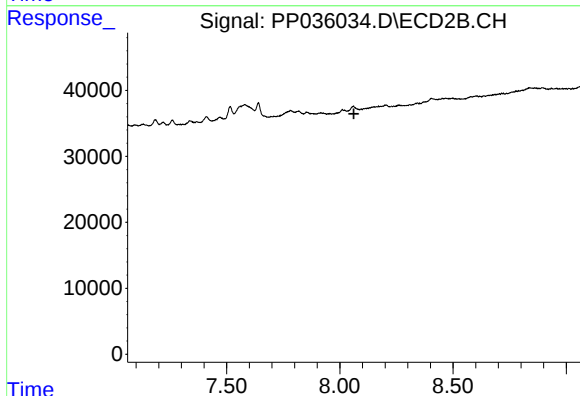


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 8.062 min
Response: 0
Conc: N.D.

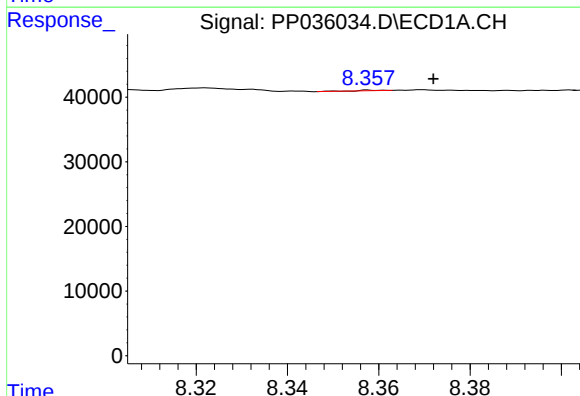


#36 AR-1262-1

R.T.: 8.358 min
Delta R.T.: -0.014 min
Response: 391
Conc: 0.37 ng/ml

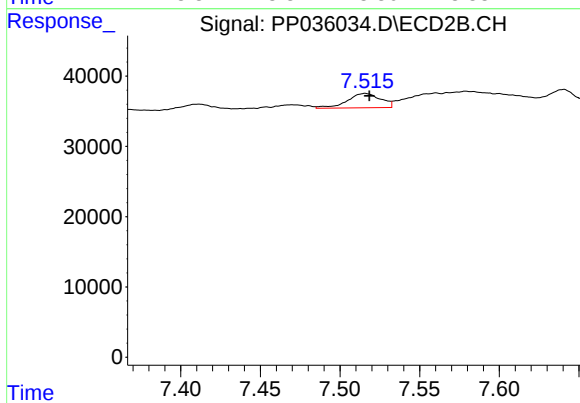

#36 AR-1262-1


R.T.: 7.516 min
Delta R.T.: -0.003 min
Response: 29566
Conc: 33.44 ng/ml

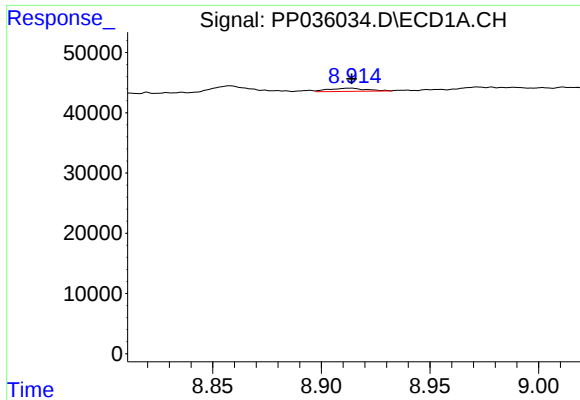

#37 AR-1262-2


R.T.: 8.914 min
Delta R.T.: 0.000 min
Response: 6093
Conc: 3.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
VAN-REIPEN-A

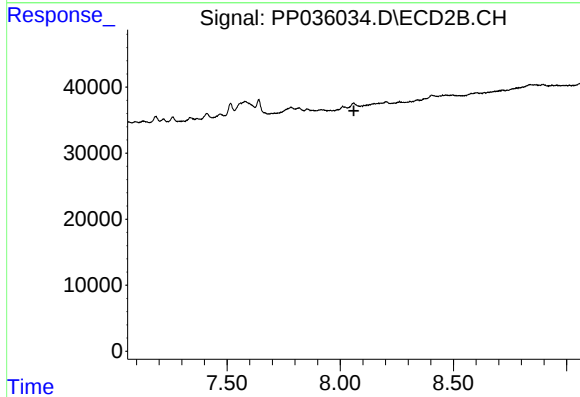


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.060 min
Response: 0
Conc: N.D.

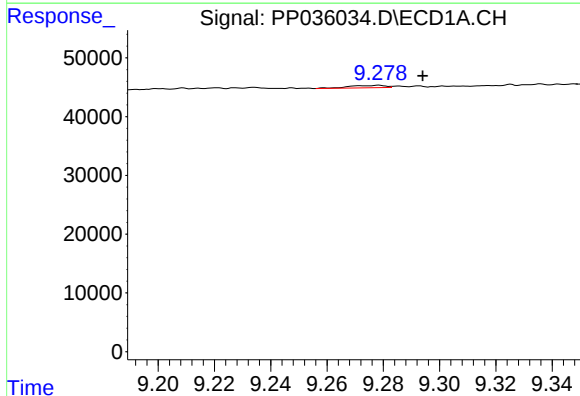


#39 AR-1262-4

R.T.: 9.278 min
Delta R.T.: -0.016 min
Response: 3685
Conc: 3.70 ng/ml

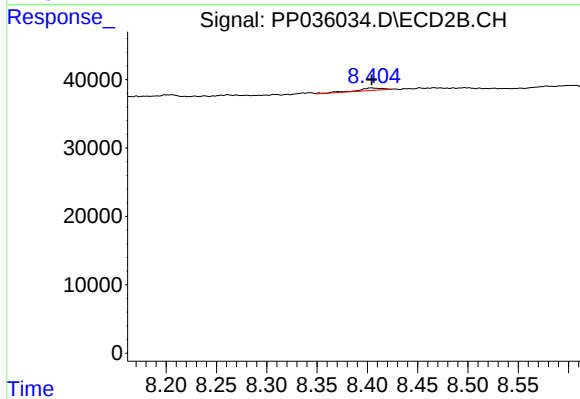

#39 AR-1262-4


R.T.: 8.404 min
Delta R.T.: 0.000 min
Response: 5993
Conc: 2.62 ng/ml

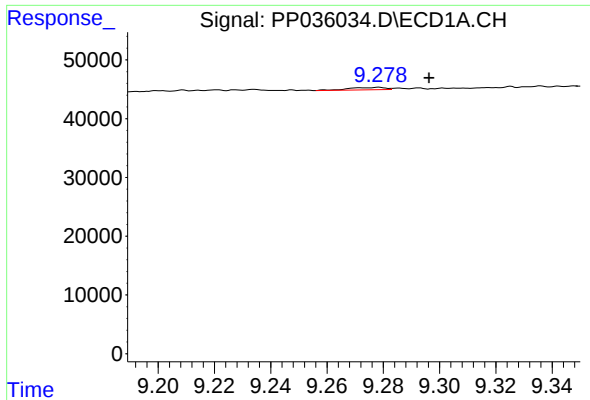

#42 AR-1268-2

R.T.: 9.278 min
Delta R.T.: -0.018 min
Response: 3685
Conc: 1.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
VAN-REIPEN-A

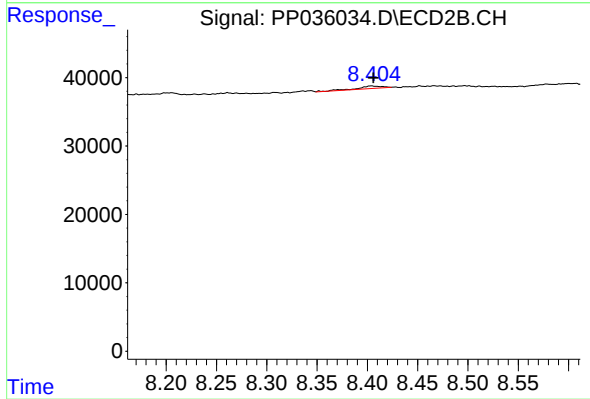

#42 AR-1268-2

R.T.: 8.404 min
Delta R.T.: -0.002 min
Response: 5993
Conc: 1.90 ng/ml