

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051821\
 Data File : PP036020.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 May 2021 13:13
 Operator : DD\AJ
 Sample : M2392-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-06-COMP

Manual Integrations
 APPROVED

Ankita
 5/19/2021 3:13:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 18:02:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 18 06:25:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.775	4.190	432499	629212	20.022	19.685
2) SA Decachlor...	10.601	9.421	222206	315829	16.417	15.995
Target Compounds						
31) L7 AR-1260-1	7.743	6.990	74033	129688	94.242m	103.950
32) L7 AR-1260-2	8.007	7.184	85677	134199	98.248m	87.548
33) L7 AR-1260-3	8.369	7.337	65261	123763	97.108	89.254
34) L7 AR-1260-4	8.593	7.812	110669	68641	127.755	57.796 #
35) L7 AR-1260-5	8.911	8.057	110576	157035	72.154	60.798

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051821\
Data File : PP036020.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 May 2021 13:13
Operator : DD\AJ
Sample : M2392-17
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
SB-06-COMP


Manual Integrations
APPROVED

Ankita
5/19/2021 3:13:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 18:02:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 18 06:25:23 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

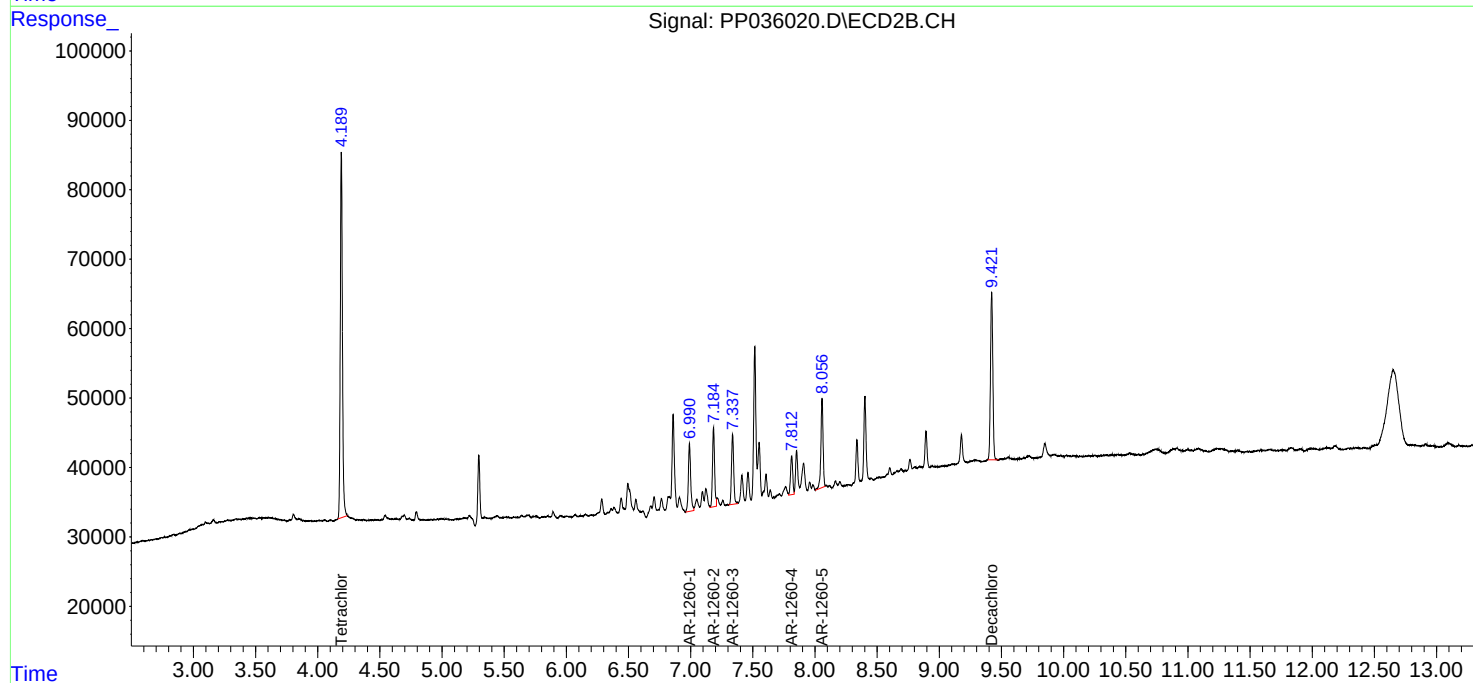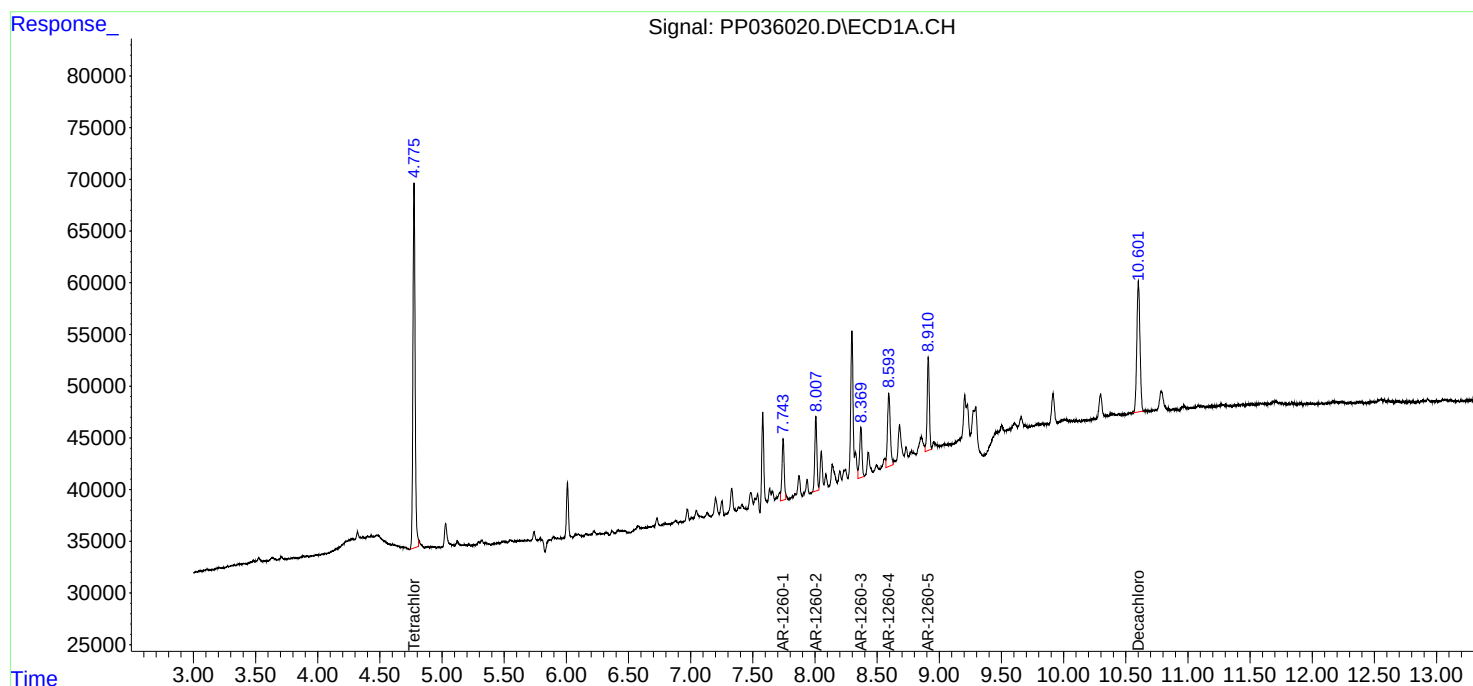

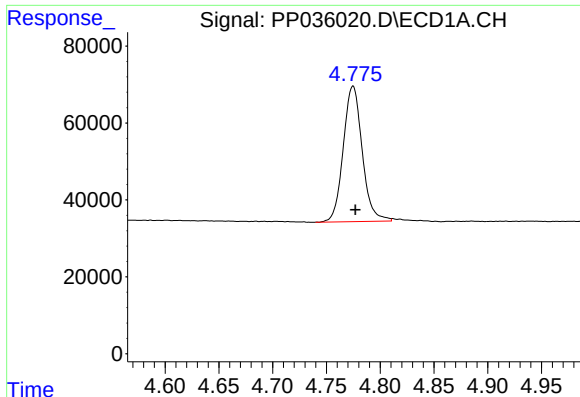


#1 Tetrachloro-m-xylene

R.T.: 4.775 min
Delta R.T.: -0.002 min
Response: 432499
Conc: 20.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-06-COMP


Manual Integrations
APPROVED

Ankita
5/19/2021 3:13:25 PM

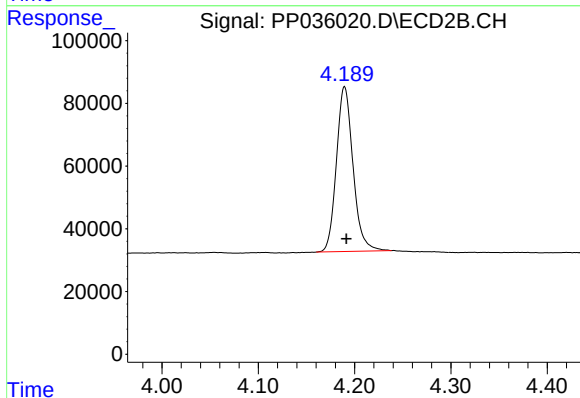


#1 Tetrachloro-m-xylene

R.T.: 4.190 min
Delta R.T.: -0.002 min
Response: 629212
Conc: 19.68 ng/ml

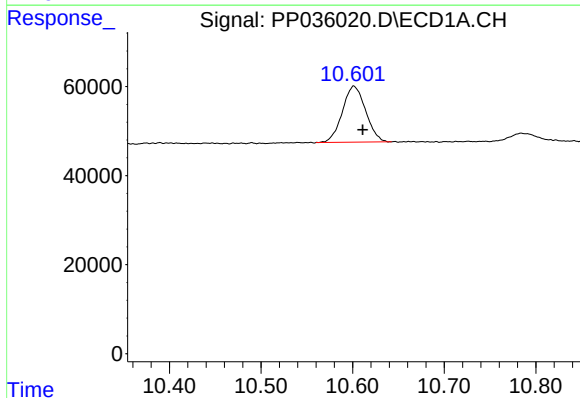


#2 Decachlorobiphenyl

R.T.: 10.601 min
Delta R.T.: -0.010 min
Response: 222206
Conc: 16.42 ng/ml

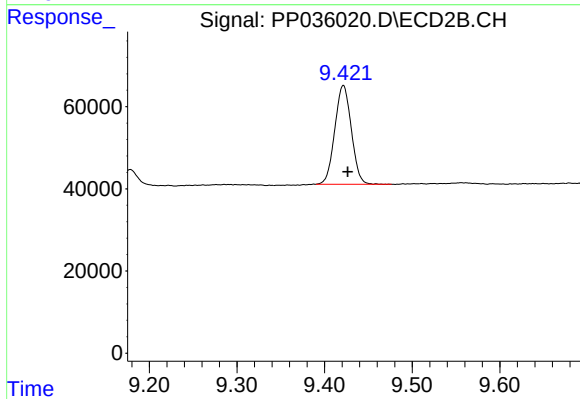

#2 Decachlorobiphenyl

R.T.: 9.421 min
Delta R.T.: -0.005 min
Response: 315829
Conc: 15.99 ng/ml

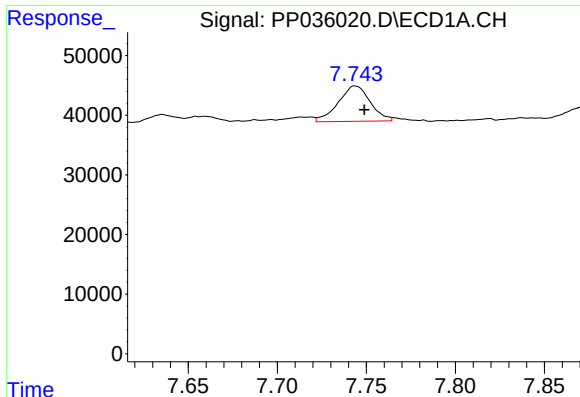


#31 AR-1260-1

R.T.: 7.743 min
Delta R.T.: -0.006 min
Response: 74033
Conc: 94.24 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SB-06-COMP


Manual Integrations
APPROVED

Ankita
5/19/2021 3:13:25 PM

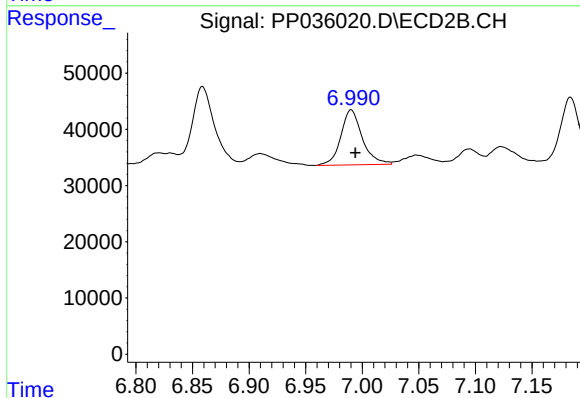


#31 AR-1260-1

R.T.: 6.990 min
Delta R.T.: -0.004 min
Response: 129688
Conc: 103.95 ng/ml

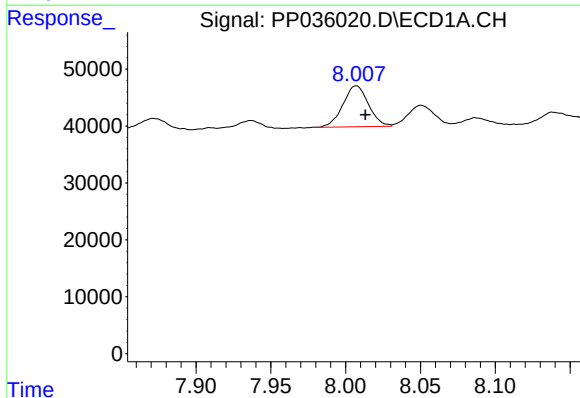


#32 AR-1260-2

R.T.: 8.007 min
Delta R.T.: -0.006 min
Response: 85677
Conc: 98.25 ng/ml m

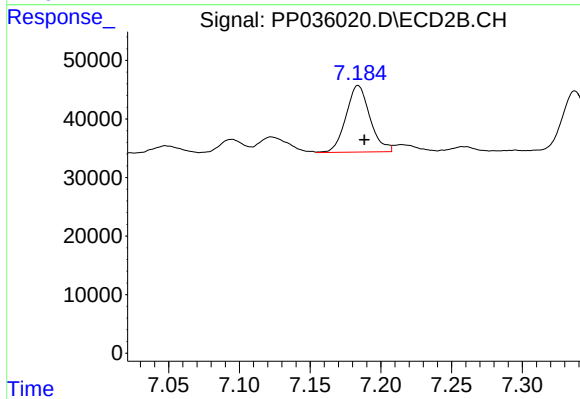

#32 AR-1260-2

R.T.: 7.184 min
Delta R.T.: -0.004 min
Response: 134199
Conc: 87.55 ng/ml

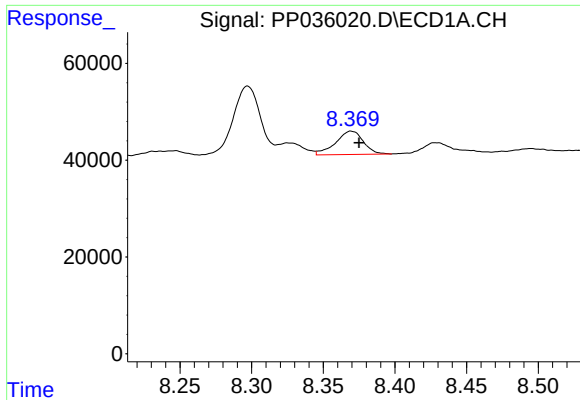


#33 AR-1260-3

R.T.: 8.369 min
Delta R.T.: -0.006 min
Response: 65261
Conc: 97.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-06-COMP


Manual Integrations
APPROVED

Ankita
5/19/2021 3:13:25 PM

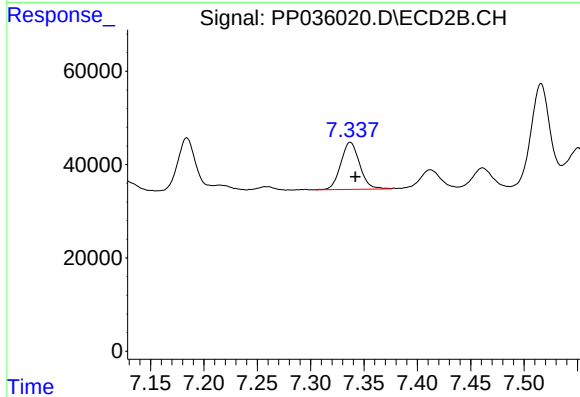


#33 AR-1260-3

R.T.: 7.337 min
Delta R.T.: -0.005 min
Response: 123763
Conc: 89.25 ng/ml

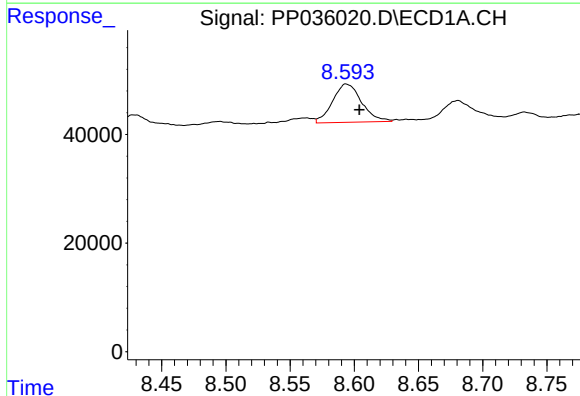


#34 AR-1260-4

R.T.: 8.593 min
Delta R.T.: -0.011 min
Response: 110669
Conc: 127.75 ng/ml

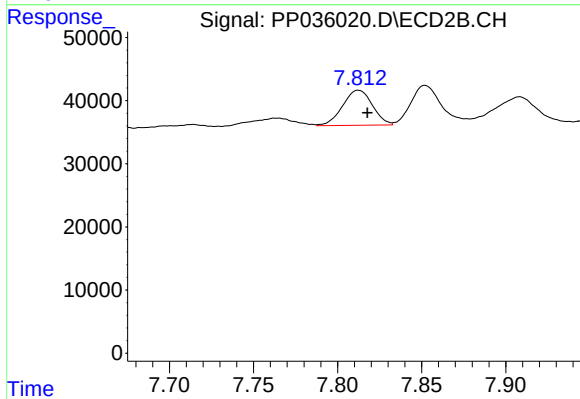

#34 AR-1260-4

R.T.: 7.812 min
Delta R.T.: -0.005 min
Response: 68641
Conc: 57.80 ng/ml

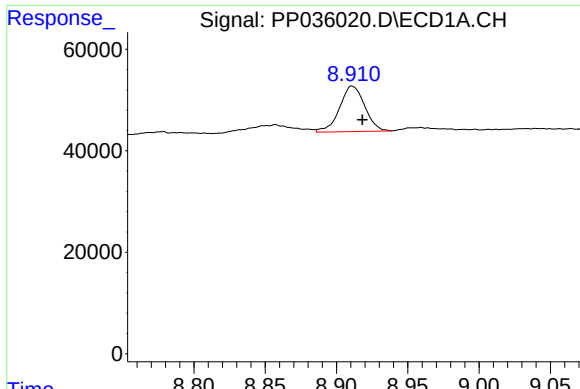


#35 AR-1260-5

R.T.: 8.911 min
Delta R.T.: -0.007 min
Response: 110576
Conc: 72.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-06-COMP

Manual Integrations
APPROVED

Ankita
5/19/2021 3:13:25 PM

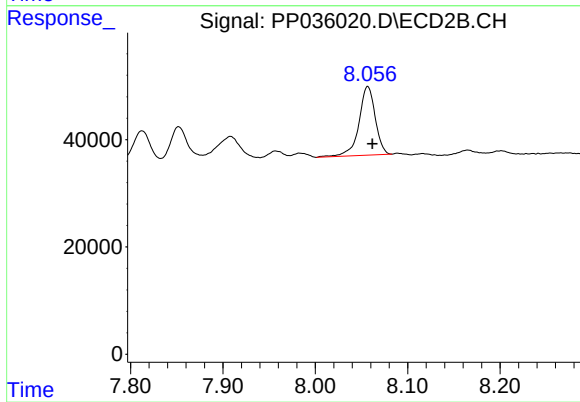

#35 AR-1260-5

R.T.: 8.057 min
Delta R.T.: -0.005 min
Response: 157035
Conc: 60.80 ng/ml