

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051821\
 Data File : PP036035.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 May 2021 18:08
 Operator : DD\AJ
 Sample : M2435-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VAN-REIPEN-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 18:54:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 18 06:25:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.775	4.190	499857	751476	23.140	23.510
2) SA Decachlor...	10.601	9.422	278523	395172	20.577	20.013

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051821\
Data File : PP036035.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 May 2021 18:08
Operator : DD\AJ
Sample : M2435-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
VAN-REIPEN-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 18:54:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 18 06:25:23 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

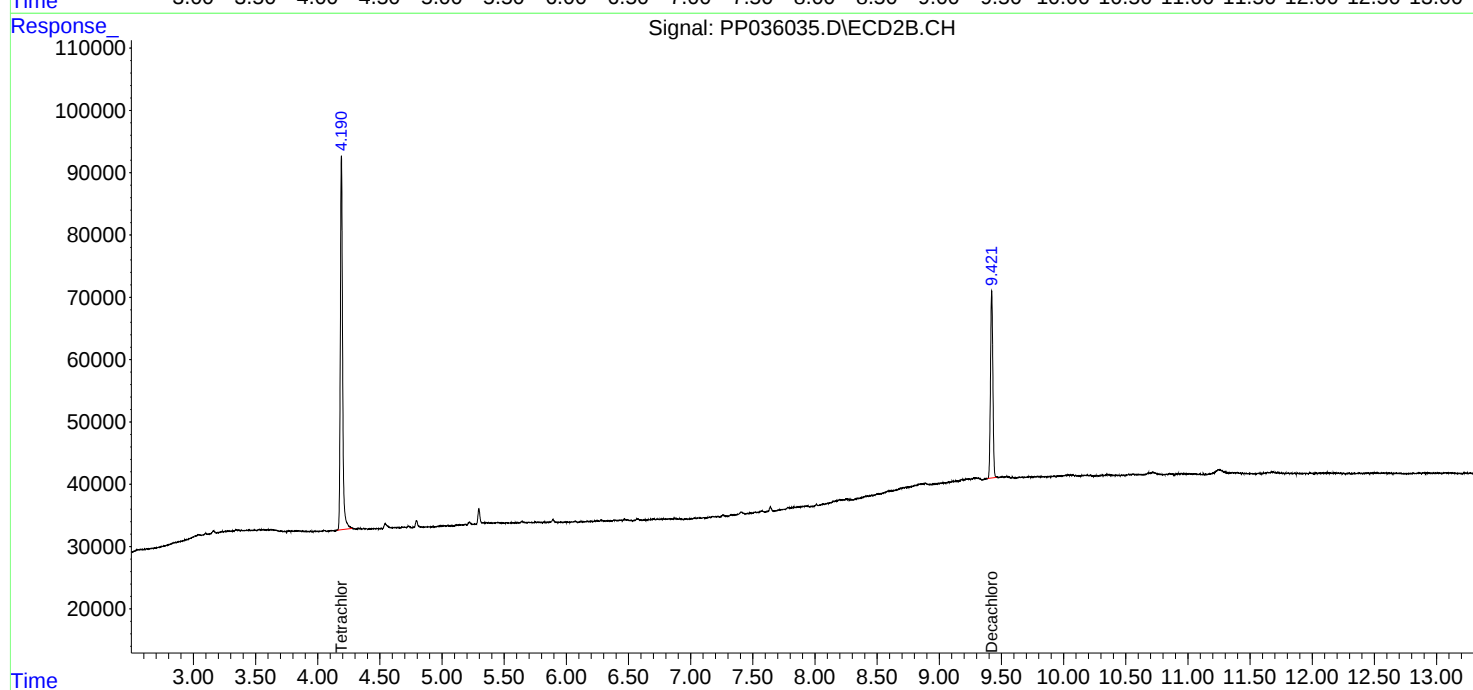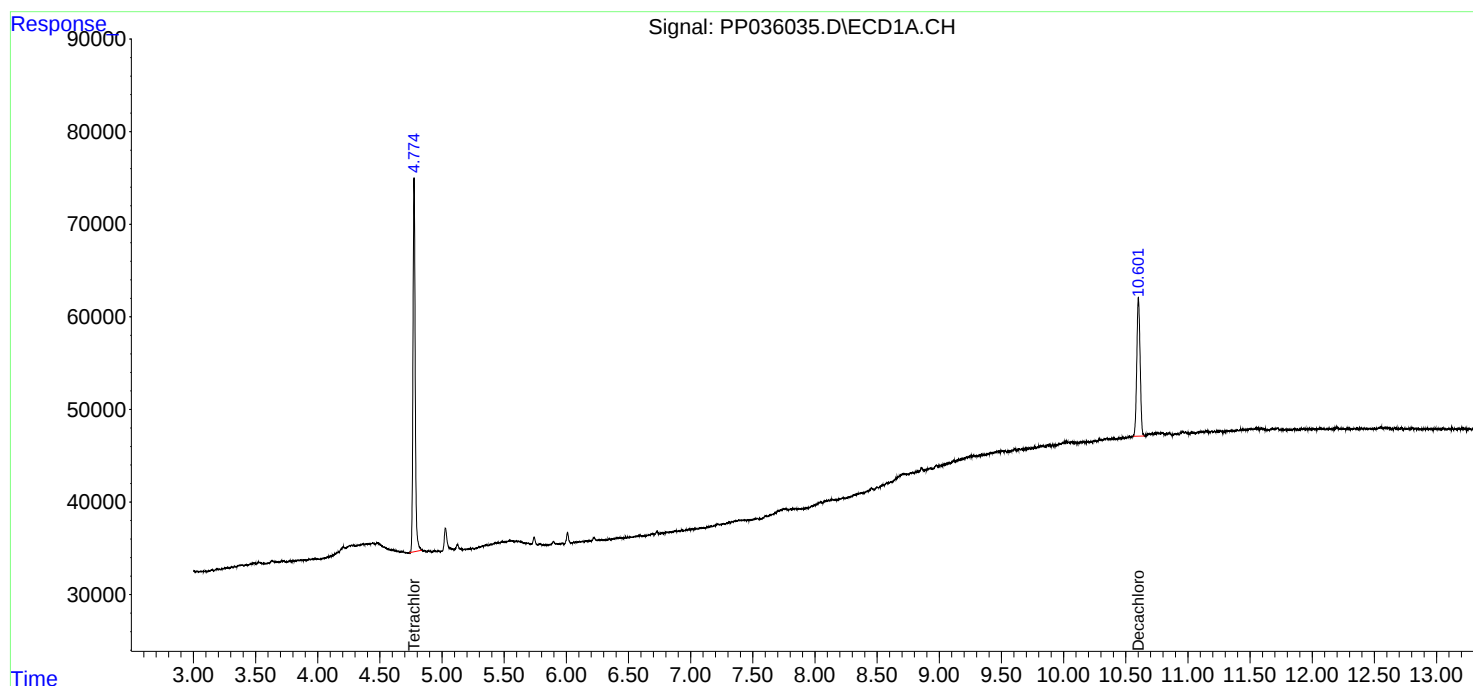


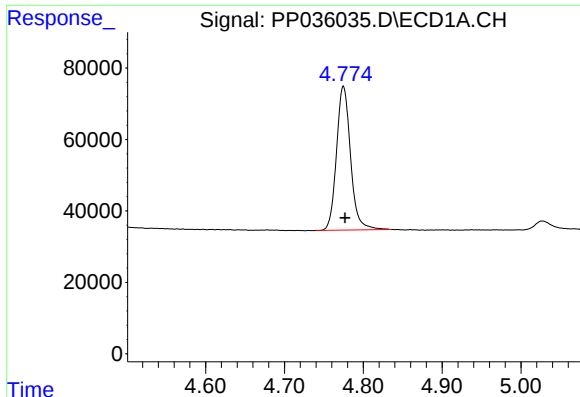

#1 Tetrachloro-m-xylene


R.T.: 4.775 min
Delta R.T.: -0.002 min
Response: 499857
Conc: 23.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
VAN-REIPEN-B

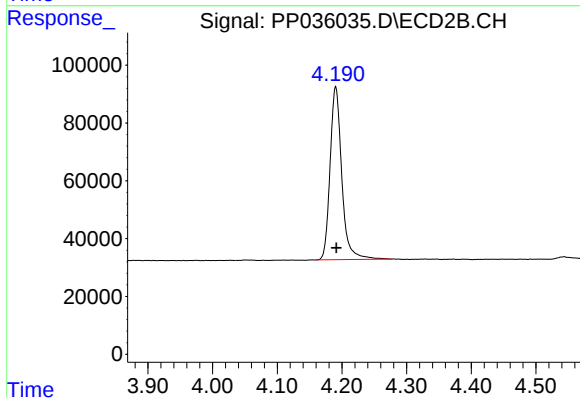


#1 Tetrachloro-m-xylene

R.T.: 4.190 min
Delta R.T.: -0.001 min
Response: 751476
Conc: 23.51 ng/ml

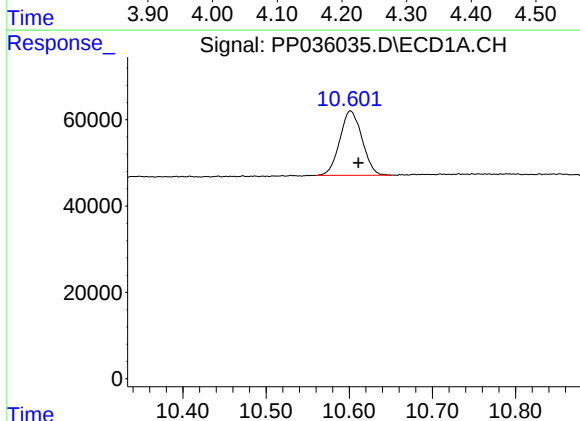

#2 Decachlorobiphenyl

R.T.: 10.601 min
Delta R.T.: -0.010 min
Response: 278523
Conc: 20.58 ng/ml

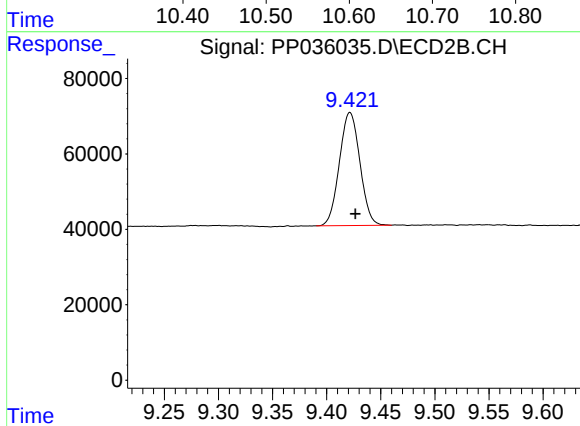

#2 Decachlorobiphenyl

R.T.: 9.422 min
Delta R.T.: -0.005 min
Response: 395172
Conc: 20.01 ng/ml