

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051822\
 Data File : PP047730.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2022 18:15
 Operator : YP\AJ
 Sample : N2904-01 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FCA566M-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 00:36:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 11 13:10:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.842	3.109	3073085	4647034	1.209	1.411
2) SA Decachlor...	9.900	8.408	3471642	4866952	2.427m	1.788 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051822\
Data File : PP047730.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2022 18:15
Operator : YP\AJ
Sample : N2904-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
FCA566M-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 00:36:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 11 13:10:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

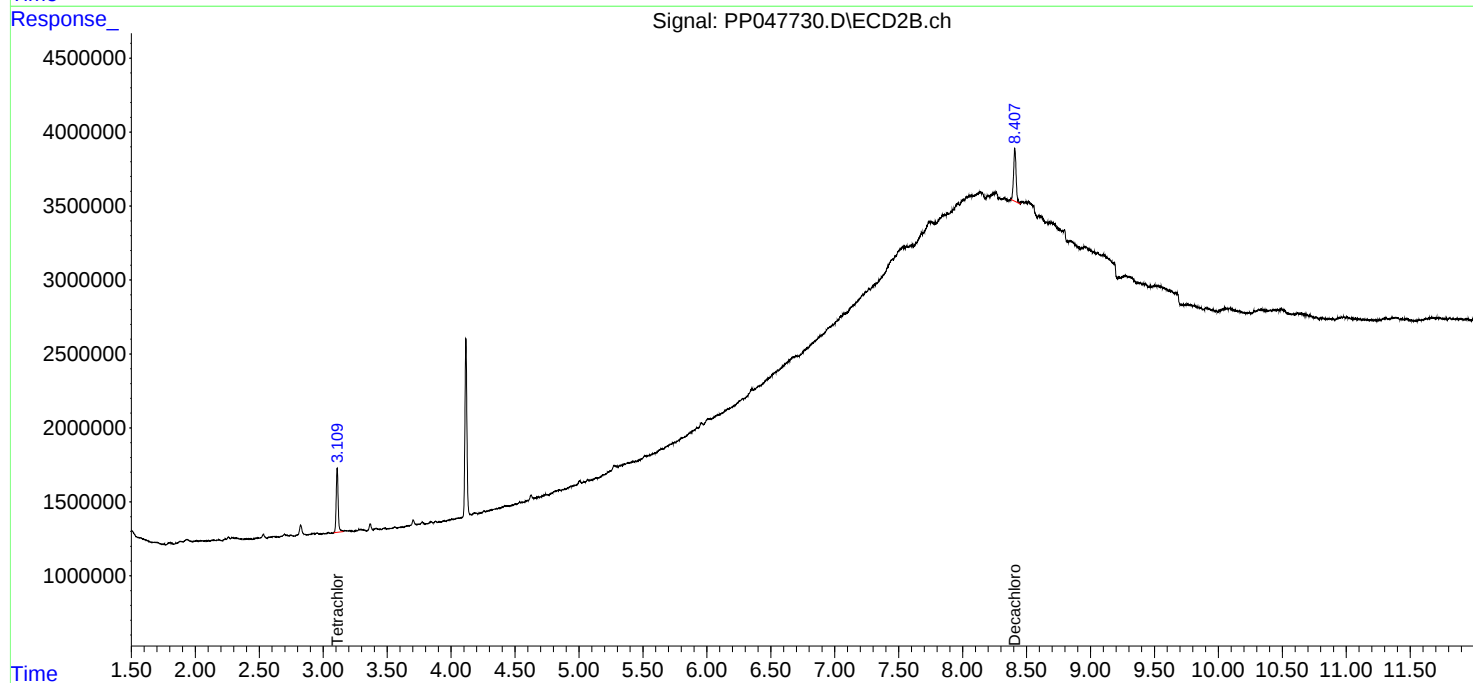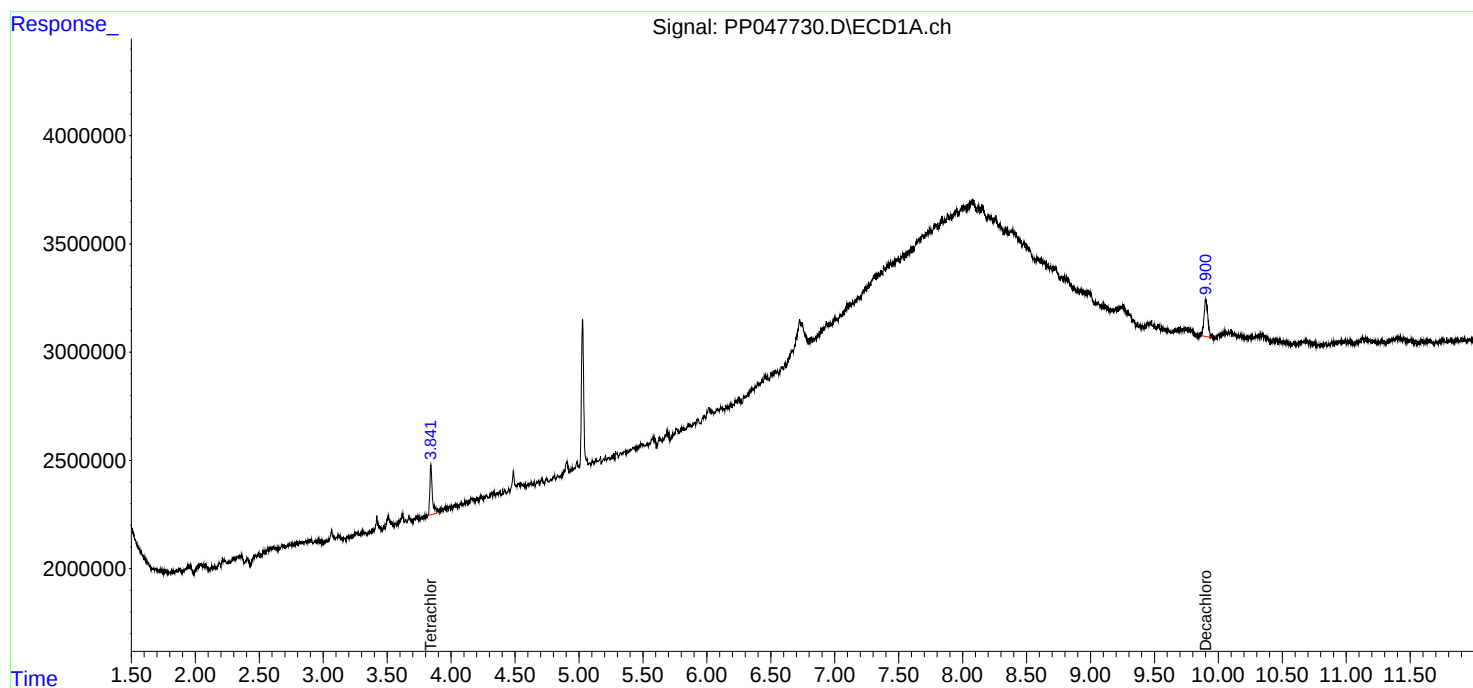

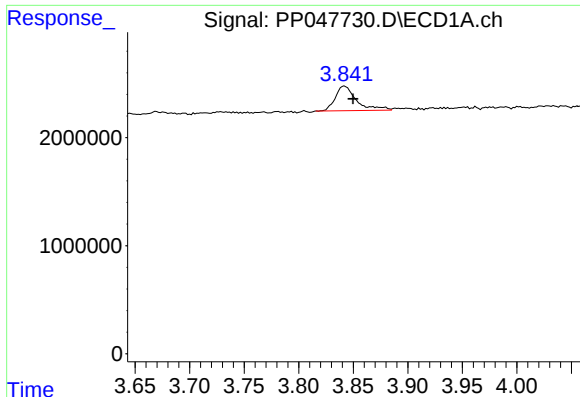


#1 Tetrachloro-m-xylene

R.T.: 3.842 min
Delta R.T.: -0.008 min
Response: 3073085
Conc: 1.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
FCA566M-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

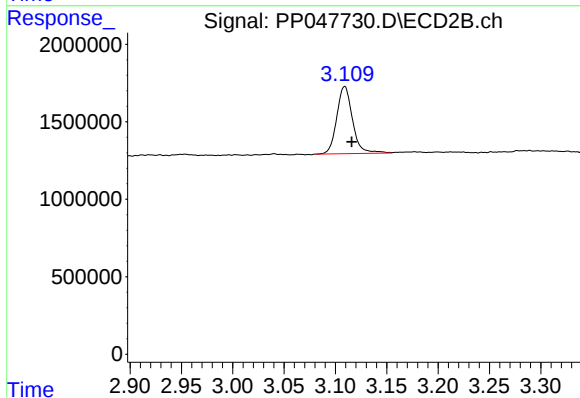


#1 Tetrachloro-m-xylene

R.T.: 3.109 min
Delta R.T.: -0.007 min
Response: 4647034
Conc: 1.41 ng/ml

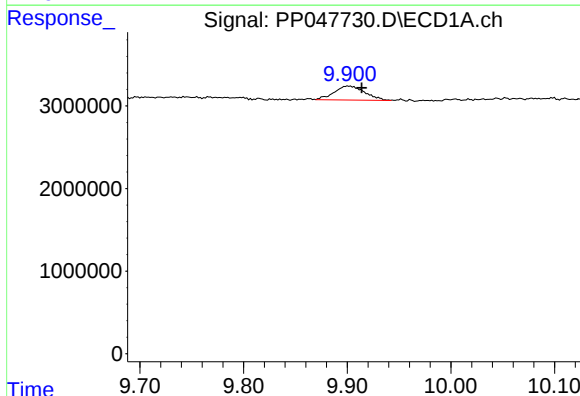

#2 Decachlorobiphenyl

R.T.: 9.900 min
Delta R.T.: -0.014 min
Response: 3471642
Conc: 2.43 ng/ml m

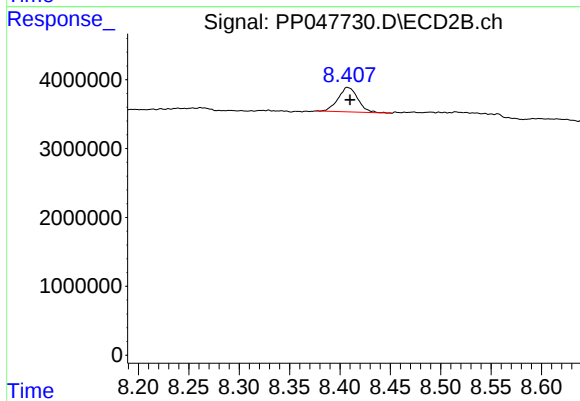

#2 Decachlorobiphenyl

R.T.: 8.408 min
Delta R.T.: -0.002 min
Response: 4866952
Conc: 1.79 ng/ml