

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051822\
 Data File : PP047731.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2022 18:30
 Operator : YP\AJ
 Sample : PB144912BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB144912BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/31/2022
 Supervised By :Ankita Jodhani 05/31/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 00:37:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 11 13:10:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.843	3.110	55386578	73167215	21.786	22.222
2) SA Decachlor...	9.903	8.408	41260382	64998494	28.842m	23.880

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051822\
Data File : PP047731.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2022 18:30
Operator : YP\AJ
Sample : PB144912BL
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB144912BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/31/2022
Supervised By :Ankita Jodhani 05/31/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 00:37:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 11 13:10:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

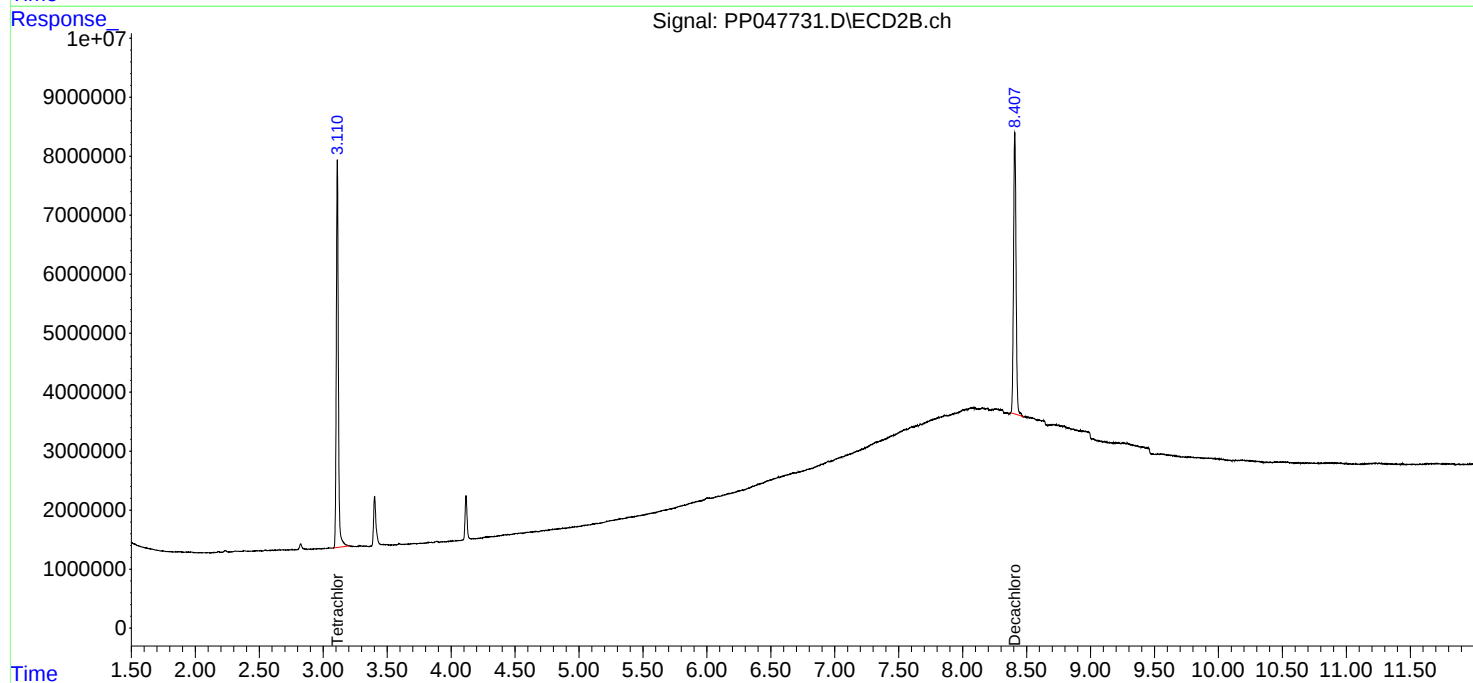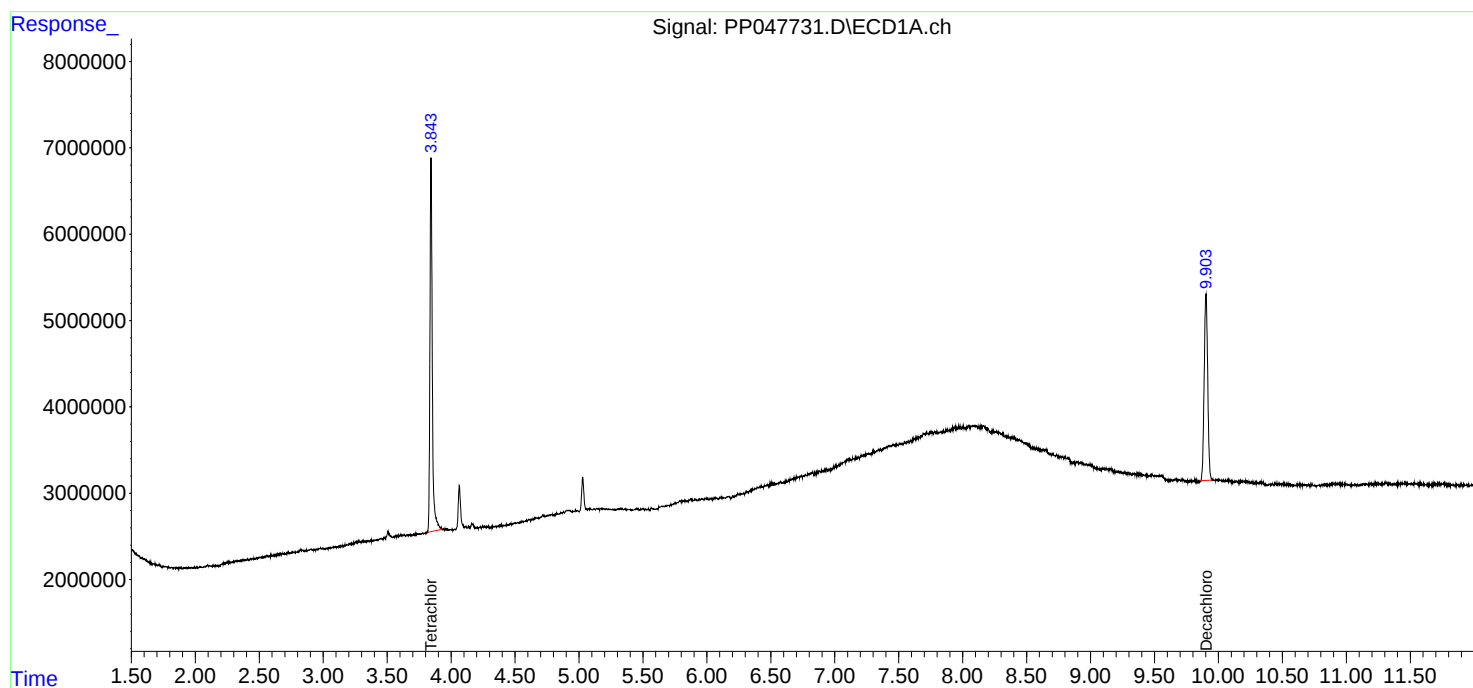

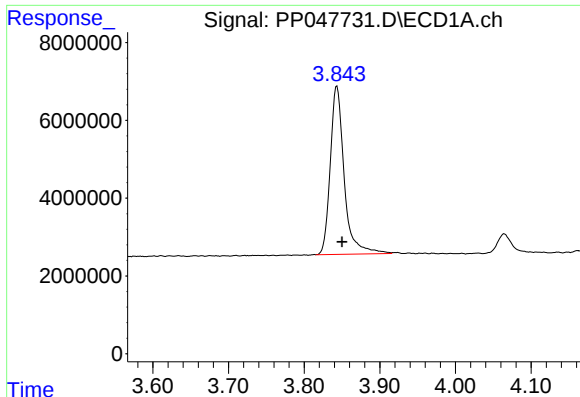


#1 Tetrachloro-m-xylene

R.T.: 3.843 min
Delta R.T.: -0.007 min
Response: 55386578
Conc: 21.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB144912BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/31/2022
Supervised By :Ankita Jodhani 05/31/2022

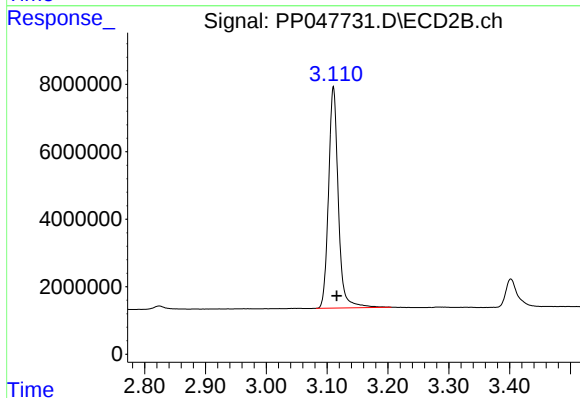


#1 Tetrachloro-m-xylene

R.T.: 3.110 min
Delta R.T.: -0.005 min
Response: 73167215
Conc: 22.22 ng/ml

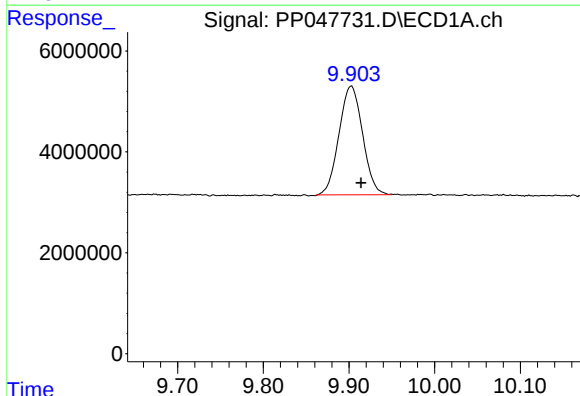

#2 Decachlorobiphenyl

R.T.: 9.903 min
Delta R.T.: -0.011 min
Response: 41260382
Conc: 28.84 ng/ml m

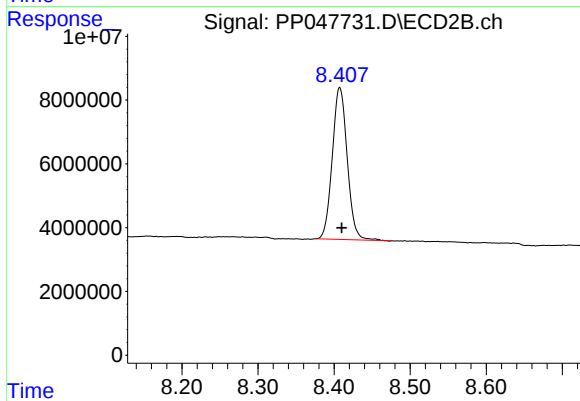

#2 Decachlorobiphenyl

R.T.: 8.408 min
Delta R.T.: -0.002 min
Response: 64998494
Conc: 23.88 ng/ml