

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051921\
 Data File : PP036075.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 May 2021 5:34 (#1); 19 May 2021 5:35 (#2)
 Operator : DD\AJ
 Sample : M2423-18
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 K328-29A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 06:19:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 18 06:25:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.772	4.189	331328	475787	15.338	14.885
2) SA Decachlor...	10.597	9.419	108143	163774	7.990	8.294

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051921\
Data File : PP036075.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 May 2021 5:34 (#1); 19 May 2021 5:35 (#2)
Operator : DD\AJ
Sample : M2423-18
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
K328-29A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 06:19:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 18 06:25:23 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

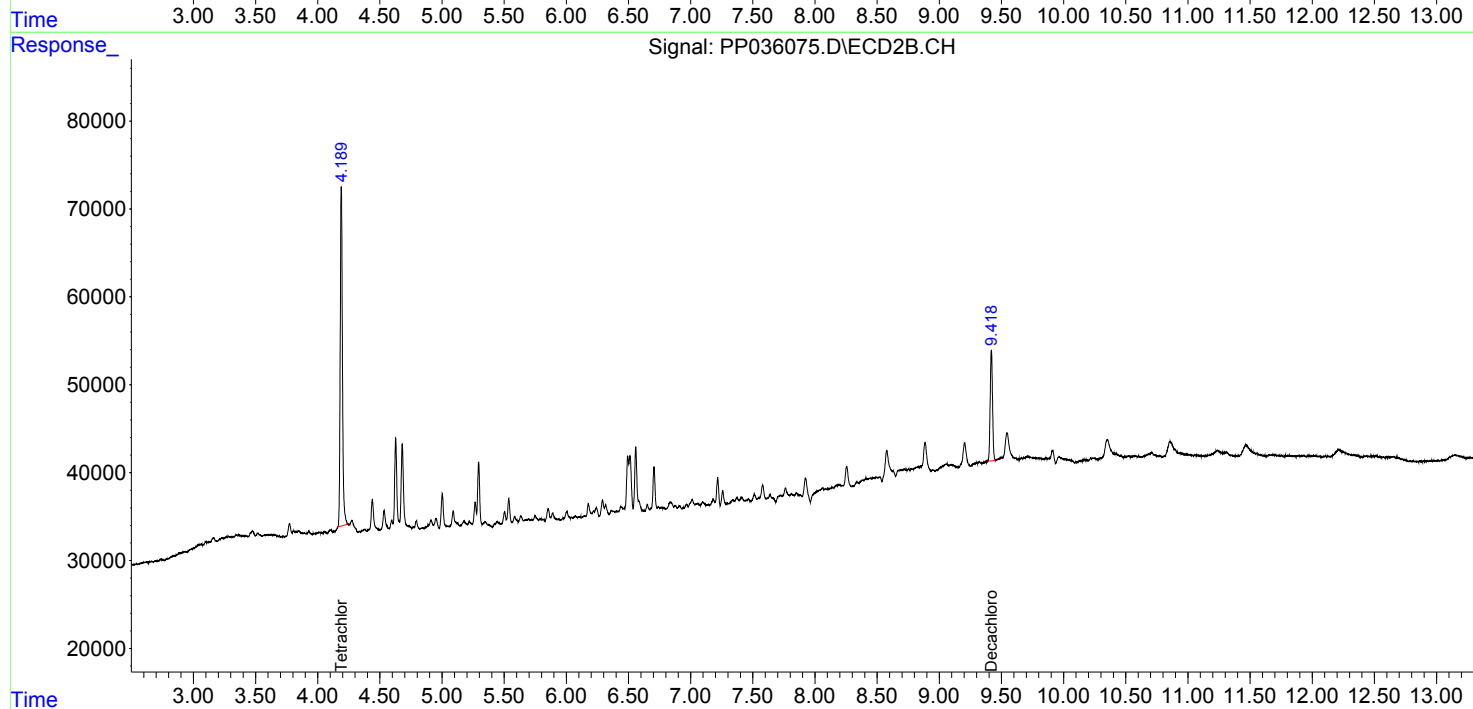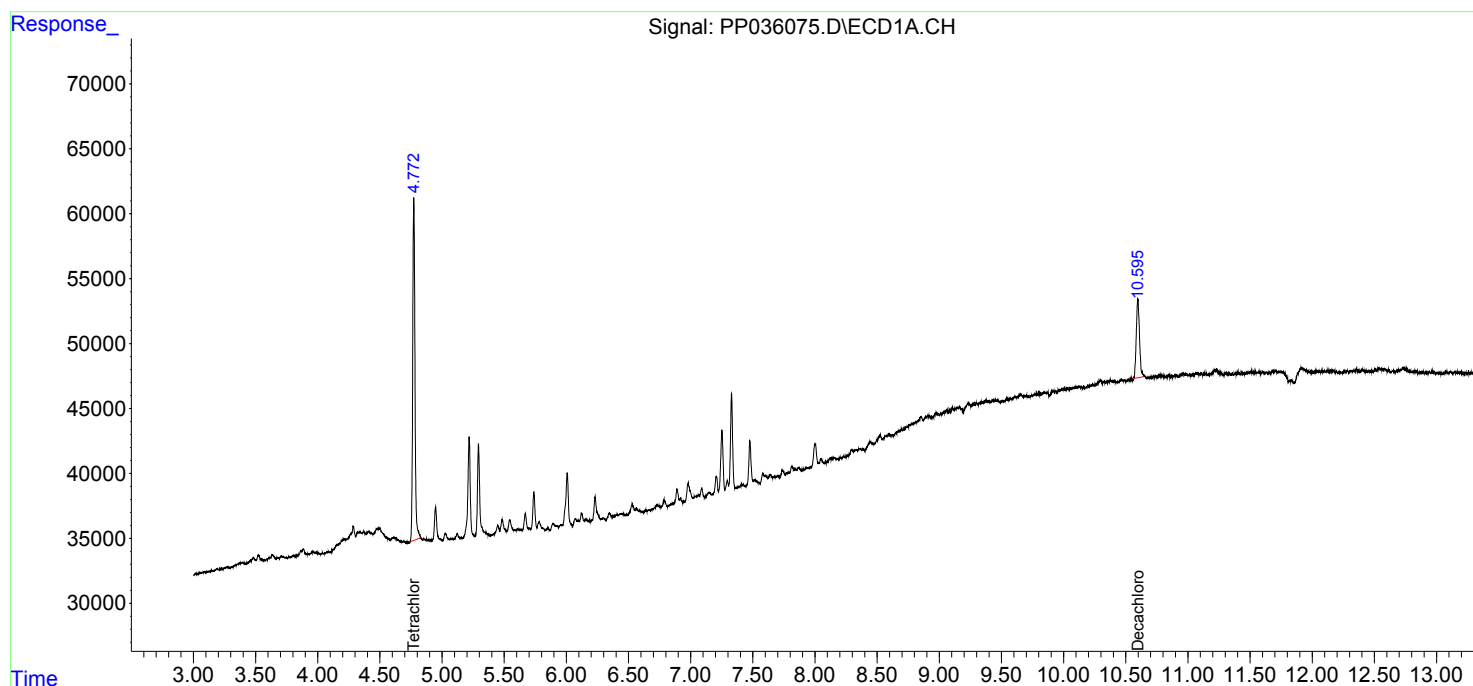


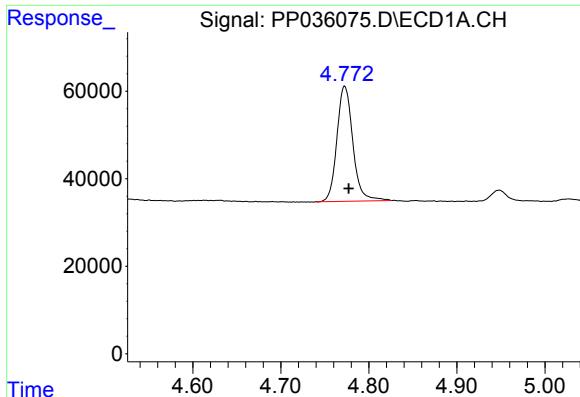

#1 Tetrachloro-m-xylene


R.T.: 4.772 min
Delta R.T.: -0.005 min
Response: 331328
Conc: 15.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
K328-29A

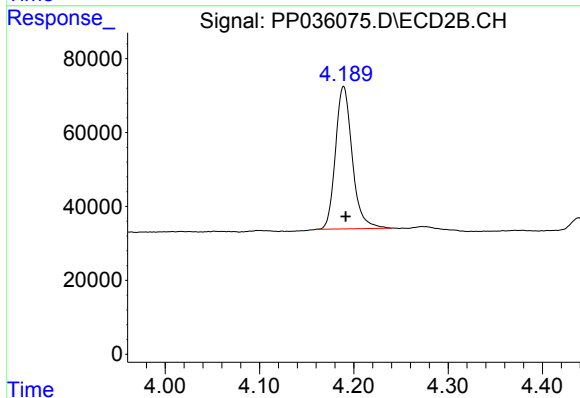


#1 Tetrachloro-m-xylene

R.T.: 4.189 min
Delta R.T.: -0.002 min
Response: 475787
Conc: 14.89 ng/ml

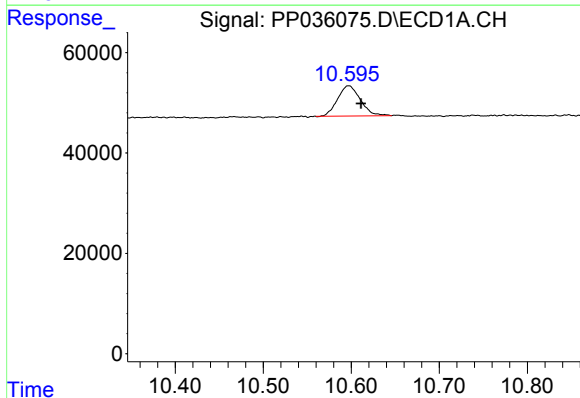

#2 Decachlorobiphenyl

R.T.: 10.597 min
Delta R.T.: -0.014 min
Response: 108143
Conc: 7.99 ng/ml

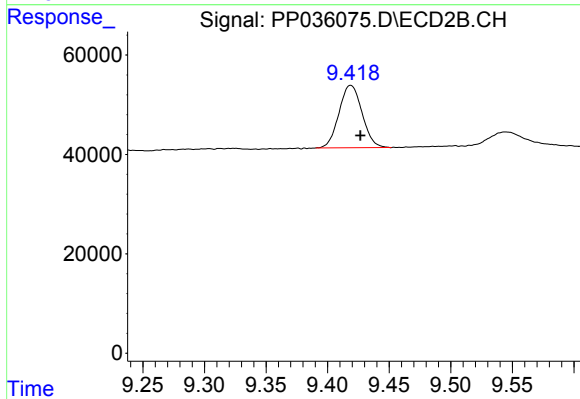

#2 Decachlorobiphenyl

R.T.: 9.419 min
Delta R.T.: -0.008 min
Response: 163774
Conc: 8.29 ng/ml