

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051921\
 Data File : PP036088.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 May 2021 12:56
 Operator : DD\AJ
 Sample : M2423-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 K328-DUP5

Manual Integrations
 APPROVED

Ankita
 5/20/2021 2:03:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 14:30:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 18 06:25:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.770	4.186	436604	613913	20.212	19.206
2) SA Decachlor...	10.595f	9.417	247522	355600	18.287	18.009m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP051921\
Data File : PP036088.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 May 2021 12:56
Operator : DD\AJ
Sample : M2423-03
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
K328-DUP5


Manual Integrations
APPROVED

Ankita
5/20/2021 2:03:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 14:30:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 18 06:25:23 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

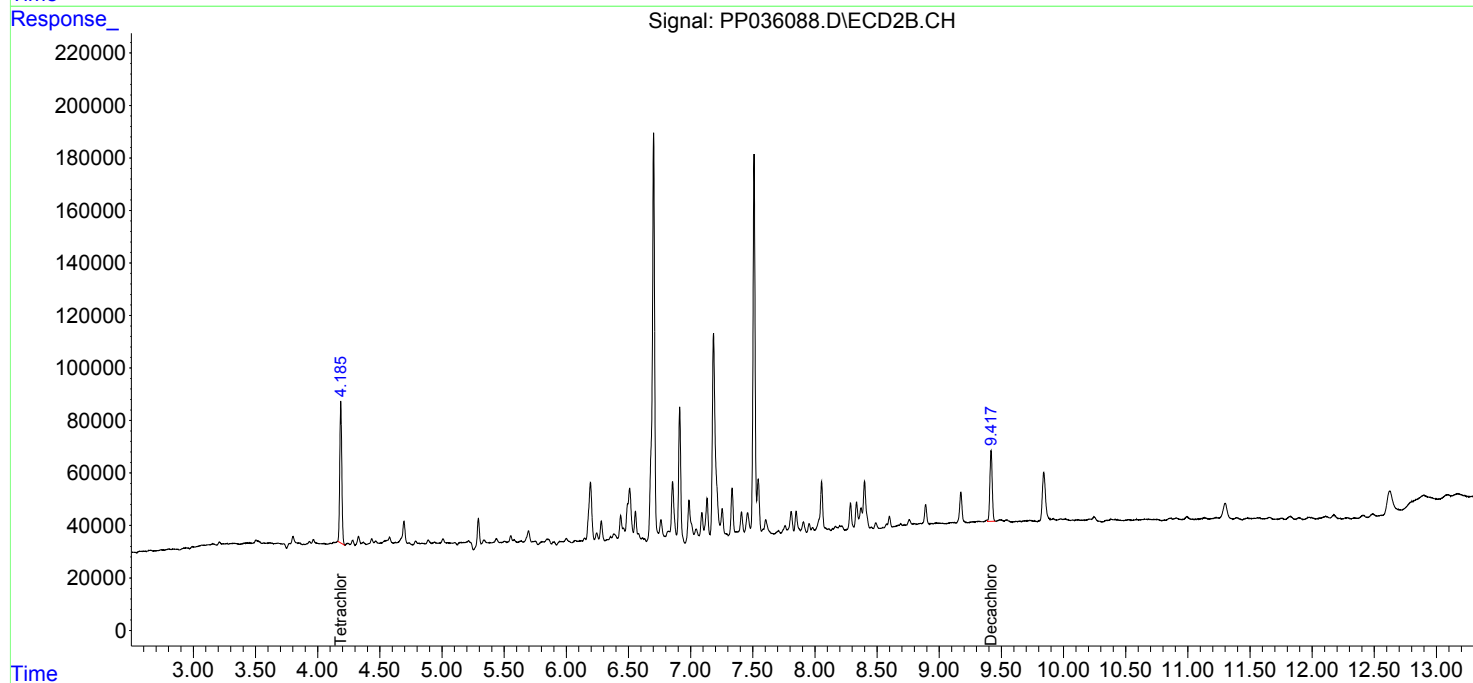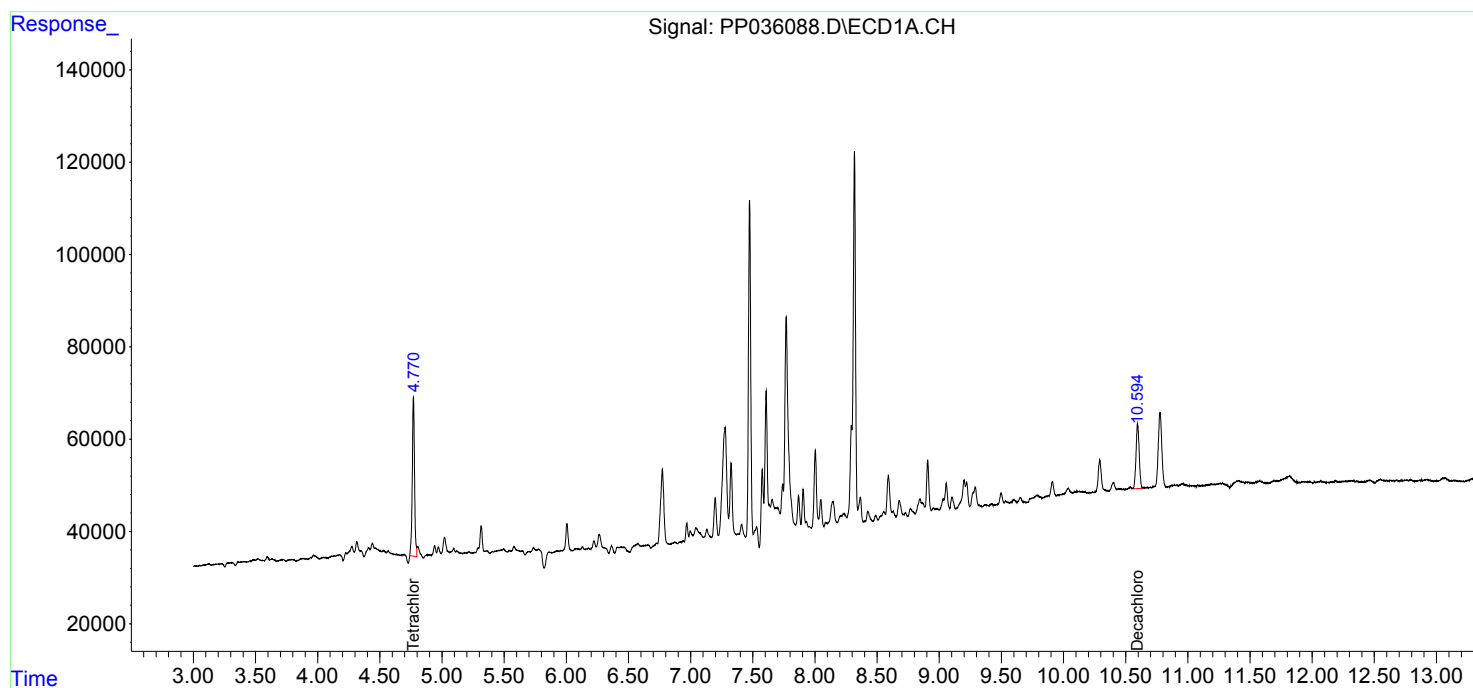

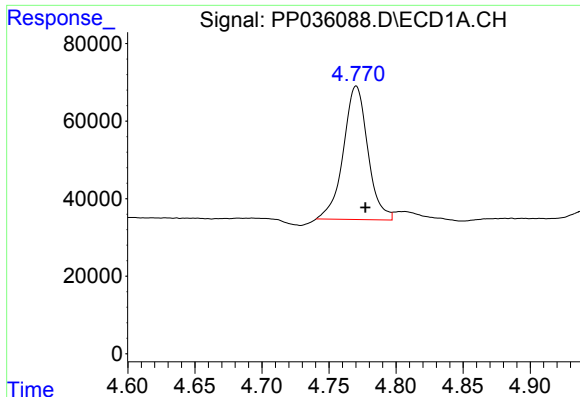


#1 Tetrachloro-m-xylene

R.T.: 4.770 min
Delta R.T.: -0.007 min
Response: 436604
Conc: 20.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
K328-DUP5


Manual Integrations
APPROVED

Ankita
5/20/2021 2:03:36 PM

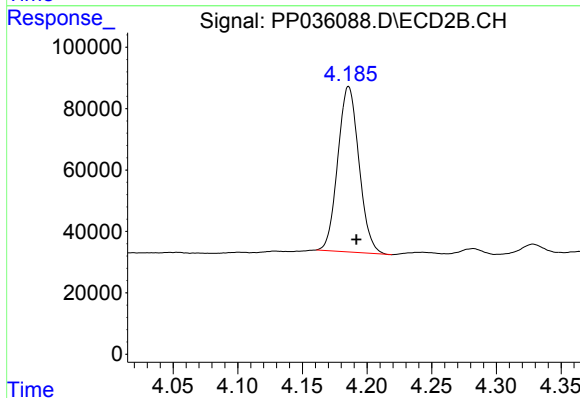


#1 Tetrachloro-m-xylene

R.T.: 4.186 min
Delta R.T.: -0.006 min
Response: 613913
Conc: 19.21 ng/ml

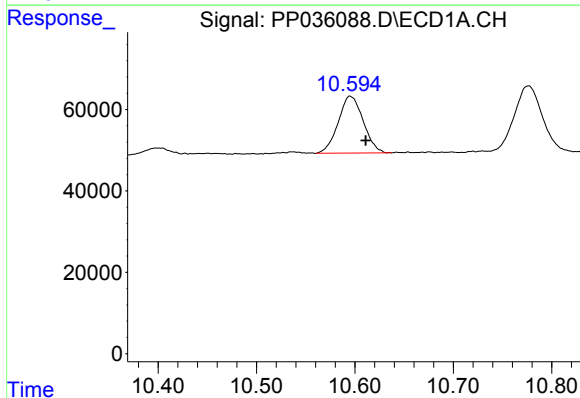

#2 Decachlorobiphenyl

R.T.: 10.595 min
Delta R.T.: -0.016 min
Response: 247522
Conc: 18.29 ng/ml

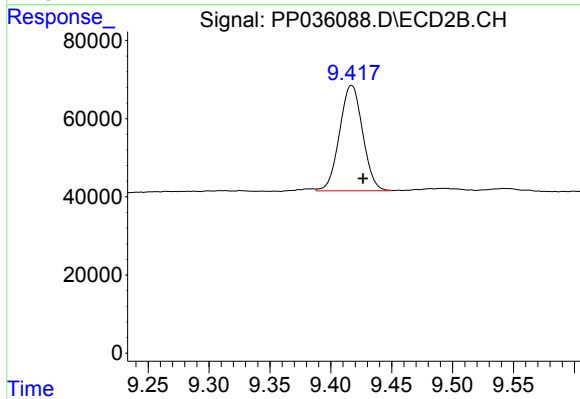

#2 Decachlorobiphenyl

R.T.: 9.417 min
Delta R.T.: -0.010 min
Response: 355600
Conc: 18.01 ng/ml m