

Data Path : P:\HPCHEM1\ECD_P\Data\PP052018\
 Data File : PP025934.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 May 2018 11:41
 Operator : UA/AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 06:47:50 2018
 Quant Method : P:\HPCHEM1\ECD_P\methods\PP051718.M
 Quant Title : 8080.M
 QLast Update : Fri May 18 00:16:42 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
Target Compounds						
5) T DICAMBA	11.748	0.000	1607740	0	0.602	N.D. #
9) T 2,4-D	13.250	0.000	54707571	0	68.836	N.D. #
10) T Pentachlo...	13.682	0.000	5049432	0	0.468	N.D. #
11) T 2,4,5-TP ...	14.558	0.000	3347973	0	0.749	N.D. #
12) T 2,4,5-T	14.973	0.000	2853189	0	0.724	N.D. #
14) T DINOSEB	17.168	0.000	1637161	0	0.680	N.D. #
15) T Picloram	16.944	0.000	1375417	0	0.283	N.D. #
16) T DCPA	17.535	0.000	5621111	0	1.031	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_P\Data\PP052018\
Data File : PP025934.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 May 2018 11:41
Operator : UA/AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 06:47:50 2018
Quant Method : P:\HPCHEM1\ECD_P\methods\PP051718.M
Quant Title : 8080.M
QLast Update : Fri May 18 00:16:42 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

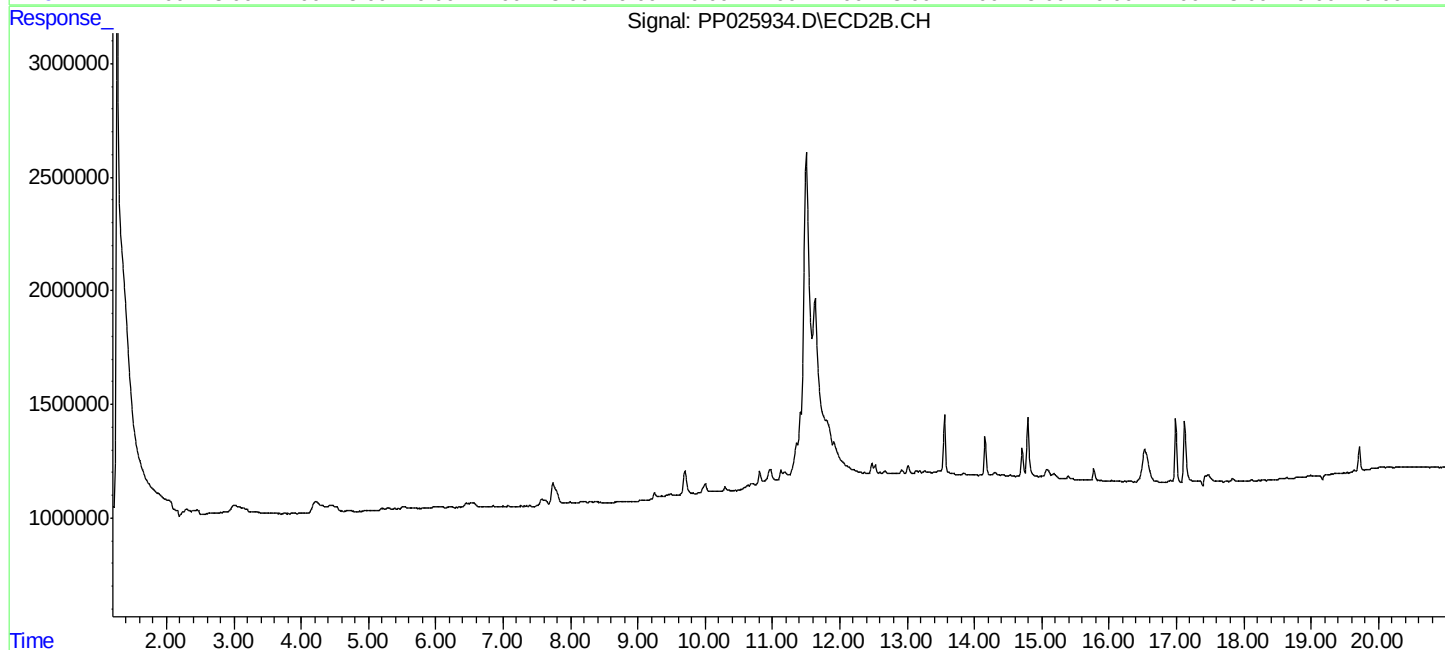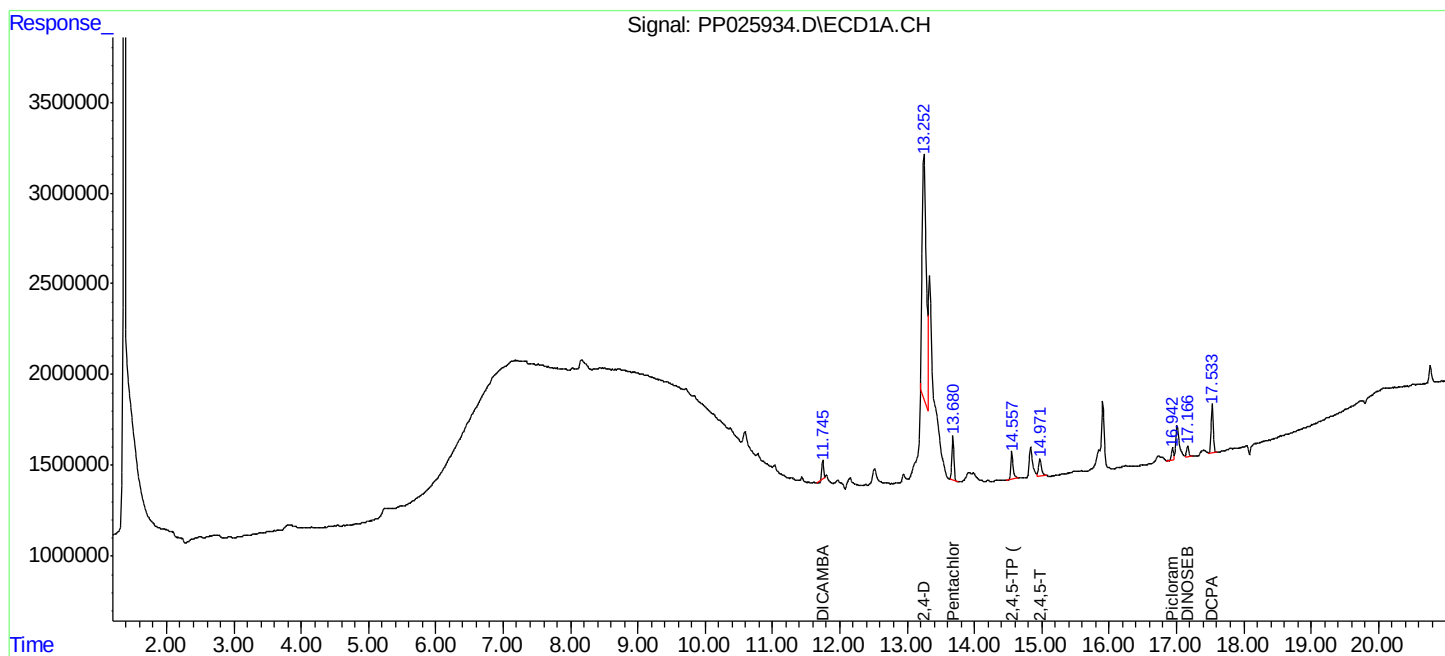


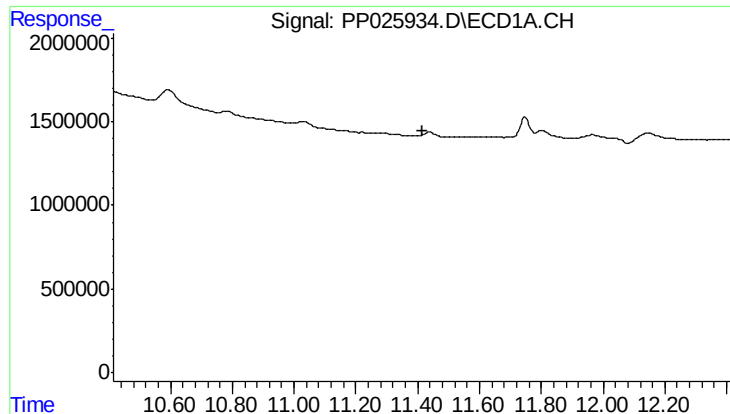

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.415 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

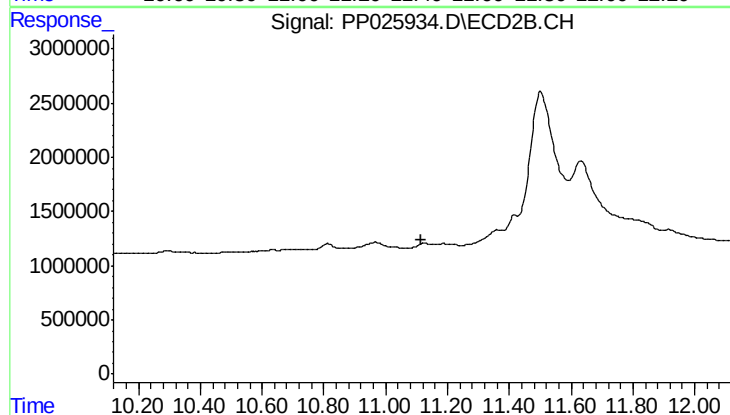


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.117 min
Response: 0
Conc: N.D.

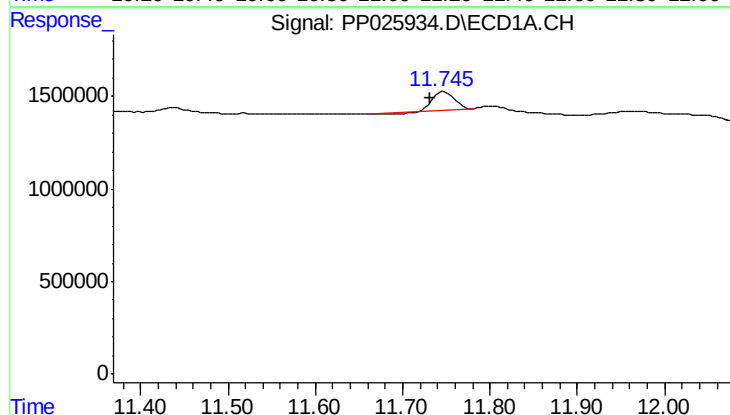


#5 DICAMBA

R.T.: 11.748 min
Delta R.T.: 0.016 min
Response: 1607740
Conc: 0.60 ng/ml

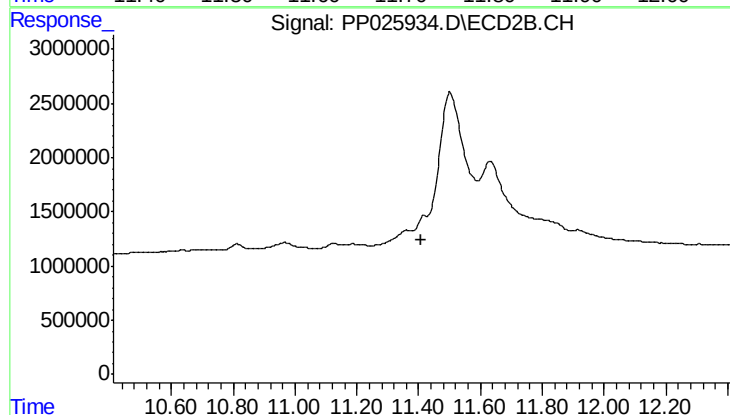

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.410 min
Response: 0
Conc: N.D.

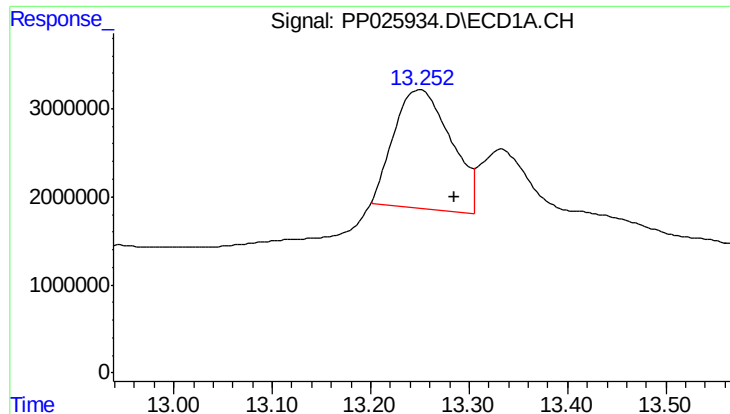

#9 2,4-D


R.T.: 13.250 min
Delta R.T.: -0.035 min
Response: 54707571
Conc: 68.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

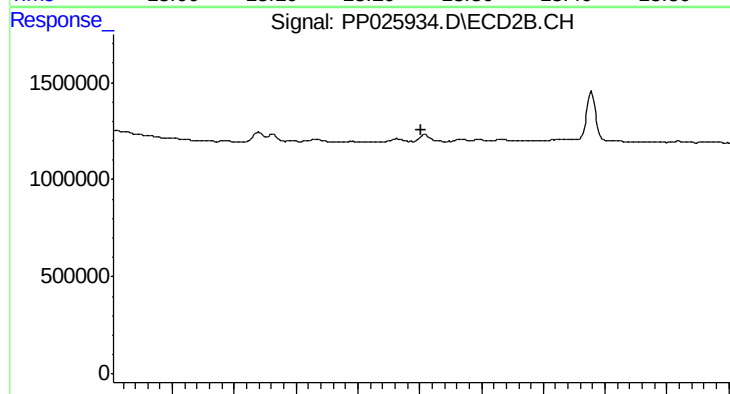


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.006 min
Response: 0
Conc: N.D.

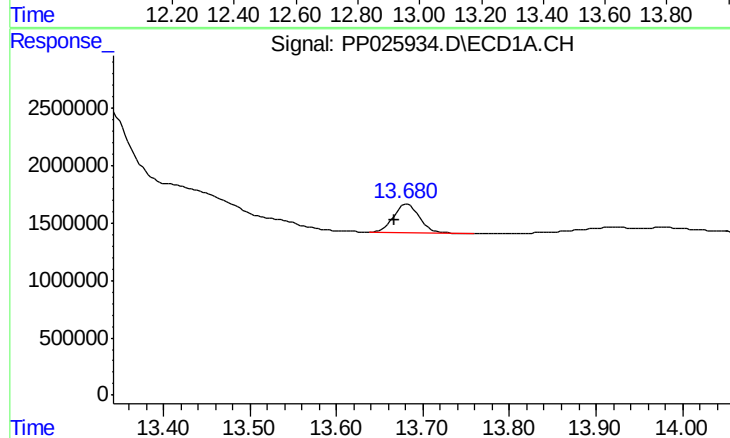


#10 Pentachlorophenol

R.T.: 13.682 min
Delta R.T.: 0.015 min
Response: 5049432
Conc: 0.47 ng/ml

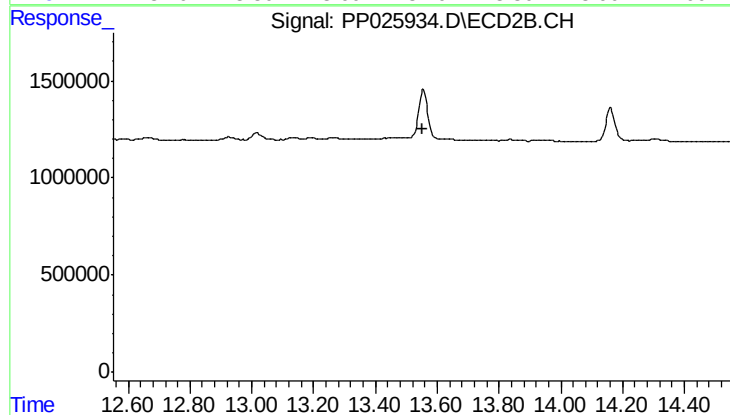

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.552 min
Response: 0
Conc: N.D.

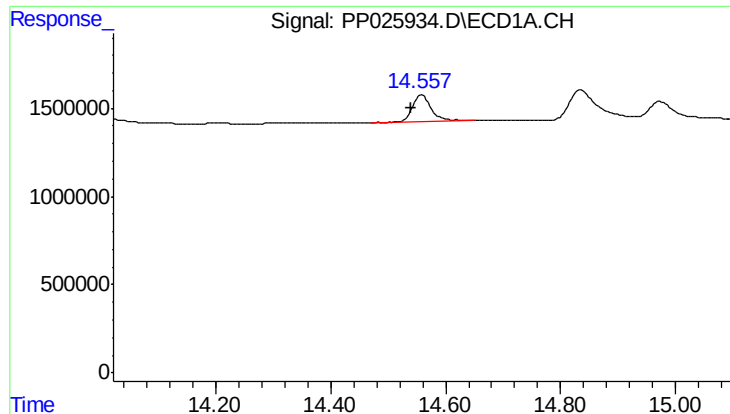

#11 2,4,5-TP (SILVEX)


R.T.: 14.558 min
Delta R.T.: 0.019 min
Response: 3347973
Conc: 0.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

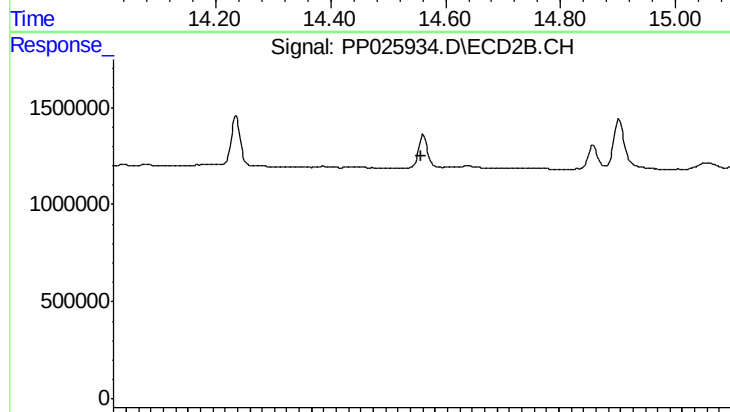


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.156 min
Response: 0
Conc: N.D.

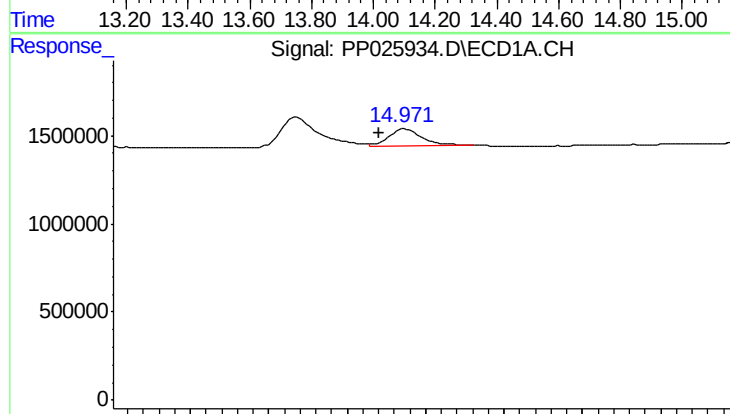


#12 2,4,5-T

R.T.: 14.973 min
Delta R.T.: 0.032 min
Response: 2853189
Conc: 0.72 ng/ml

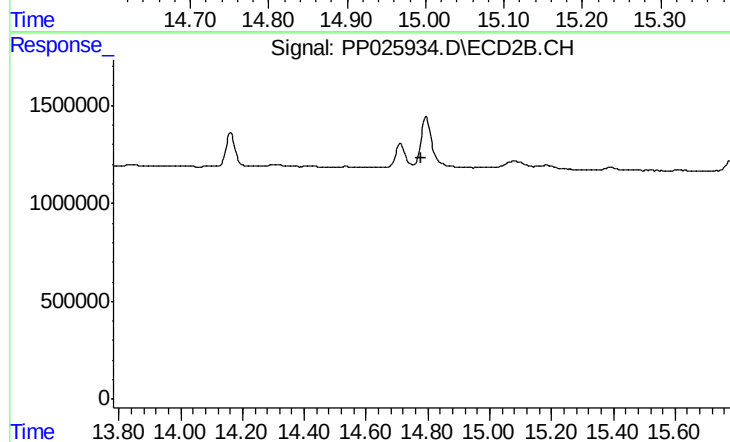

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.781 min
Response: 0
Conc: N.D.

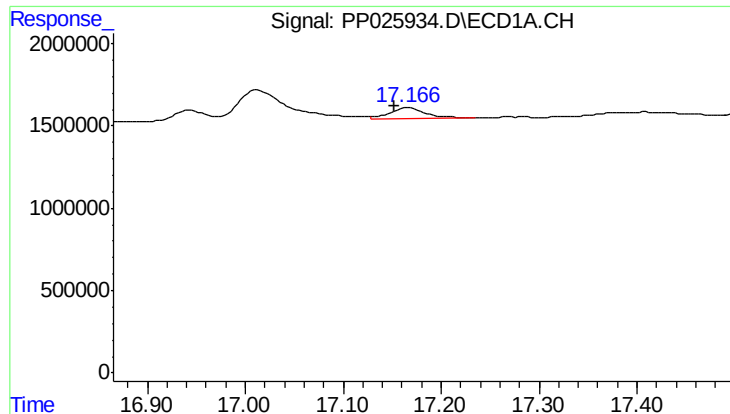

#14 DINOSEB


R.T.: 17.168 min
Delta R.T.: 0.015 min
Response: 1637161
Conc: 0.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

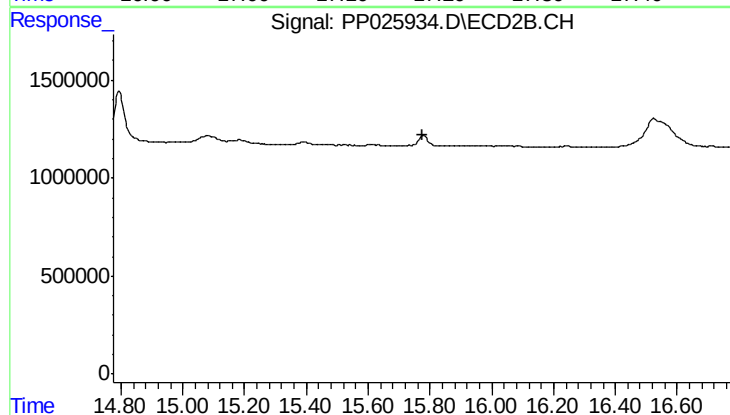


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 15.774 min
Response: 0
Conc: N.D.

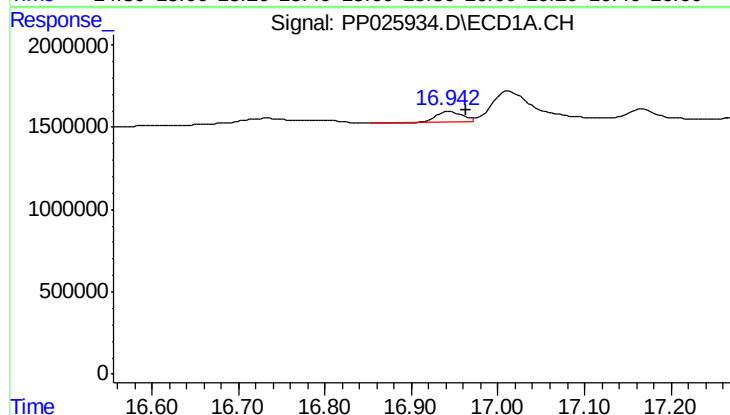


#15 Picloram

R.T.: 16.944 min
Delta R.T.: -0.019 min
Response: 1375417
Conc: 0.28 ng/ml

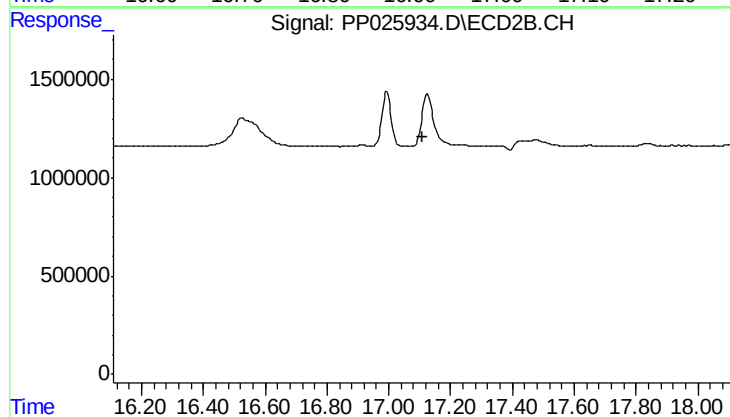

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.109 min
Response: 0
Conc: N.D.

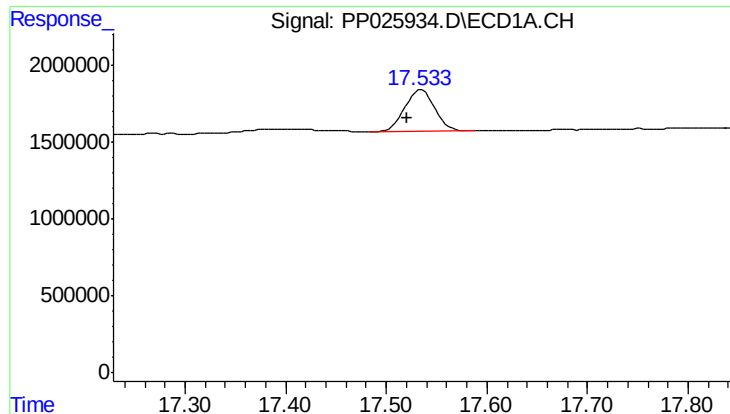

#16 DCPA

R.T.: 17.535 min
Delta R.T.: 0.013 min
Response: 5621111
Conc: 1.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

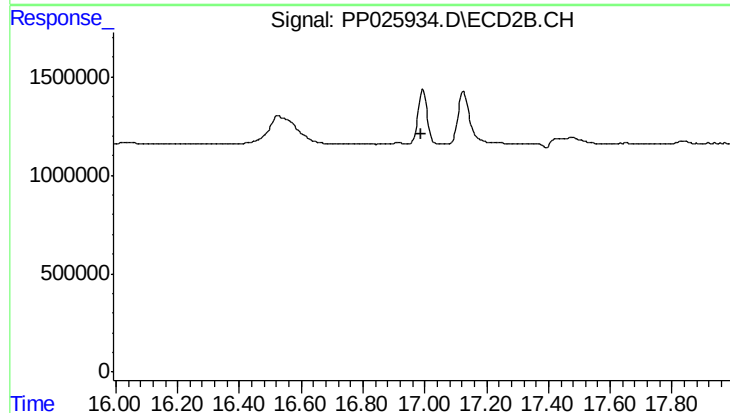

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.