

Data Path : P:\HPCHEM1\ECD_P\Data\PP052018\
 Data File : PP025946.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 May 2018 16:51
 Operator : UA/AJ
 Sample : J3004-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-10-WC-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 06:52:19 2018
 Quant Method : P:\HPCHEM1\ECD_P\methods\PP051718.M
 Quant Title : 8080.M
 QLast Update : Fri May 18 00:16:42 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	11.417	11.119	193.1E6	188.3E6	322.534	294.285
Target Compounds						
1) T Dalapon	2.852	0.000	5589127	0	7.483	N.D. #
2) T 3,5-DICHL...	0.000	9.223	0	8886156	N.D.	10.415 #
3) T 4-Nitroph...	11.052	0.000	8844167	0	27.080	N.D. #
6) T MCPP	12.001	0.000	2279218	0	1.419	N.D. #
7) T MCPA	12.388	0.000	1936526	0	0.791	N.D. #
8) T DICHLORPROP	12.870	0.000	2597742	0	3.965	N.D. #
14) T DINOSEB	17.187	0.000	2296968	0	0.953	N.D. #
15) T Picloram	16.925	0.000	5523125	0	1.137	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_P\Data\PP052018\
Data File : PP025946.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 May 2018 16:51
Operator : UA/AJ
Sample : J3004-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
TP-10-WC-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 06:52:19 2018
Quant Method : P:\HPCHEM1\ECD_P\methods\PP051718.M
Quant Title : 8080.M
QLast Update : Fri May 18 00:16:42 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

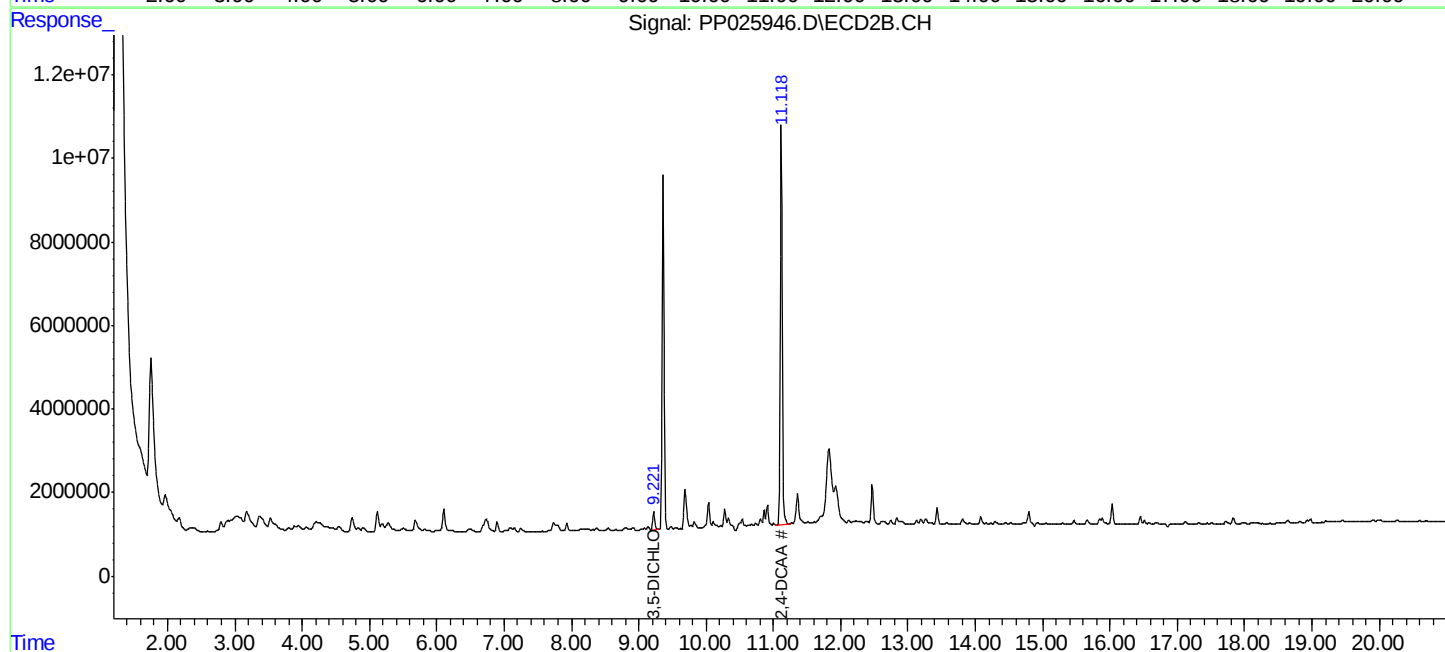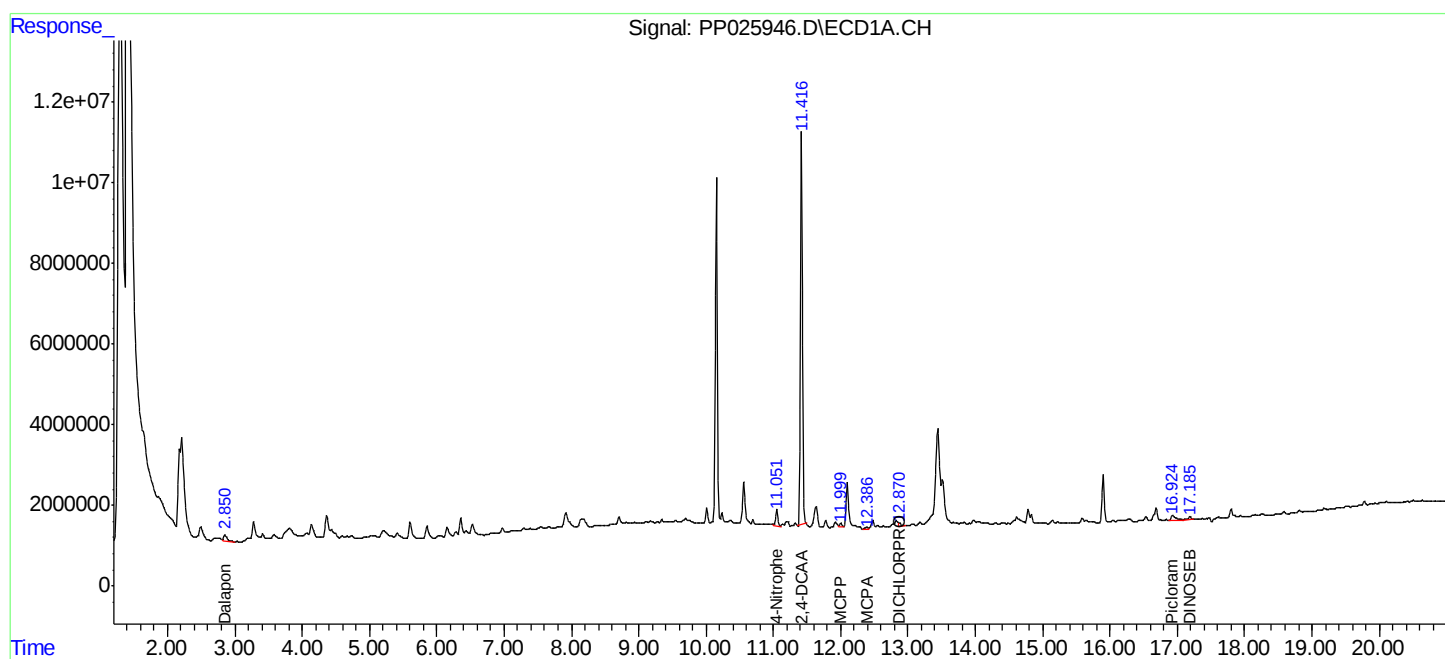


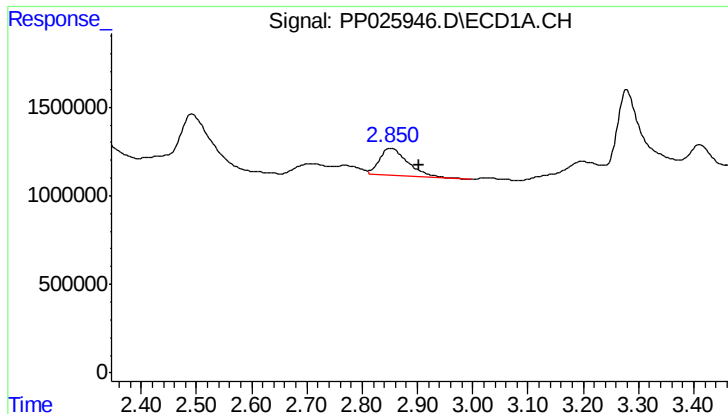

#1 Dalapon


R.T.: 2.852 min
Delta R.T.: -0.051 min
Response: 5589127
Conc: 7.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-10-WC-2

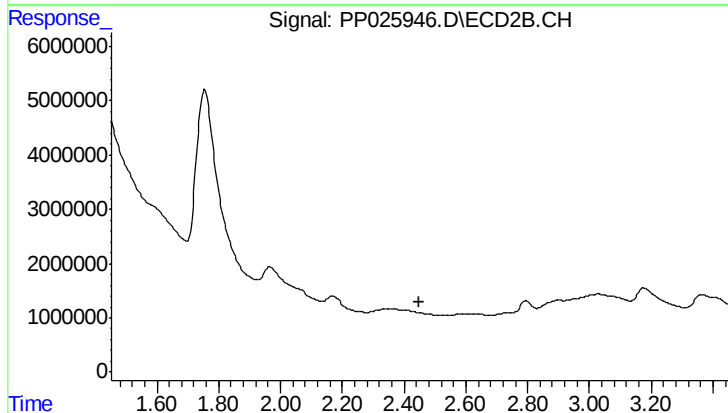


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.450 min
Response: 0
Conc: N.D.

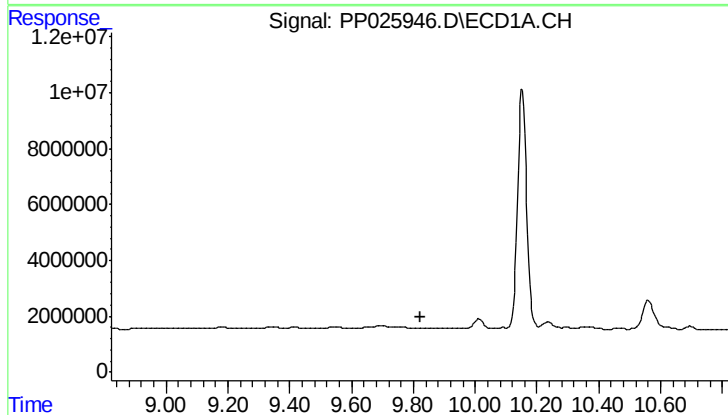


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.822 min
Response: 0
Conc: N.D.

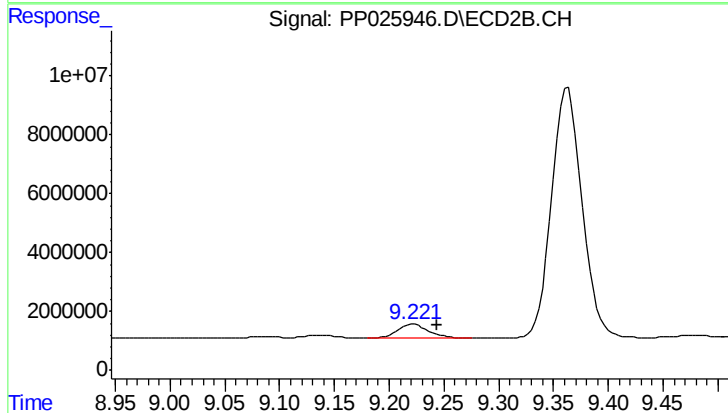

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.223 min
Delta R.T.: -0.021 min
Response: 8886156
Conc: 10.41 ng/ml

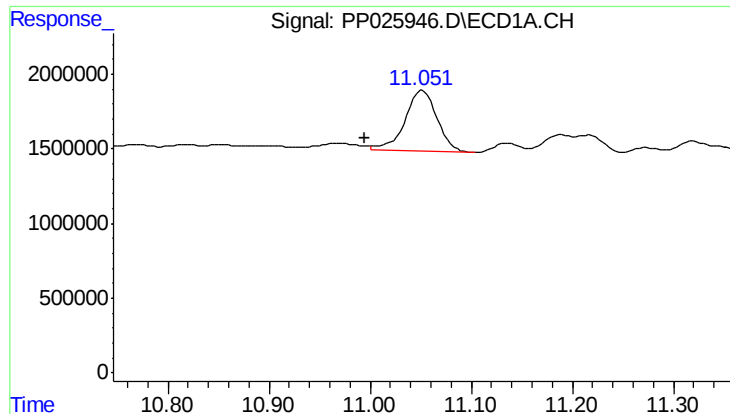

#3 4-Nitrophenol


R.T.: 11.052 min
Delta R.T.: 0.057 min
Response: 8844167
Conc: 27.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-10-WC-2

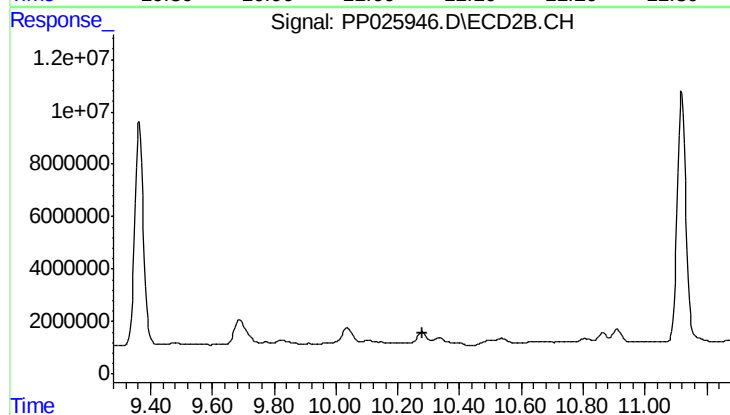


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.279 min
Response: 0
Conc: N.D.

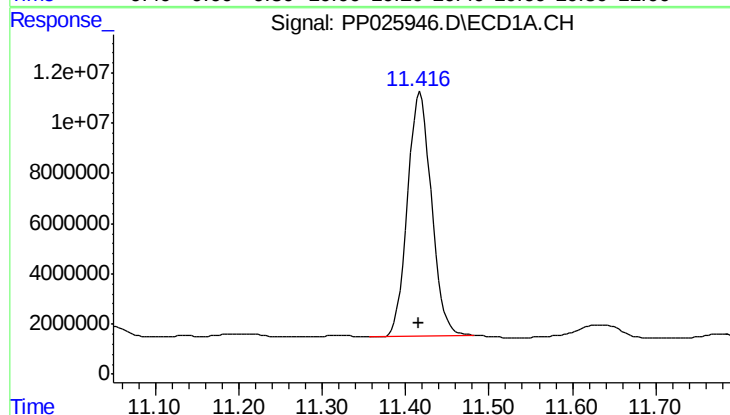


#4 2,4-DCAA

R.T.: 11.417 min
Delta R.T.: 0.002 min
Response: 193126591
Conc: 322.53 ng/ml

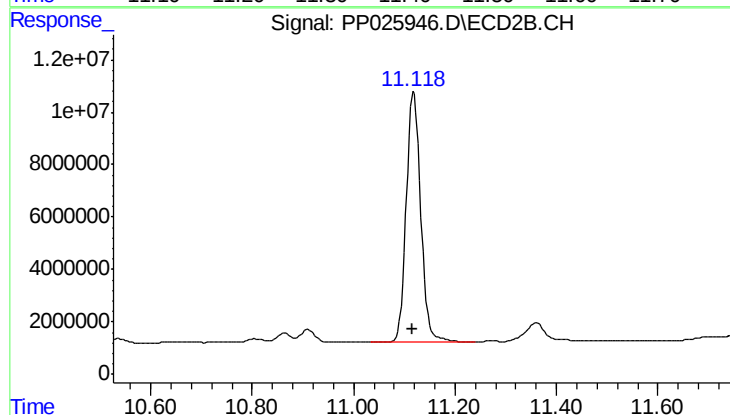

#4 2,4-DCAA


R.T.: 11.119 min
Delta R.T.: 0.002 min
Response: 188312622
Conc: 294.28 ng/ml

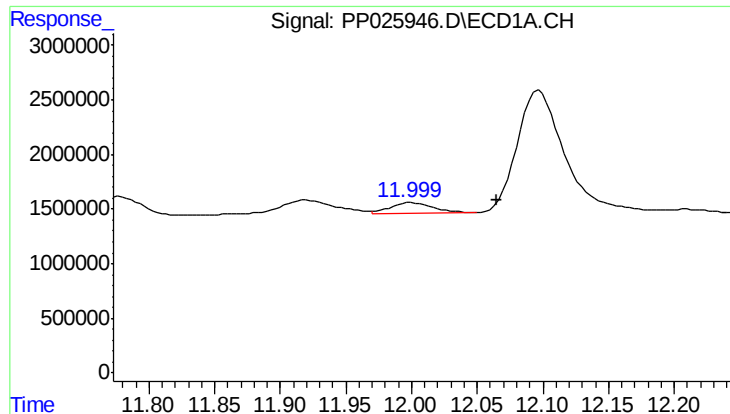

#6 MCPP


R.T.: 12.001 min
Delta R.T.: -0.065 min
Response: 2279218
Conc: 1.42 ug/ml

Instrument :
ECD_P
ClientSampleId :
TP-10-WC-2

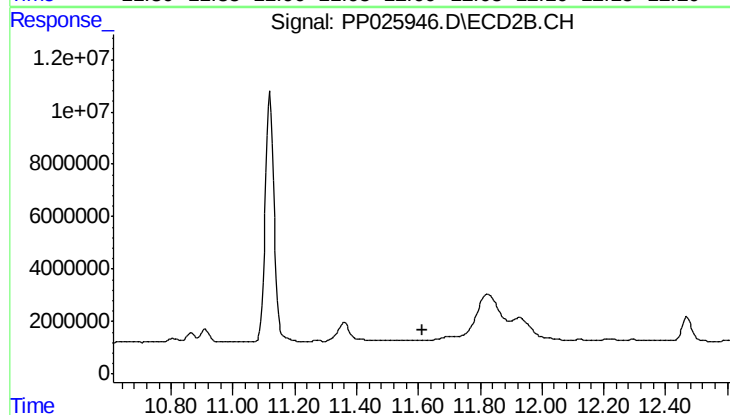


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 11.612 min
Response: 0
Conc: N.D.

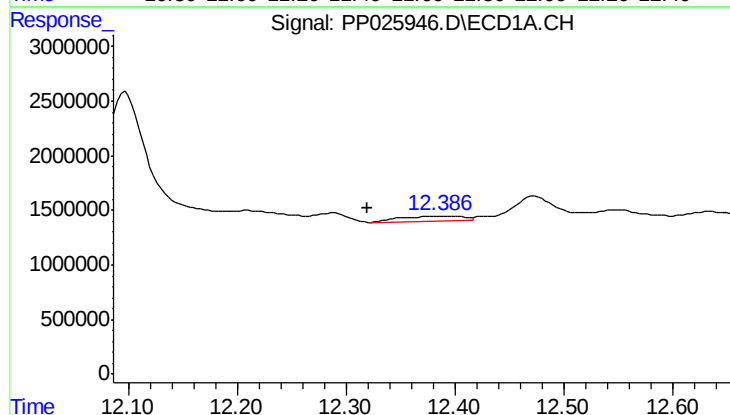


#7 MCPA

R.T.: 12.388 min
Delta R.T.: 0.069 min
Response: 1936526
Conc: 0.79 ug/ml

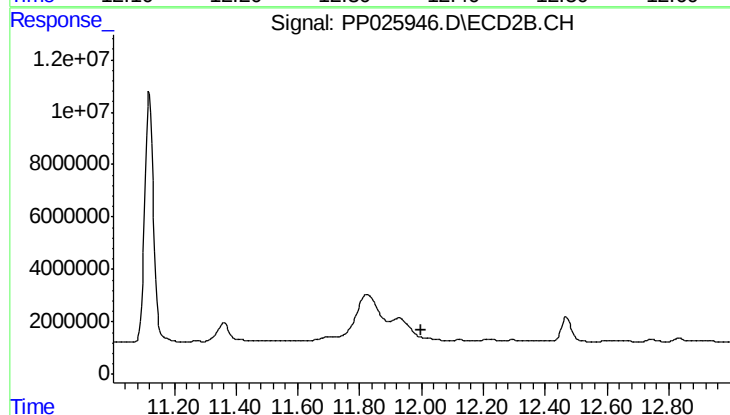

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.001 min
Response: 0
Conc: N.D.

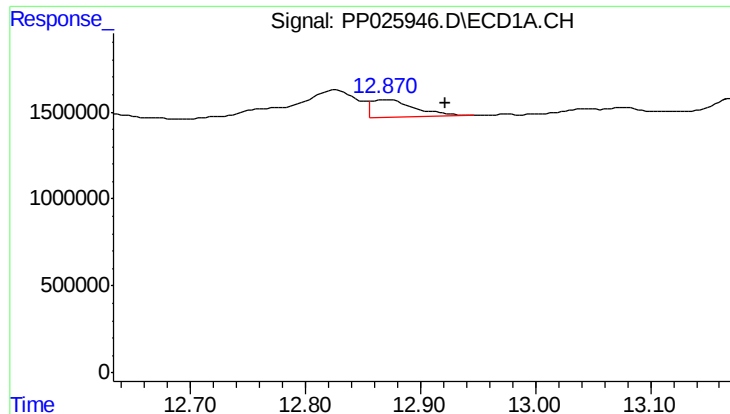

#8 DICHLORPROP


R.T.: 12.870 min
Delta R.T.: -0.052 min
Response: 2597742
Conc: 3.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-10-WC-2

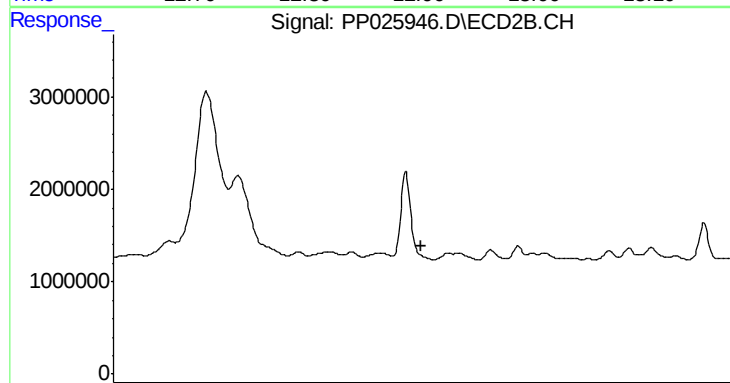


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.521 min
Response: 0
Conc: N.D.

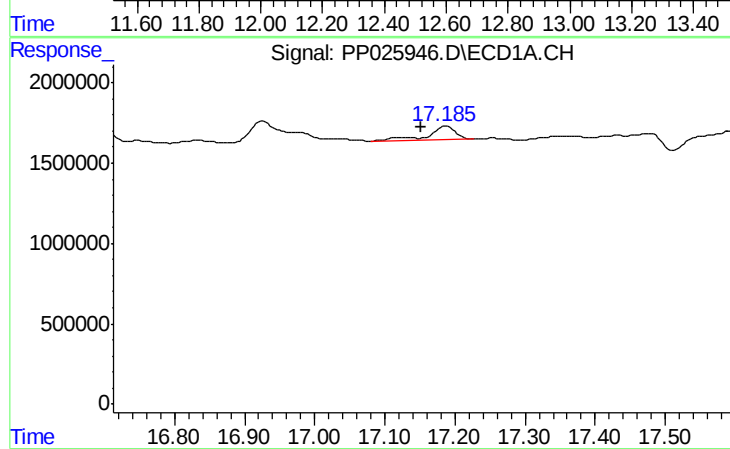


#14 DINOSEB

R.T.: 17.187 min
Delta R.T.: 0.034 min
Response: 2296968
Conc: 0.95 ng/ml

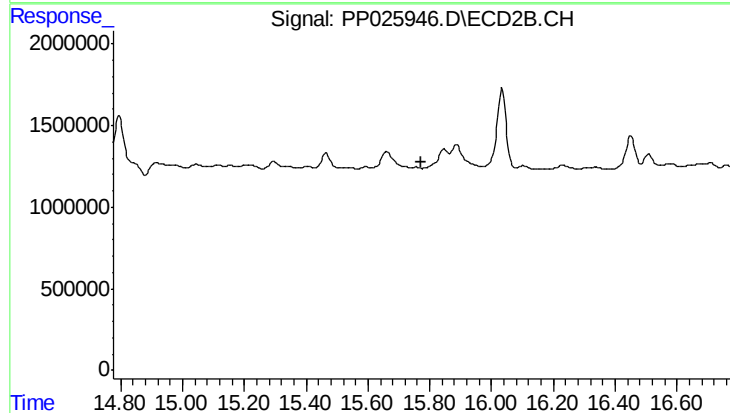

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 15.774 min
Response: 0
Conc: N.D.

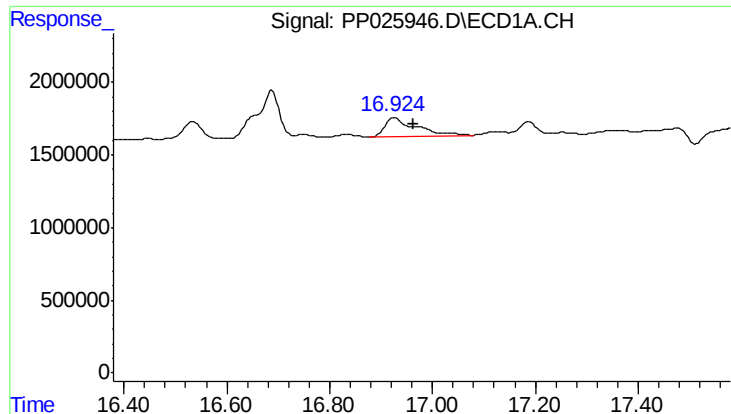

#15 Picloram

R.T.: 16.925 min
Delta R.T.: -0.038 min
Response: 5523125
Conc: 1.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-10-WC-2

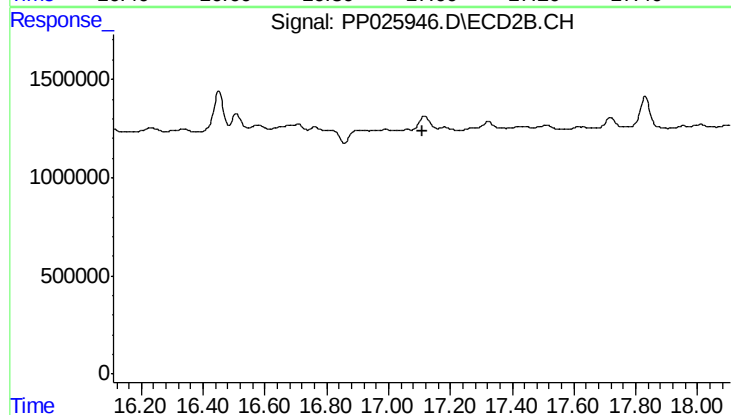

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.109 min
Response: 0
Conc: N.D.