

Data Path : P:\HPCHEM1\ECD_P\Data\PP052118\
Data File : PP025974.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 May 2018 19:45
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 03:17:46 2018
Quant Method : P:\HPCHEM1\ECD_P\methods\PP052118.M
Quant Title : 8080.M
QLast Update : Tue May 22 02:19:00 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.400	11.110	273.9E6	262.0E6	489.103	452.273
Target Compounds							
15) T	Picloram	16.909	0.000	12402234	0	2.093	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_P\Data\PP052118\
Data File : PP025974.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 May 2018 19:45
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 03:17:46 2018
Quant Method : P:\HPCHEM1\ECD_P\methods\PP052118.M
Quant Title : 8080.M
QLast Update : Tue May 22 02:19:00 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

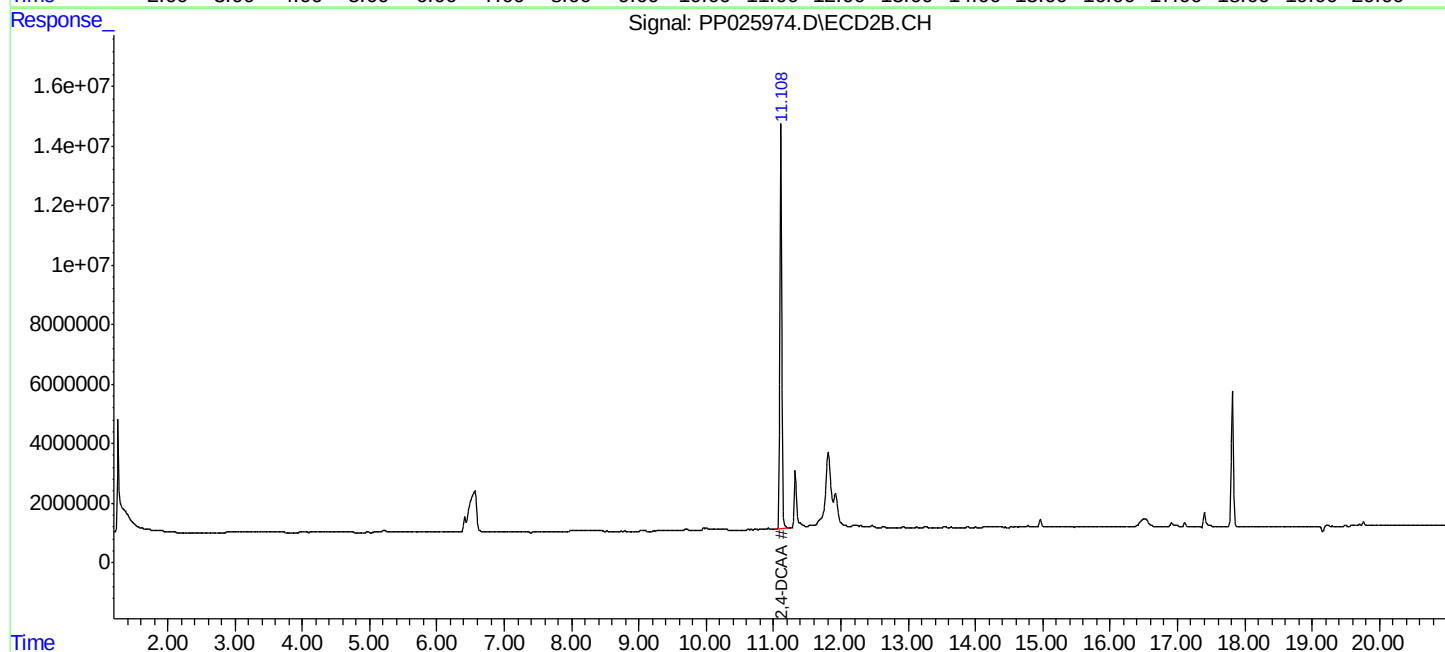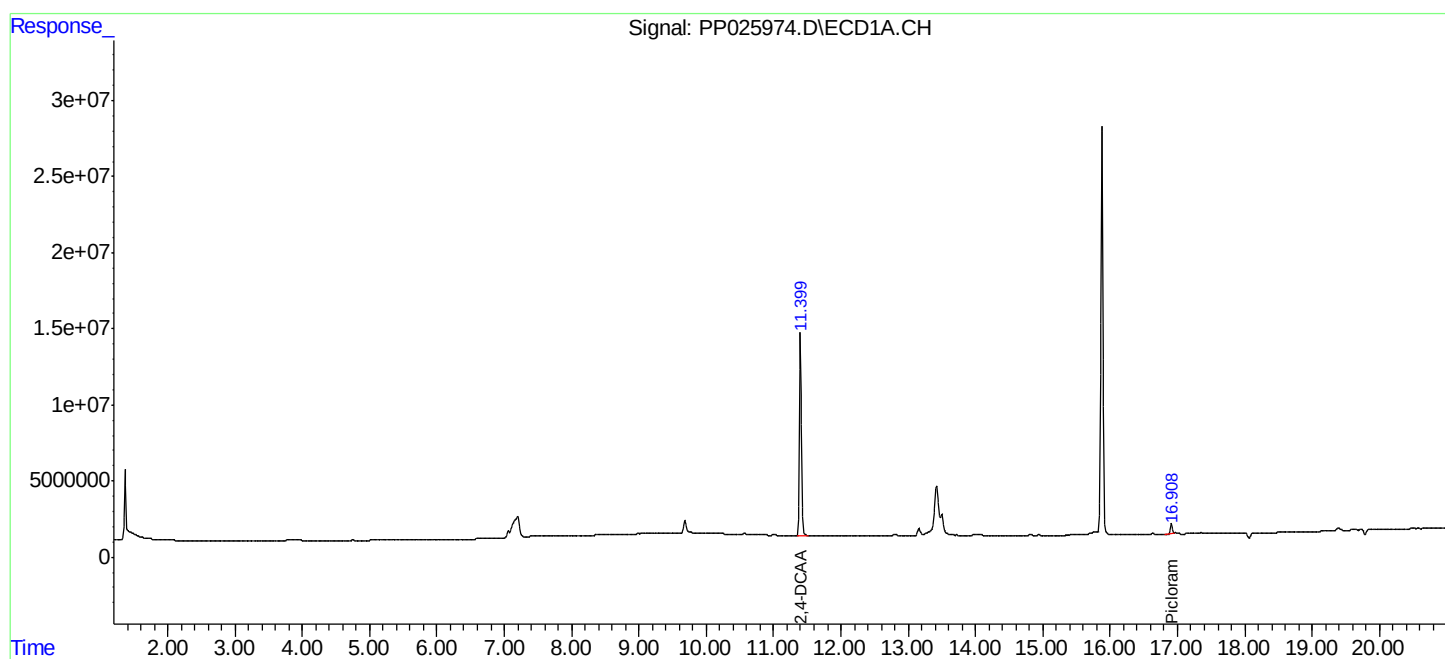


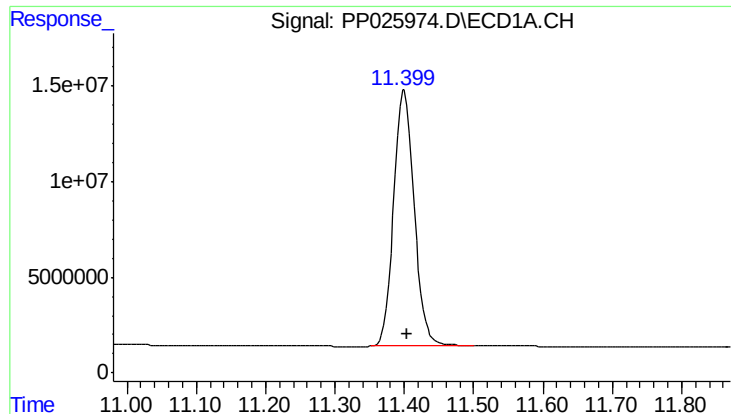

#4 2,4-DCAA


R.T.: 11.400 min
Delta R.T.: -0.005 min
Response: 273897282
Conc: 489.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

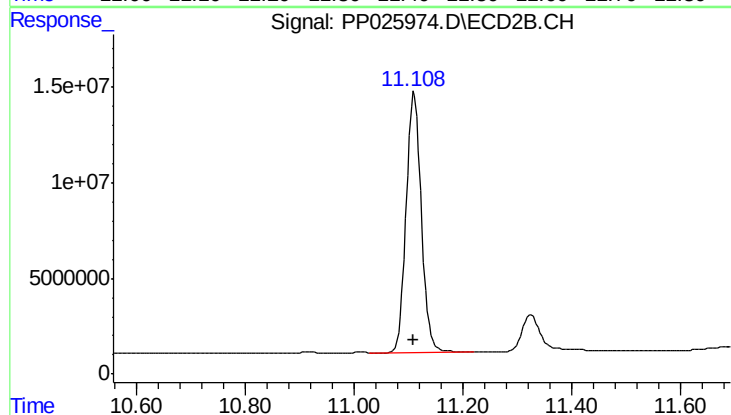


#4 2,4-DCAA

R.T.: 11.110 min
Delta R.T.: 0.000 min
Response: 262039346
Conc: 452.27 ng/ml

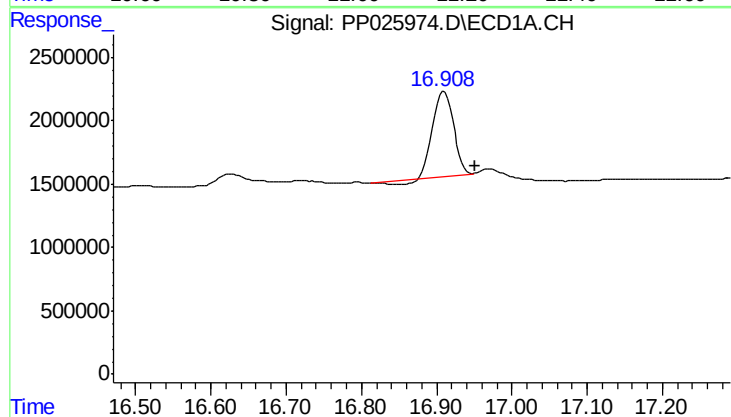

#15 Picloram

R.T.: 16.909 min
Delta R.T.: -0.041 min
Response: 12402234
Conc: 2.09 ng/ml

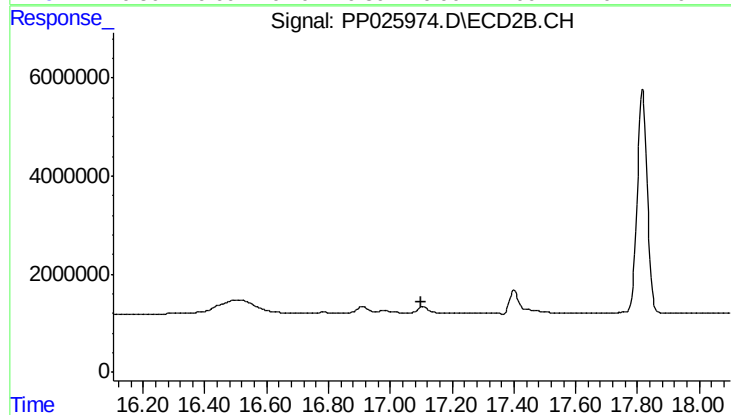

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.101 min
Response: 0
Conc: N.D.