

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052122\
 Data File : PP047839.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2022 16:49
 Operator : YP\AJ
 Sample : N2965-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 31508

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/23/2022
 Supervised By :Ankita Jodhani 05/24/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 14:51:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 21 06:22:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.839	3.109	36966020	56202971	13.975m	15.936
2) SA Decachlor...	9.889	8.403	27565528	50504938	18.200	17.330

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052122\
Data File : PP047839.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2022 16:49
Operator : YP\AJ
Sample : N2965-04
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
31508


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/23/2022
Supervised By :Ankita Jodhani 05/24/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 14:51:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 21 06:22:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

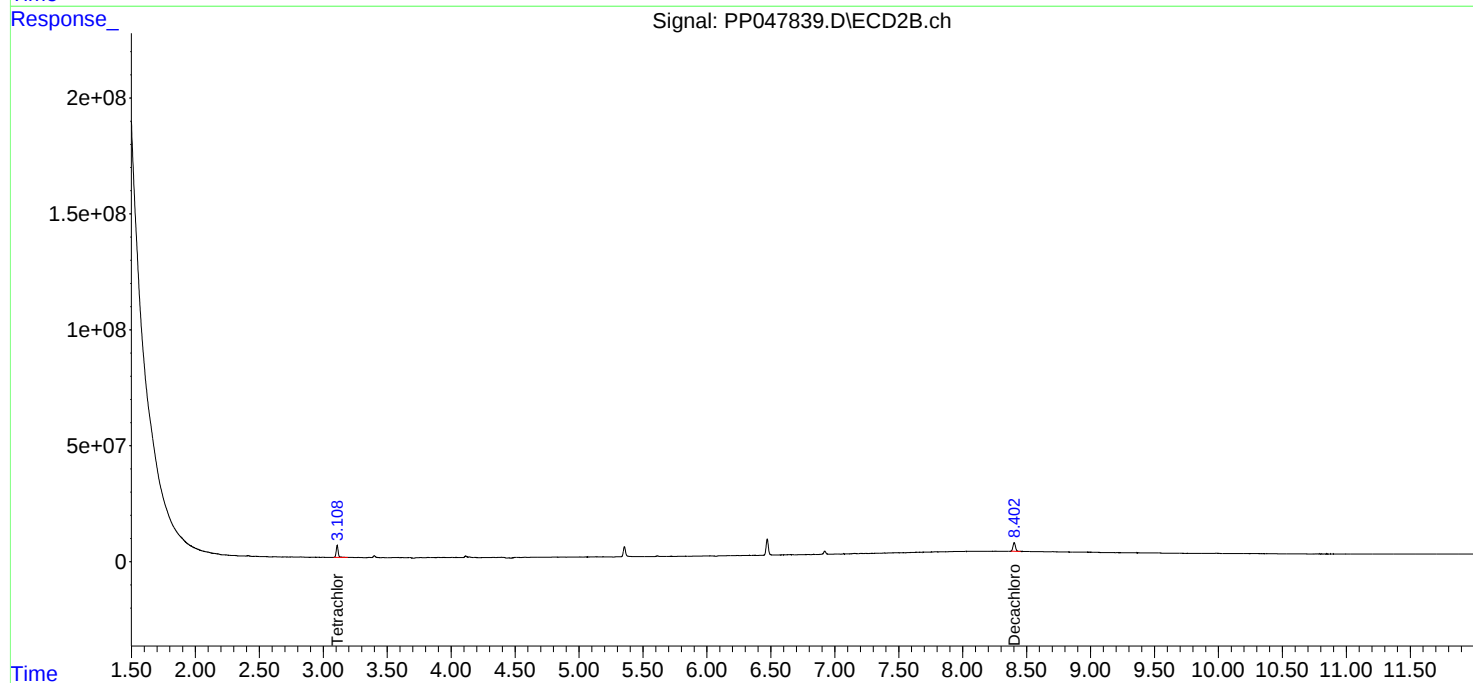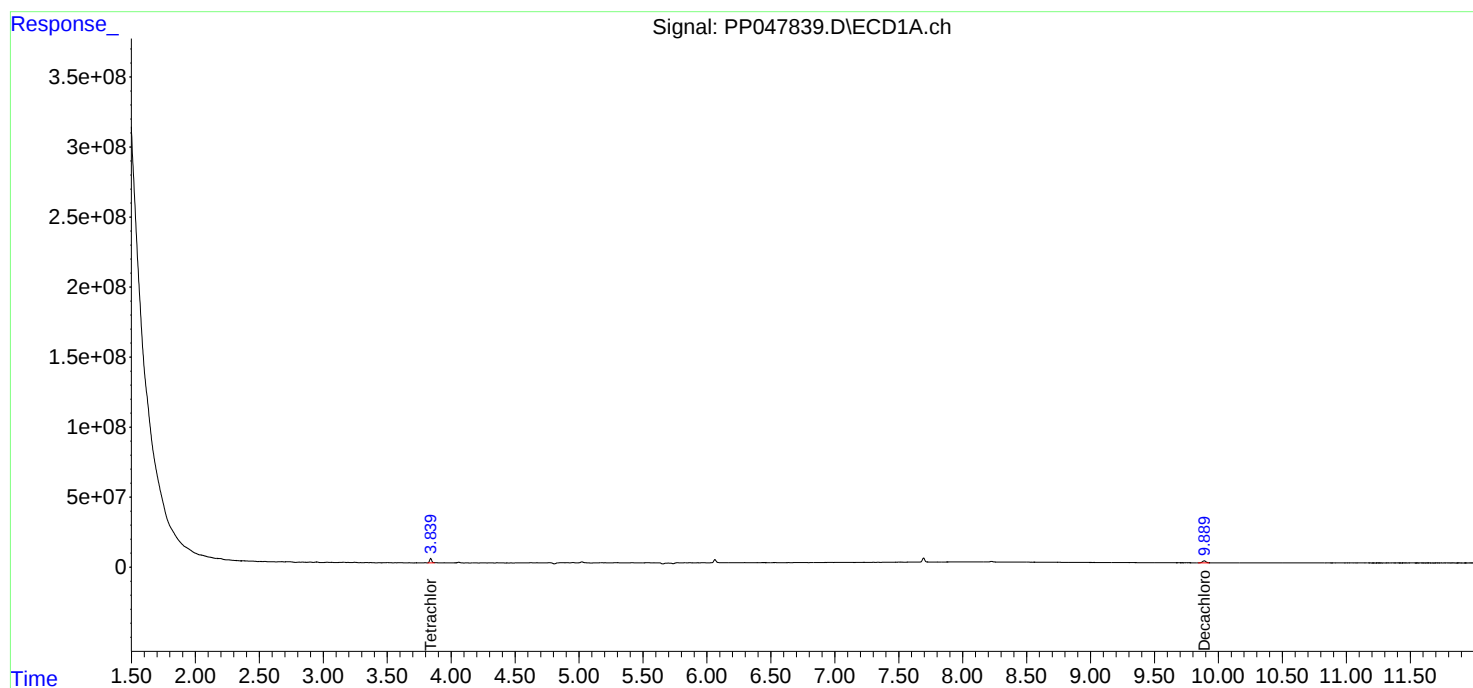

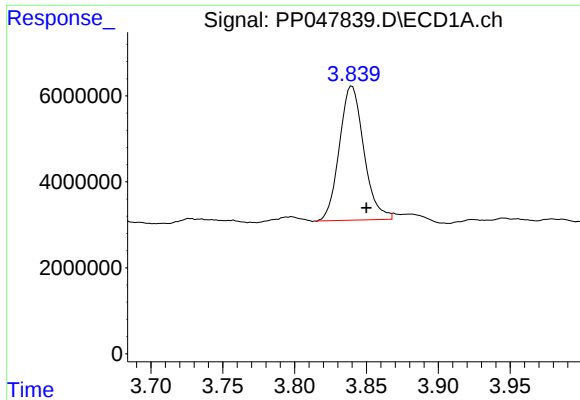


#1 Tetrachloro-m-xylene

R.T.: 3.839 min
Delta R.T.: -0.011 min
Response: 36966020
Conc: 13.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
31508


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/23/2022
Supervised By :Ankita Jodhani 05/24/2022

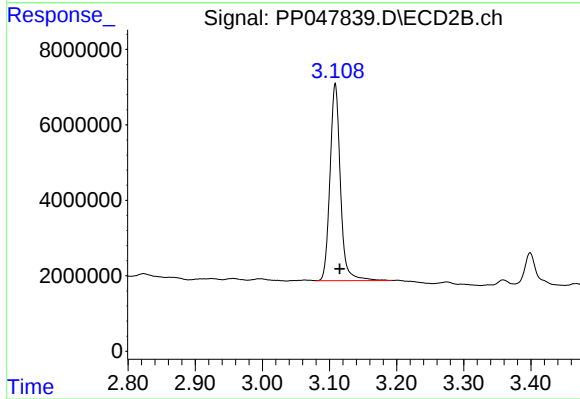


#1 Tetrachloro-m-xylene

R.T.: 3.109 min
Delta R.T.: -0.007 min
Response: 56202971
Conc: 15.94 ng/ml

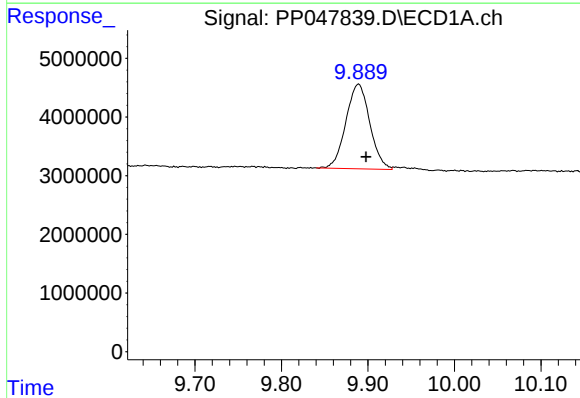

#2 Decachlorobiphenyl

R.T.: 9.889 min
Delta R.T.: -0.009 min
Response: 27565528
Conc: 18.20 ng/ml

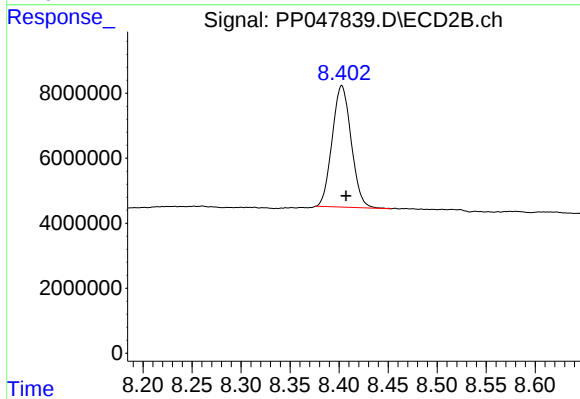

#2 Decachlorobiphenyl

R.T.: 8.403 min
Delta R.T.: -0.004 min
Response: 50504938
Conc: 17.33 ng/ml