

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052224\
 Data File : PP065176.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2024 23:16
 Operator : YP\AJ
 Sample : P2557-05 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KZZ380A-1-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 02:09:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 18:19:41 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.469	3.753	2263577	2651352	1.434	1.746
2) SA Decachlor...	10.207	8.827	2641538	2194328	2.031	1.665
Target Compounds						
28) L6 AR-1254-3	7.075	0.000	180453	0	1.940	N.D. #
30) L6 AR-1254-5	7.773	0.000	82969	0	1.181	N.D. #
31) L7 AR-1260-1	7.246	0.000	167204	0	2.423	N.D. #
32) L7 AR-1260-2	7.489	0.000	136898	0	1.773	N.D. #
33) L7 AR-1260-3	7.857	0.000	140278	0	2.343	N.D. #
34) L7 AR-1260-4	8.088	0.000	238807	0	3.547	N.D. #
35) L7 AR-1260-5	8.388	0.000	47897	0	0.404	N.D. #
36) L8 AR-1262-1	7.935f	0.000	92158	0	2.399	N.D. #
37) L8 AR-1262-2	8.388	0.000	47897	0	0.332	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052224\
Data File : PP065176.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2024 23:16
Operator : YP\AJ
Sample : P2557-05 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
KZZ380A-1-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 02:09:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052124.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 18:19:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

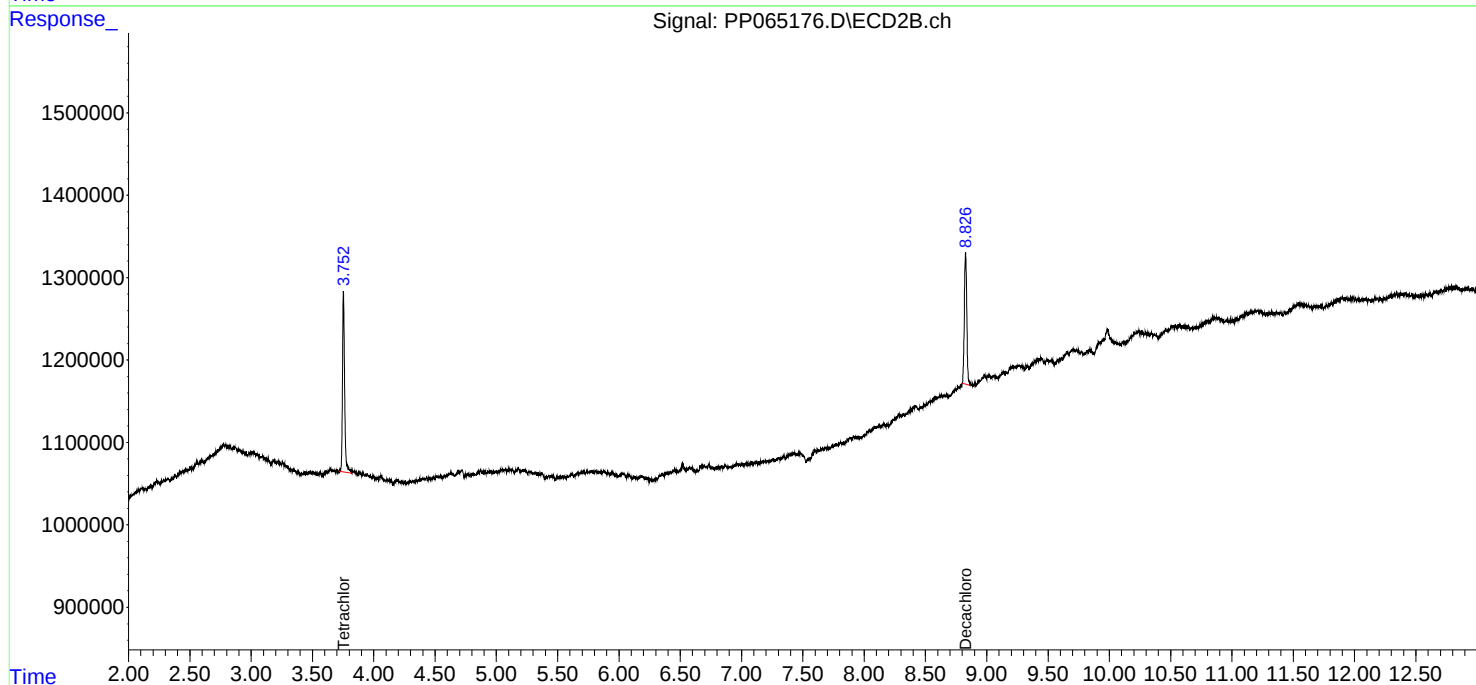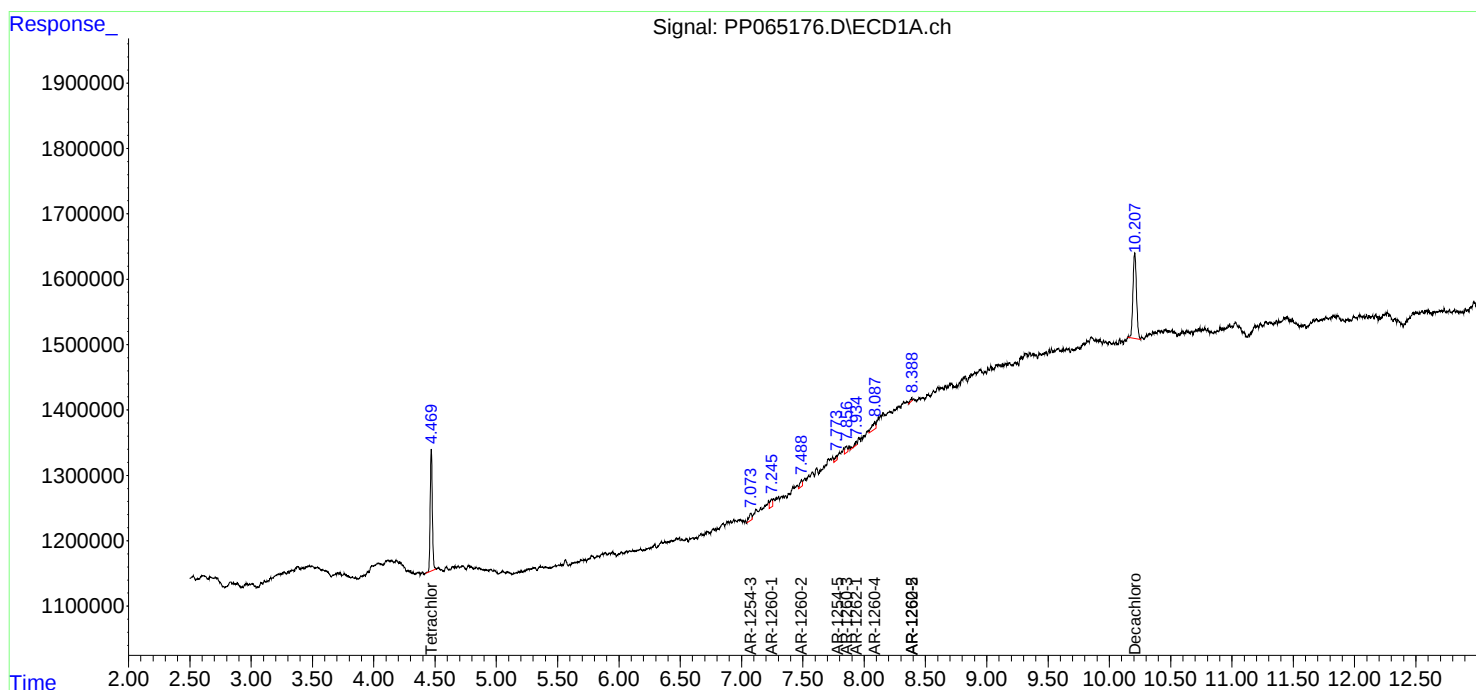


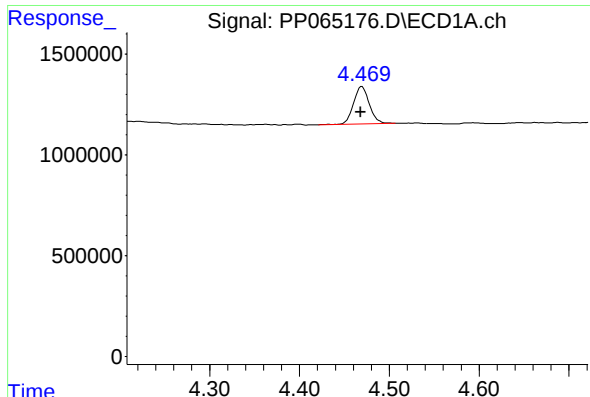

#1 Tetrachloro-m-xylene


R.T.: 4.469 min
Delta R.T.: 0.001 min
Response: 2263577
Conc: 1.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
KZZ380A-1-1

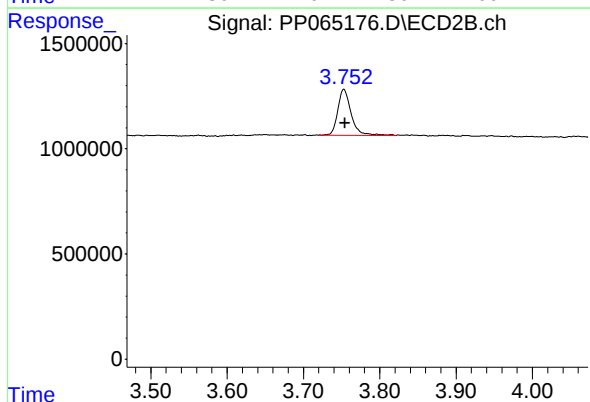


#1 Tetrachloro-m-xylene

R.T.: 3.753 min
Delta R.T.: -0.002 min
Response: 2651352
Conc: 1.75 ng/ml

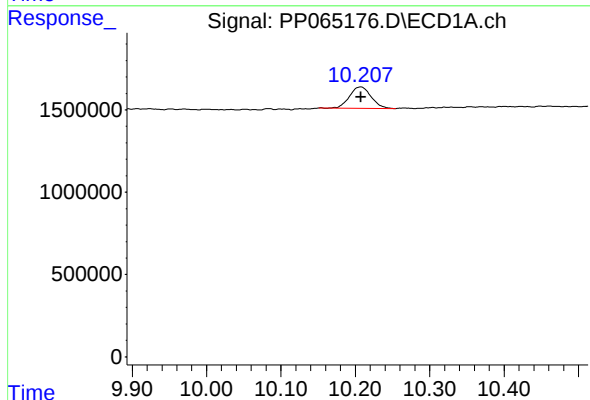


#2 Decachlorobiphenyl

R.T.: 10.207 min
Delta R.T.: 0.000 min
Response: 2641538
Conc: 2.03 ng/ml

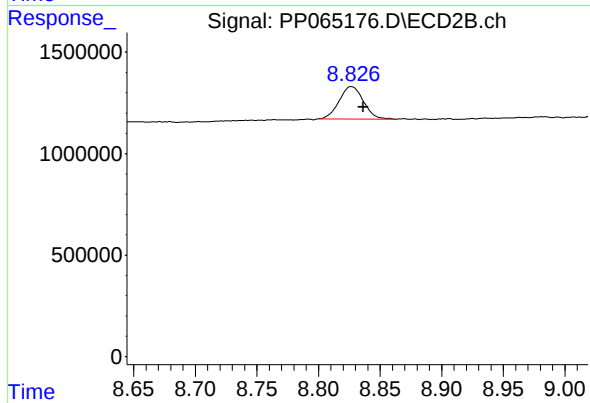

#2 Decachlorobiphenyl


R.T.: 8.827 min
Delta R.T.: -0.010 min
Response: 2194328
Conc: 1.66 ng/ml

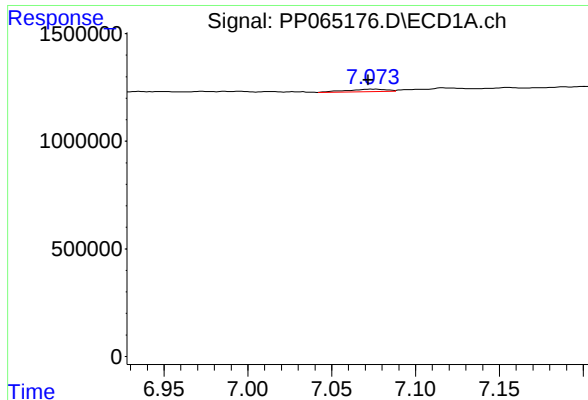

#28 AR-1254-3


R.T.: 7.075 min
Delta R.T.: 0.003 min
Response: 180453
Conc: 1.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
KZZ380A-1-1

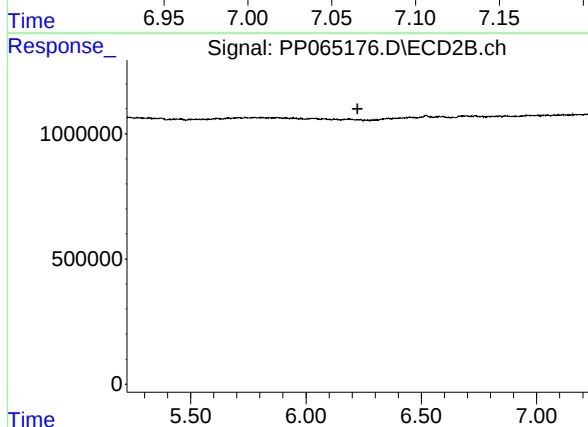


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.223 min
Response: 0
Conc: N.D.

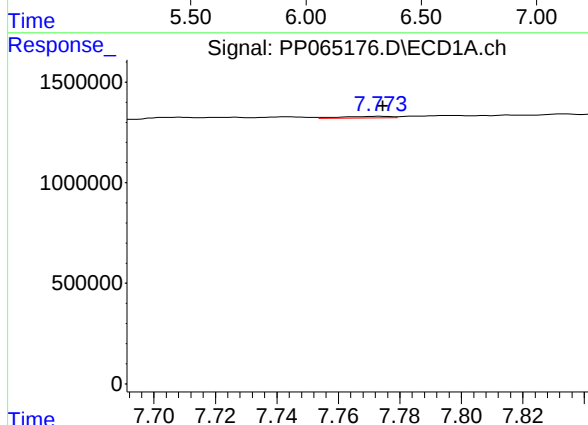


#30 AR-1254-5

R.T.: 7.773 min
Delta R.T.: -0.001 min
Response: 82969
Conc: 1.18 ng/ml

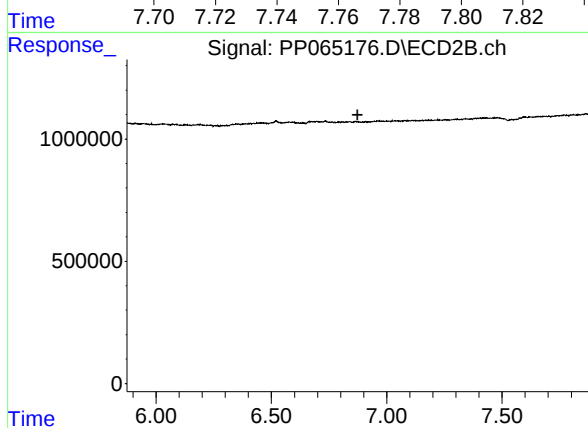

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.873 min
Response: 0
Conc: N.D.

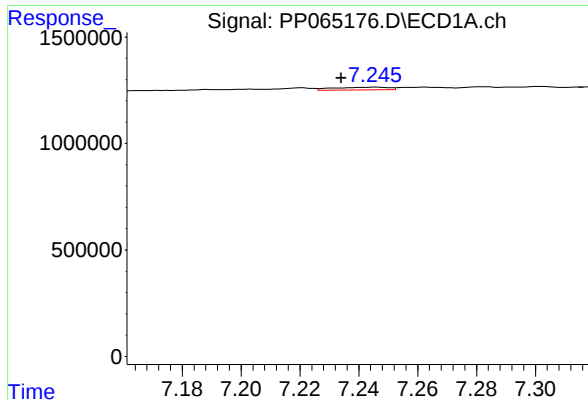

#31 AR-1260-1


R.T.: 7.246 min
Delta R.T.: 0.012 min
Response: 167204
Conc: 2.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
KZZ380A-1-1

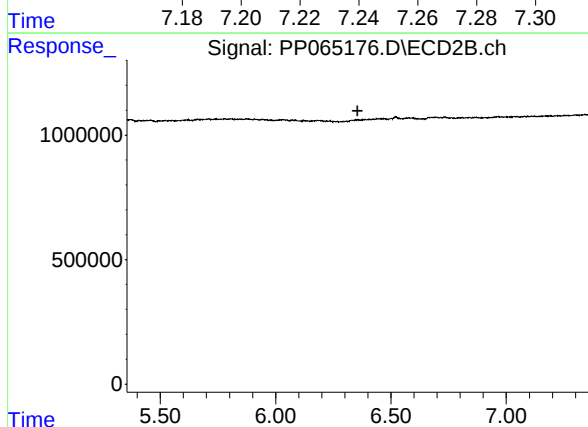


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

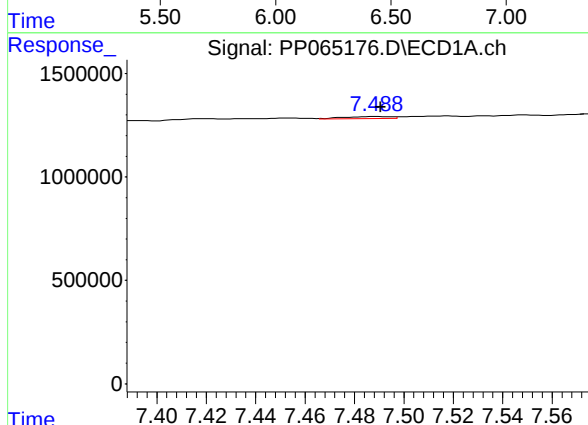


#32 AR-1260-2

R.T.: 7.489 min
Delta R.T.: -0.002 min
Response: 136898
Conc: 1.77 ng/ml

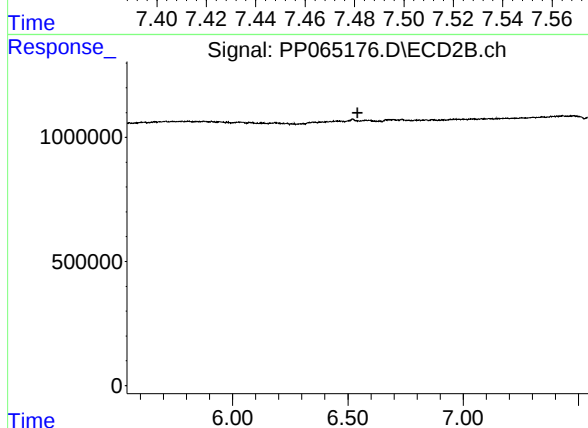

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.542 min
Response: 0
Conc: N.D.

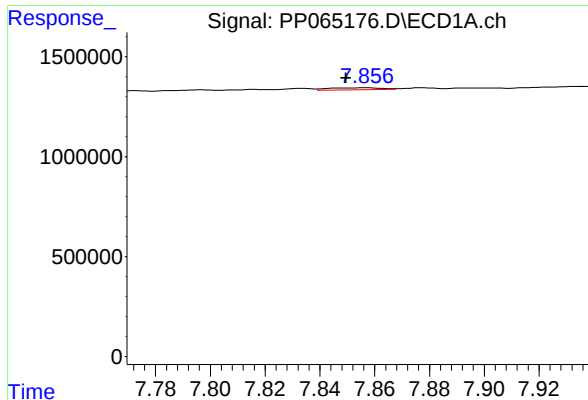

#33 AR-1260-3


R.T.: 7.857 min
Delta R.T.: 0.007 min
Response: 140278
Conc: 2.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
KZZ380A-1-1

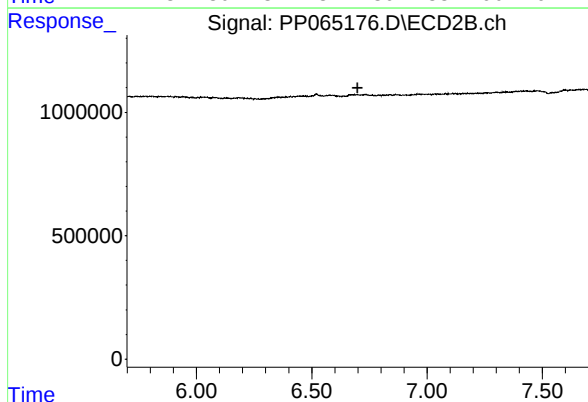


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.699 min
Response: 0
Conc: N.D.

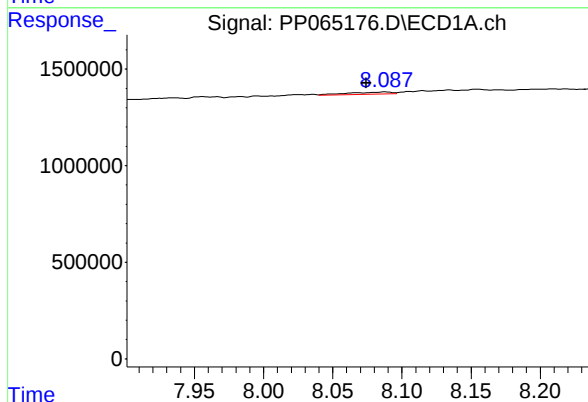


#34 AR-1260-4

R.T.: 8.088 min
Delta R.T.: 0.013 min
Response: 238807
Conc: 3.55 ng/ml

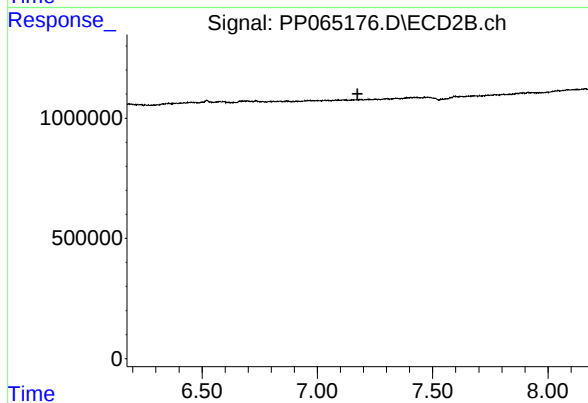

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.174 min
Response: 0
Conc: N.D.

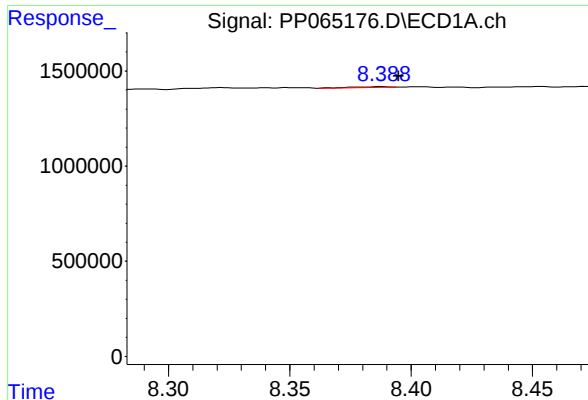

#35 AR-1260-5


R.T.: 8.388 min
Delta R.T.: -0.007 min
Response: 47897
Conc: 0.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
KZZ380A-1-1

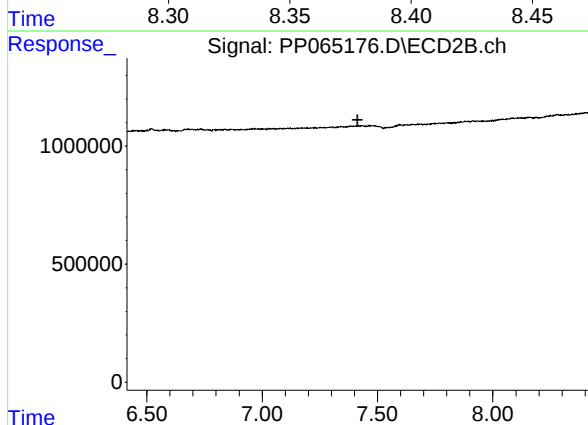


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 7.413 min
Response: 0
Conc: N.D.

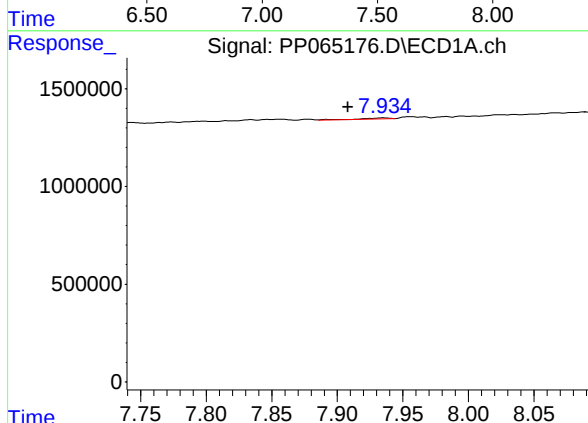


#36 AR-1262-1

R.T.: 7.935 min
Delta R.T.: 0.027 min
Response: 92158
Conc: 2.40 ng/ml

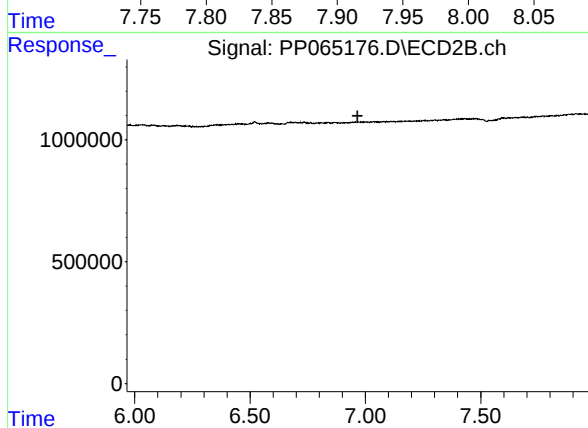

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 6.966 min
Response: 0
Conc: N.D.

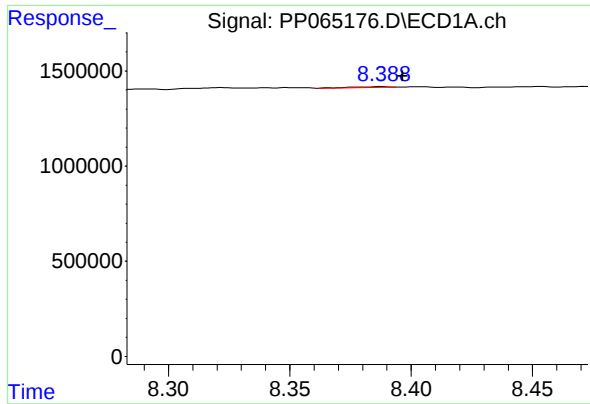

#37 AR-1262-2

R.T.: 8.388 min
Delta R.T.: -0.008 min
Response: 47897
Conc: 0.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
KZZ380A-1-1

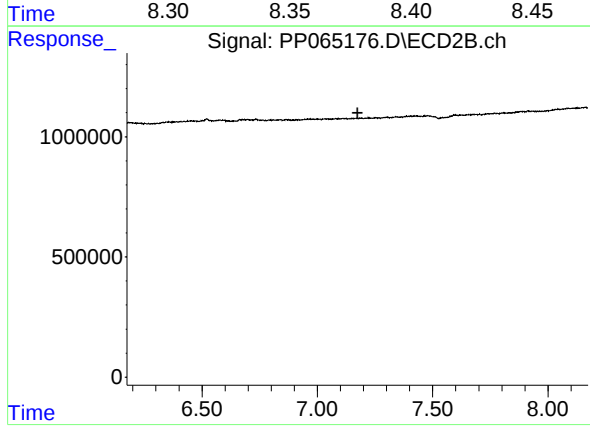

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.174 min
Response: 0
Conc: N.D.