

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052224\
 Data File : PP065177.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2024 23:32
 Operator : YP\AJ
 Sample : P2557-06 10X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KZZ380A-1-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 02:09:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 18:19:41 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.469	3.753	2878240	2805129	1.824	1.848
2) SA Decachlor...	10.205	8.828	3071629	2257656	2.362	1.713 #
Target Compounds						
28) L6 AR-1254-3	7.071	0.000	159501	0	1.715	N.D. #
29) L6 AR-1254-4	7.361	0.000	47509	0	0.784	N.D. #
30) L6 AR-1254-5	7.775	0.000	58648	0	0.835	N.D. #
31) L7 AR-1260-1	7.236	0.000	146710	0	2.126	N.D. #
32) L7 AR-1260-2	7.499	0.000	156989	0	2.033	N.D. #
33) L7 AR-1260-3	7.842	0.000	115222	0	1.925	N.D. #
34) L7 AR-1260-4	8.067	0.000	121250	0	1.801	N.D. #
36) L8 AR-1262-1	7.907	0.000	38974	0	1.015	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052224\
Data File : PP065177.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2024 23:32
Operator : YP\AJ
Sample : P2557-06 10X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
KZZ380A-1-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 02:09:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052124.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 18:19:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

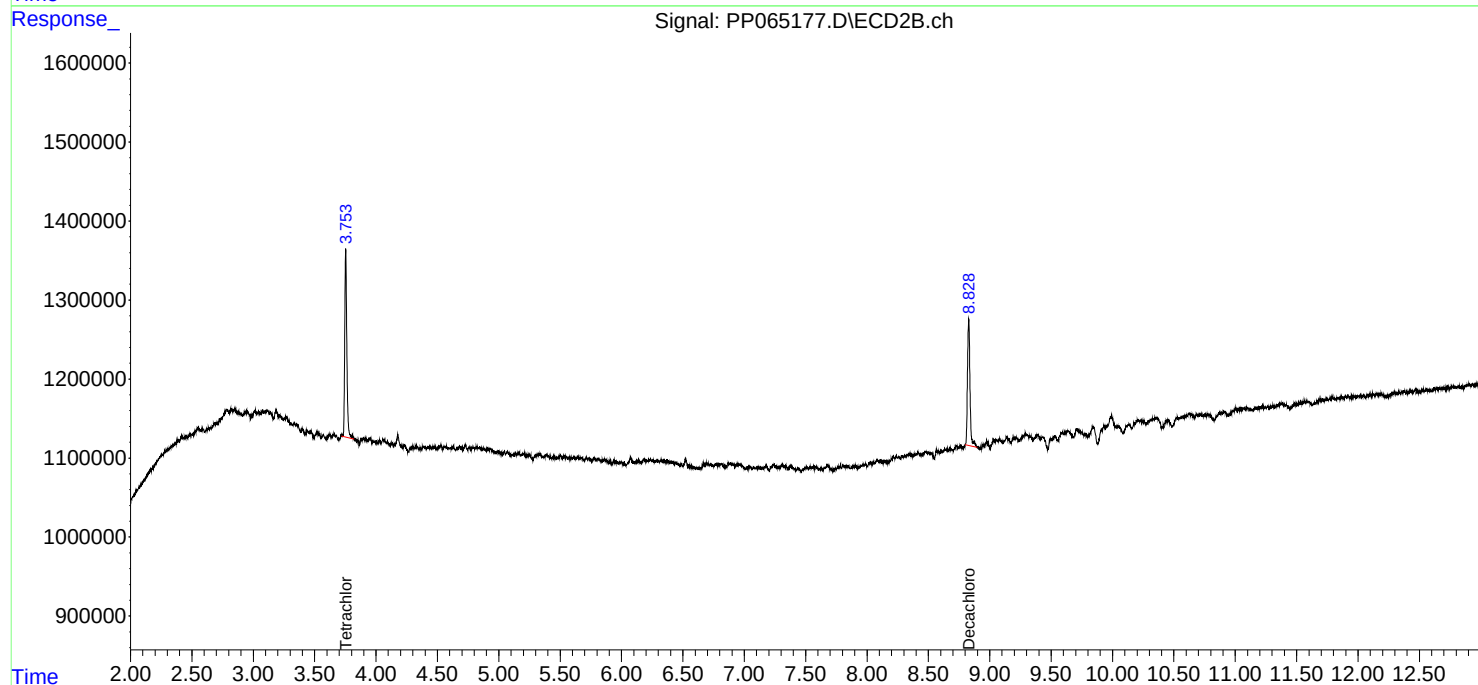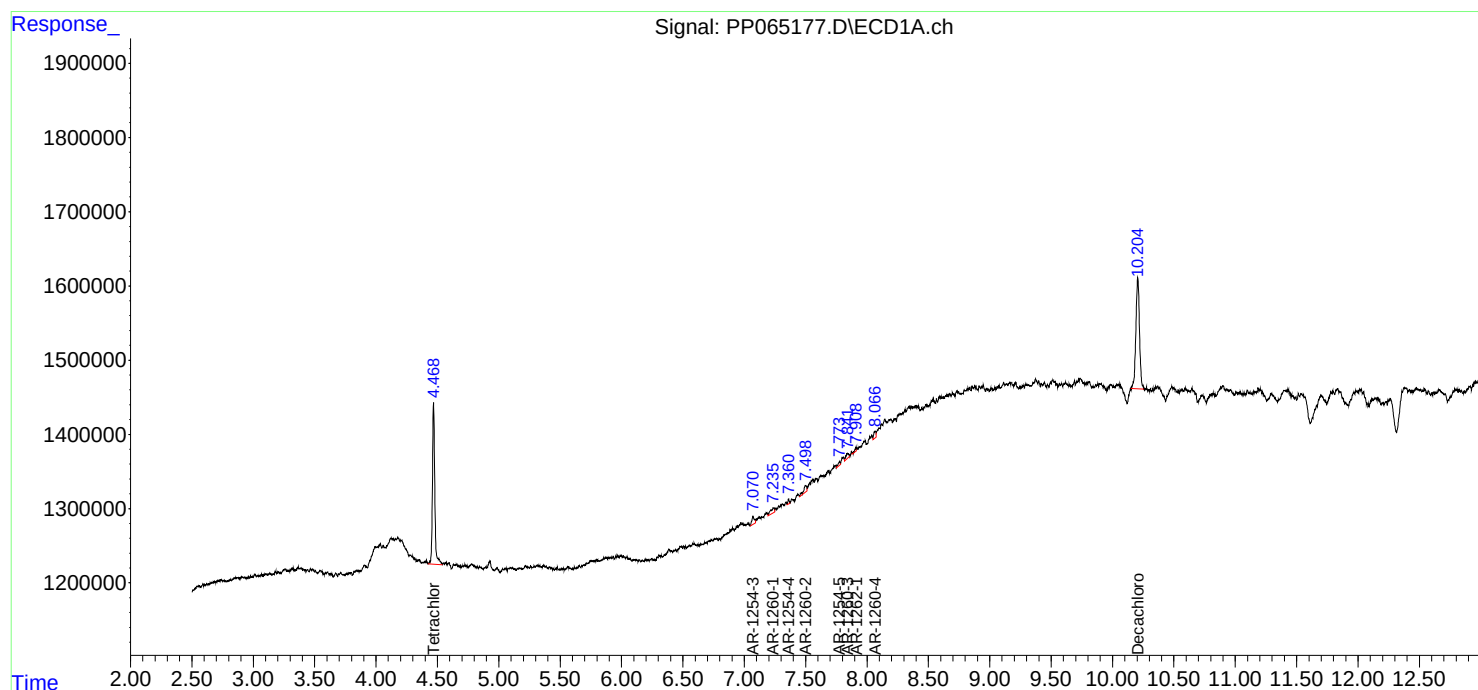


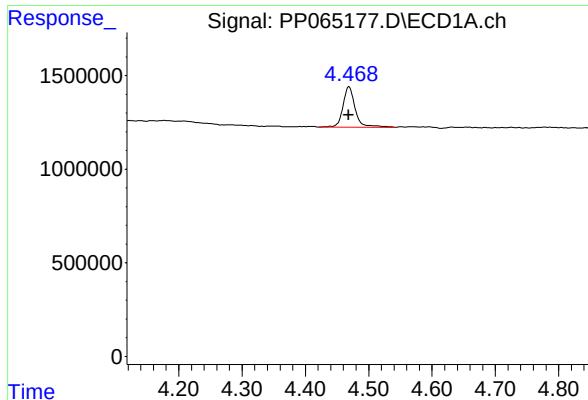

#1 Tetrachloro-m-xylene


R.T.: 4.469 min
Delta R.T.: 0.000 min
Response: 2878240
Conc: 1.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
KZZ380A-1-2

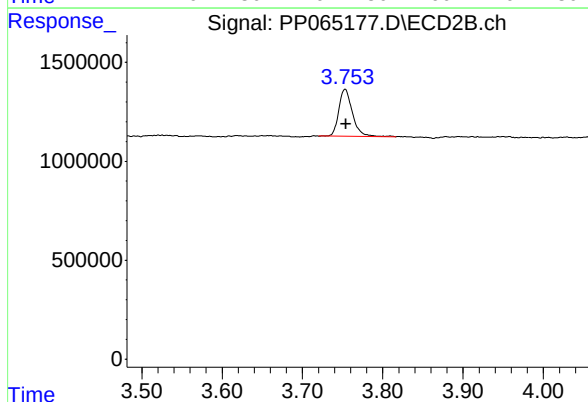


#1 Tetrachloro-m-xylene

R.T.: 3.753 min
Delta R.T.: -0.001 min
Response: 2805129
Conc: 1.85 ng/ml

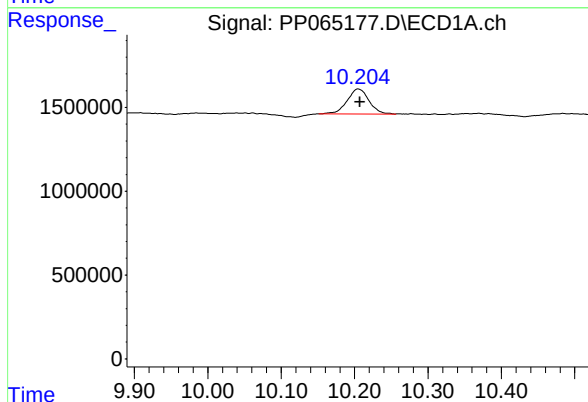


#2 Decachlorobiphenyl

R.T.: 10.205 min
Delta R.T.: -0.002 min
Response: 3071629
Conc: 2.36 ng/ml

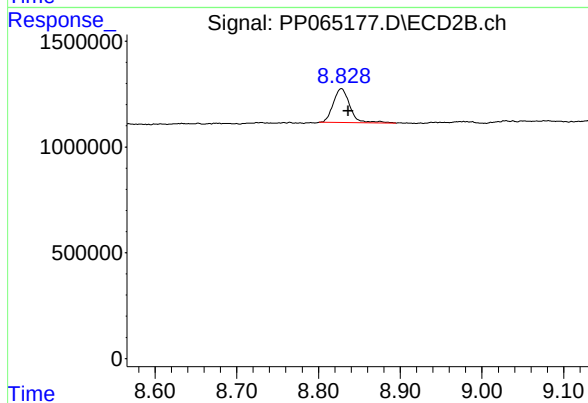

#2 Decachlorobiphenyl


R.T.: 8.828 min
Delta R.T.: -0.008 min
Response: 2257656
Conc: 1.71 ng/ml

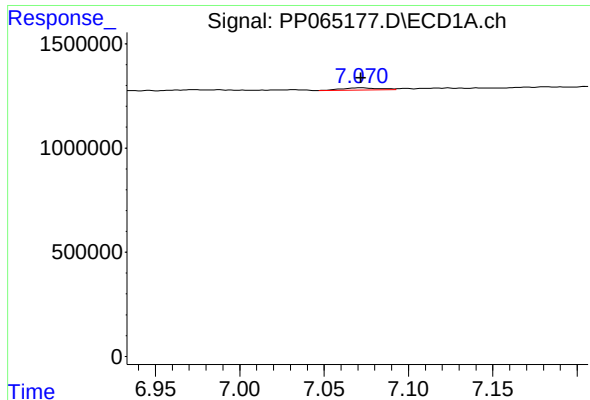

#28 AR-1254-3


R.T.: 7.071 min
Delta R.T.: 0.000 min
Response: 159501
Conc: 1.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
KZZ380A-1-2

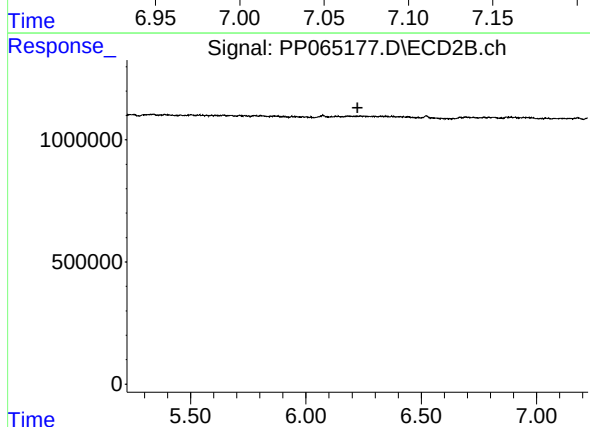


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.223 min
Response: 0
Conc: N.D.

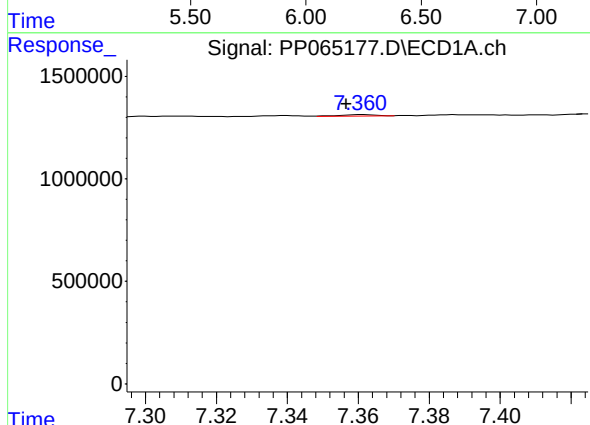


#29 AR-1254-4

R.T.: 7.361 min
Delta R.T.: 0.004 min
Response: 47509
Conc: 0.78 ng/ml

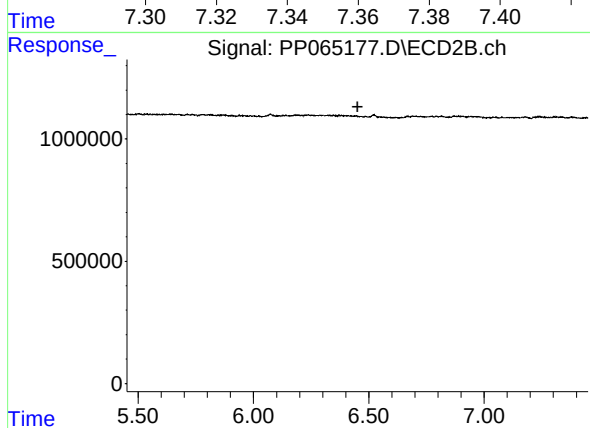

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

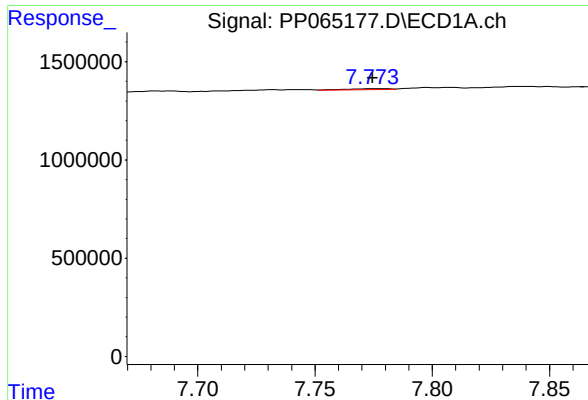

#30 AR-1254-5


R.T.: 7.775 min
Delta R.T.: 0.000 min
Response: 58648
Conc: 0.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
KZZ380A-1-2

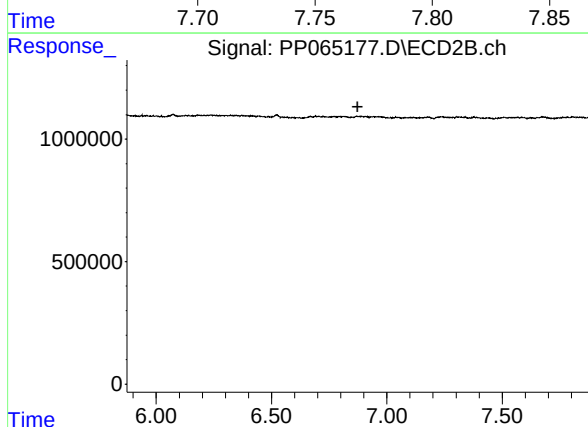


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.873 min
Response: 0
Conc: N.D.

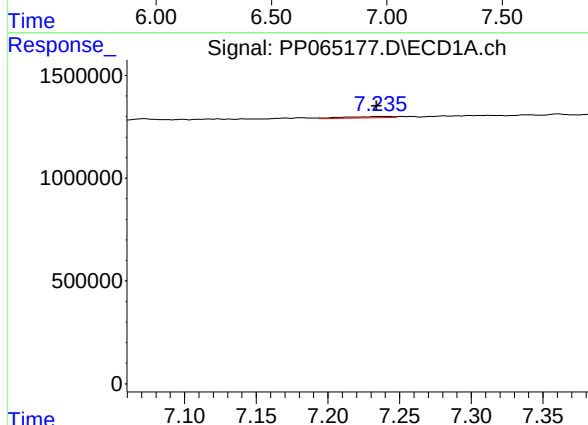


#31 AR-1260-1

R.T.: 7.236 min
Delta R.T.: 0.002 min
Response: 146710
Conc: 2.13 ng/ml

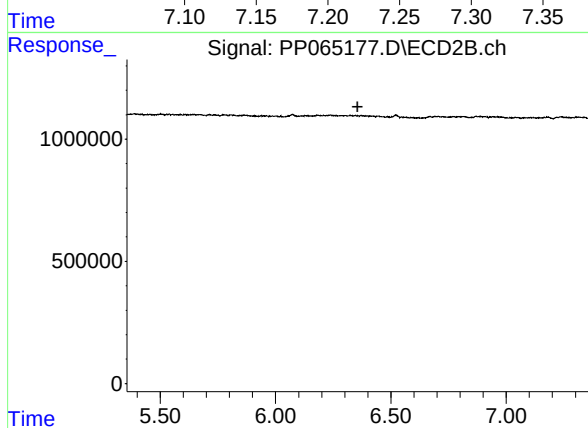

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

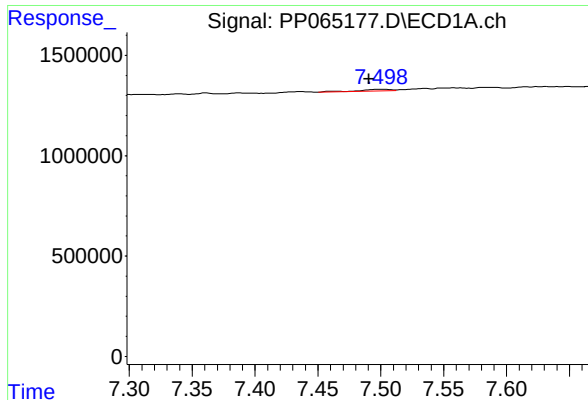

#32 AR-1260-2


R.T.: 7.499 min
Delta R.T.: 0.008 min
Response: 156989
Conc: 2.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
KZZ380A-1-2

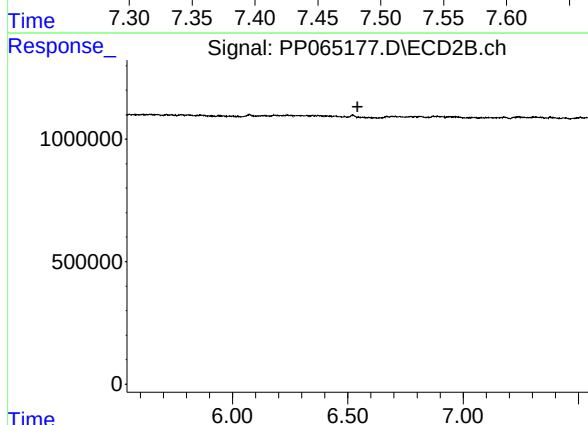


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.542 min
Response: 0
Conc: N.D.

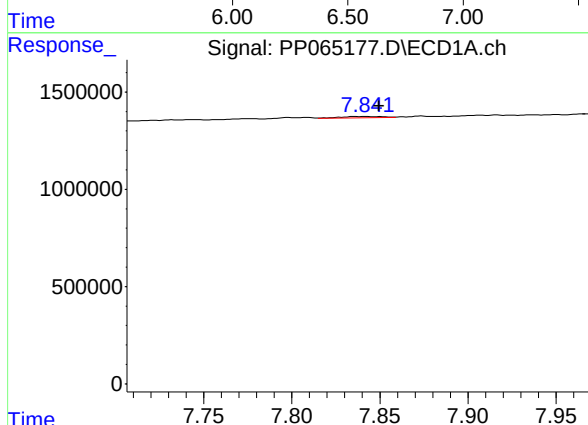


#33 AR-1260-3

R.T.: 7.842 min
Delta R.T.: -0.007 min
Response: 115222
Conc: 1.92 ng/ml

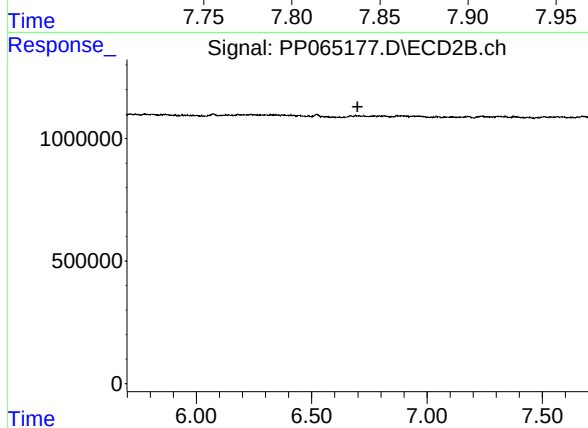

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 6.699 min
Response: 0
Conc: N.D.

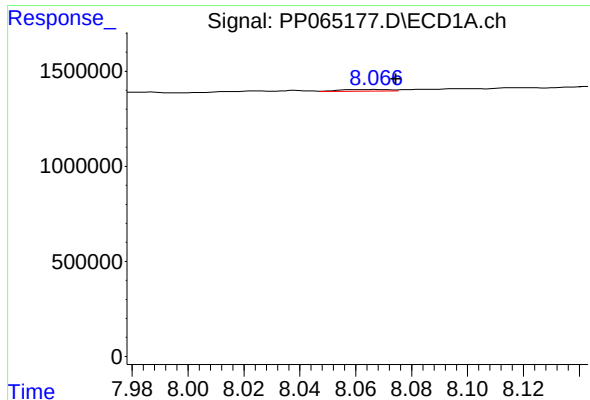

#34 AR-1260-4


R.T.: 8.067 min
Delta R.T.: -0.008 min
Response: 121250
Conc: 1.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
KZZ380A-1-2

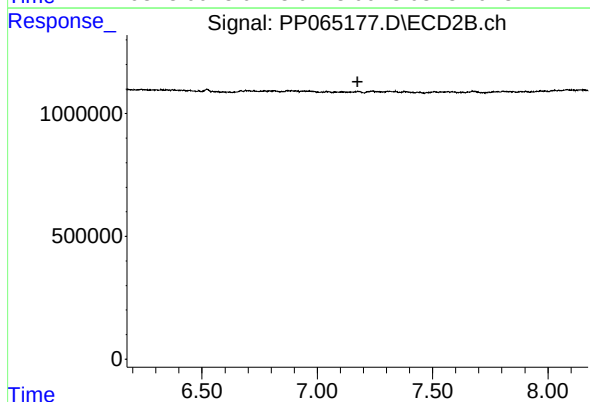


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.174 min
Response: 0
Conc: N.D.

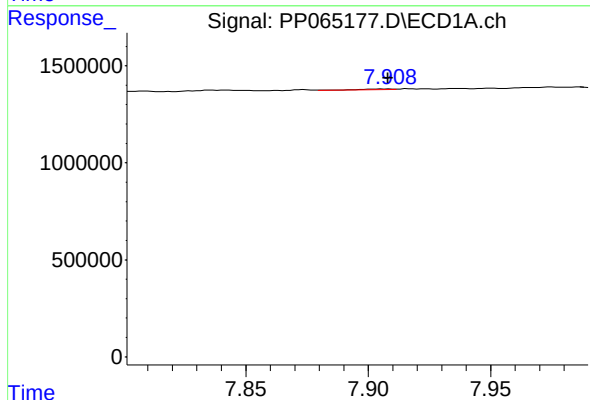

#36 AR-1262-1

R.T.: 7.907 min
Delta R.T.: 0.000 min
Response: 38974
Conc: 1.01 ng/ml

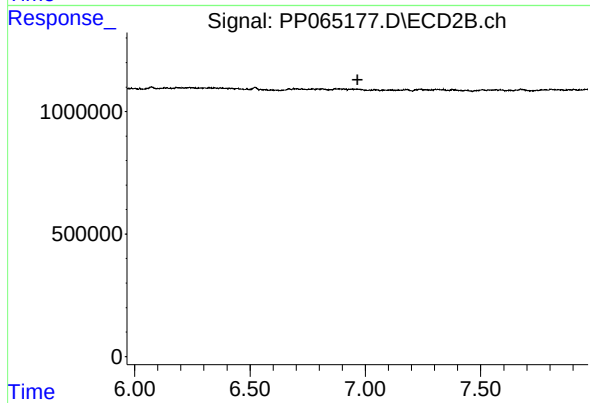

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 6.966 min
Response: 0
Conc: N.D.