

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052224\
 Data File : PP065178.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2024 23:48
 Operator : YP\AJ
 Sample : P2557-07 10X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC1976A3LOK-1-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 02:09:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 18:19:41 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.469	3.753	2469588	2847716	1.565	1.876
2) SA Decachlor...	10.206	8.825	2948656	2256232	2.268	1.712
Target Compounds						
24) L5 AR-1248-4	6.485f	0.000	279091	0	5.097	N.D. #
26) L6 AR-1254-1	6.485	0.000	279091	0	4.520	N.D. #
28) L6 AR-1254-3	7.072	0.000	133637	0	1.437	N.D. #
30) L6 AR-1254-5	7.776	0.000	576770	0	8.210	N.D. #
32) L7 AR-1260-2	7.496	0.000	334462	0	4.331	N.D. #
33) L7 AR-1260-3	7.869f	0.000	176916	0	2.955	N.D. #
35) L7 AR-1260-5	8.393	0.000	219583	0	1.853	N.D. #
37) L8 AR-1262-2	8.393	0.000	219583	0	1.521	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052224\
Data File : PP065178.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2024 23:48
Operator : YP\AJ
Sample : P2557-07 10X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BC1976A3LOK-1-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 02:09:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052124.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 18:19:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

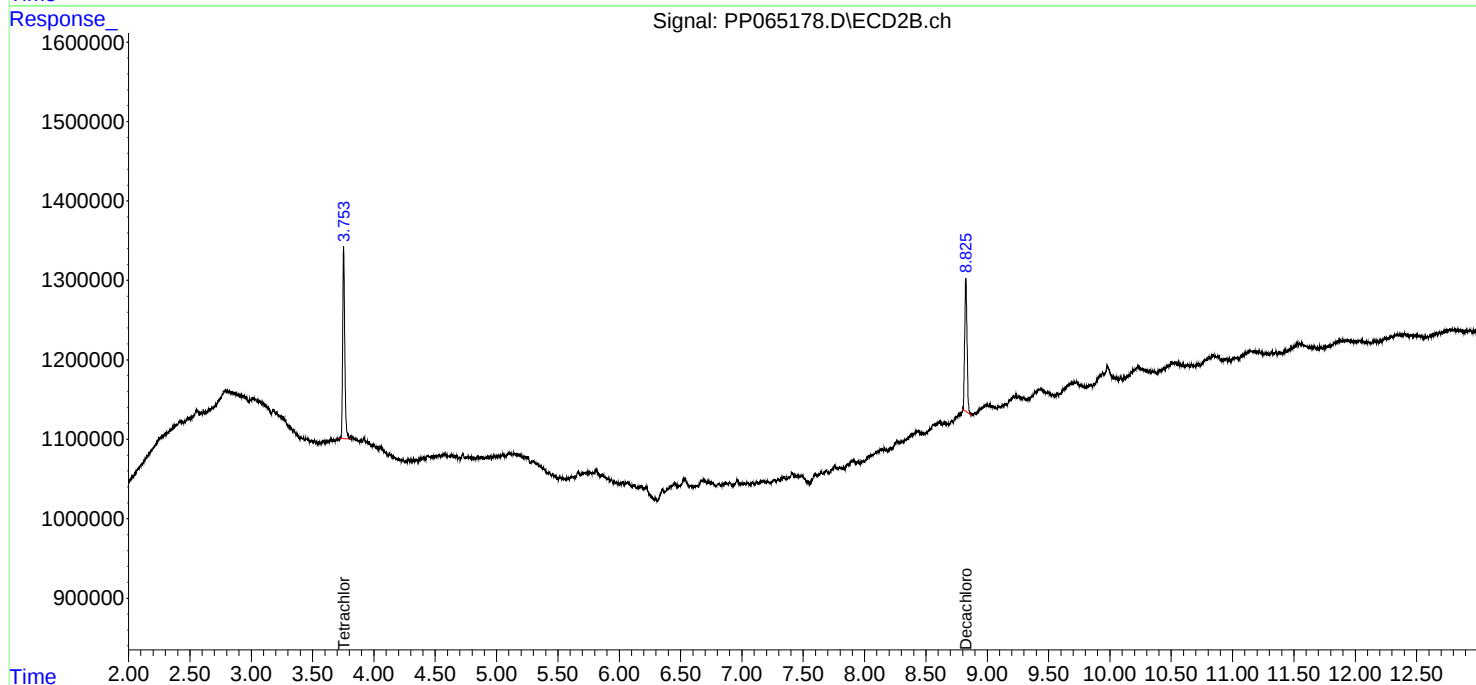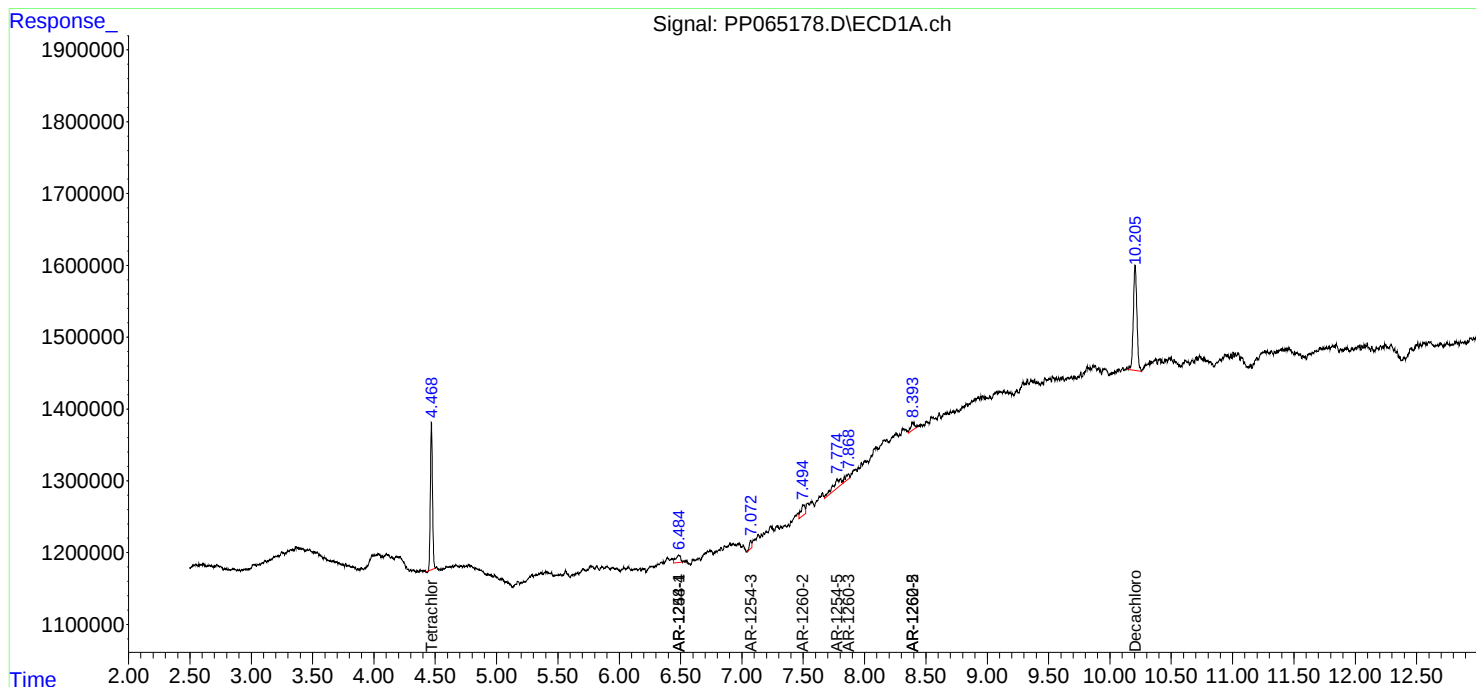


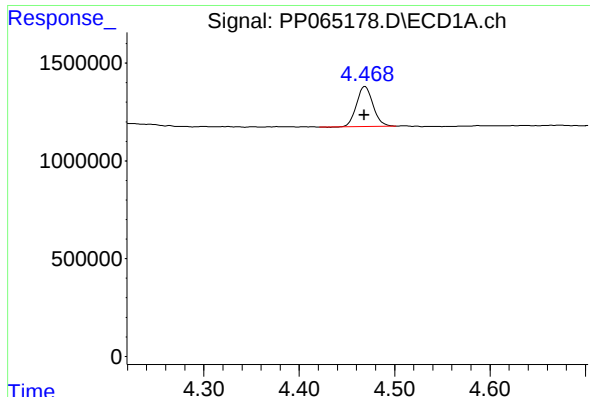

#1 Tetrachloro-m-xylene


R.T.: 4.469 min
Delta R.T.: 0.001 min
Response: 2469588
Conc: 1.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC1976A3LOK-1-1

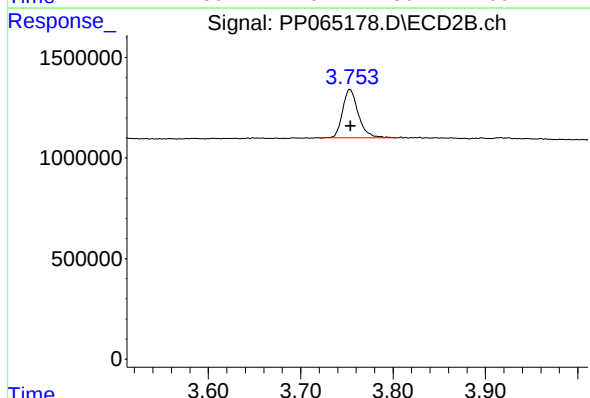


#1 Tetrachloro-m-xylene

R.T.: 3.753 min
Delta R.T.: 0.000 min
Response: 2847716
Conc: 1.88 ng/ml

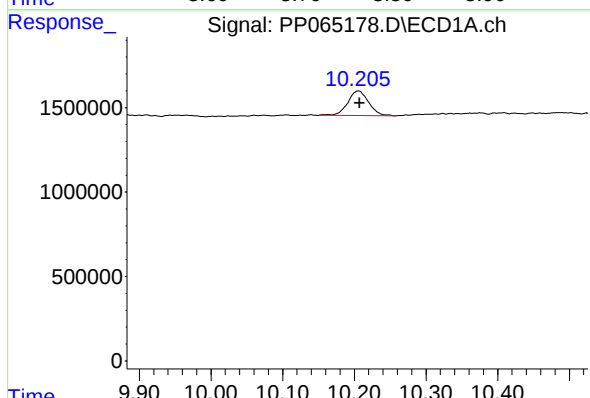


#2 Decachlorobiphenyl

R.T.: 10.206 min
Delta R.T.: -0.002 min
Response: 2948656
Conc: 2.27 ng/ml

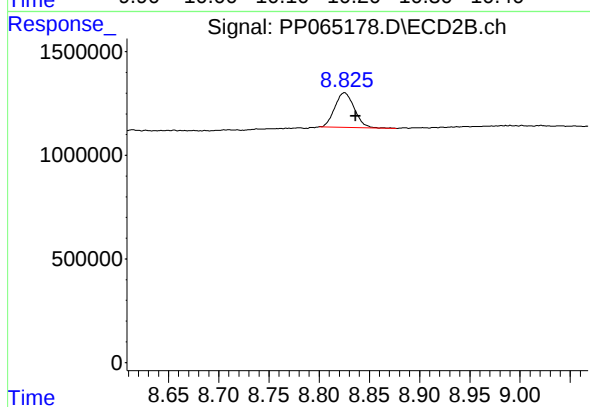

#2 Decachlorobiphenyl


R.T.: 8.825 min
Delta R.T.: -0.011 min
Response: 2256232
Conc: 1.71 ng/ml

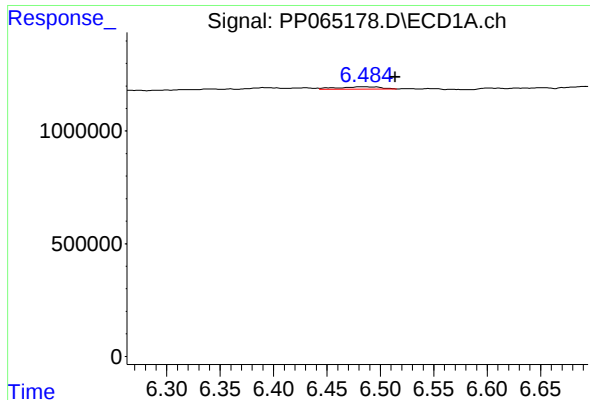

#24 AR-1248-4


R.T.: 6.485 min
Delta R.T.: -0.029 min
Response: 279091
Conc: 5.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC1976A3LOK-1-1

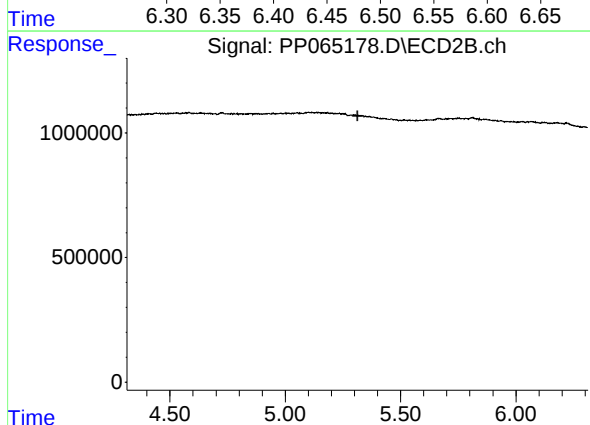


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.313 min
Response: 0
Conc: N.D.

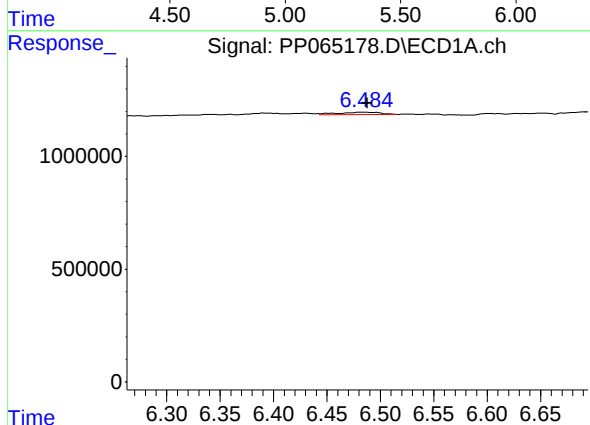


#26 AR-1254-1

R.T.: 6.485 min
Delta R.T.: -0.003 min
Response: 279091
Conc: 4.52 ng/ml

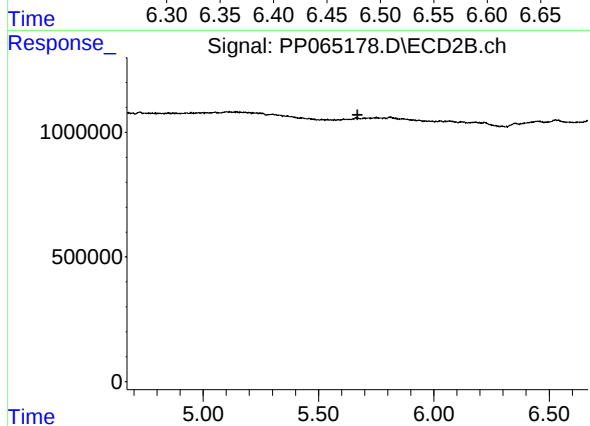

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.669 min
Response: 0
Conc: N.D.

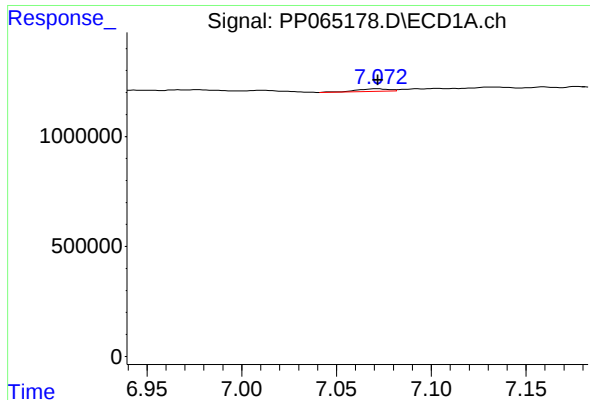

#28 AR-1254-3


R.T.: 7.072 min
Delta R.T.: 0.000 min
Response: 133637
Conc: 1.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC1976A3LOK-1-1

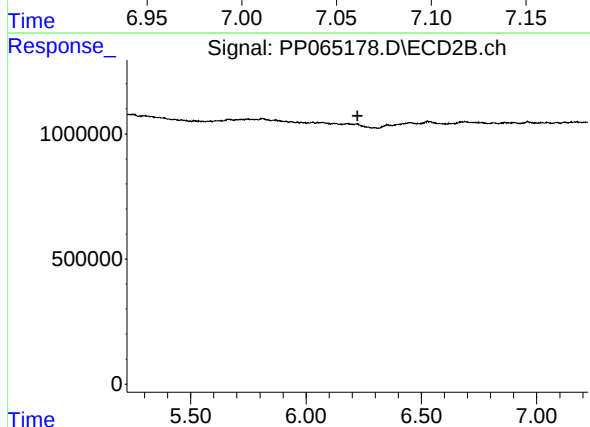


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.223 min
Response: 0
Conc: N.D.

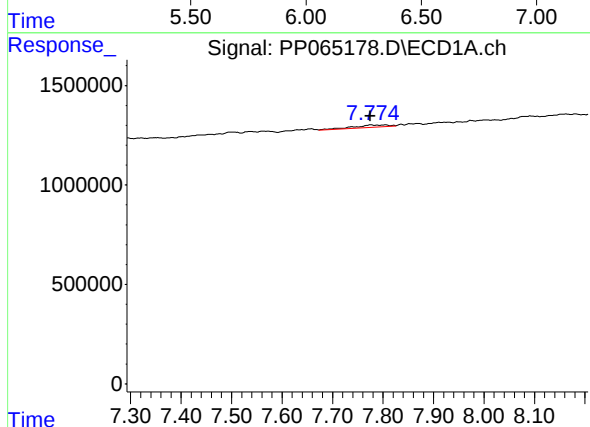


#30 AR-1254-5

R.T.: 7.776 min
Delta R.T.: 0.001 min
Response: 576770
Conc: 8.21 ng/ml

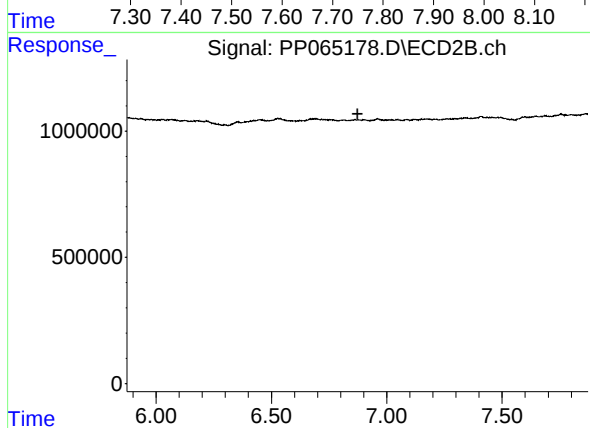

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.873 min
Response: 0
Conc: N.D.

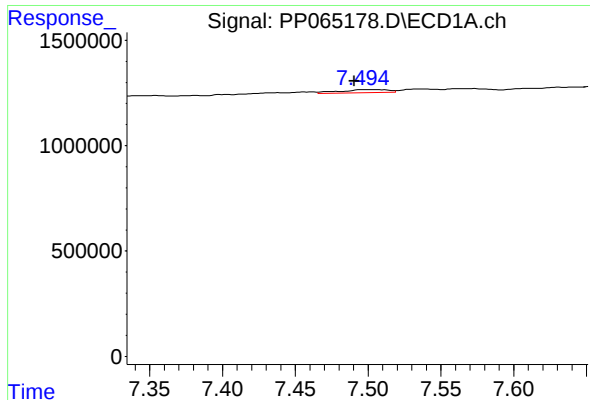

#32 AR-1260-2


R.T.: 7.496 min
Delta R.T.: 0.005 min
Response: 334462
Conc: 4.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC1976A3LOK-1-1

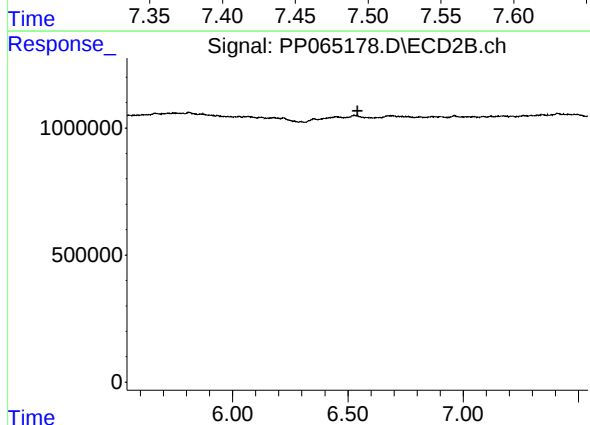


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.542 min
Response: 0
Conc: N.D.

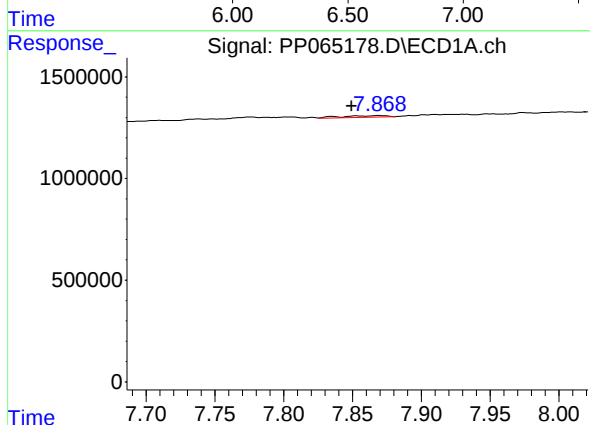


#33 AR-1260-3

R.T.: 7.869 min
Delta R.T.: 0.020 min
Response: 176916
Conc: 2.96 ng/ml

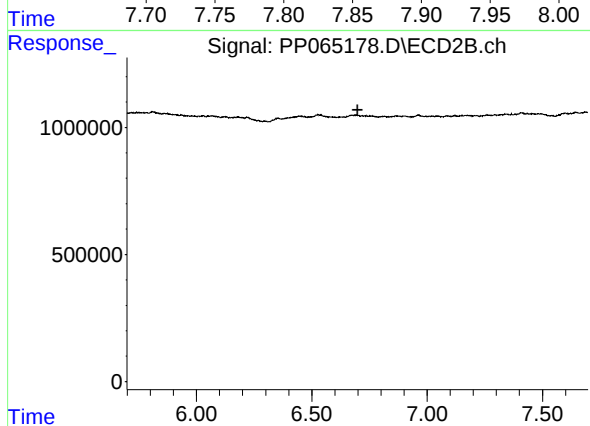

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 6.699 min
Response: 0
Conc: N.D.

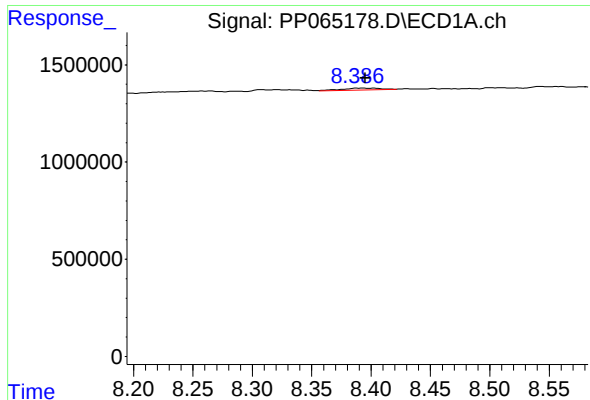

#35 AR-1260-5


R.T.: 8.393 min
Delta R.T.: -0.002 min
Response: 219583
Conc: 1.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC1976A3LOK-1-1

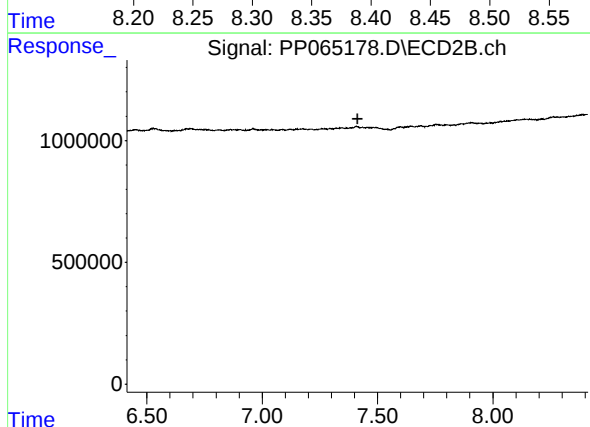


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.413 min
Response: 0
Conc: N.D.

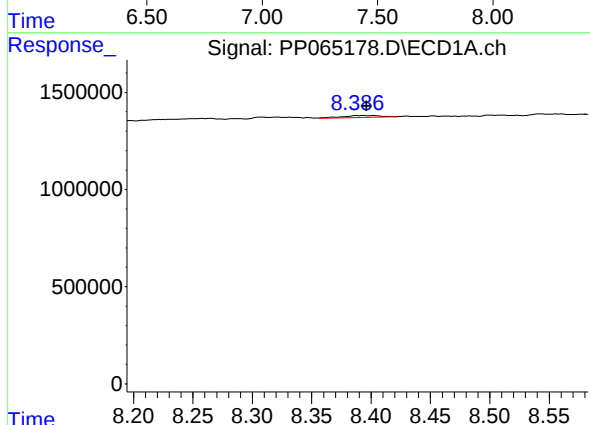

#37 AR-1262-2

R.T.: 8.393 min
Delta R.T.: -0.003 min
Response: 219583
Conc: 1.52 ng/ml

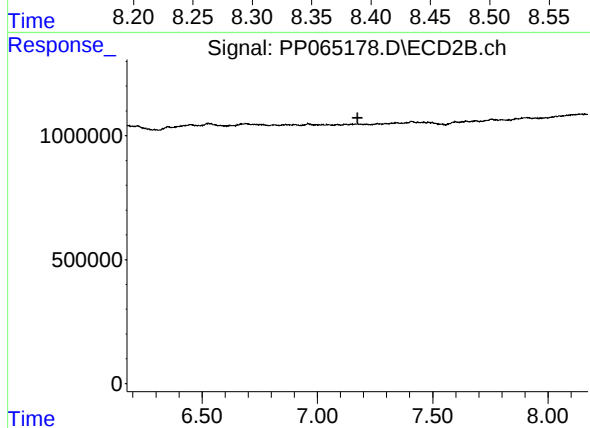

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.174 min
Response: 0
Conc: N.D.