

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052224\
 Data File : PP065181.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2024 00:37
 Operator : YP\AJ
 Sample : P2559-02 10X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC10941LOK-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/23/2024
 Supervised By :Ankita Jodhani 05/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 02:10:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 21 18:19:41 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.469	3.753	2339514	2887920	1.482	1.902 #
2) SA Decachlor...	10.208	8.828	2616725	2278989	2.012	1.729m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052224\
Data File : PP065181.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2024 00:37
Operator : YP\AJ
Sample : P2559-02 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
BC10941LOK-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/23/2024
Supervised By :Ankita Jodhani 05/23/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 02:10:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052124.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 21 18:19:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

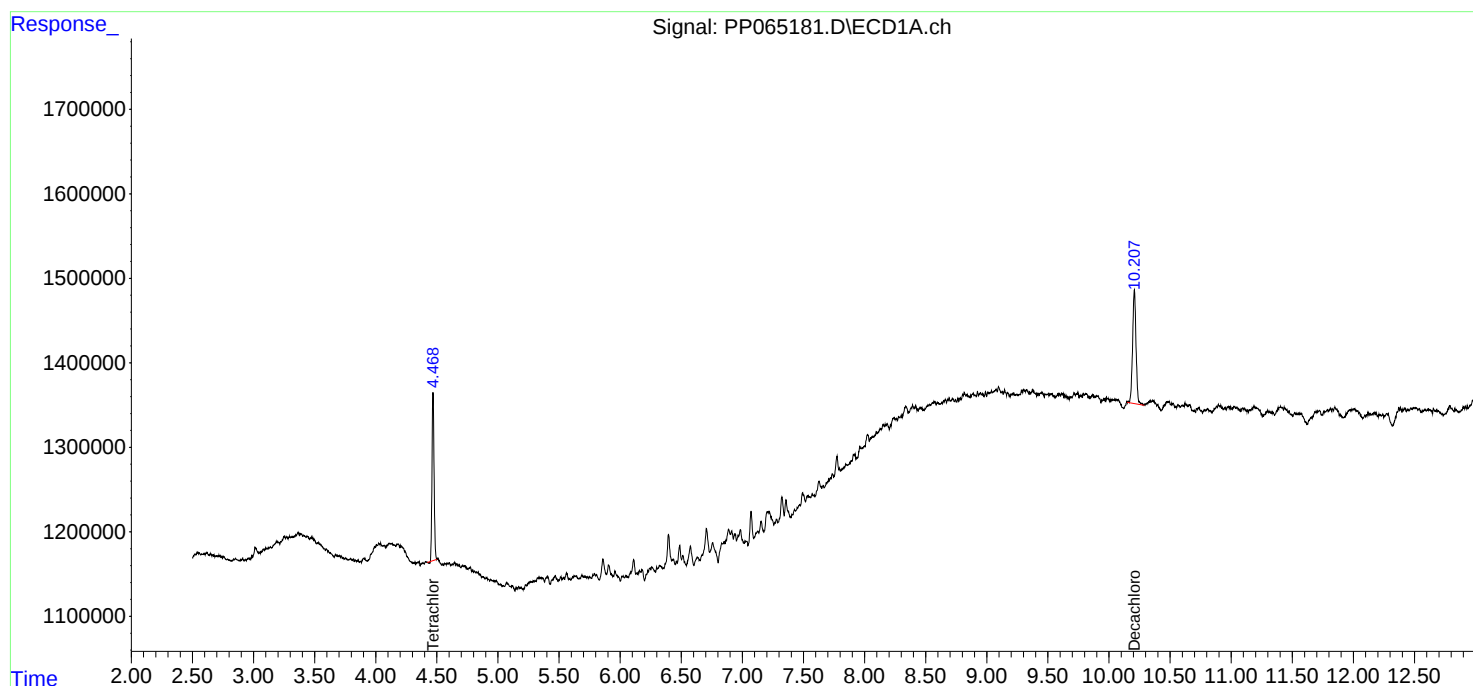

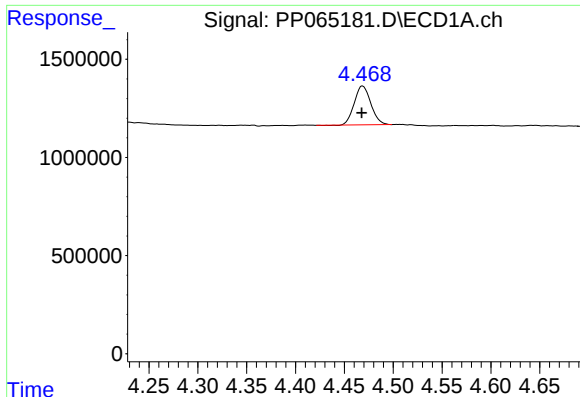


#1 Tetrachloro-m-xylene

R.T.: 4.469 min
Delta R.T.: 0.000 min
Response: 2339514
Conc: 1.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC10941LOK-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/23/2024
Supervised By :Ankita Jodhani 05/23/2024

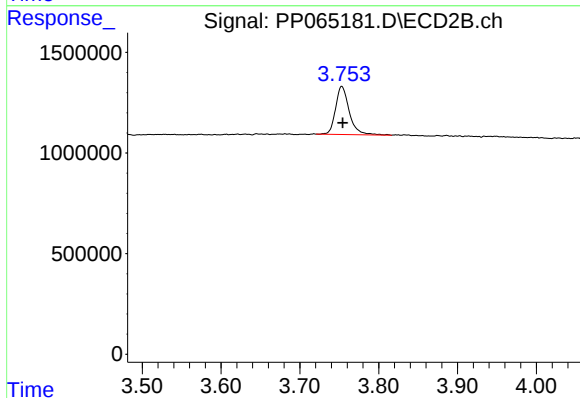


#1 Tetrachloro-m-xylene

R.T.: 3.753 min
Delta R.T.: -0.001 min
Response: 2887920
Conc: 1.90 ng/ml

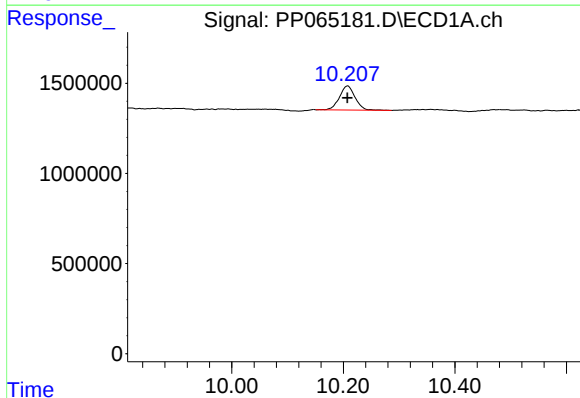

#2 Decachlorobiphenyl

R.T.: 10.208 min
Delta R.T.: 0.000 min
Response: 2616725
Conc: 2.01 ng/ml

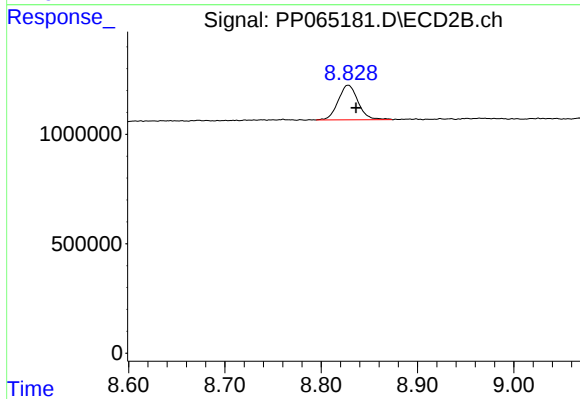

#2 Decachlorobiphenyl

R.T.: 8.828 min
Delta R.T.: -0.008 min
Response: 2278989
Conc: 1.73 ng/ml m