

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052322\
 Data File : PP047887.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2022 11:02
 Operator : YP\AJ
 Sample : N2942-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RATZER-RD-SP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/24/2022
 Supervised By :Ankita Jodhani 05/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 11:24:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 23 09:44:20 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.840	3.109	53832606	70365332	20.351m	19.952
2) SA Decachlor...	9.888	8.401	35564696	59226316	23.481	20.323m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052322\
Data File : PP047887.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2022 11:02
Operator : YP\AJ
Sample : N2942-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
RATZER-RD-SP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/24/2022
Supervised By :Ankita Jodhani 05/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 11:24:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051022.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 23 09:44:20 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

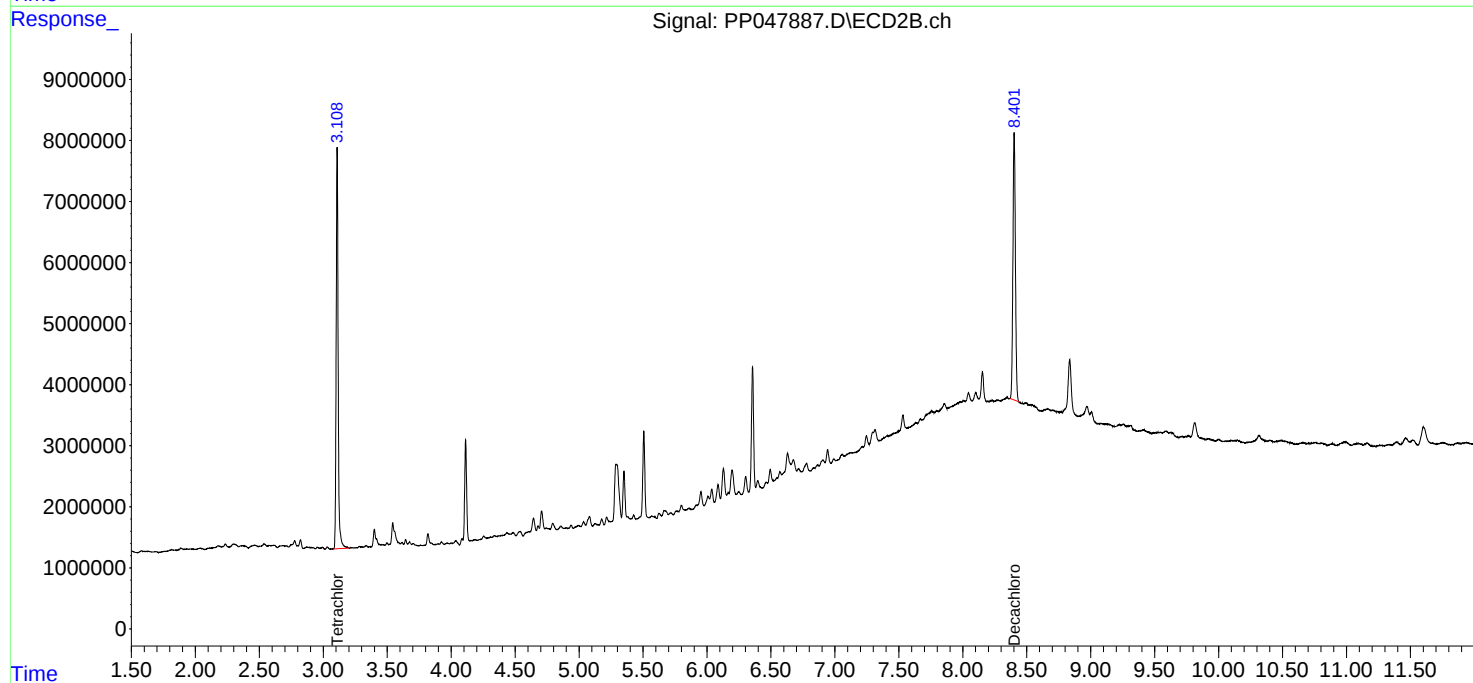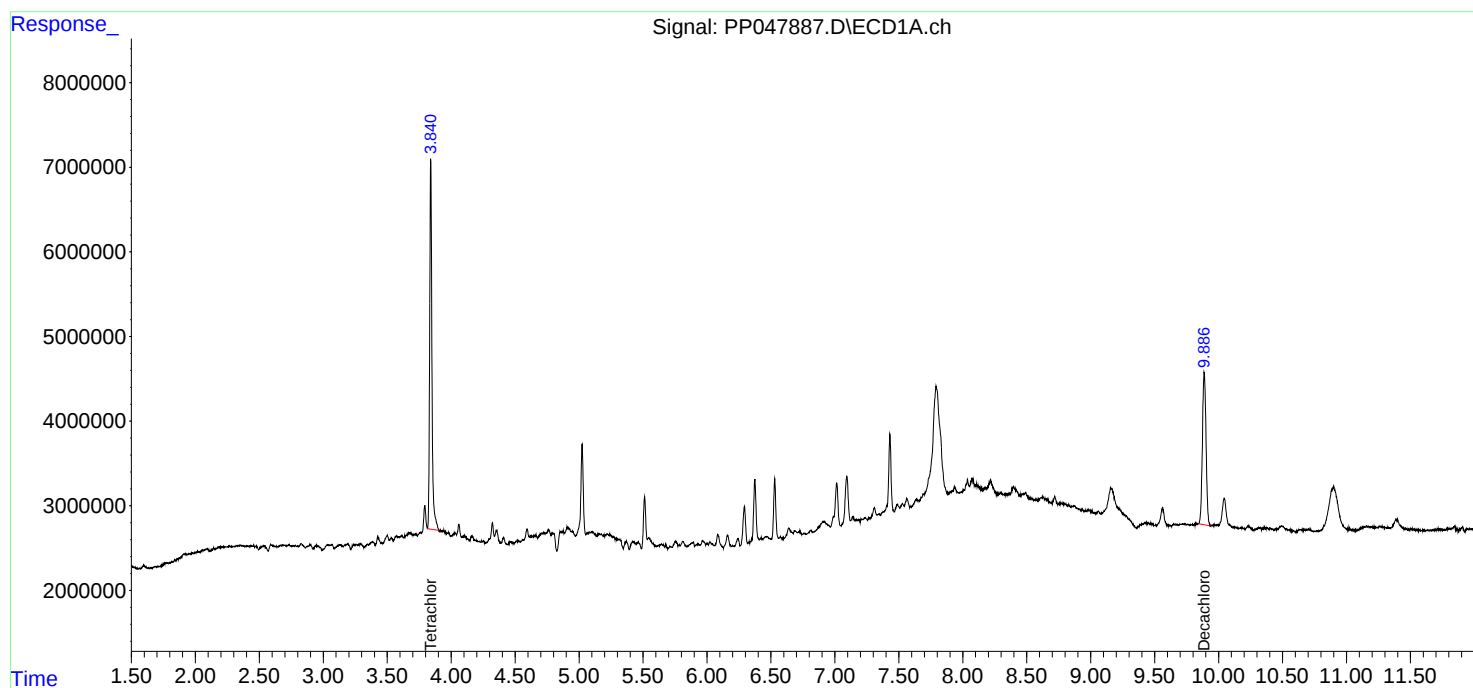

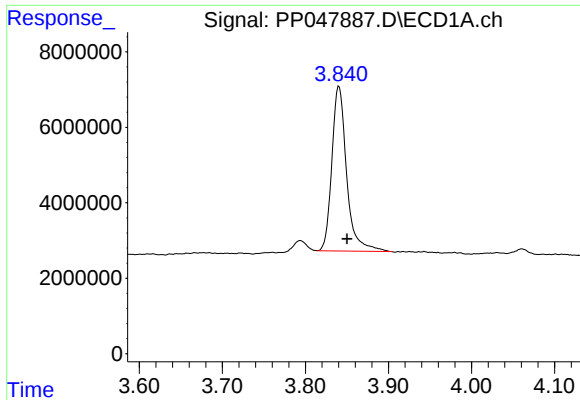


#1 Tetrachloro-m-xylene

R.T.: 3.840 min
Delta R.T.: -0.010 min
Response: 53832606
Conc: 20.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
RATZER-RD-SP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/24/2022
Supervised By :Ankita Jodhani 05/25/2022

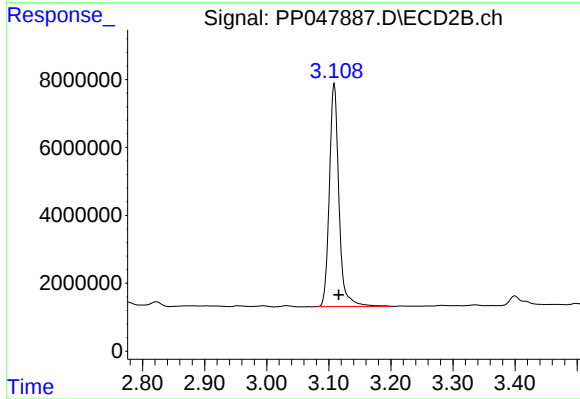


#1 Tetrachloro-m-xylene

R.T.: 3.109 min
Delta R.T.: -0.007 min
Response: 70365332
Conc: 19.95 ng/ml

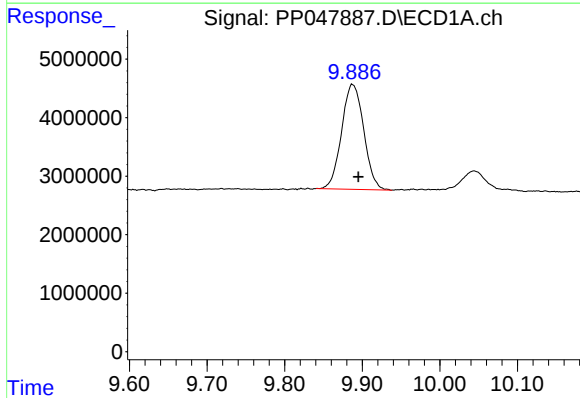

#2 Decachlorobiphenyl

R.T.: 9.888 min
Delta R.T.: -0.007 min
Response: 35564696
Conc: 23.48 ng/ml

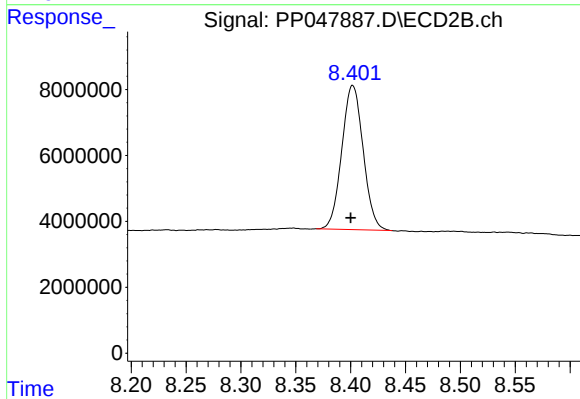

#2 Decachlorobiphenyl

R.T.: 8.401 min
Delta R.T.: 0.001 min
Response: 59226316
Conc: 20.32 ng/ml m