

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052325\
 Data File : PP072317.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2025 14:55
 Operator : YP\AJ
 Sample : Q2111-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 34899

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/27/2025
 Supervised By :mohammad ahmed 05/28/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 22:33:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 20 03:29:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.504	3.799	35218439	24437166	17.515m	15.289m
2) SA Decachlor...	10.238	8.845	18819854	12799064	11.552	12.091

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052325\
Data File : PP072317.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2025 14:55
Operator : YP\AJ
Sample : Q2111-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
34899


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/27/2025
Supervised By :mohammad ahmed 05/28/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 22:33:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 20 03:29:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

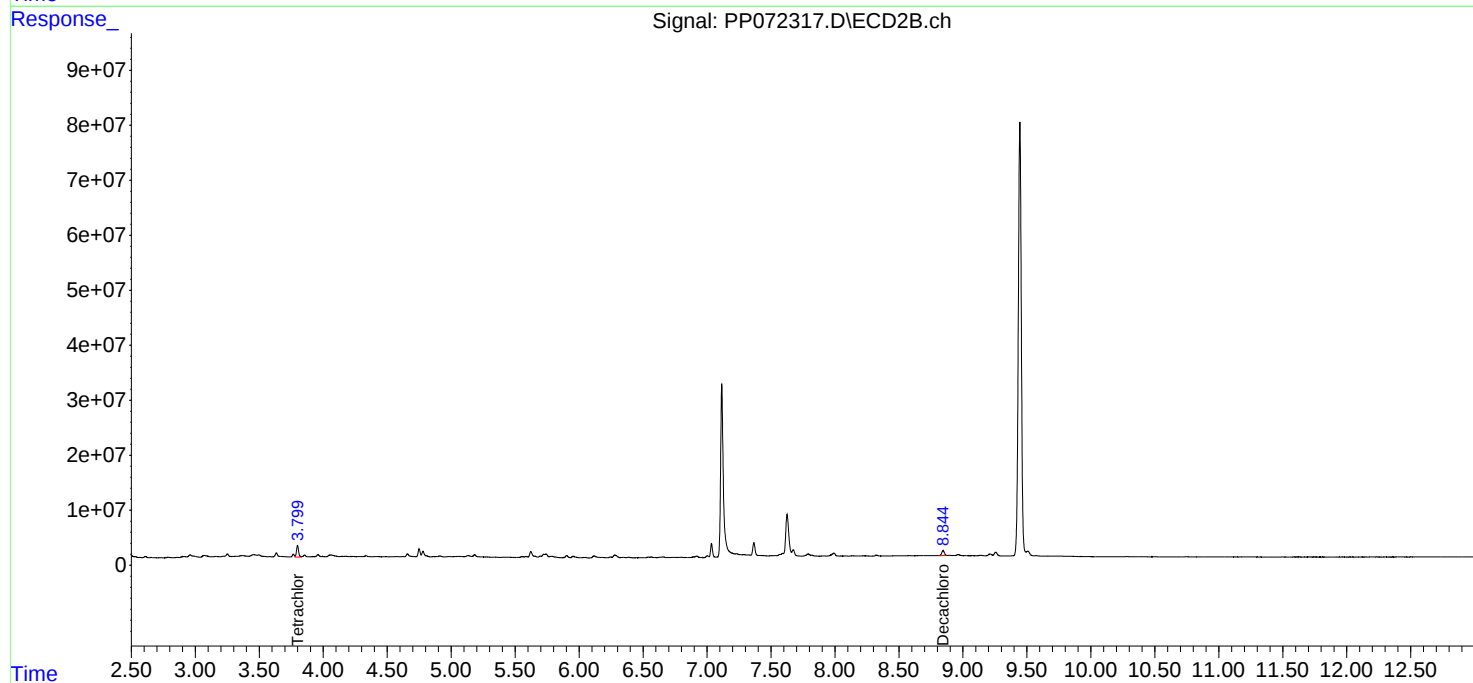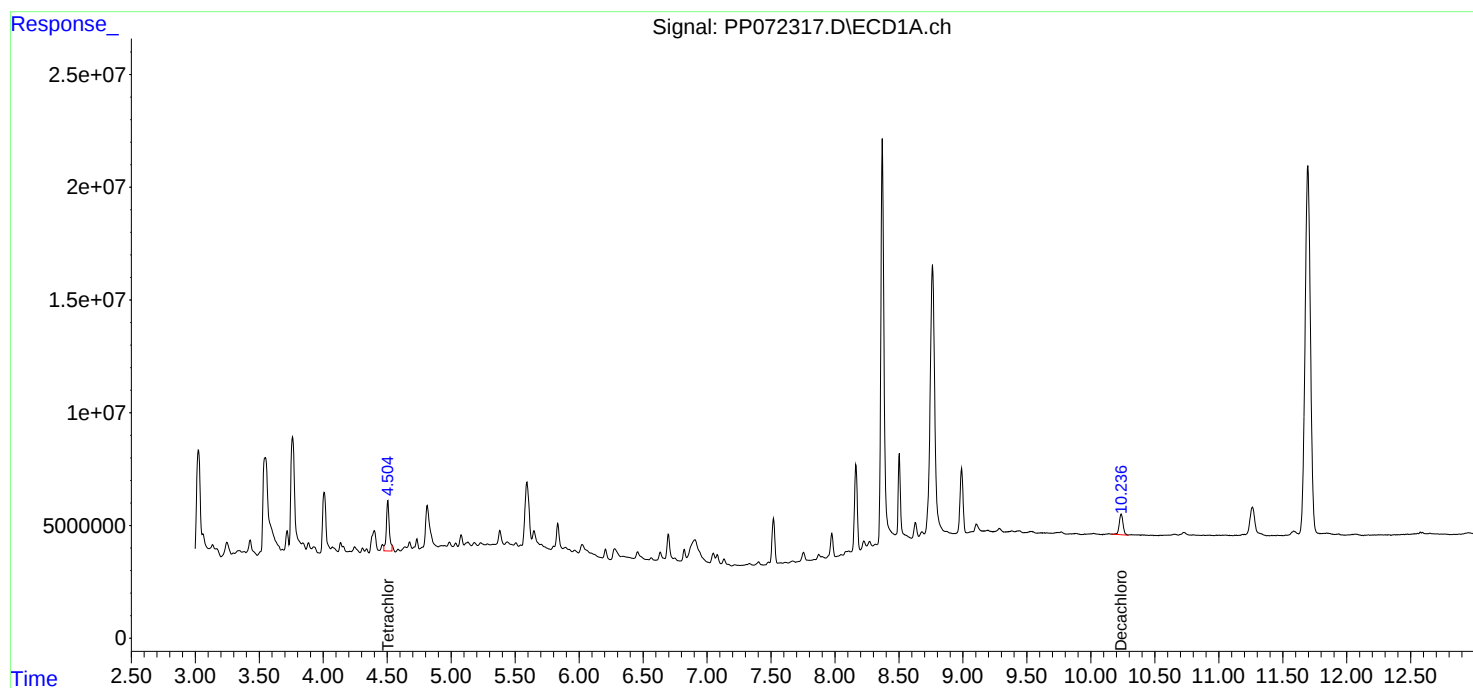

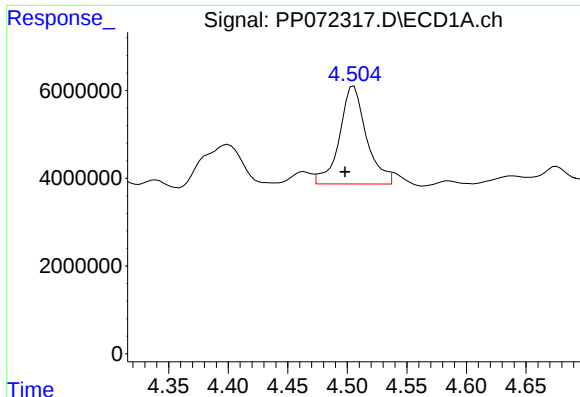


#1 Tetrachloro-m-xylene

R.T.: 4.504 min
Delta R.T.: 0.006 min
Response: 35218439
Conc: 17.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
34899


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/27/2025
Supervised By :mohammad ahmed 05/28/2025

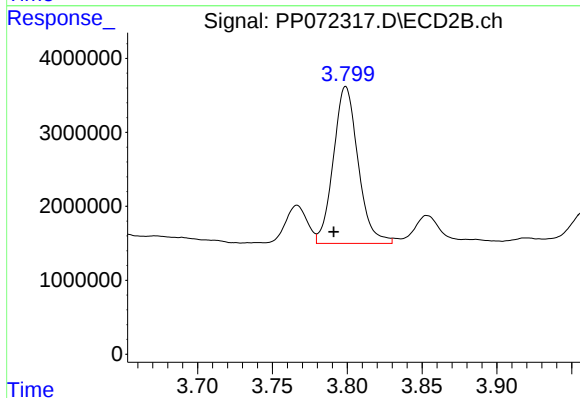


#1 Tetrachloro-m-xylene

R.T.: 3.799 min
Delta R.T.: 0.008 min
Response: 24437166
Conc: 15.29 ng/ml m

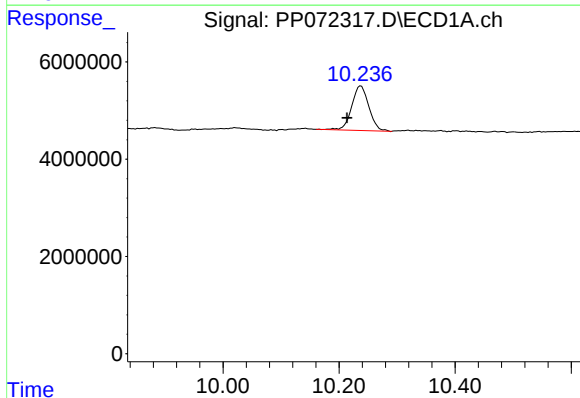

#2 Decachlorobiphenyl

R.T.: 10.238 min
Delta R.T.: 0.024 min
Response: 18819854
Conc: 11.55 ng/ml

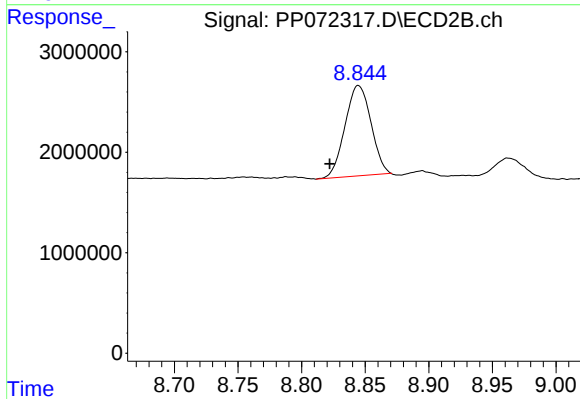

#2 Decachlorobiphenyl

R.T.: 8.845 min
Delta R.T.: 0.023 min
Response: 12799064
Conc: 12.09 ng/ml