

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052325\
 Data File : PP072333.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2025 20:22
 Operator : YP\AJ
 Sample : Q2110-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 60458

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/27/2025
 Supervised By :mohammad ahmed 05/28/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 22:39:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 20 03:29:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.498	3.796	17189861	14933222	8.549m	9.343m
2) SA Decachlor...	10.204	8.817	4694304	3775268	2.881	3.566

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052325\
Data File : PP072333.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2025 20:22
Operator : YP\AJ
Sample : Q2110-02
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
60458


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/27/2025
Supervised By :mohammad ahmed 05/28/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 22:39:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP051925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 20 03:29:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

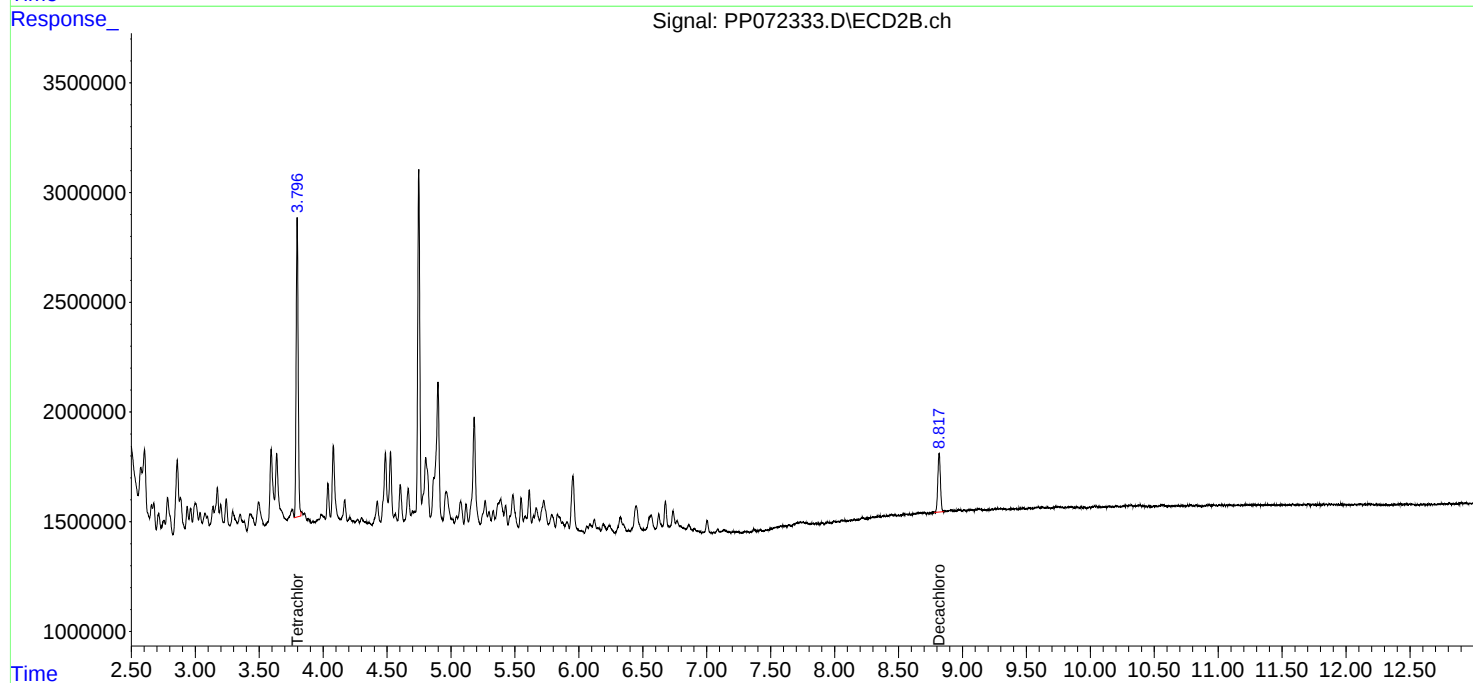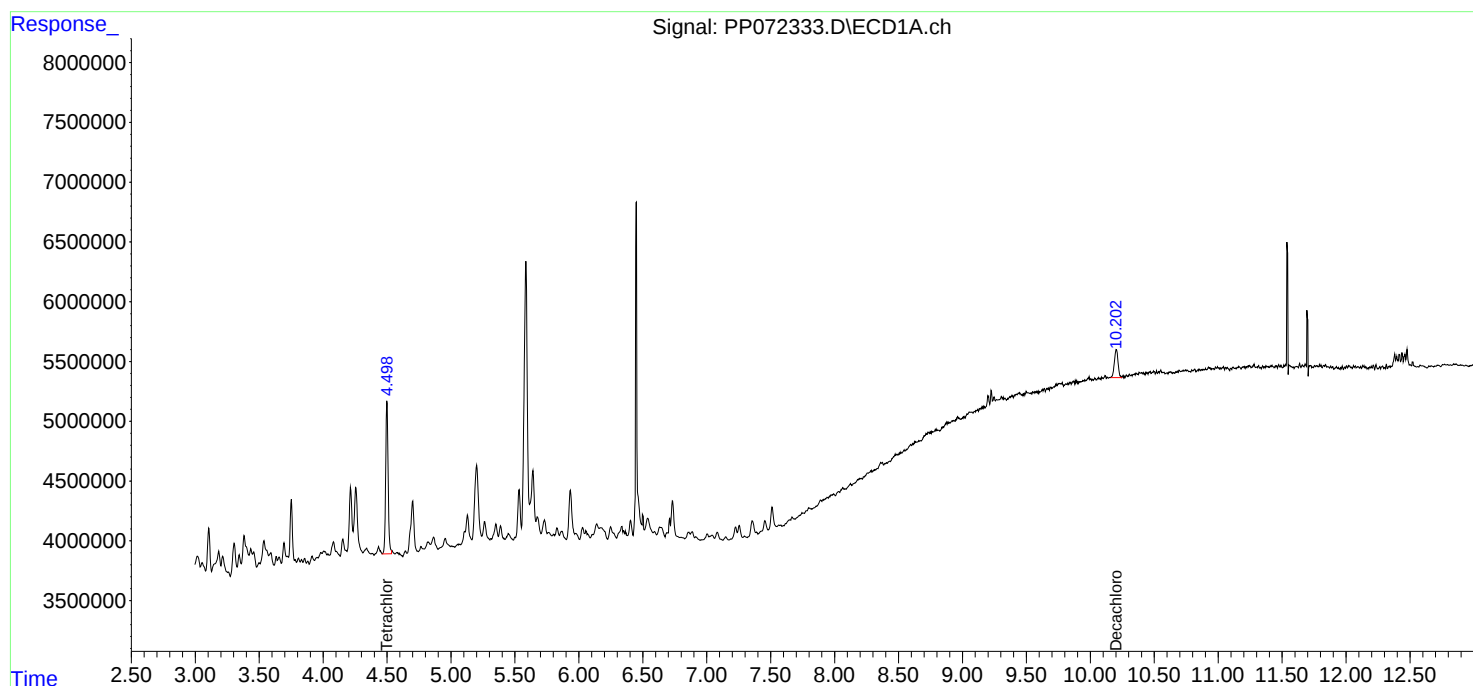

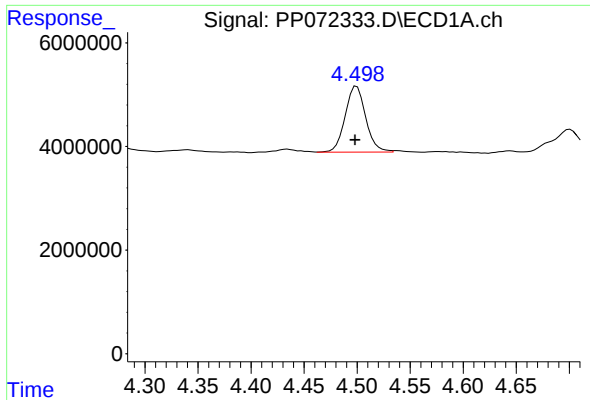


#1 Tetrachloro-m-xylene

R.T.: 4.498 min
Delta R.T.: 0.000 min
Response: 17189861
Conc: 8.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
60458


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/27/2025
Supervised By :mohammad ahmed 05/28/2025

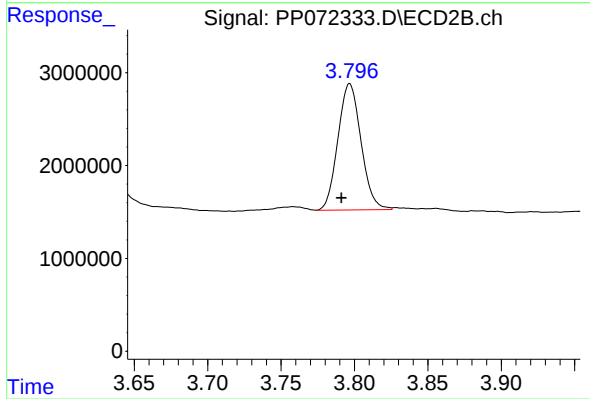


#1 Tetrachloro-m-xylene

R.T.: 3.796 min
Delta R.T.: 0.005 min
Response: 14933222
Conc: 9.34 ng/ml m

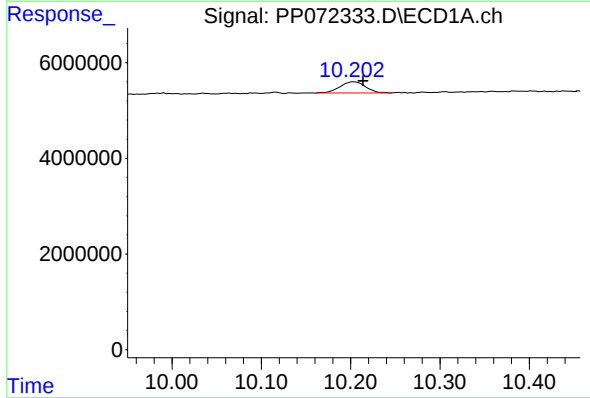

#2 Decachlorobiphenyl

R.T.: 10.204 min
Delta R.T.: -0.010 min
Response: 4694304
Conc: 2.88 ng/ml

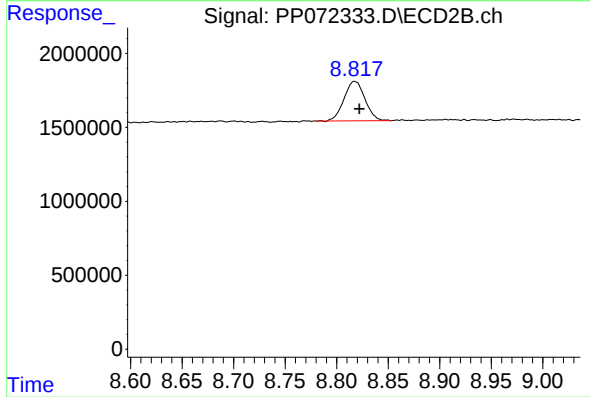

#2 Decachlorobiphenyl

R.T.: 8.817 min
Delta R.T.: -0.005 min
Response: 3775268
Conc: 3.57 ng/ml