

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052423\
 Data File : PP057843.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2023 16:07
 Operator : YP\AJ
 Sample : 02899-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/25/2023
 Supervised By :Ankita Jodhani 05/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 02:26:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 08 19:18:05 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.383	3.621	52397797	51942124	23.884	22.899
2) SA Decachlor...	10.210	8.682	31833822	30359718	28.091	19.341 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052423\
Data File : PP057843.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2023 16:07
Operator : YP\AJ
Sample : 02899-04
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/25/2023
Supervised By :Ankita Jodhani 05/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 02:26:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050823.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 08 19:18:05 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

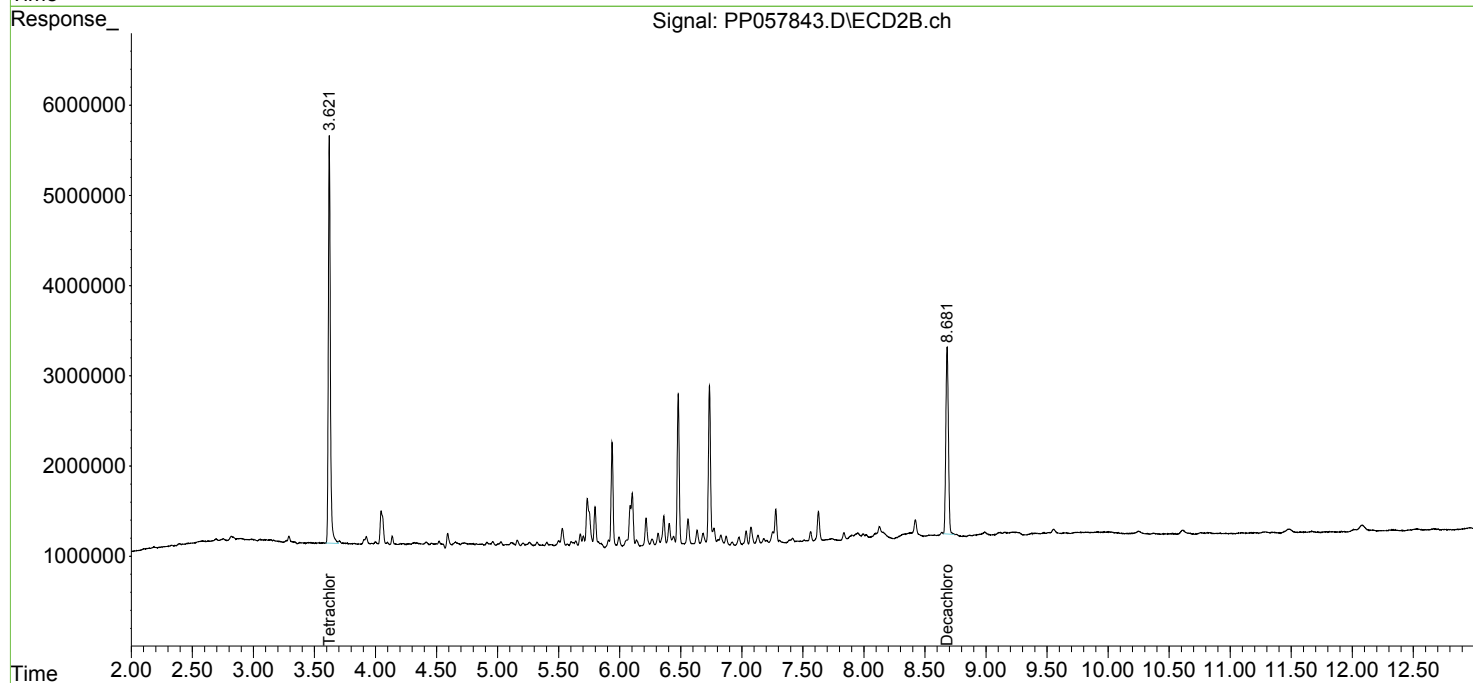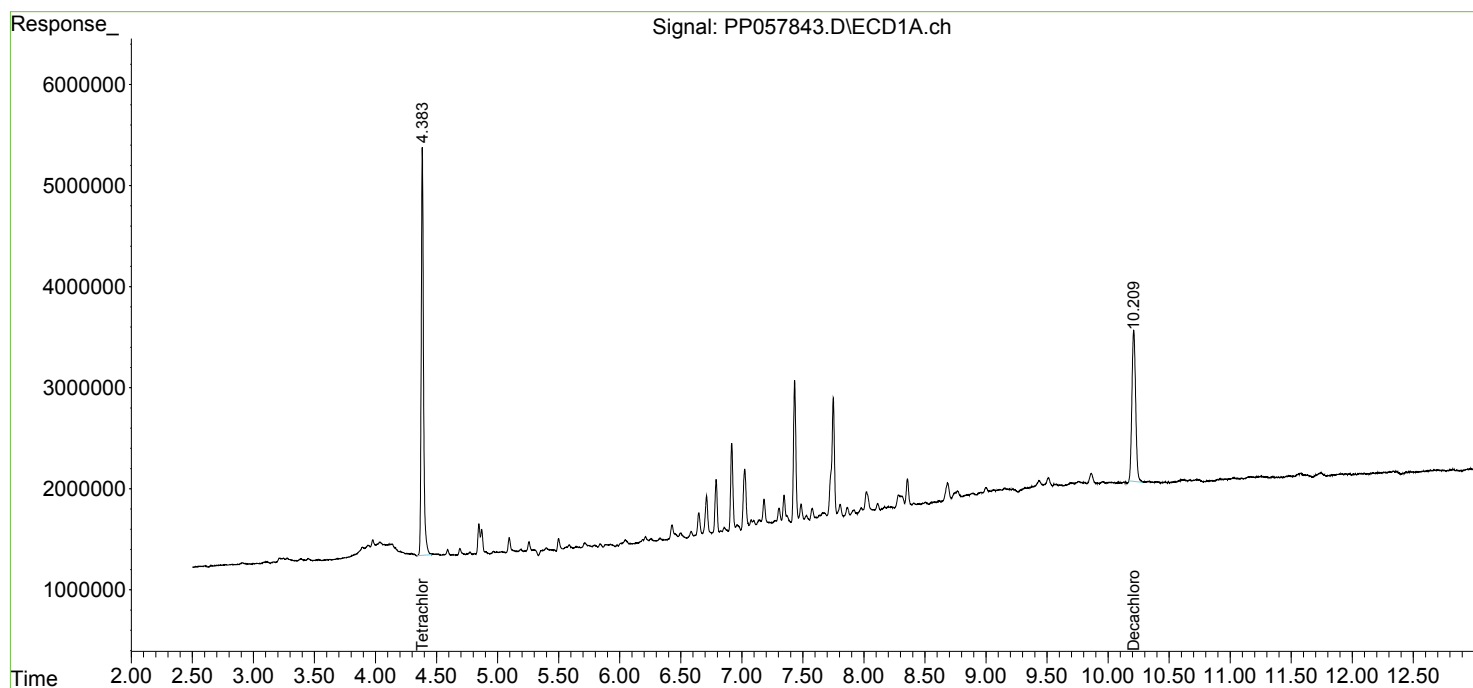

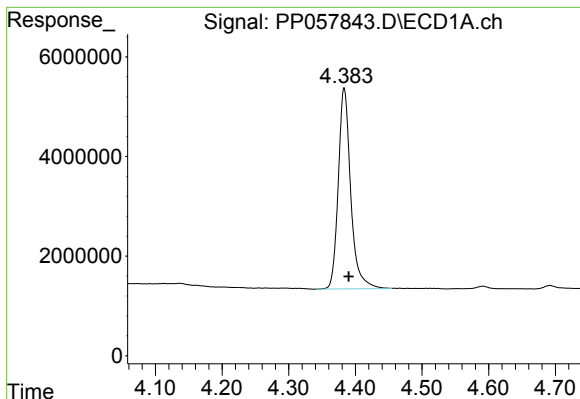

#1 Tetrachloro-m-xylene

R.T.: 4.383 min
Delta R.T.: -0.007 min
Response: 52397797
Conc: 23.88 ng/ml

Instrument :

ECD_P


ClientSampleId :

SB01

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 05/25/2023
Supervised By :Ankita Jodhani 05/25/2023

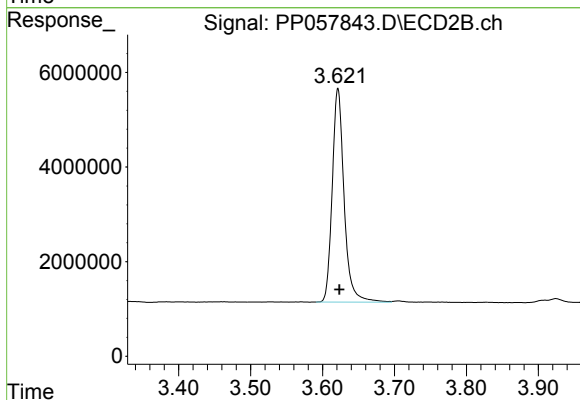


#1 Tetrachloro-m-xylene

R.T.: 3.621 min
Delta R.T.: -0.002 min
Response: 51942124
Conc: 22.90 ng/ml

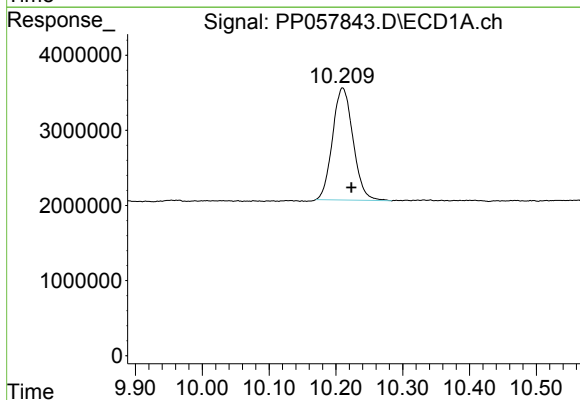

#2 Decachlorobiphenyl

R.T.: 10.210 min
Delta R.T.: -0.013 min
Response: 31833822
Conc: 28.09 ng/ml

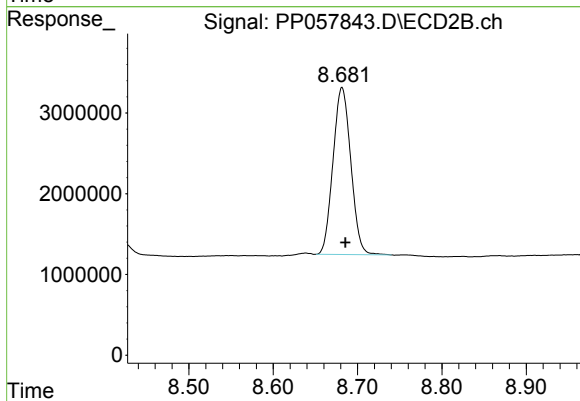

#2 Decachlorobiphenyl

R.T.: 8.682 min
Delta R.T.: -0.004 min
Response: 30359718
Conc: 19.34 ng/ml