

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP052423\  
 Data File : PP057867.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 25 May 2023 01:24  
 Operator : YP\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 25 05:50:59 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP050823.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Mon May 08 19:18:05 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound        | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|--------|-------|----------|----------|--------|--------|
| -----                       |                 |        |       |          |          |        |        |
| System Monitoring Compounds |                 |        |       |          |          |        |        |
| 1)                          | SA Tetrachlo... | 4.383  | 3.621 | 44503652 | 45451987 | 20.286 | 20.038 |
| 2)                          | SA Decachlor... | 10.207 | 8.679 | 24748206 | 27691708 | 21.838 | 17.641 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP052423\  
Data File : PP057867.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 25 May 2023 01:24  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 25 05:50:59 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP050823.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Mon May 08 19:18:05 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

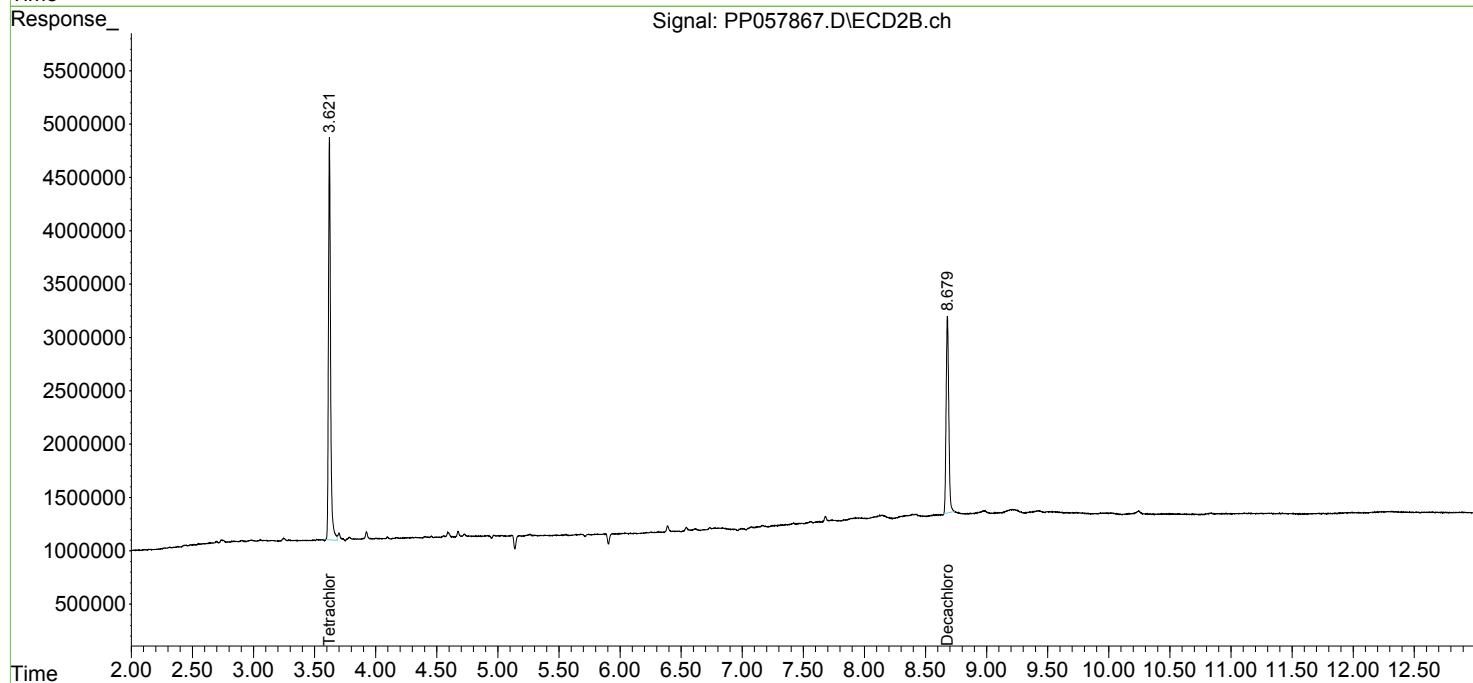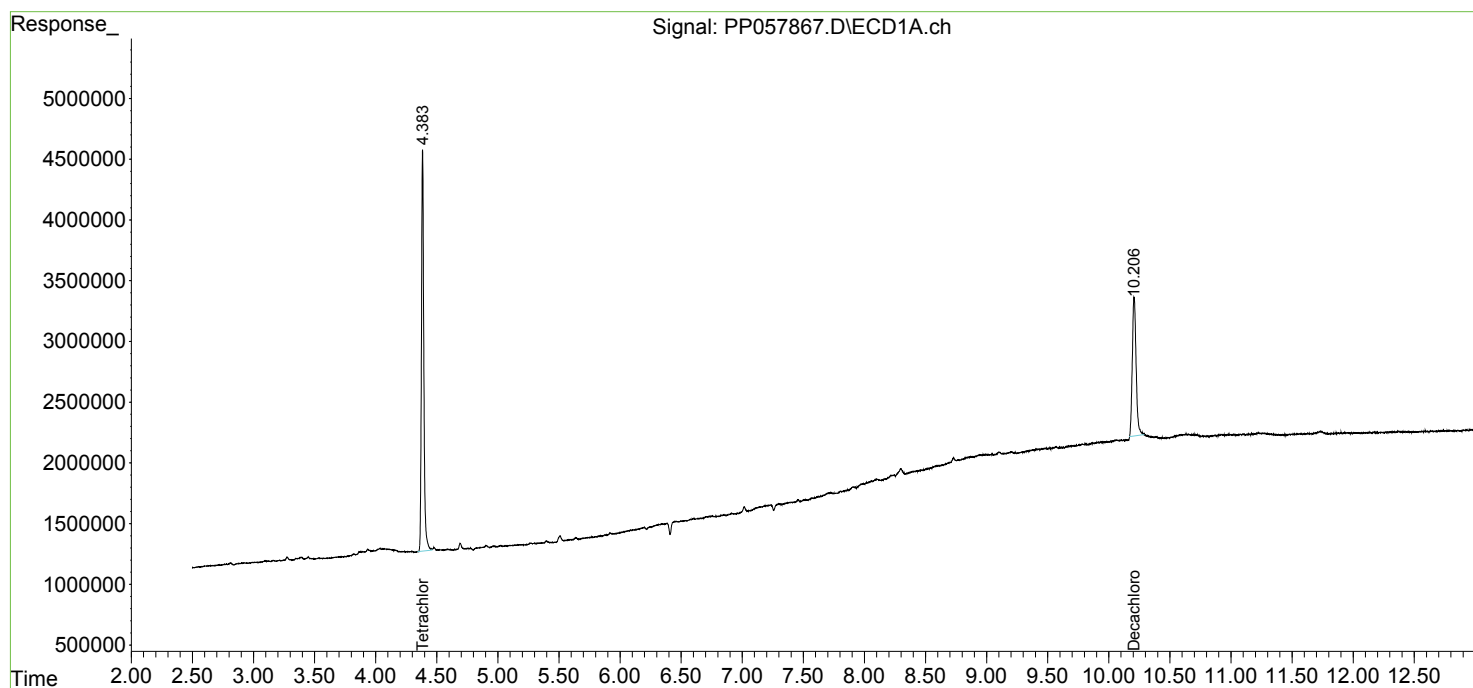


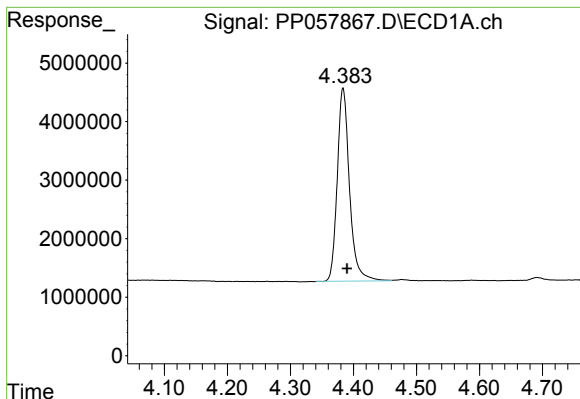

#1 Tetrachloro-m-xylene


R.T.: 4.383 min  
Delta R.T.: -0.007 min  
Response: 44503652  
Conc: 20.29 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
I.BLK

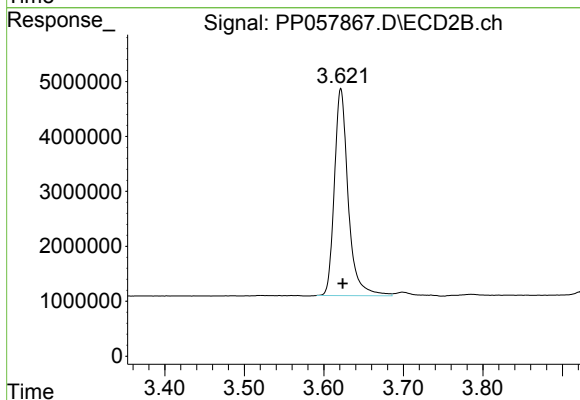


#1 Tetrachloro-m-xylene

R.T.: 3.621 min  
Delta R.T.: -0.002 min  
Response: 45451987  
Conc: 20.04 ng/ml

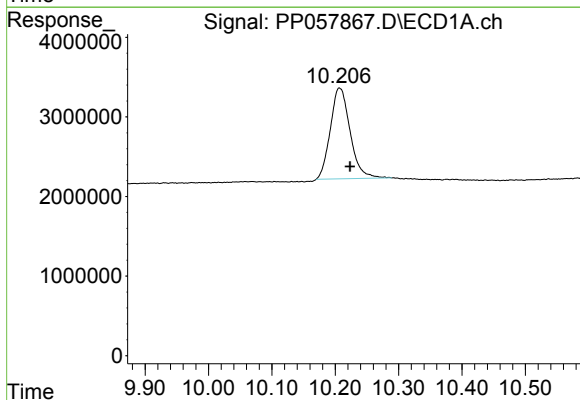

#2 Decachlorobiphenyl

R.T.: 10.207 min  
Delta R.T.: -0.017 min  
Response: 24748206  
Conc: 21.84 ng/ml

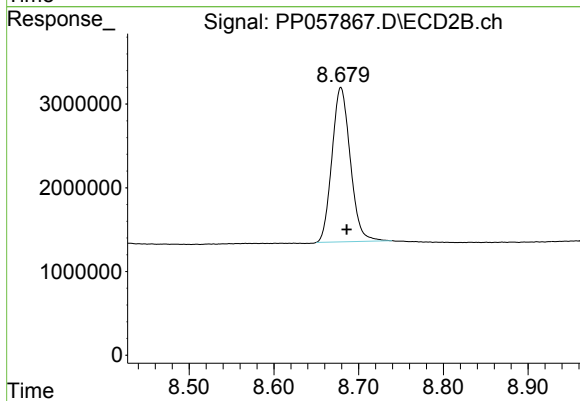

#2 Decachlorobiphenyl

R.T.: 8.679 min  
Delta R.T.: -0.007 min  
Response: 27691708  
Conc: 17.64 ng/ml