

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052522\
 Data File : PP048036.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2022 17:53
 Operator : YP\AJ
 Sample : N3024-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 31532-34-SOL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/26/2022
 Supervised By :Ankita Jodhani 05/26/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 01:39:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052522.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 25 14:26:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.830	3.099	29158209	50843054	12.954m	18.561 #
2) SA Decachlor...	9.871	8.387	18478588	30758184	13.885	12.019

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052522\
Data File : PP048036.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2022 17:53
Operator : YP\AJ
Sample : N3024-02
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
31532-34-SOL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 01:39:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052522.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 25 14:26:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

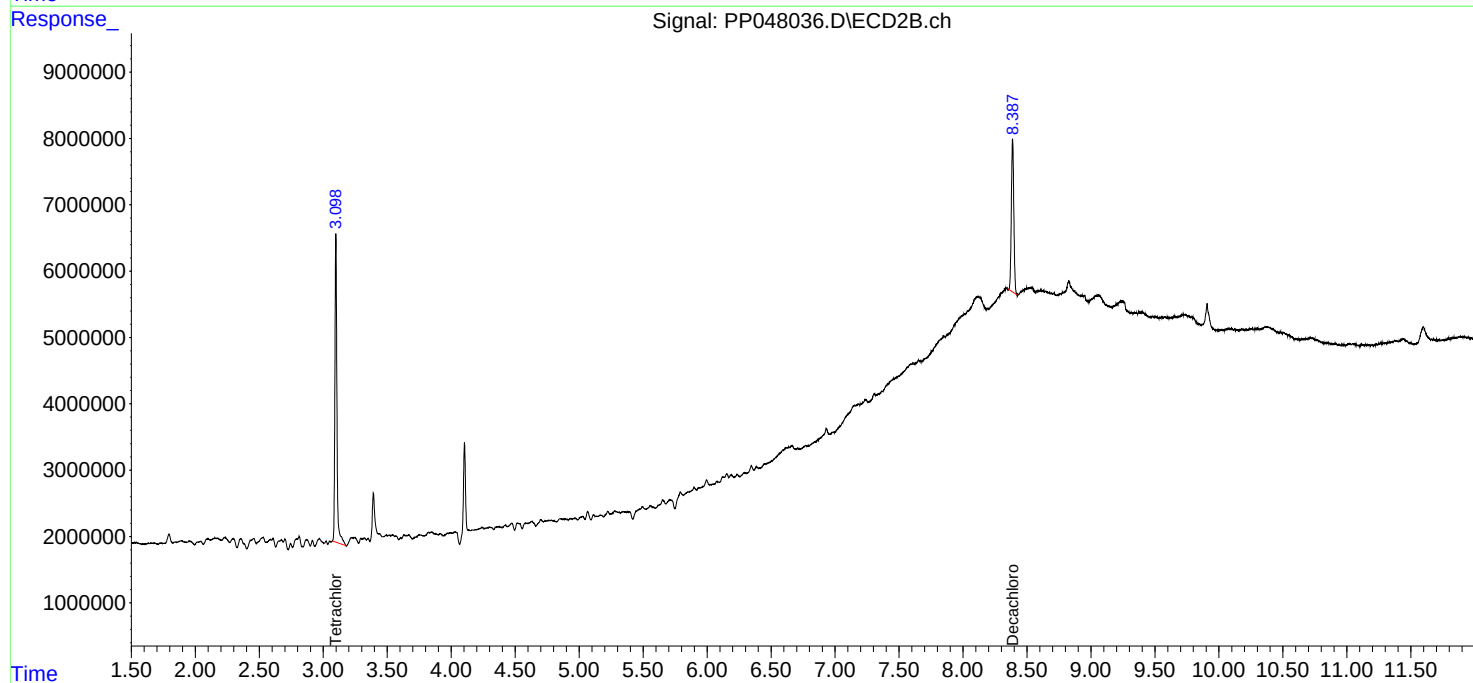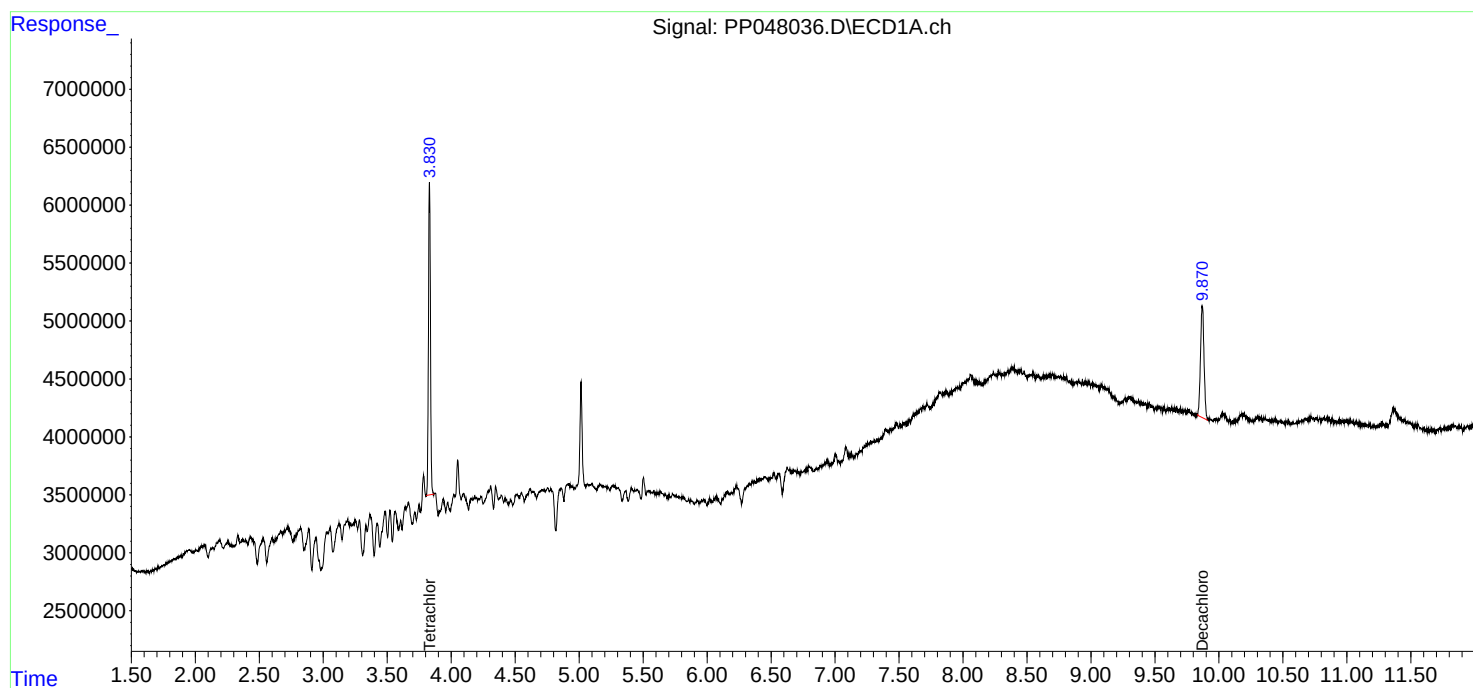

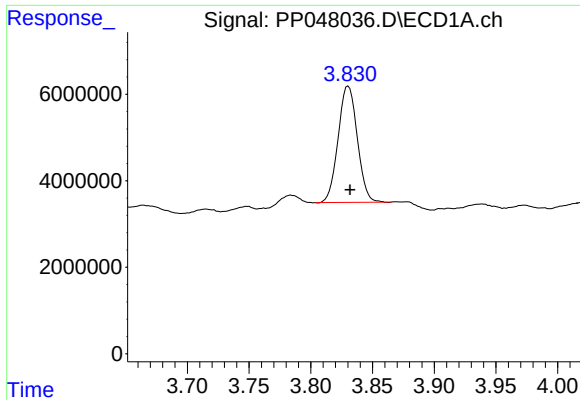


#1 Tetrachloro-m-xylene

R.T.: 3.830 min
Delta R.T.: -0.002 min
Response: 29158209
Conc: 12.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
31532-34-SOL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

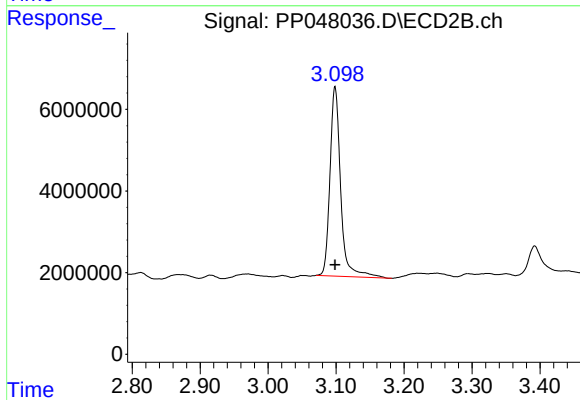


#1 Tetrachloro-m-xylene

R.T.: 3.099 min
Delta R.T.: 0.000 min
Response: 50843054
Conc: 18.56 ng/ml

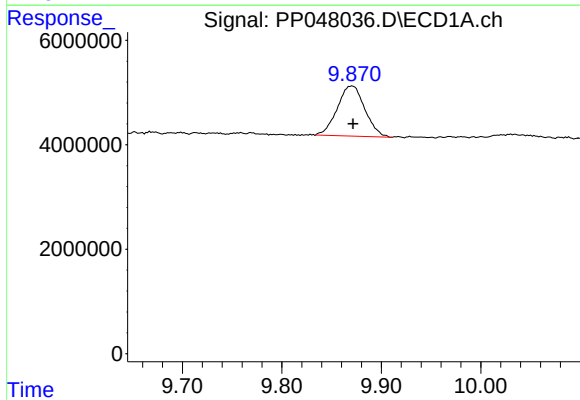

#2 Decachlorobiphenyl

R.T.: 9.871 min
Delta R.T.: 0.000 min
Response: 18478588
Conc: 13.89 ng/ml

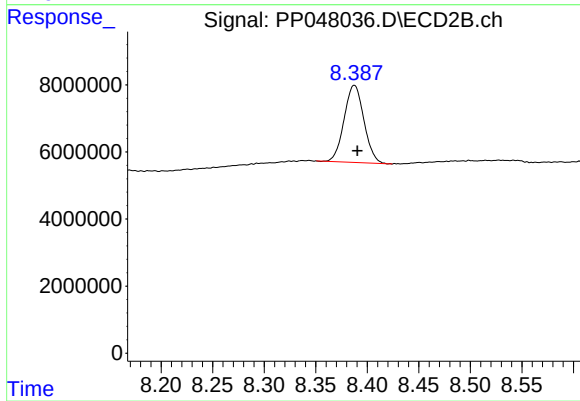

#2 Decachlorobiphenyl

R.T.: 8.387 min
Delta R.T.: -0.003 min
Response: 30758184
Conc: 12.02 ng/ml