

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052523\
 Data File : PP057920.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2023 17:16
 Operator : YP\AJ
 Sample : 02931-01 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEE103S-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/26/2023
 Supervised By :Ankita Jodhani 05/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 21:25:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 08 19:18:05 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.382	3.620	5476887	5505536	2.496	2.427
2) SA Decachlor...	10.206	8.680	3986920	3699642	3.518	2.357 #
Target Compounds						
26) L6 AR-1254-1	6.424	5.527	2280814	3169023	33.982	28.381
27) L6 AR-1254-2	6.646	5.675	3114595	2716944	32.924	27.223
28) L6 AR-1254-3	7.014	6.083	2857081	3284089	31.366	20.991 #
29) L6 AR-1254-4	7.302	6.313	1734144	1653829	29.115	17.927 #
30) L6 AR-1254-5	7.726	6.734	1382542	2340895	20.138m	16.171

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052523\
Data File : PP057920.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2023 17:16
Operator : YP\AJ
Sample : 02931-01 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HEE103S-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2023
Supervised By :Ankita Jodhani 05/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 21:25:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050823.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 08 19:18:05 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

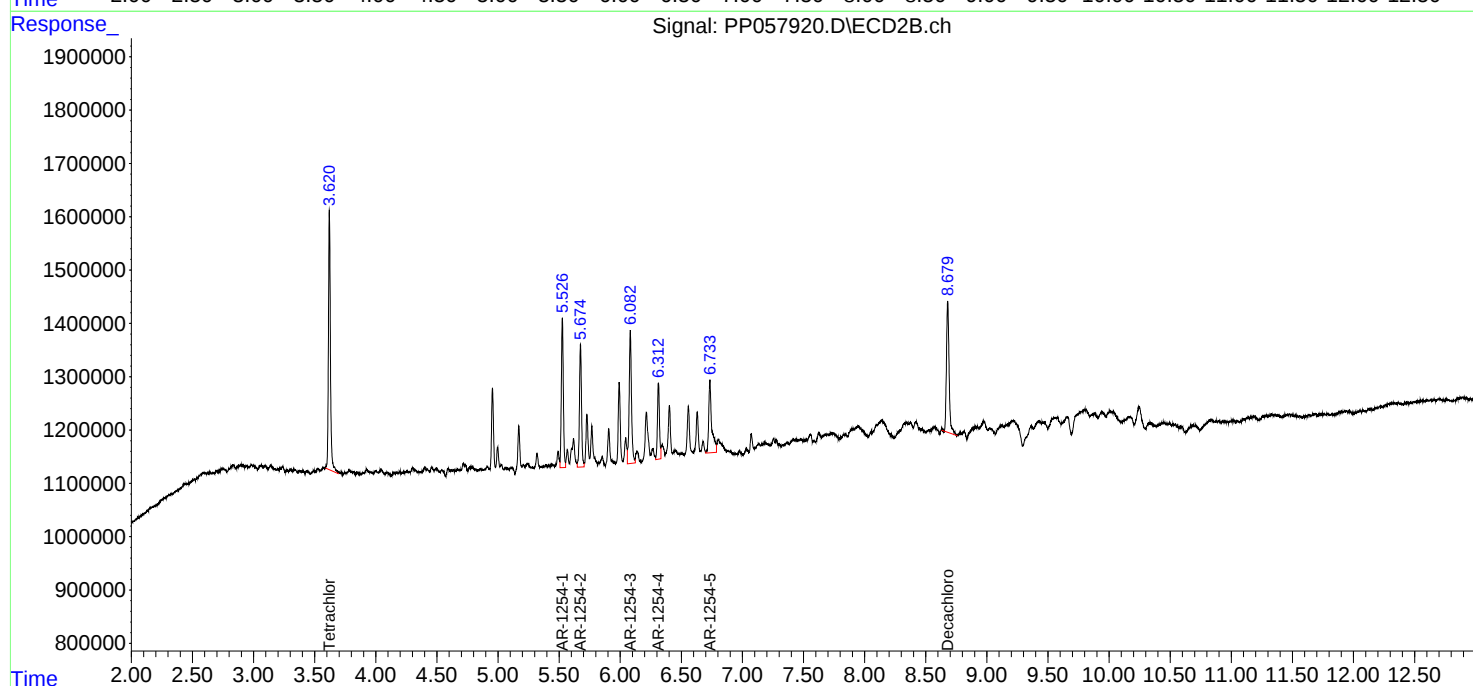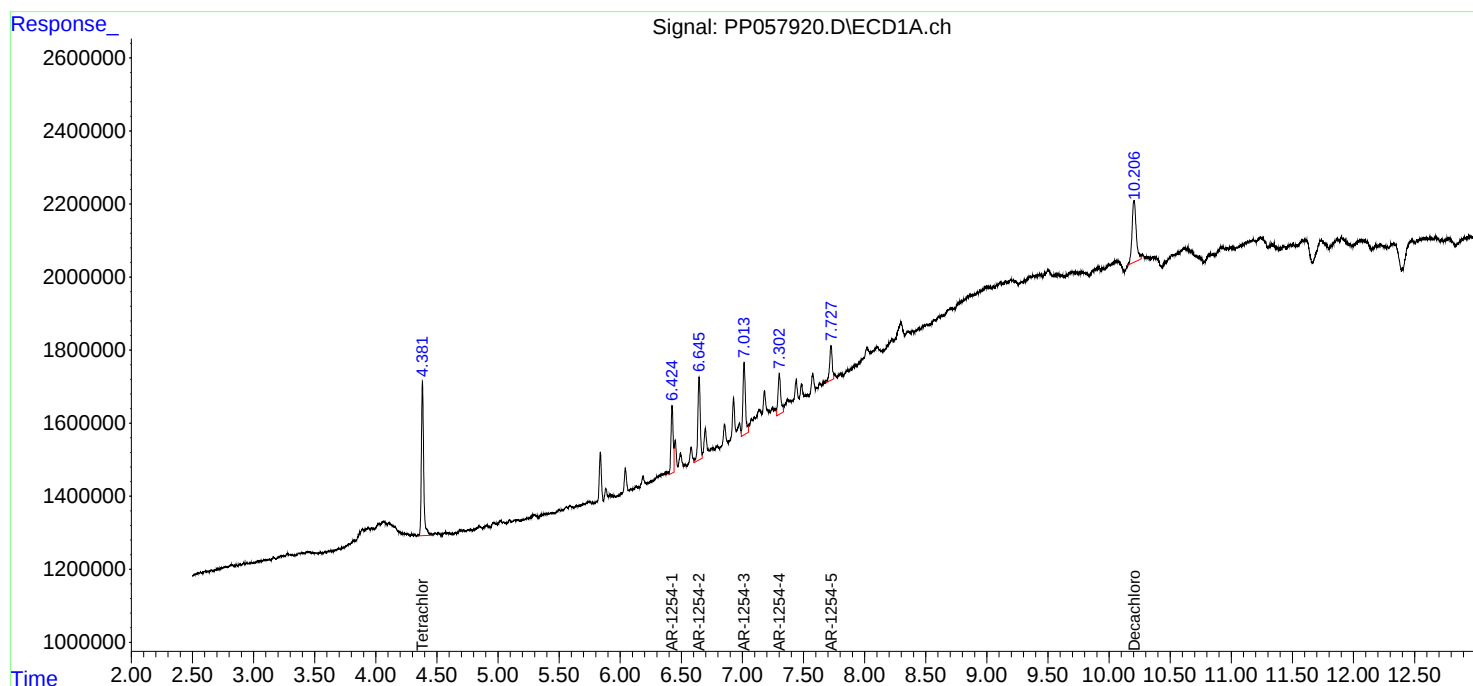

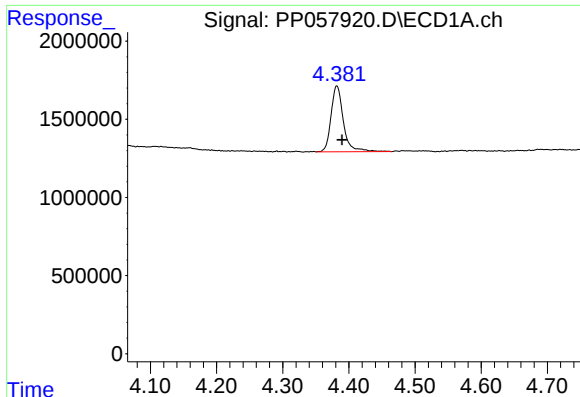


#1 Tetrachloro-m-xylene

R.T.: 4.382 min
Delta R.T.: -0.008 min
Response: 5476887
Conc: 2.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEE103S-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2023
Supervised By :Ankita Jodhani 05/26/2023

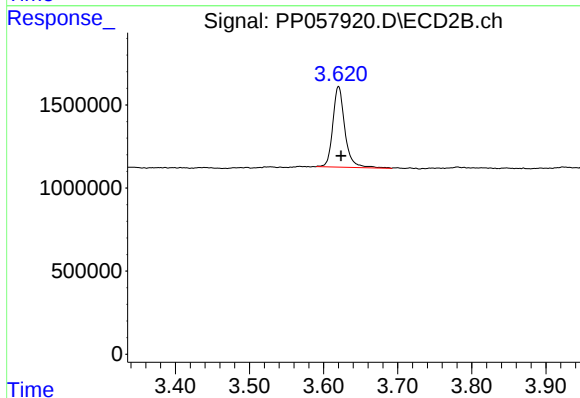


#1 Tetrachloro-m-xylene

R.T.: 3.620 min
Delta R.T.: -0.003 min
Response: 5505536
Conc: 2.43 ng/ml

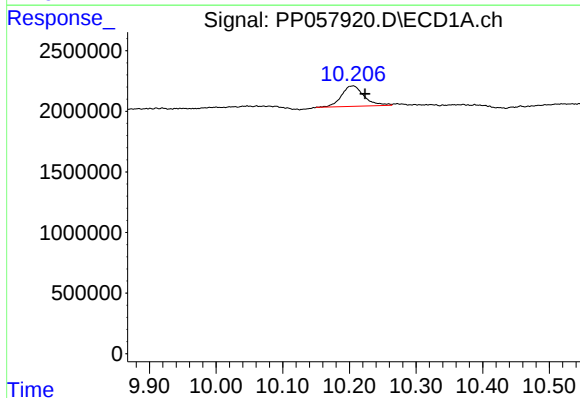


#2 Decachlorobiphenyl

R.T.: 10.206 min
Delta R.T.: -0.018 min
Response: 3986920
Conc: 3.52 ng/ml

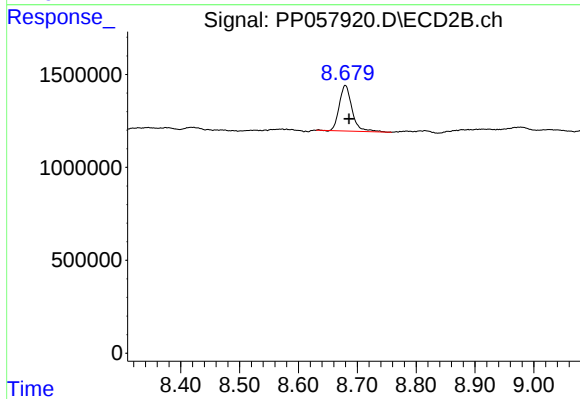

#2 Decachlorobiphenyl

R.T.: 8.680 min
Delta R.T.: -0.006 min
Response: 3699642
Conc: 2.36 ng/ml

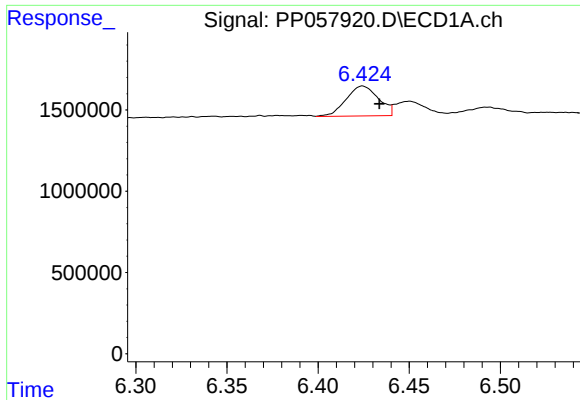


#26 AR-1254-1

R.T.: 6.424 min
Delta R.T.: -0.009 min
Response: 2280814
Conc: 33.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEE103S-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2023
Supervised By :Ankita Jodhani 05/26/2023

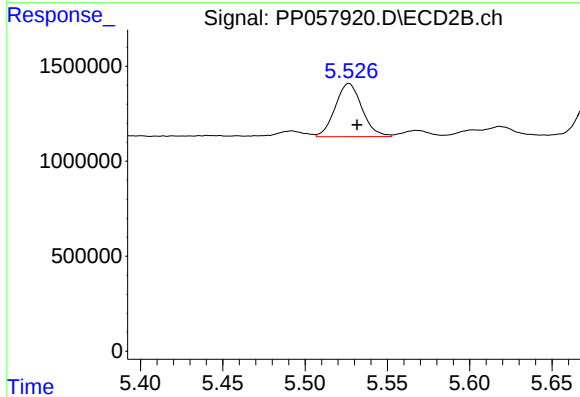


#26 AR-1254-1

R.T.: 5.527 min
Delta R.T.: -0.005 min
Response: 3169023
Conc: 28.38 ng/ml

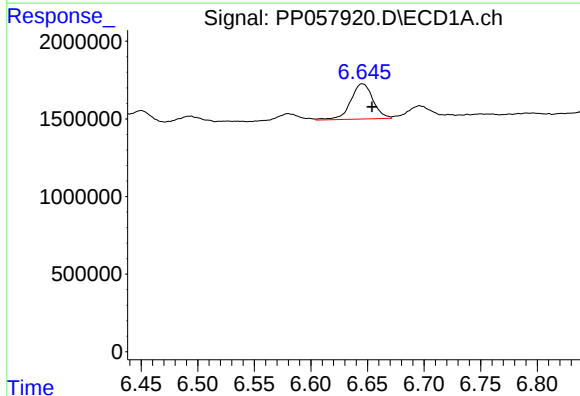


#27 AR-1254-2

R.T.: 6.646 min
Delta R.T.: -0.008 min
Response: 3114595
Conc: 32.92 ng/ml

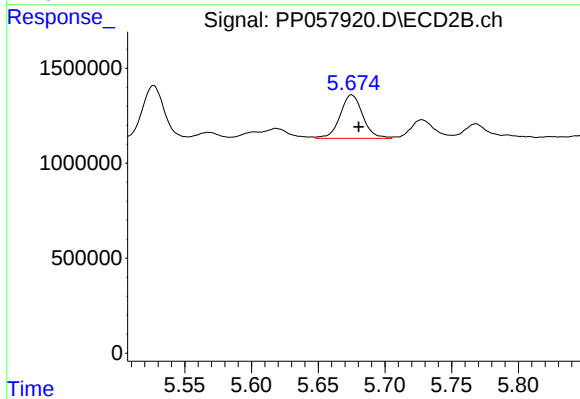

#27 AR-1254-2

R.T.: 5.675 min
Delta R.T.: -0.005 min
Response: 2716944
Conc: 27.22 ng/ml

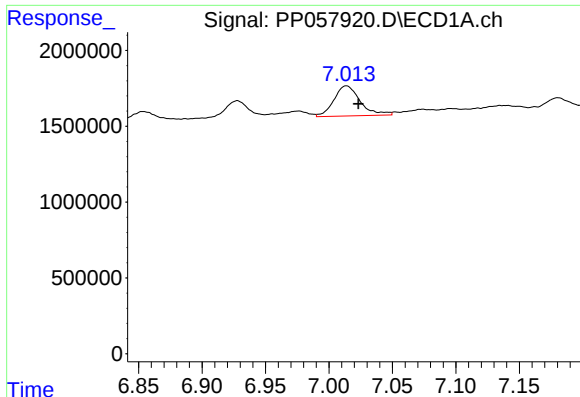


#28 AR-1254-3

R.T.: 7.014 min
Delta R.T.: -0.009 min
Response: 2857081
Conc: 31.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEE103S-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2023
Supervised By :Ankita Jodhani 05/26/2023

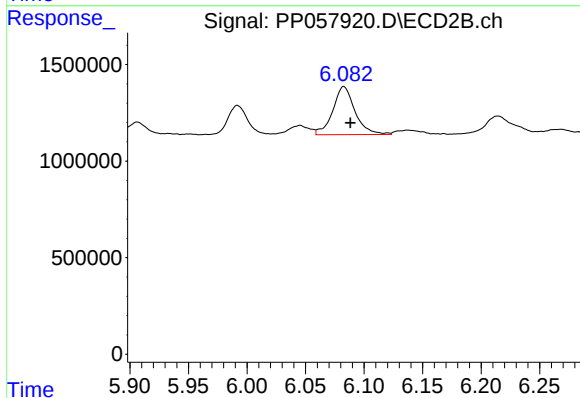


#28 AR-1254-3

R.T.: 6.083 min
Delta R.T.: -0.006 min
Response: 3284089
Conc: 20.99 ng/ml

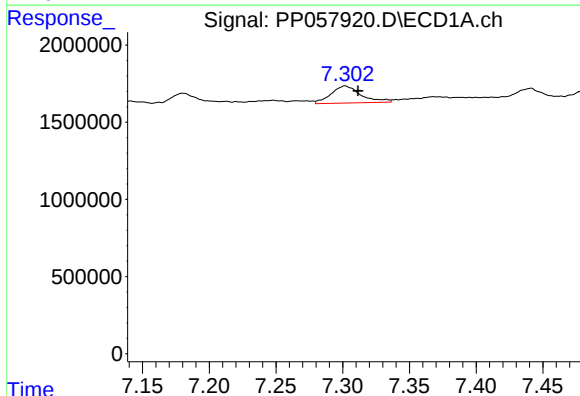


#29 AR-1254-4

R.T.: 7.302 min
Delta R.T.: -0.010 min
Response: 1734144
Conc: 29.11 ng/ml

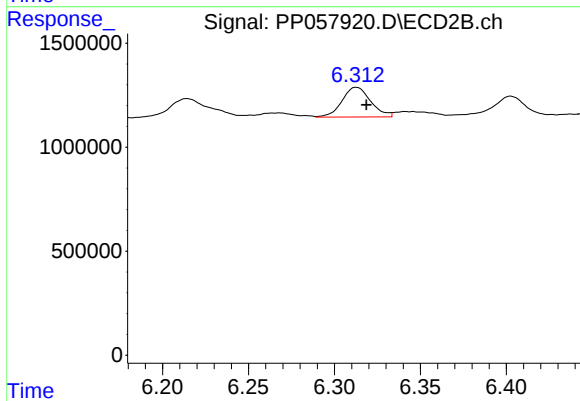

#29 AR-1254-4

R.T.: 6.313 min
Delta R.T.: -0.006 min
Response: 1653829
Conc: 17.93 ng/ml

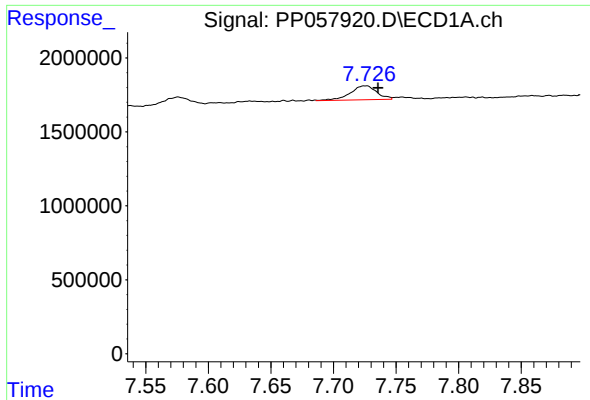

#30 AR-1254-5

R.T.: 7.726 min
Delta R.T.: -0.009 min
Response: 1382542
Conc: 20.14 ng/ml

Instrument :

ECD_P

ClientSampleId :


HEE103S-1-1

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 05/26/2023

Supervised By :Ankita Jodhani 05/26/2023

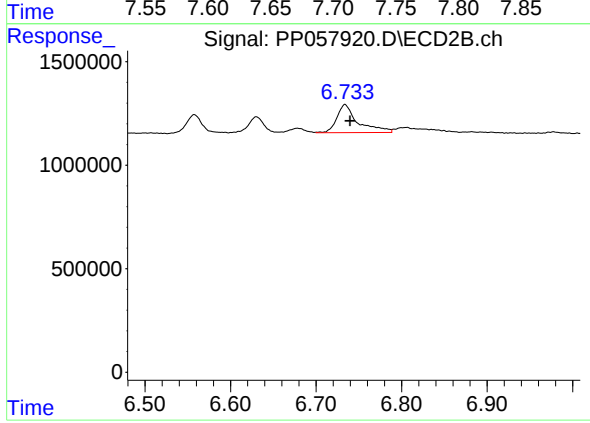

#30 AR-1254-5

R.T.: 6.734 min
Delta R.T.: -0.006 min
Response: 2340895
Conc: 16.17 ng/ml