

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052523\
 Data File : PP057952.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2023 04:03
 Operator : YP\AJ
 Sample : 02934-05 10X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KMA864L-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/26/2023
 Supervised By :Ankita Jodhani 05/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 06:06:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 08 19:18:05 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.383	3.622	3741867	3859526	1.706m	1.701
2) SA Decachlor...	10.205	8.678	3052650	3501822	2.694	2.231

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052523\
Data File : PP057952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2023 04:03
Operator : YP\AJ
Sample : 02934-05 10X
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KMA864L-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2023
Supervised By :Ankita Jodhani 05/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 06:06:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050823.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 08 19:18:05 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

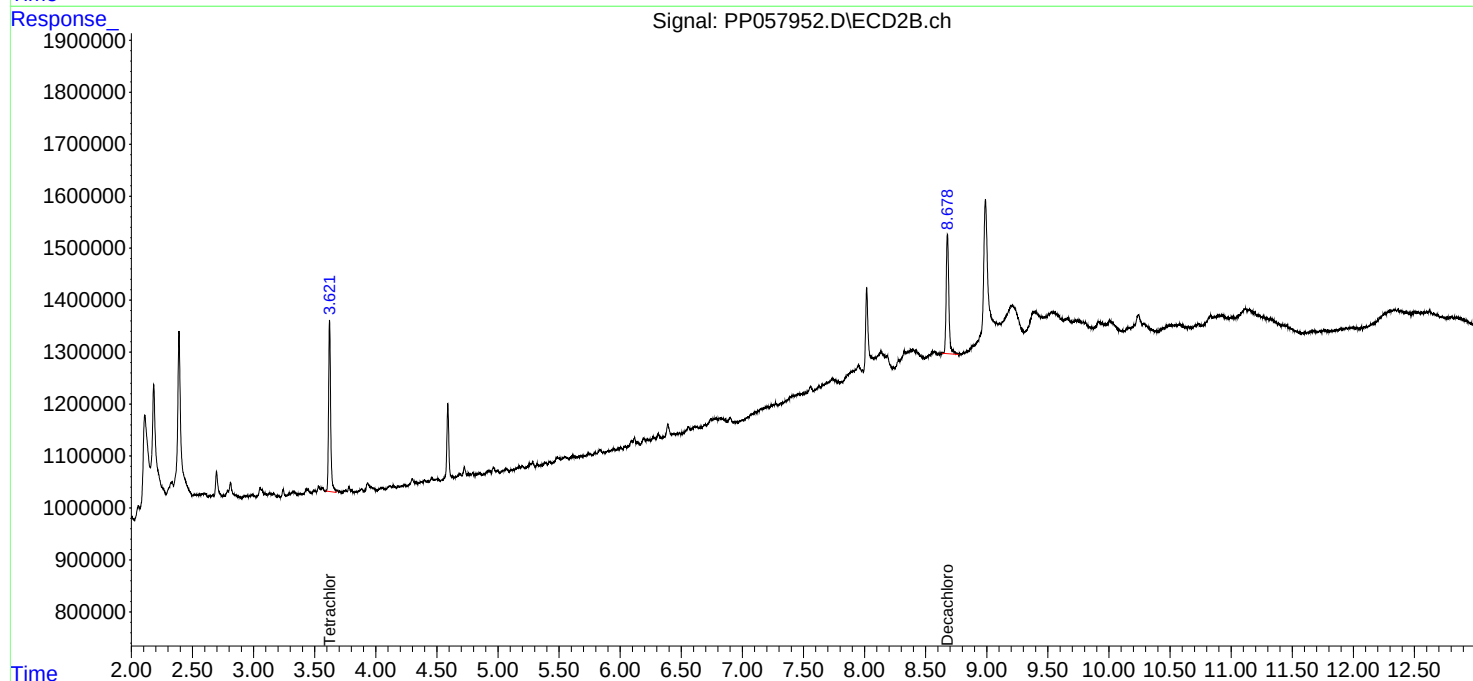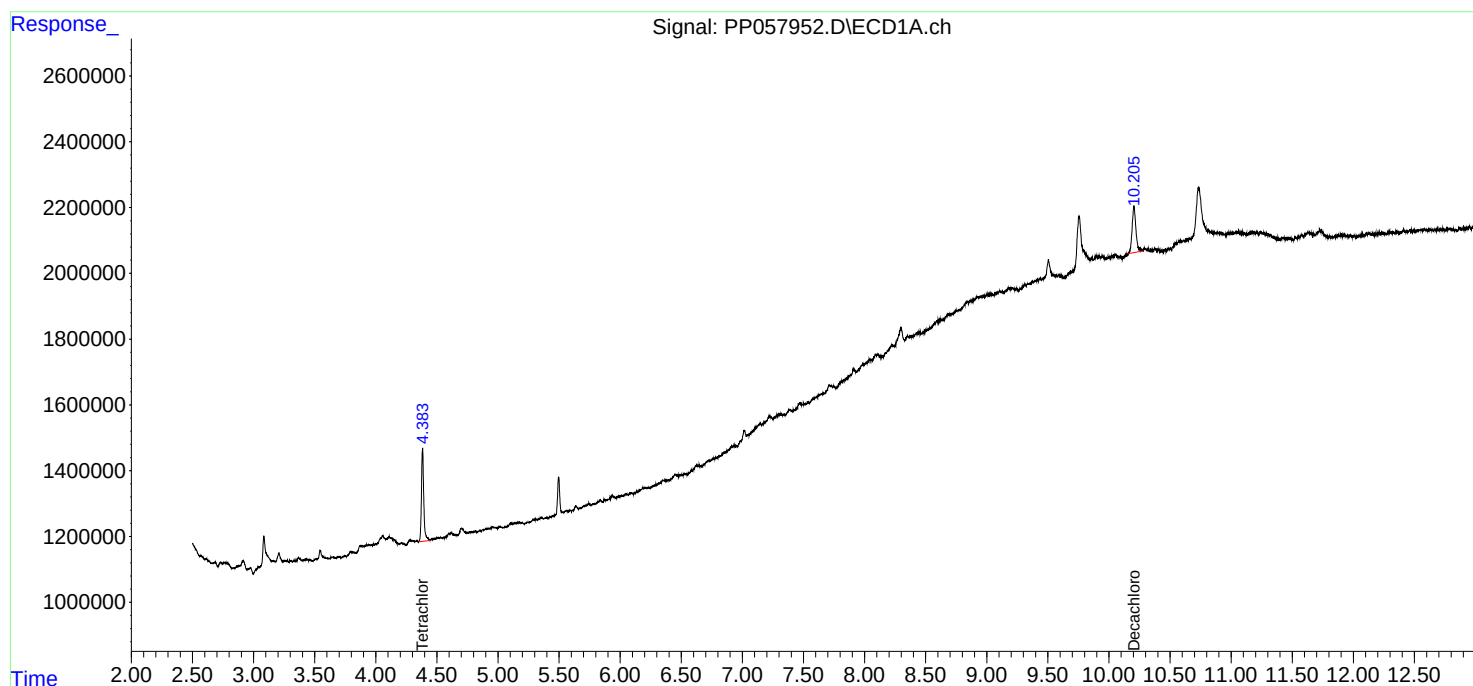

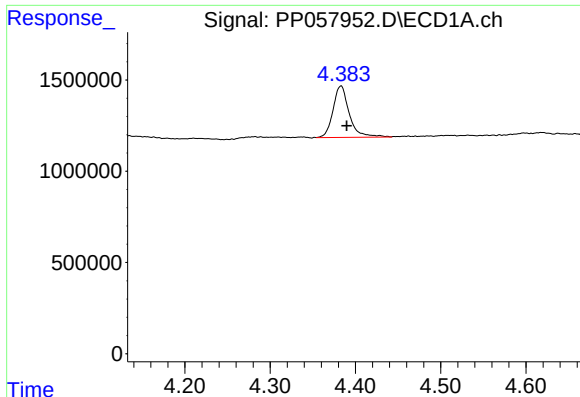

#1 Tetrachloro-m-xylene

R.T.: 4.383 min
Delta R.T.: -0.007 min
Response: 3741867
Conc: 1.71 ng/ml

Instrument :

ECD_P


ClientSampleId :

KMA864L-1-1

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 05/26/2023
Supervised By :Ankita Jodhani 05/26/2023

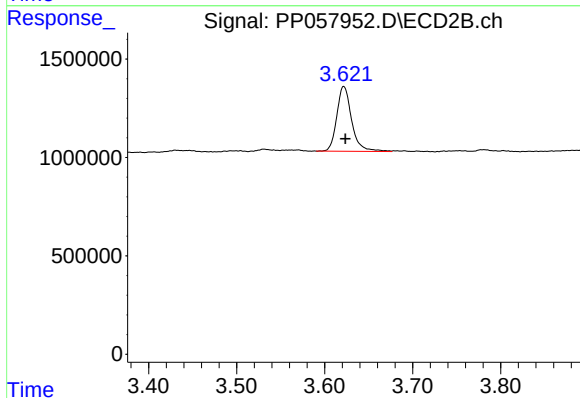


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.002 min
Response: 3859526
Conc: 1.70 ng/ml

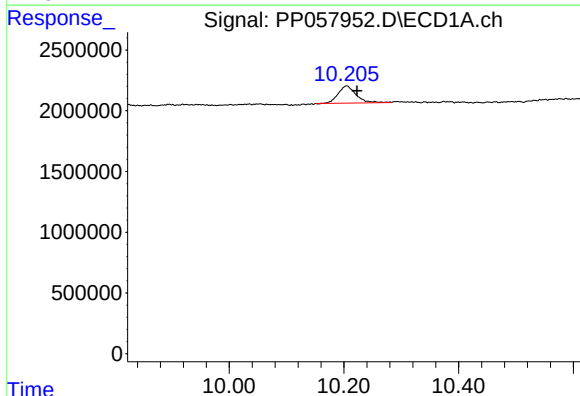

#2 Decachlorobiphenyl

R.T.: 10.205 min
Delta R.T.: -0.018 min
Response: 3052650
Conc: 2.69 ng/ml

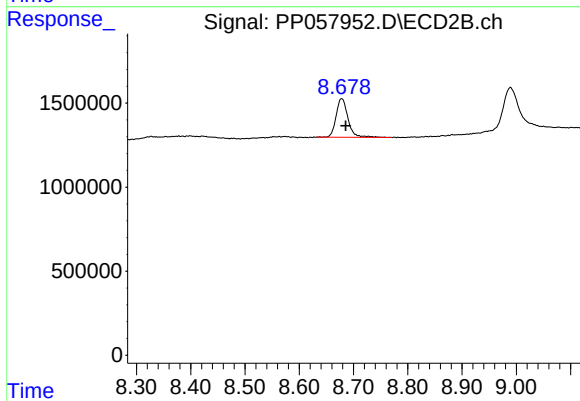

#2 Decachlorobiphenyl

R.T.: 8.678 min
Delta R.T.: -0.008 min
Response: 3501822
Conc: 2.23 ng/ml