

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052523\
 Data File : PP057965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2023 08:36
 Operator : YP\AJ
 Sample : 02939-03 10X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEE595N-2-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/26/2023
 Supervised By :Ankita Jodhani 05/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 08:50:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 08 19:18:05 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.382	3.621	3410724	3899982	1.555	1.719
2) SA Decachlor...	10.200	8.678	2467280	2905465	2.177m	1.851m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052523\
Data File : PP057965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2023 08:36
Operator : YP\AJ
Sample : 02939-03 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HEE595N-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2023
Supervised By :Ankita Jodhani 05/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 08:50:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP050823.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 08 19:18:05 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

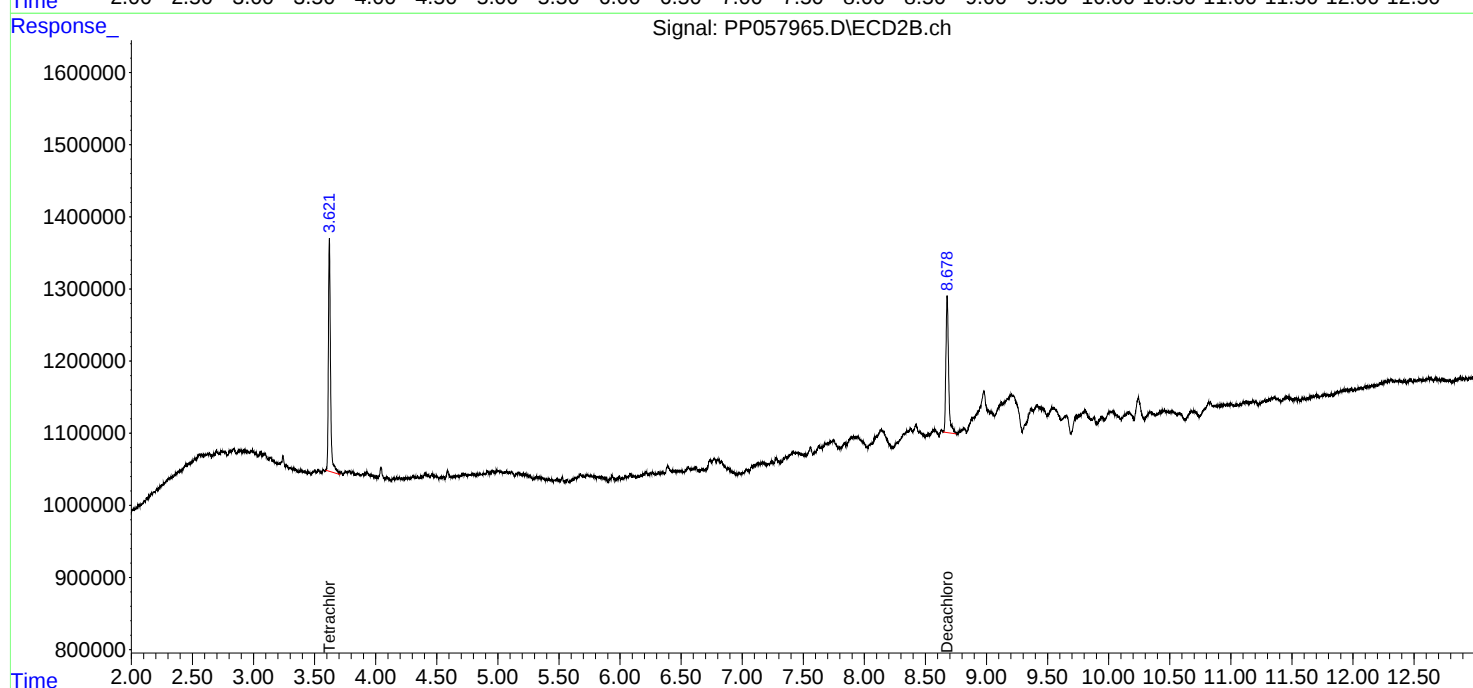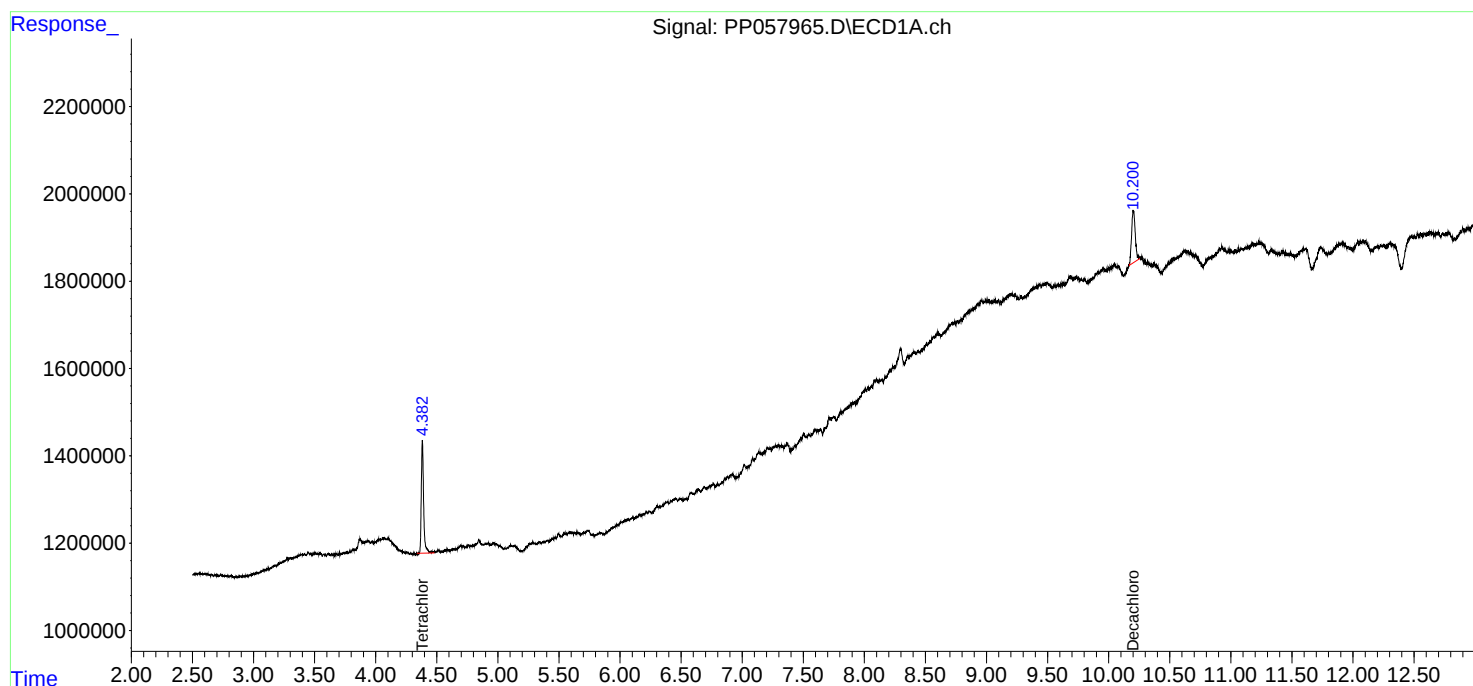

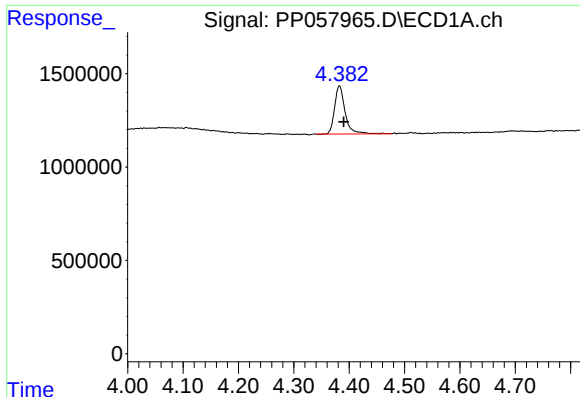


#1 Tetrachloro-m-xylene

R.T.: 4.382 min
Delta R.T.: -0.008 min
Response: 3410724
Conc: 1.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEE595N-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/26/2023
Supervised By :Ankita Jodhani 05/26/2023

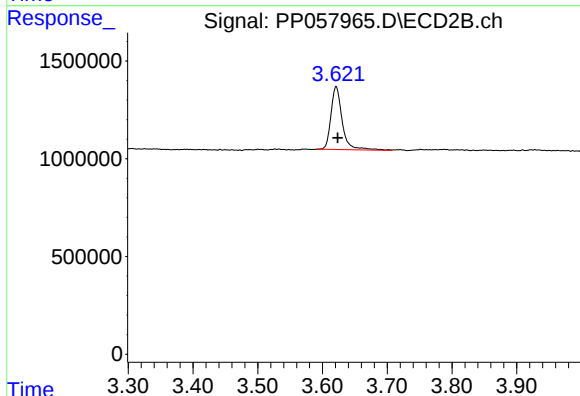


#1 Tetrachloro-m-xylene

R.T.: 3.621 min
Delta R.T.: -0.003 min
Response: 3899982
Conc: 1.72 ng/ml

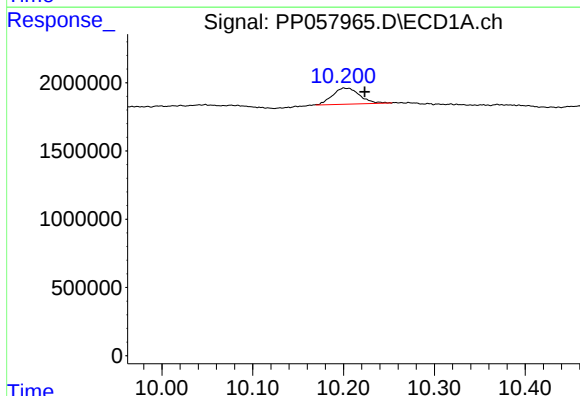

#2 Decachlorobiphenyl

R.T.: 10.200 min
Delta R.T.: -0.024 min
Response: 2467280
Conc: 2.18 ng/ml m

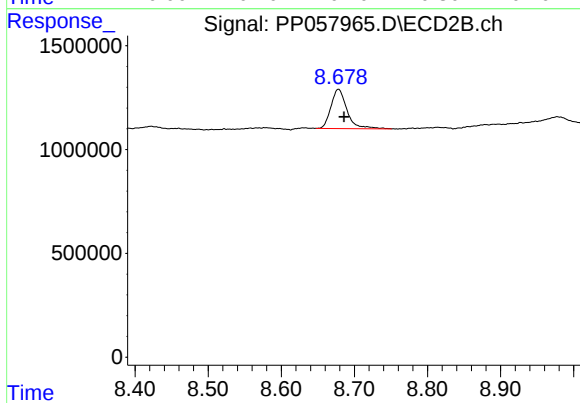

#2 Decachlorobiphenyl

R.T.: 8.678 min
Delta R.T.: -0.008 min
Response: 2905465
Conc: 1.85 ng/ml m