

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052621\
 Data File : PP036186.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 May 2021 7:56
 Operator : DD\AJ
 Sample : PB136340BL
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 09:58:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 26 00:48:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.966	3.963	948588	591880	21.312	21.207
2)	SA Decachlor...	10.994	9.271	991751	535082	23.206	23.323
Target Compounds							
8)	L2 AR-1221-1	5.217	0.000	23228	0	42.267	N.D. #
9)	L2 AR-1221-2	5.317	0.000	13851	0	33.229	N.D. #
12)	L3 AR-1232-2	5.975	0.000	34025	0	67.710	N.D. #
24)	L5 AR-1248-4	7.200f	0.000	7497	0	4.708	N.D. #
26)	L6 AR-1254-1	7.200	0.000	7497	0	4.628	N.D. #
38)	L8 AR-1262-3	0.000	8.177	0	18985	N.D.	15.977 #
41)	L9 AR-1268-1	0.000	8.177	0	18985	N.D.	5.590 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052621\
Data File : PP036186.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 May 2021 7:56
Operator : DD\AJ
Sample : PB136340BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 09:58:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 26 00:48:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

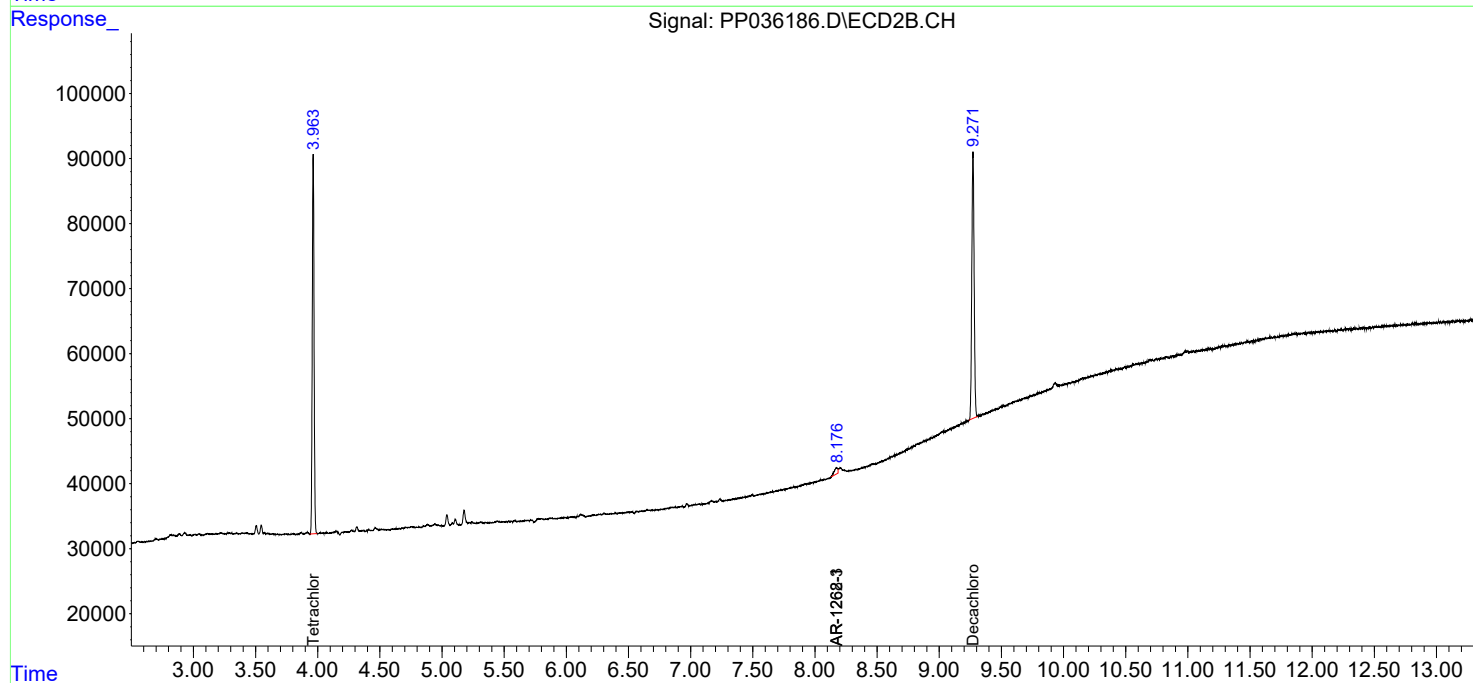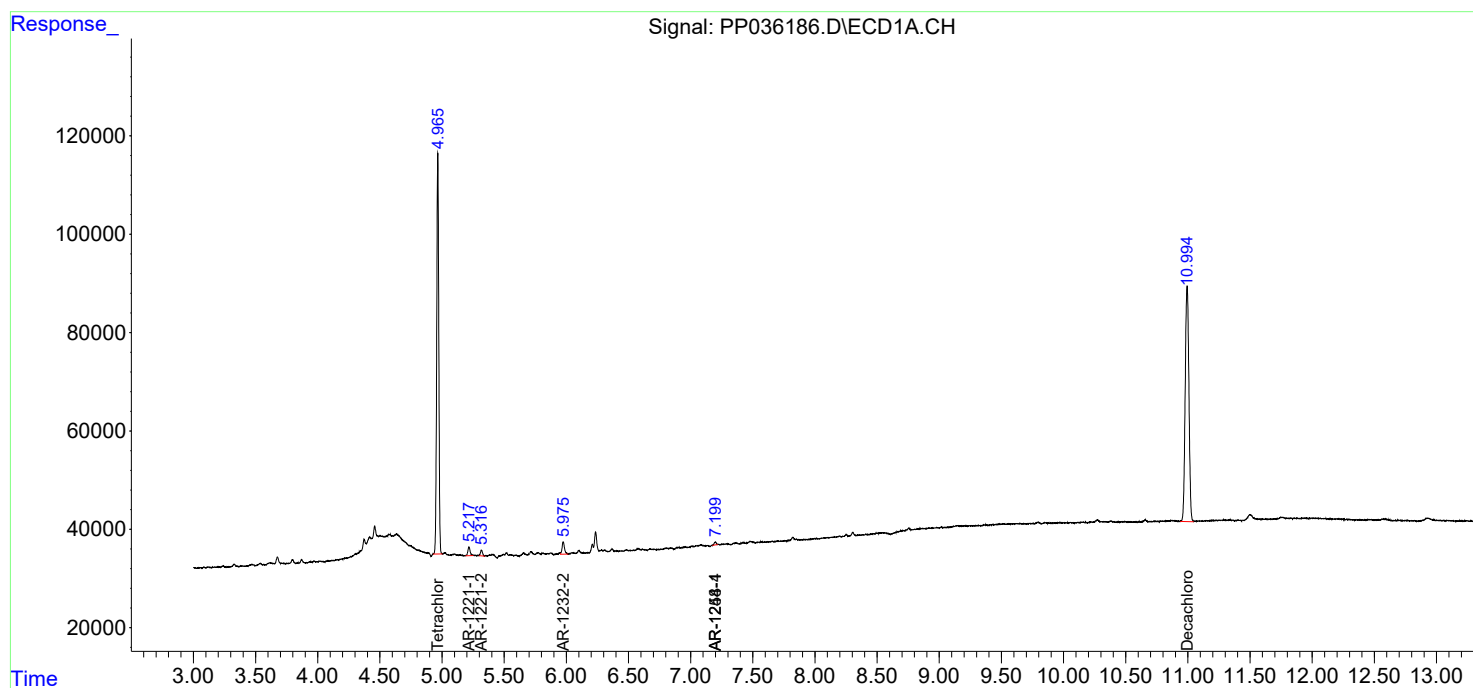


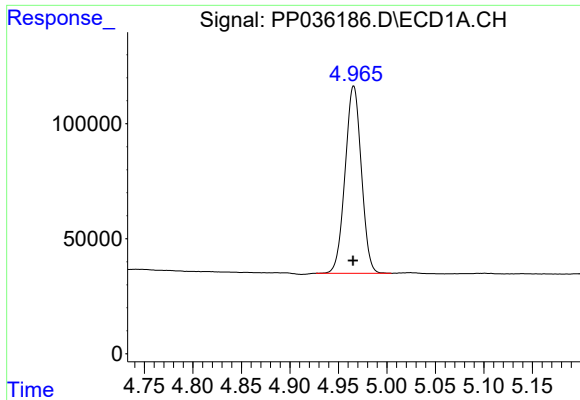

#1 Tetrachloro-m-xylene


R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 948588
Conc: 21.31 ng/ml

Instrument :
ECD_P
ClientSampleId :

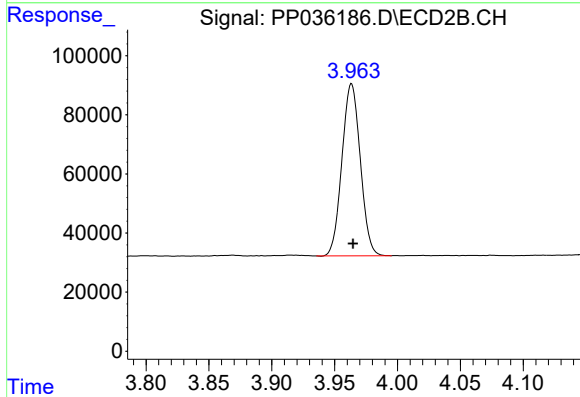


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: -0.001 min
Response: 591880
Conc: 21.21 ng/ml

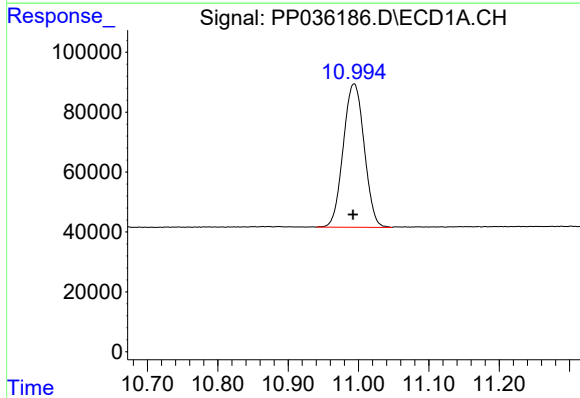


#2 Decachlorobiphenyl

R.T.: 10.994 min
Delta R.T.: 0.002 min
Response: 991751
Conc: 23.21 ng/ml

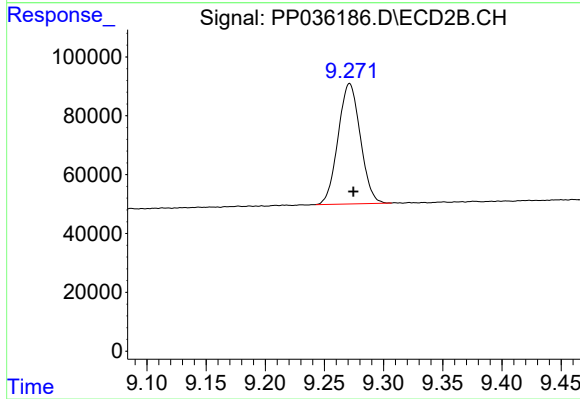

#2 Decachlorobiphenyl


R.T.: 9.271 min
Delta R.T.: -0.003 min
Response: 535082
Conc: 23.32 ng/ml

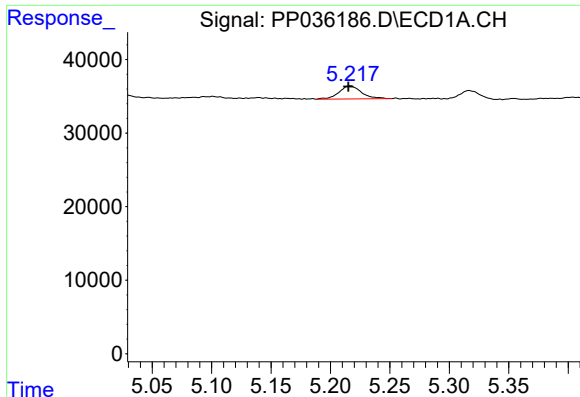

#8 AR-1221-1


R.T.: 5.217 min
Delta R.T.: 0.002 min
Response: 23228
Conc: 42.27 ng/ml

Instrument :
ECD_P
ClientSampleId :

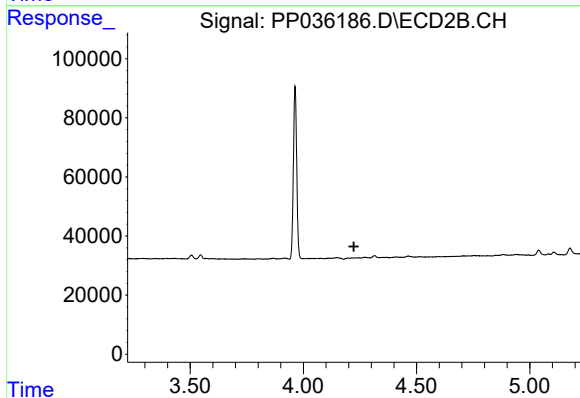


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.223 min
Response: 0
Conc: N.D.

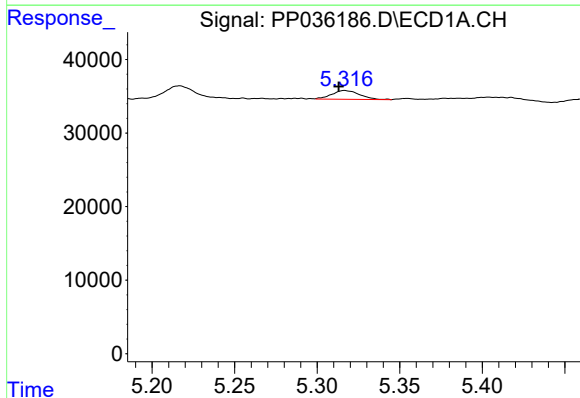


#9 AR-1221-2

R.T.: 5.317 min
Delta R.T.: 0.003 min
Response: 13851
Conc: 33.23 ng/ml

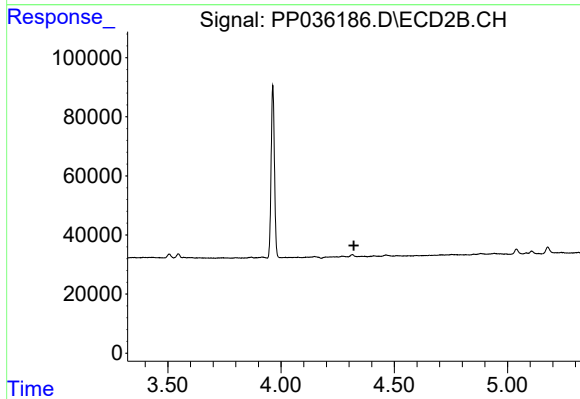

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.322 min
Response: 0
Conc: N.D.

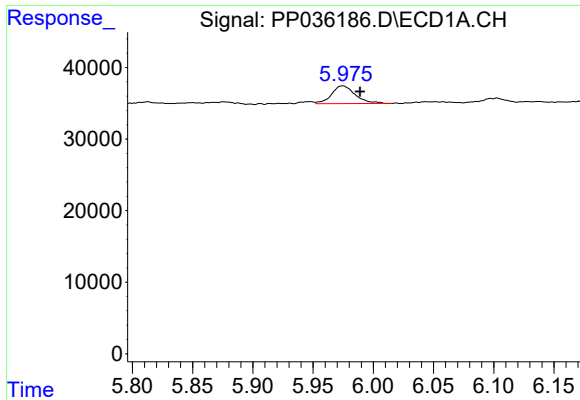

#12 AR-1232-2


R.T.: 5.975 min
Delta R.T.: -0.014 min
Response: 34025
Conc: 67.71 ng/ml

Instrument :
ECD_P
ClientSampleId :

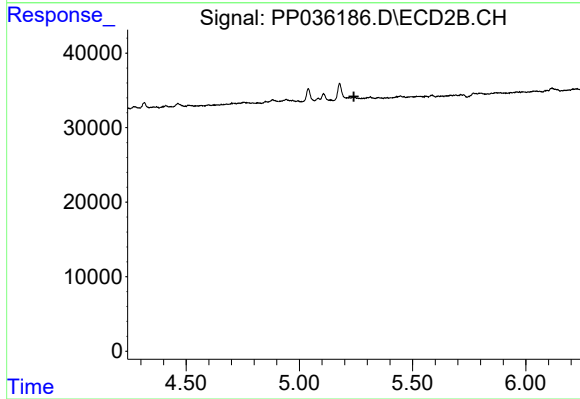


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.241 min
Response: 0
Conc: N.D.

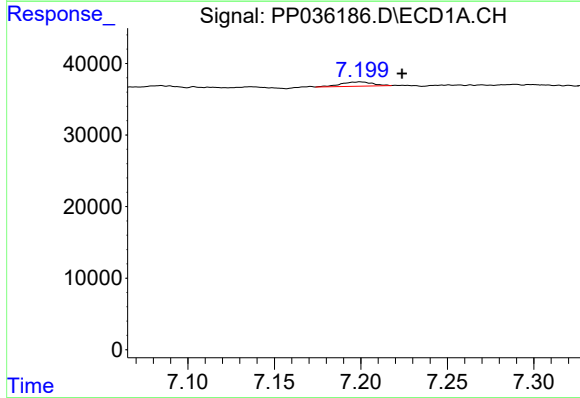


#24 AR-1248-4

R.T.: 7.200 min
Delta R.T.: -0.024 min
Response: 7497
Conc: 4.71 ng/ml

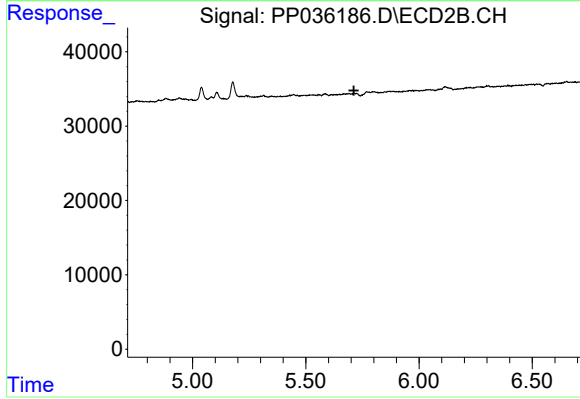

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.712 min
Response: 0
Conc: N.D.

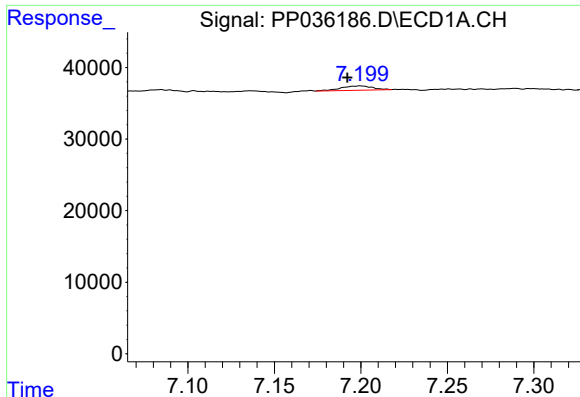

#26 AR-1254-1


R.T.: 7.200 min
Delta R.T.: 0.008 min
Response: 7497
Conc: 4.63 ng/ml

Instrument :
ECD_P
ClientSampleId :

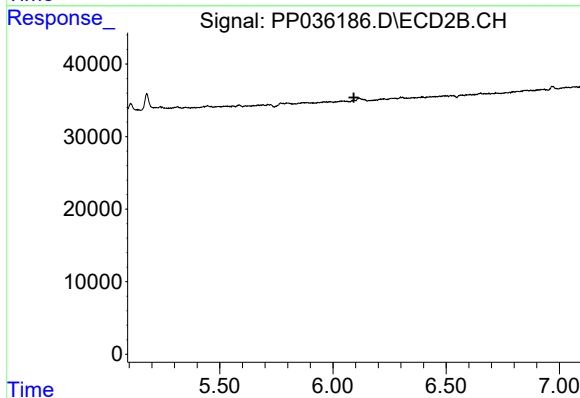


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.092 min
Response: 0
Conc: N.D.

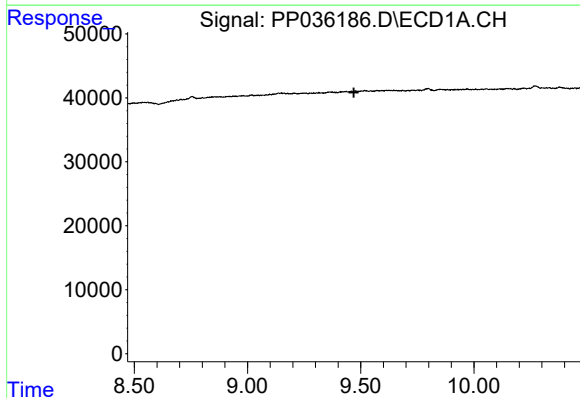


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.470 min
Response: 0
Conc: N.D.

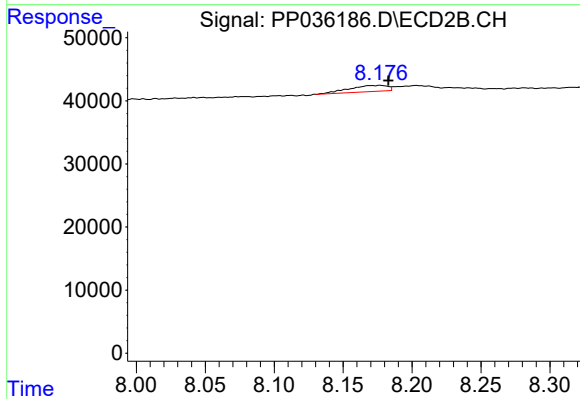

#38 AR-1262-3


R.T.: 8.177 min
Delta R.T.: -0.006 min
Response: 18985
Conc: 15.98 ng/ml

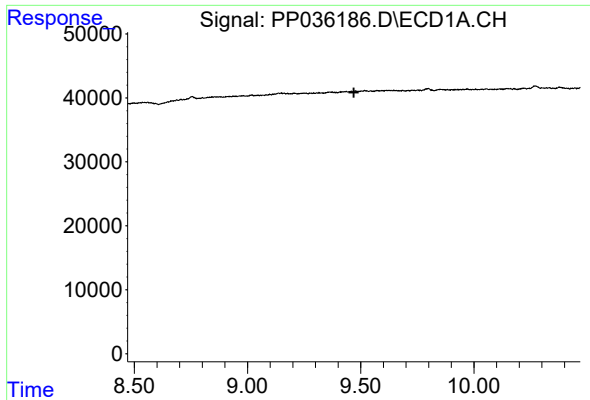

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.470 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

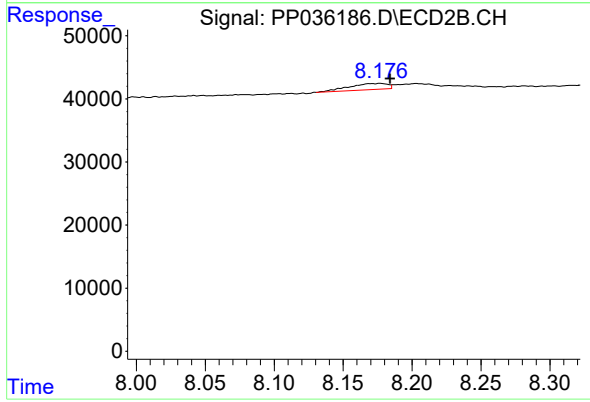

#41 AR-1268-1

R.T.: 8.177 min
Delta R.T.: -0.007 min
Response: 18985
Conc: 5.59 ng/ml