

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052621\
 Data File : PS015084.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2021 23:00
 Operator : DD\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 08:59:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052621.M
 Quant Title : 8080.M
 QLast Update : Thu May 27 05:20:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.150	6.862	1040.6E6	285.0E6	787.892	789.917
Target Compounds							
1) T	Dalapon	2.988	2.587	1106.9E6	376.3E6	718.744	718.144
2) T	3,5-DICHL...	6.378	6.031	1381.4E6	453.4E6	730.901	733.709
3) T	4-Nitroph...	6.986	6.492	531.3E6	161.8E6	721.225	731.780
5) T	DICAMBA	7.335	7.023	3839.1E6	1311.4E6	737.545	738.445
6) T	MCPD	7.500	7.115	286.5E6	106.9E6	74.235	73.920
7) T	MCPA	7.648	7.329	407.7E6	151.2E6	73.249	73.278
8) T	DICHLORPROP	8.024	7.649	941.1E6	323.3E6	739.322	740.065
9) T	2,4-D	8.257	7.951	1095.8E6	378.0E6	736.952	743.066
10) T	Pentachlo...	8.555	8.361	14246.8E6	4579.0E6	740.489	741.791
11) T	2,4,5-TP ...	9.104	8.726	5518.4E6	1824.1E6	745.280	747.636
12) T	2,4,5-T	9.392	9.107	5888.5E6	1607.0E6	746.909	751.361
13) T	2,4-DB	9.941	9.613	1081.8E6	213.5E6	752.475	754.624
14) T	DINOSEB	11.087	9.937	4269.2E6	1273.8E6	733.906	736.435
15) T	Picloram	10.916	10.926	8284.3E6	2583.4E6	760.580	761.940
16) T	DCPA	11.353	10.861	8325.8E6	2752.9E6	751.024	750.955



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052621\
Data File : PS015084.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2021 23:00
Operator : DD\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 08:59:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052621.M
Quant Title : 8080.M
QLast Update : Thu May 27 05:20:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

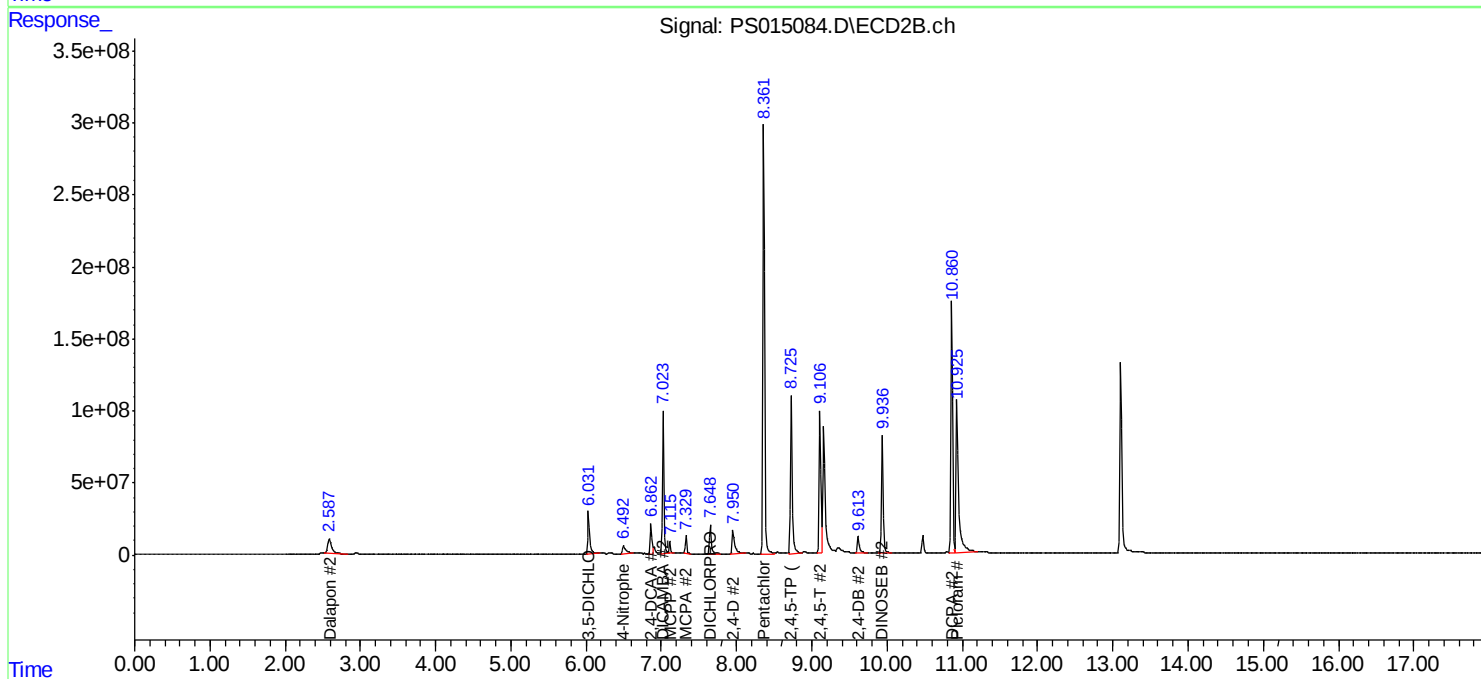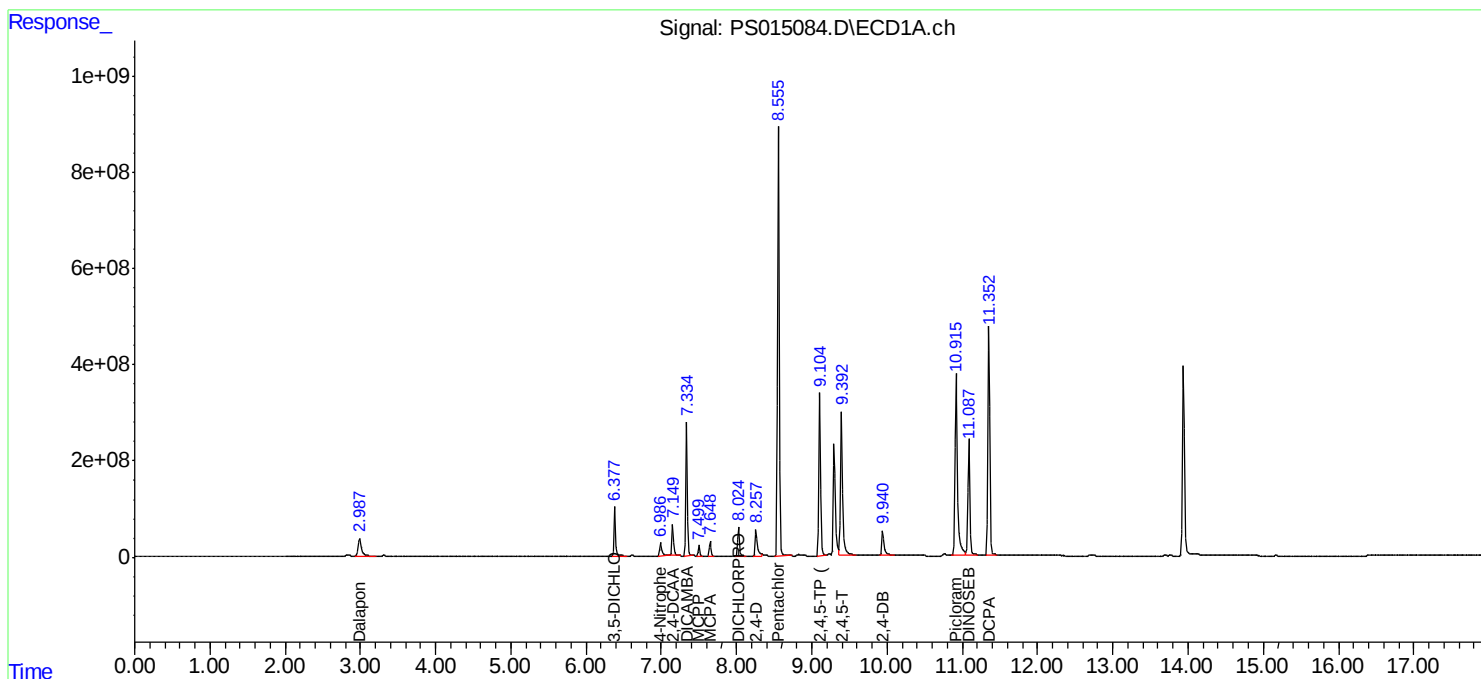


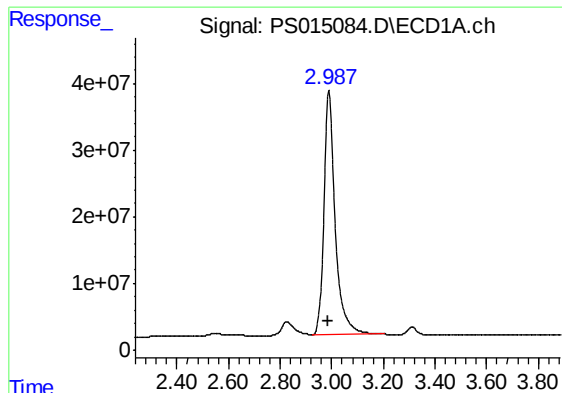

#1 Dalapon


R.T.: 2.988 min
Delta R.T.: 0.000 min
Response: 1106924418
Conc: 718.74 ng/ml

Instrument :
ECD_P
ClientSampleId :

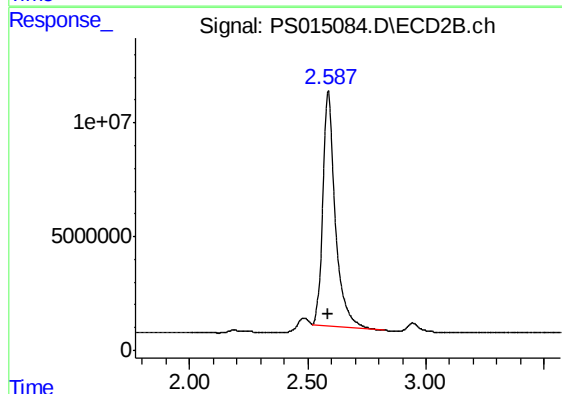


#1 Dalapon

R.T.: 2.587 min
Delta R.T.: 0.000 min
Response: 376309136
Conc: 718.14 ng/ml

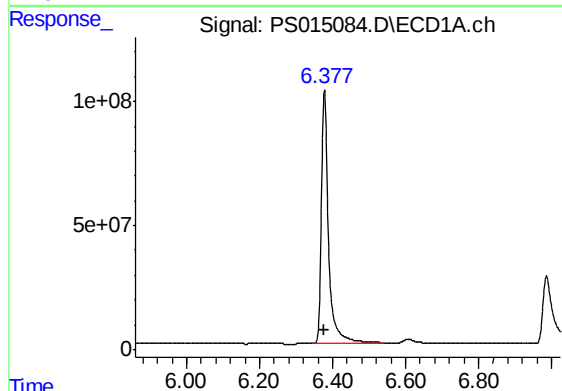


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.378 min
Delta R.T.: 0.000 min
Response: 1381362493
Conc: 730.90 ng/ml

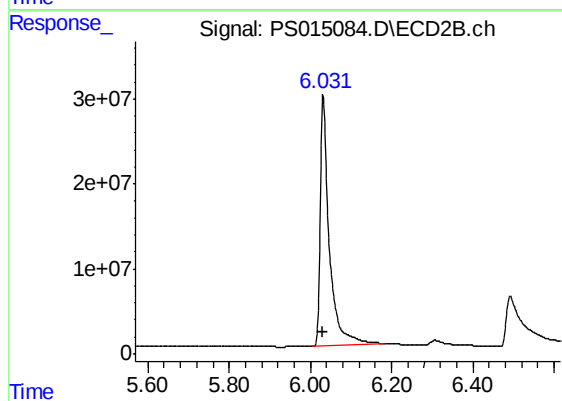

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.031 min
Delta R.T.: 0.000 min
Response: 453423782
Conc: 733.71 ng/ml

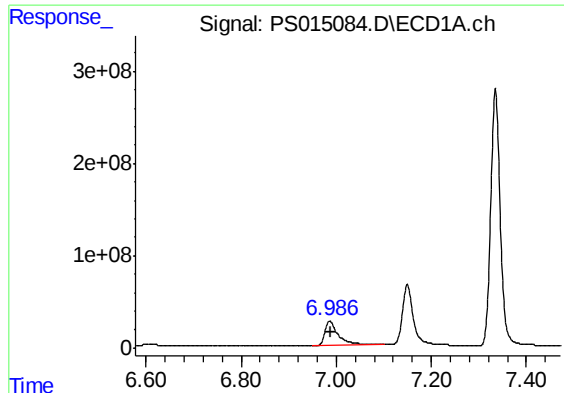

#3 4-Nitrophenol


R.T.: 6.986 min
Delta R.T.: -0.001 min
Response: 531257362
Conc: 721.23 ng/ml

Instrument :
ECD_P
ClientSampleId :

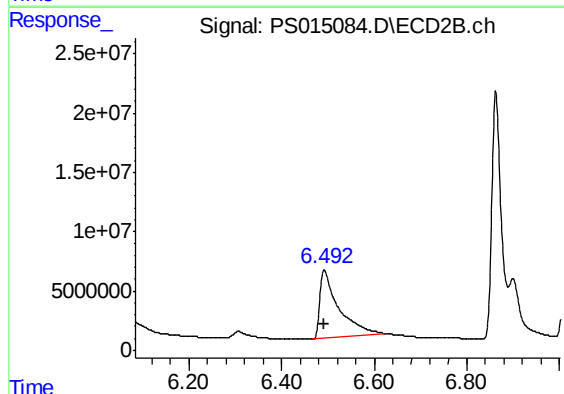


#3 4-Nitrophenol

R.T.: 6.492 min
Delta R.T.: -0.001 min
Response: 161762804
Conc: 731.78 ng/ml

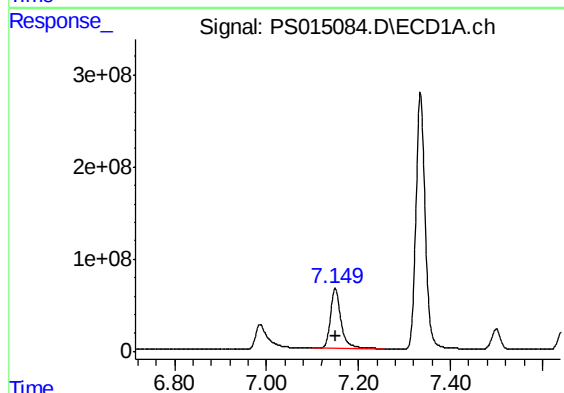


#4 2,4-DCAA

R.T.: 7.150 min
Delta R.T.: 0.000 min
Response: 1040628431
Conc: 787.89 ng/ml

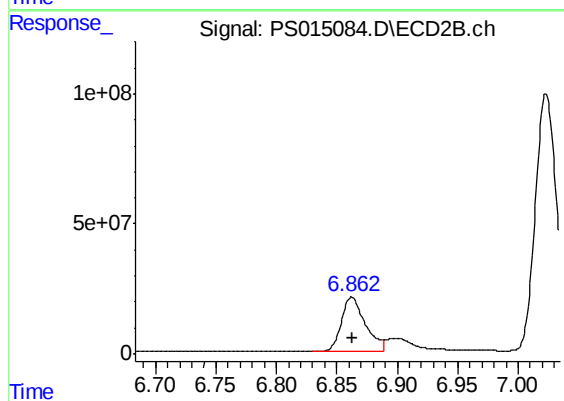

#4 2,4-DCAA


R.T.: 6.862 min
Delta R.T.: 0.000 min
Response: 284962588
Conc: 789.92 ng/ml

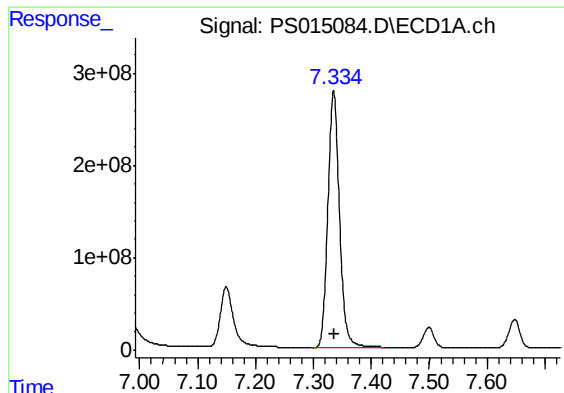

#5 DICAMBA


R.T.: 7.335 min
Delta R.T.: 0.000 min
Response: 3839094540
Conc: 737.55 ng/ml

Instrument :
ECD_P
ClientSampleId :

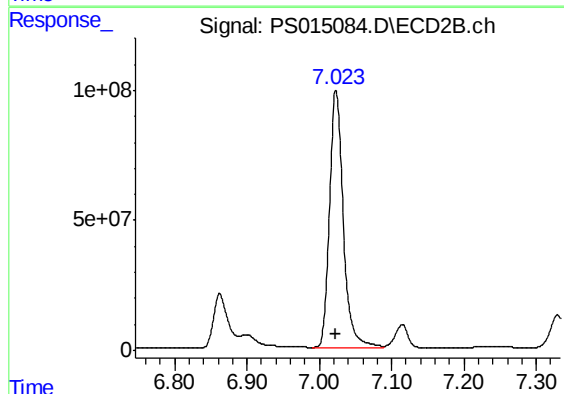


#5 DICAMBA

R.T.: 7.023 min
Delta R.T.: 0.000 min
Response: 1311427719
Conc: 738.45 ng/ml

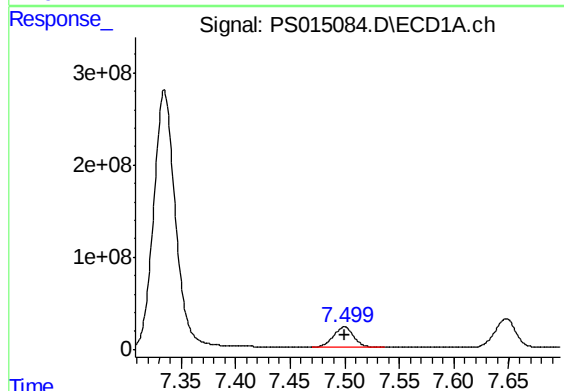


#6 MCPP

R.T.: 7.500 min
Delta R.T.: 0.000 min
Response: 286488841
Conc: 74.24 ug/ml

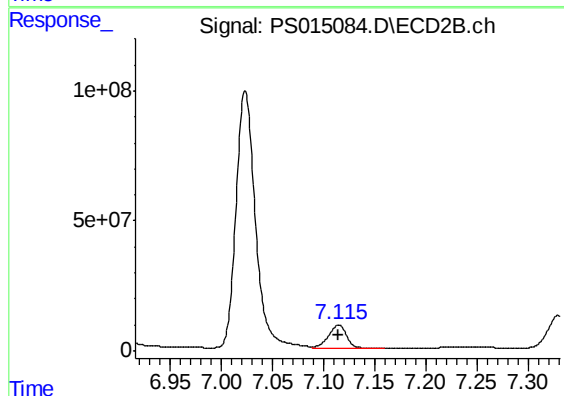

#6 MCPP


R.T.: 7.115 min
Delta R.T.: 0.000 min
Response: 106890237
Conc: 73.92 ug/ml

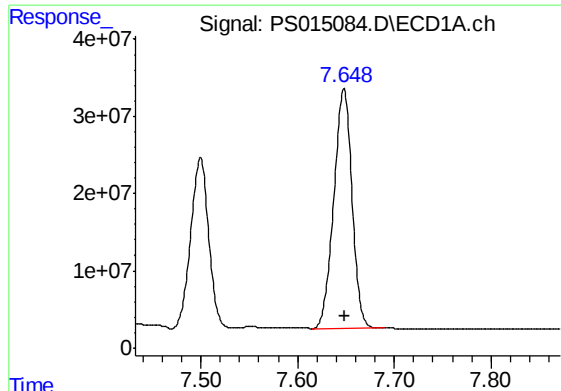

#7 MCPA


R.T.: 7.648 min
Delta R.T.: 0.000 min
Response: 407730539
Conc: 73.25 ug/ml

Instrument :
ECD_P
ClientSampleId :

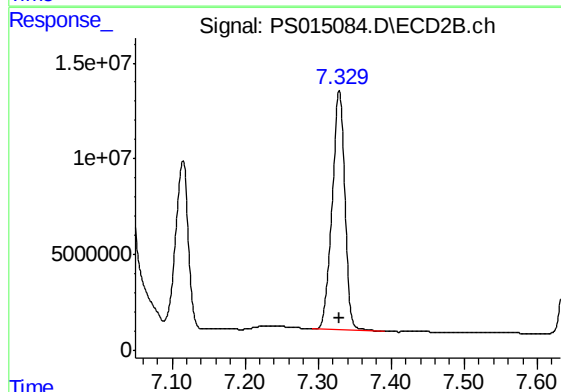


#7 MCPA

R.T.: 7.329 min
Delta R.T.: 0.000 min
Response: 151198196
Conc: 73.28 ug/ml

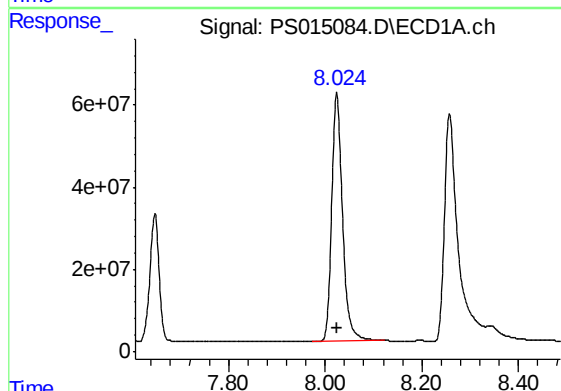


#8 DICHLORPROP

R.T.: 8.024 min
Delta R.T.: 0.000 min
Response: 941056214
Conc: 739.32 ng/ml

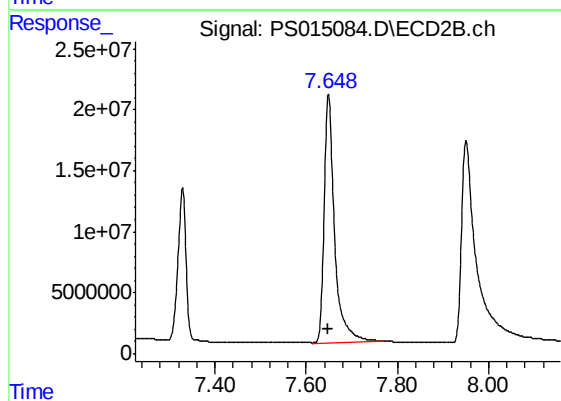

#8 DICHLORPROP


R.T.: 7.649 min
Delta R.T.: 0.000 min
Response: 323265130
Conc: 740.07 ng/ml

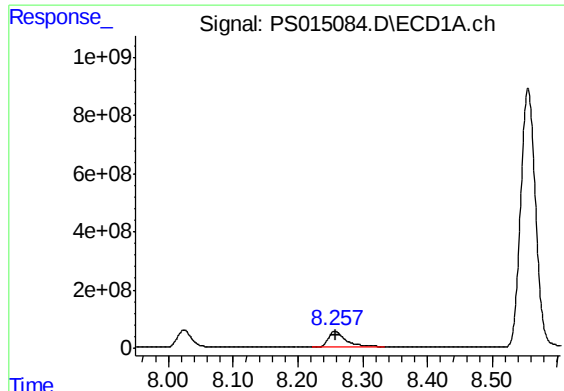

#9 2,4-D


R.T.: 8.257 min
Delta R.T.: -0.001 min
Response: 1095846640
Conc: 736.95 ng/ml

Instrument :
ECD_P
ClientSampleId :

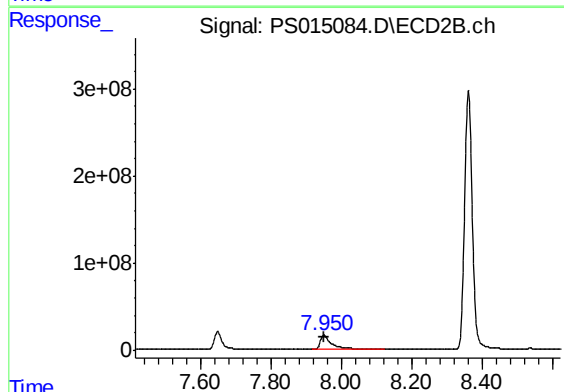


#9 2,4-D

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 377959717
Conc: 743.07 ng/ml

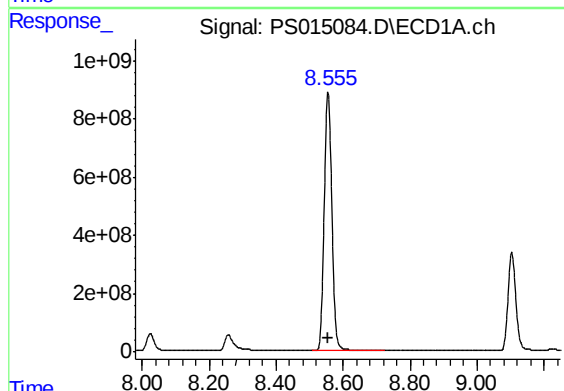


#10 Pentachlorophenol

R.T.: 8.555 min
Delta R.T.: 0.000 min
Response: 14246817180
Conc: 740.49 ng/ml

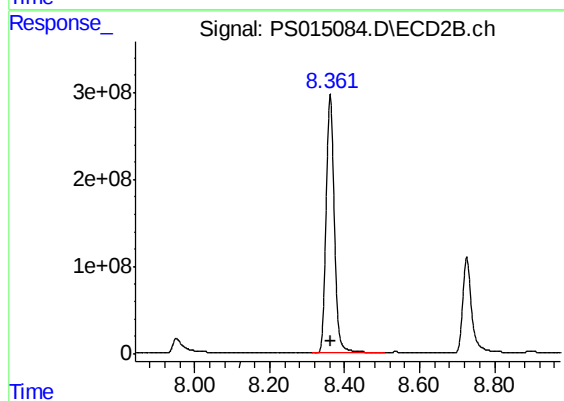

#10 Pentachlorophenol


R.T.: 8.361 min
Delta R.T.: 0.000 min
Response: 4578984637
Conc: 741.79 ng/ml

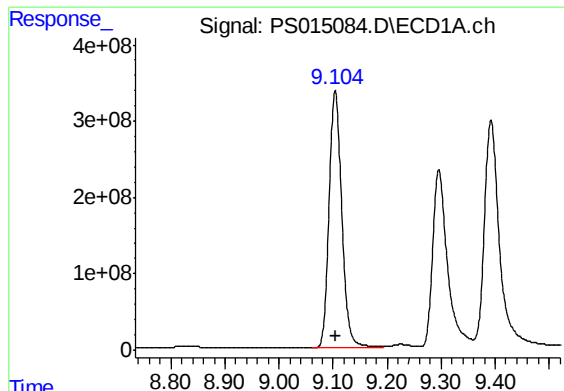

#11 2,4,5-TP (SILVEX)


R.T.: 9.104 min
Delta R.T.: 0.000 min
Response: 5518352414
Conc: 745.28 ng/ml

Instrument :
ECD_P
ClientSampleId :

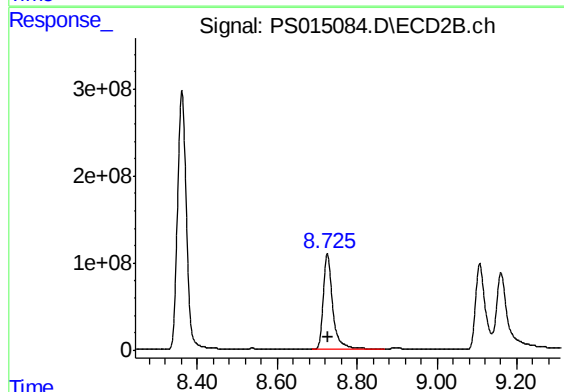


#11 2,4,5-TP (SILVEX)

R.T.: 8.726 min
Delta R.T.: 0.000 min
Response: 1824097524
Conc: 747.64 ng/ml

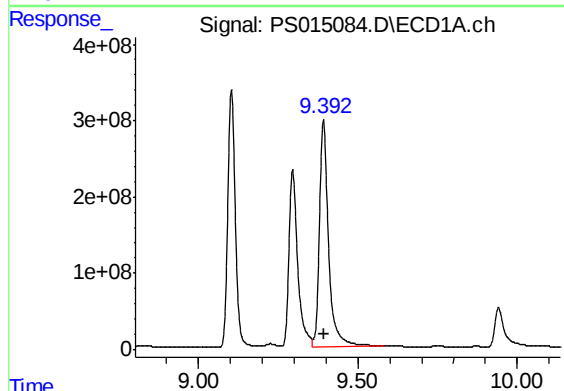


#12 2,4,5-T

R.T.: 9.392 min
Delta R.T.: 0.000 min
Response: 5888539698
Conc: 746.91 ng/ml

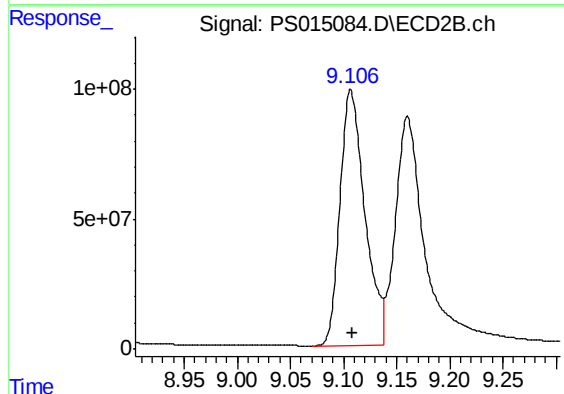

#12 2,4,5-T


R.T.: 9.107 min
Delta R.T.: -0.002 min
Response: 1606986985
Conc: 751.36 ng/ml

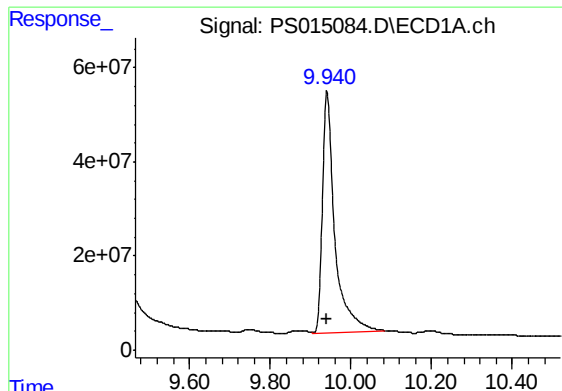

#13 2,4-DB


R.T.: 9.941 min
Delta R.T.: 0.000 min
Response: 1081848462
Conc: 752.48 ng/ml

Instrument :
ECD_P
ClientSampleId :

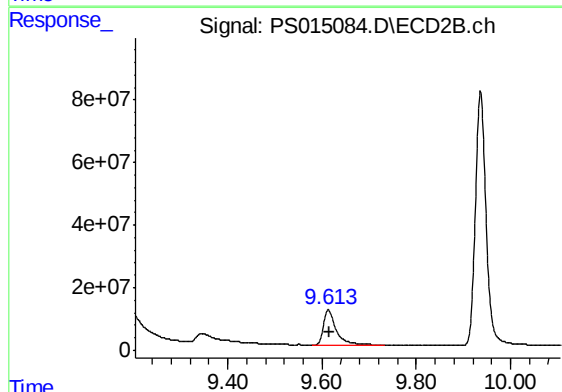


#13 2,4-DB

R.T.: 9.613 min
Delta R.T.: -0.001 min
Response: 213475521
Conc: 754.62 ng/ml

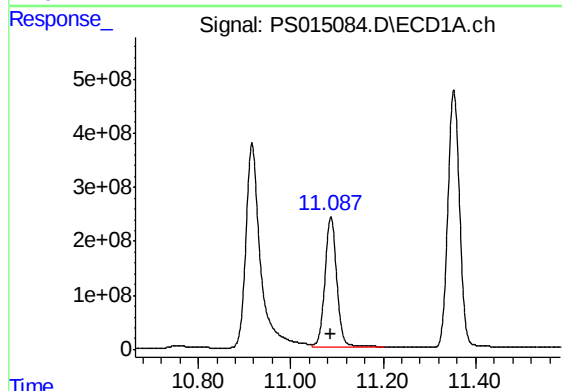


#14 DINOSEB

R.T.: 11.087 min
Delta R.T.: 0.000 min
Response: 4269161815
Conc: 733.91 ng/ml

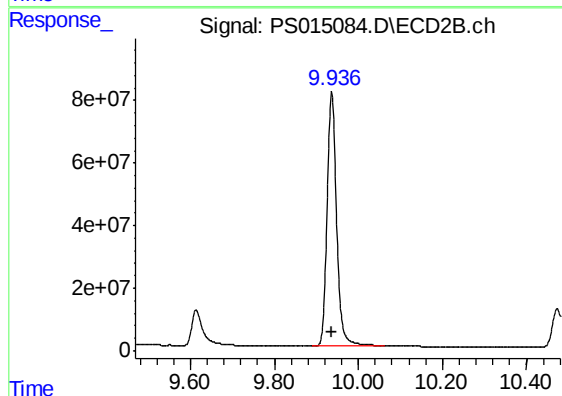

#14 DINOSEB


R.T.: 9.937 min
Delta R.T.: -0.001 min
Response: 1273761320
Conc: 736.43 ng/ml

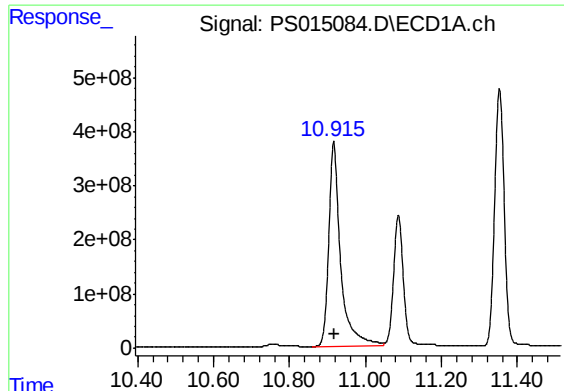

#15 Picloram


R.T.: 10.916 min
Delta R.T.: -0.002 min
Response: 8284284239
Conc: 760.58 ng/ml

Instrument :
ECD_P
ClientSampleId :

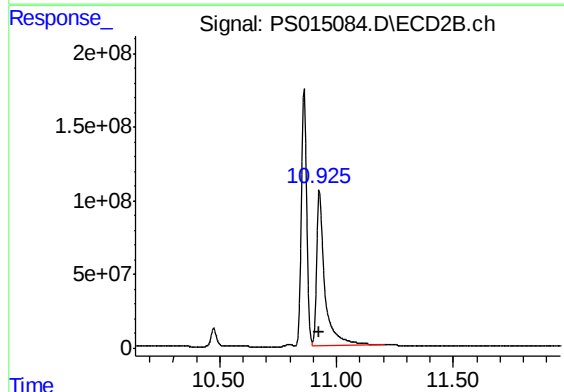


#15 Picloram

R.T.: 10.926 min
Delta R.T.: -0.001 min
Response: 2583440306
Conc: 761.94 ng/ml

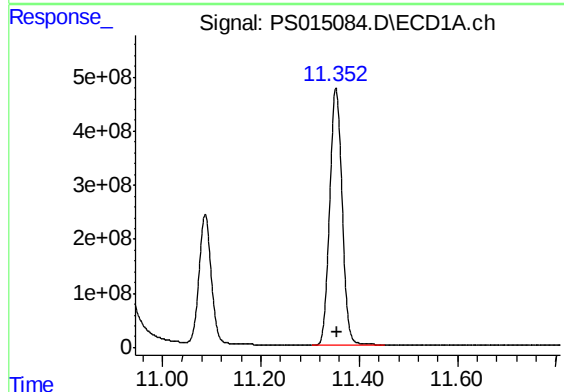

#16 DCPA

R.T.: 11.353 min
Delta R.T.: -0.001 min
Response: 8325788912
Conc: 751.02 ng/ml

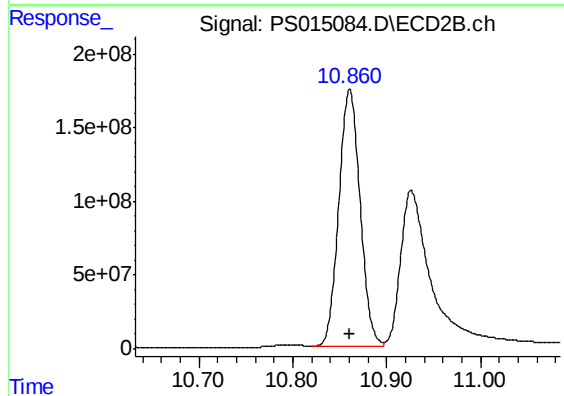

#16 DCPA

R.T.: 10.861 min
Delta R.T.: 0.000 min
Response: 2752886811
Conc: 750.96 ng/ml