

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052621\
 Data File : PP036191.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 May 2021 9:20
 Operator : DD\AJ
 Sample : M2262-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT2-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 10:00:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 26 00:48:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.966	3.964	897336	564943	20.161	20.242
2) SA Decachlor...	10.995	9.271	941725	510131	22.035	22.236
Target Compounds						
21) L5 AR-1248-1	6.285	5.217	26231	14852	28.176	27.686
22) L5 AR-1248-2	6.579	5.484	35277	18291	29.507	26.211
23) L5 AR-1248-3	6.797	5.526	39421	16605	27.208	23.072
24) L5 AR-1248-4	7.224	5.709	47708	24364	29.956	27.586
25) L5 AR-1248-5	7.263	6.133	46627	25691	29.866	29.215



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052621\
Data File : PP036191.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 May 2021 9:20
Operator : DD\AJ
Sample : M2262-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 70 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 10:00:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 26 00:48:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

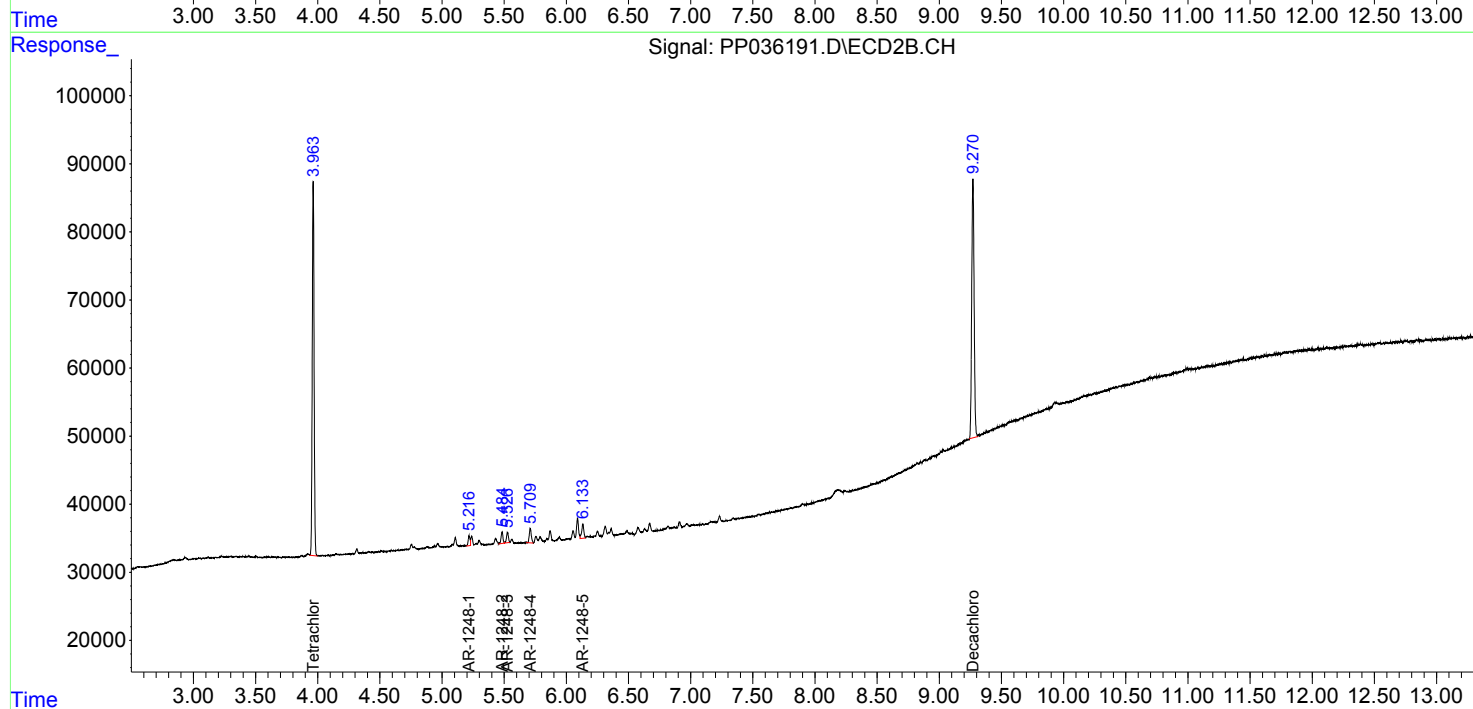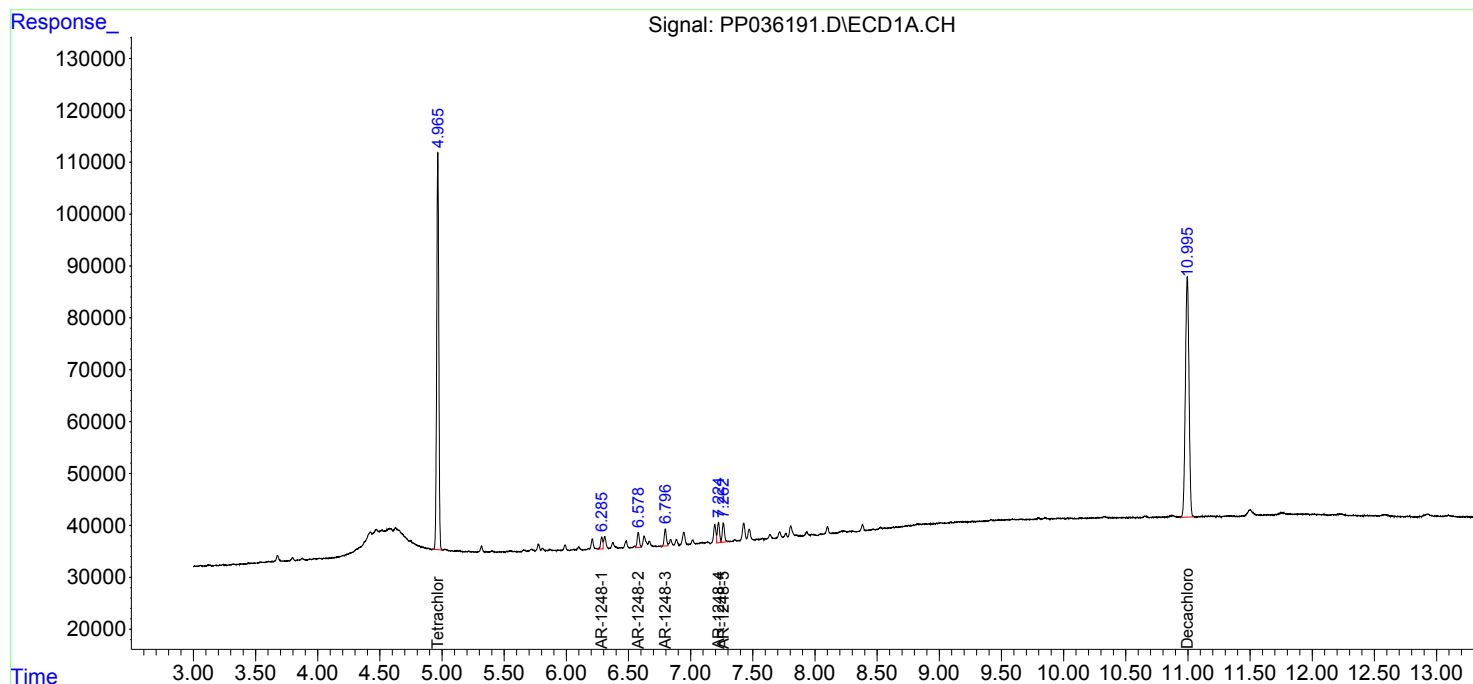


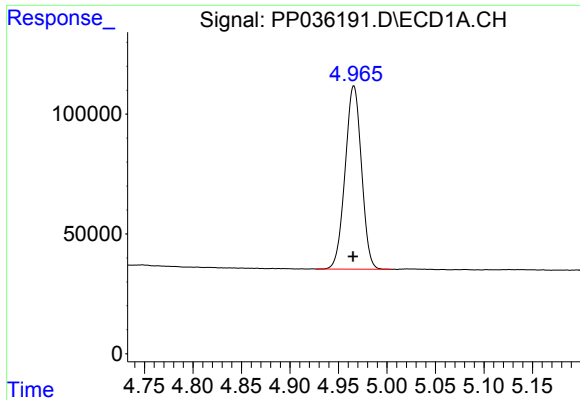

#1 Tetrachloro-m-xylene


R.T.: 4.966 min
Delta R.T.: 0.000 min
Response: 897336
Conc: 20.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2021

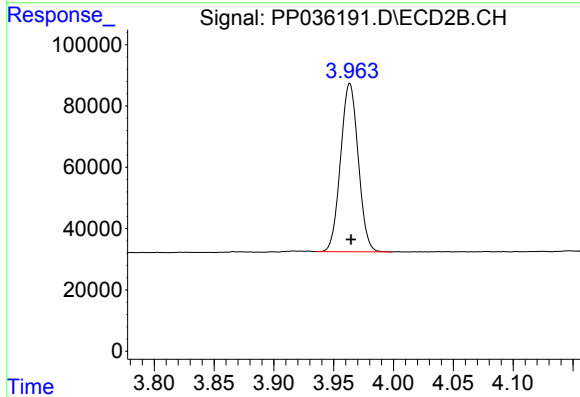


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 564943
Conc: 20.24 ng/ml

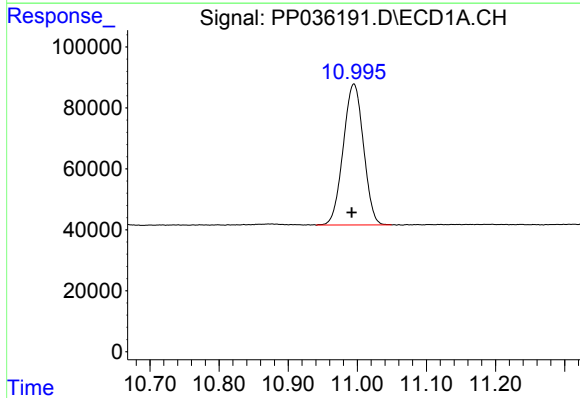


#2 Decachlorobiphenyl

R.T.: 10.995 min
Delta R.T.: 0.003 min
Response: 941725
Conc: 22.04 ng/ml

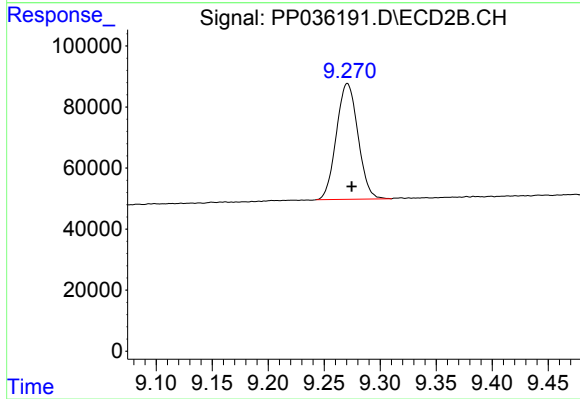

#2 Decachlorobiphenyl


R.T.: 9.271 min
Delta R.T.: -0.004 min
Response: 510131
Conc: 22.24 ng/ml

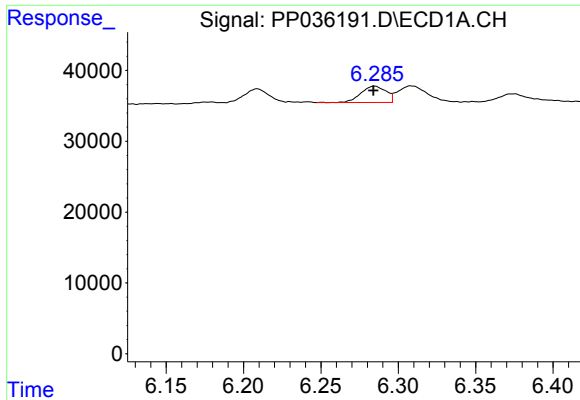

#21 AR-1248-1


R.T.: 6.285 min
Delta R.T.: 0.001 min
Response: 26231
Conc: 28.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2021

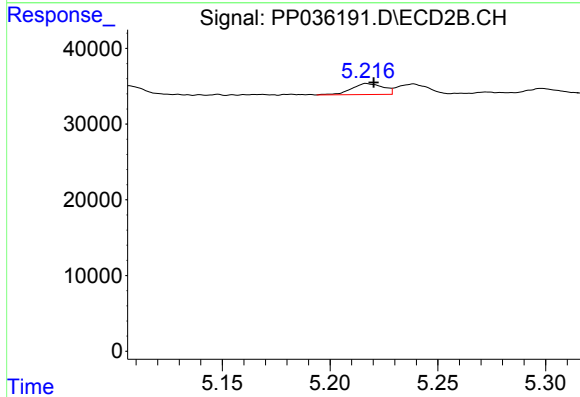


#21 AR-1248-1

R.T.: 5.217 min
Delta R.T.: -0.003 min
Response: 14852
Conc: 27.69 ng/ml

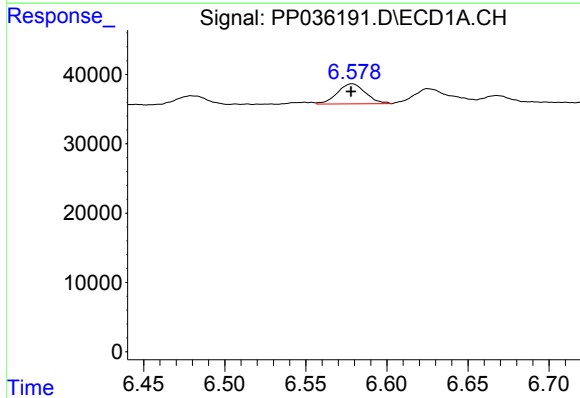


#22 AR-1248-2

R.T.: 6.579 min
Delta R.T.: 0.000 min
Response: 35277
Conc: 29.51 ng/ml

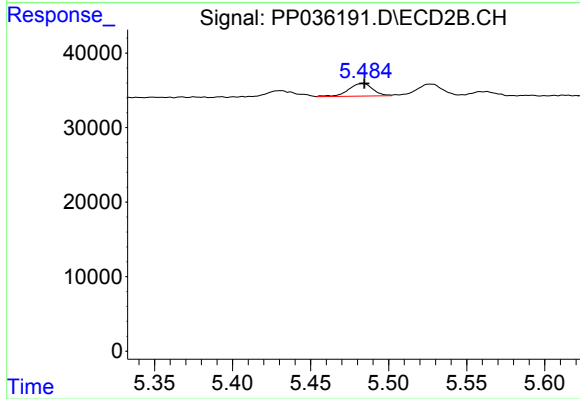

#22 AR-1248-2


R.T.: 5.484 min
Delta R.T.: 0.000 min
Response: 18291
Conc: 26.21 ng/ml

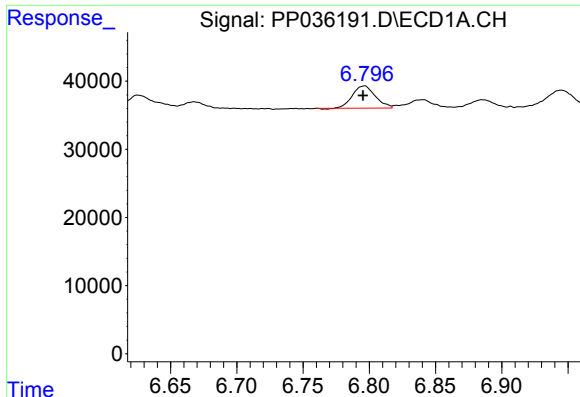

#23 AR-1248-3


R.T.: 6.797 min
Delta R.T.: 0.001 min
Response: 39421
Conc: 27.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2021

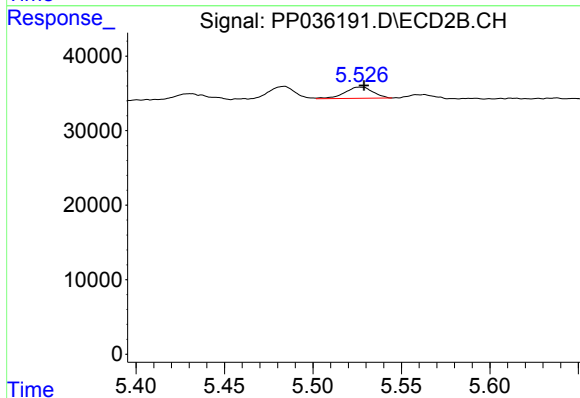


#23 AR-1248-3

R.T.: 5.526 min
Delta R.T.: -0.002 min
Response: 16605
Conc: 23.07 ng/ml

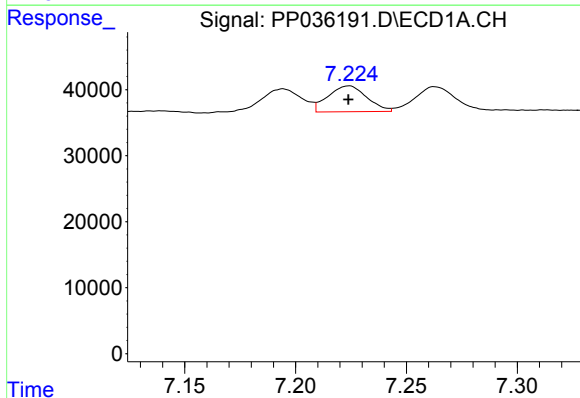


#24 AR-1248-4

R.T.: 7.224 min
Delta R.T.: 0.000 min
Response: 47708
Conc: 29.96 ng/ml

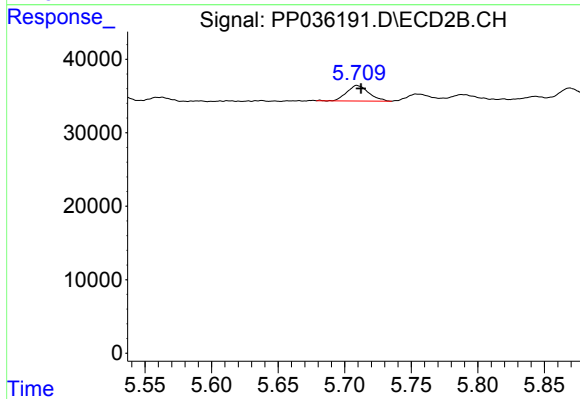

#24 AR-1248-4


R.T.: 5.709 min
Delta R.T.: -0.003 min
Response: 24364
Conc: 27.59 ng/ml

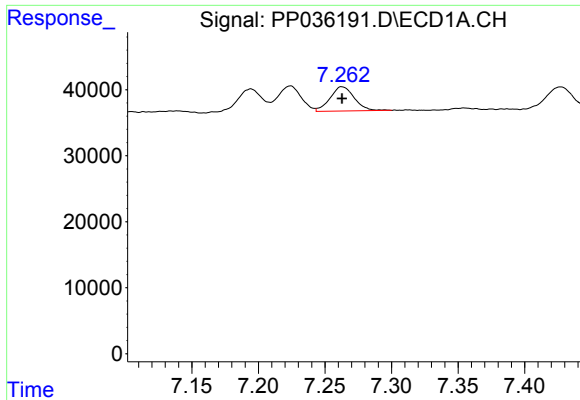

#25 AR-1248-5

R.T.: 7.263 min
Delta R.T.: 0.000 min
Response: 46627
Conc: 29.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2021

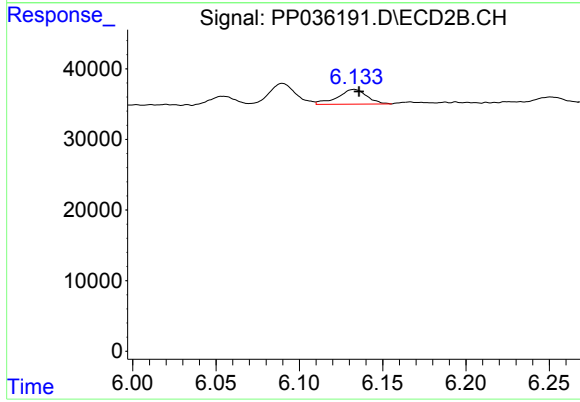

#25 AR-1248-5

R.T.: 6.133 min
Delta R.T.: -0.003 min
Response: 25691
Conc: 29.22 ng/ml