

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052621\
 Data File : PP036192.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 May 2021 9:36
 Operator : DD\AJ
 Sample : M2262-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT2-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 10:00:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 26 00:48:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.966	3.964	879593	554038	19.762	19.851
2)	SA Decachlor...	10.995	9.271	925858	497870	21.664	21.701
Target Compounds							
26)	L6 AR-1254-1	7.195	6.091	68537	34236	42.304	26.198 #
27)	L6 AR-1254-2	7.424	6.251	77338	32470	31.395	28.161
28)	L6 AR-1254-3	7.804	6.672	86153	47266	32.658	24.825
29)	L6 AR-1254-4	8.100	6.912	57743	29071	28.607	24.346
30)	L6 AR-1254-5	8.528	7.342	61245	43195	26.991	25.318



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP052621\
Data File : PP036192.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 May 2021 9:36
Operator : DD\AJ
Sample : M2262-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 71 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 10:00:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP052521.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 26 00:48:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

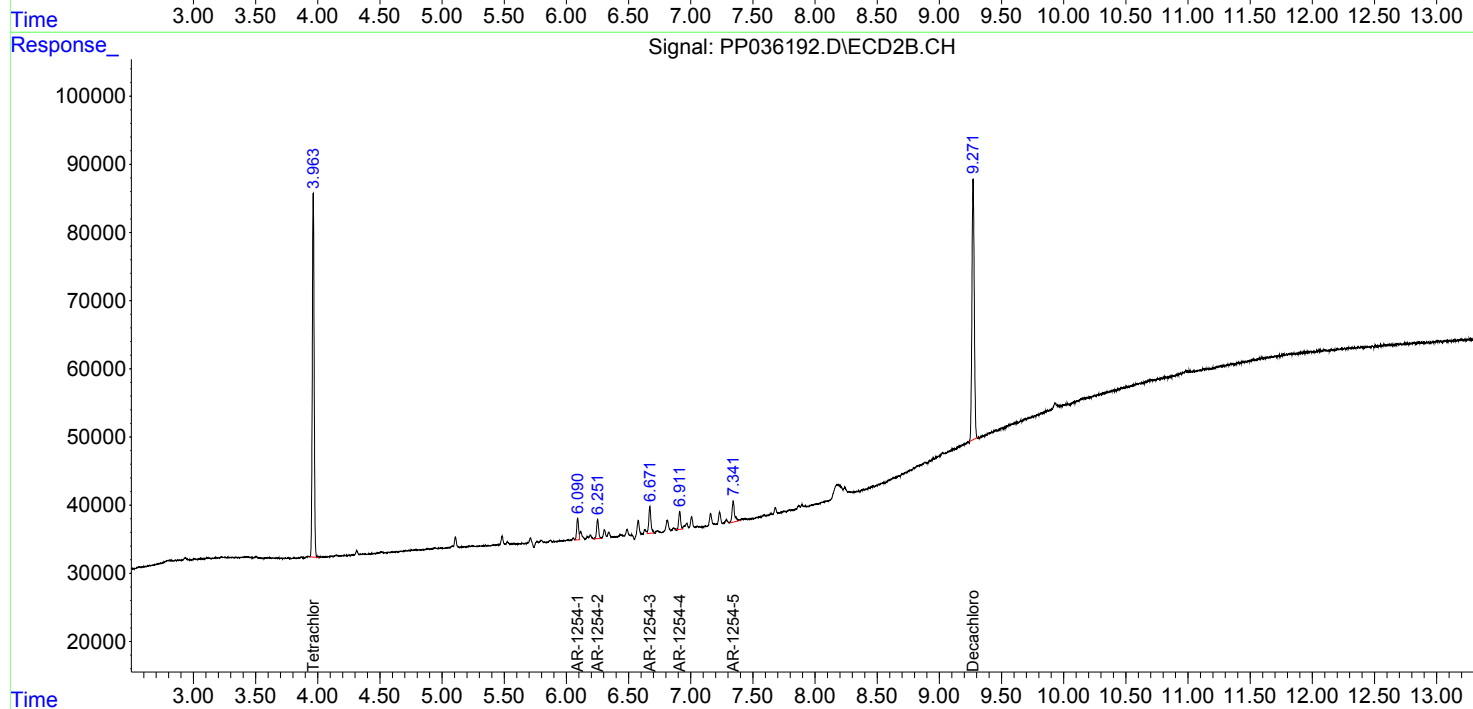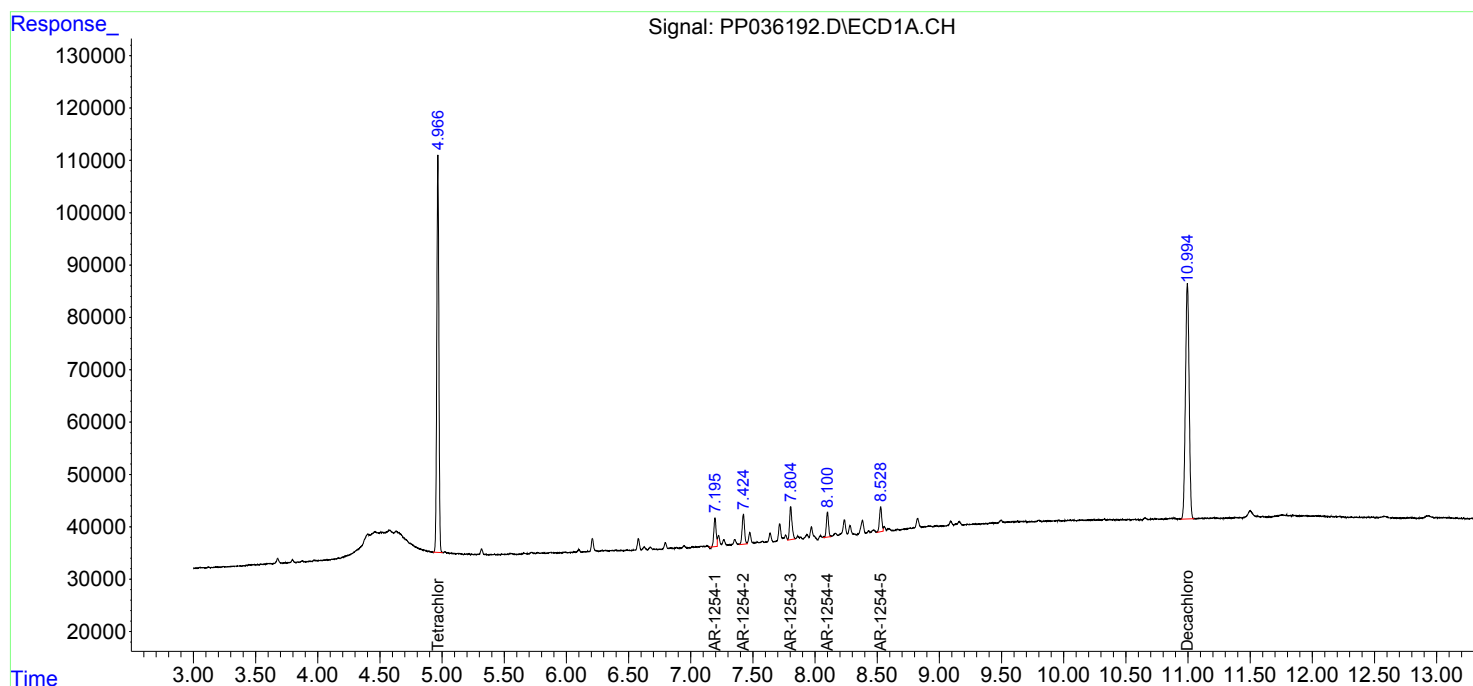


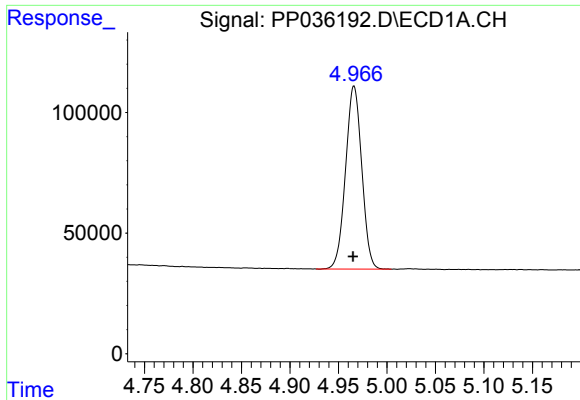

#1 Tetrachloro-m-xylene


R.T.: 4.966 min
Delta R.T.: 0.001 min
Response: 879593
Conc: 19.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2021

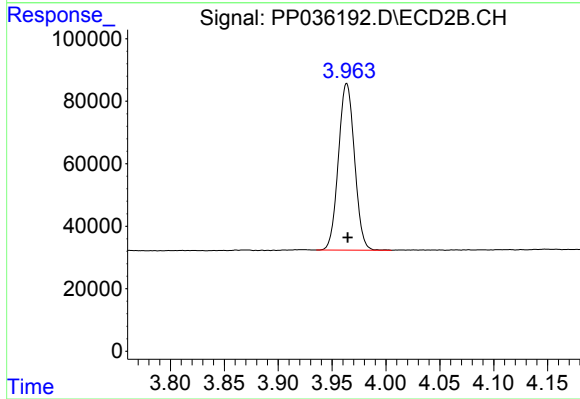


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 554038
Conc: 19.85 ng/ml

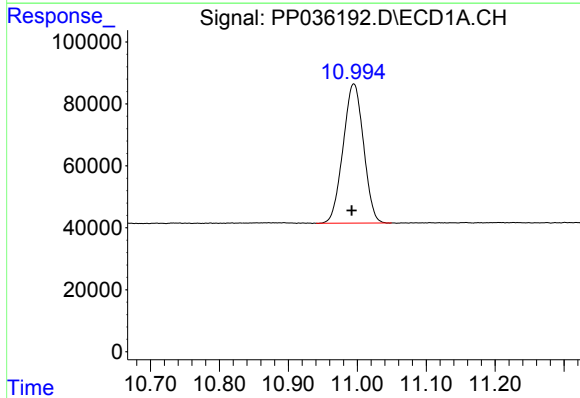


#2 Decachlorobiphenyl

R.T.: 10.995 min
Delta R.T.: 0.003 min
Response: 925858
Conc: 21.66 ng/ml

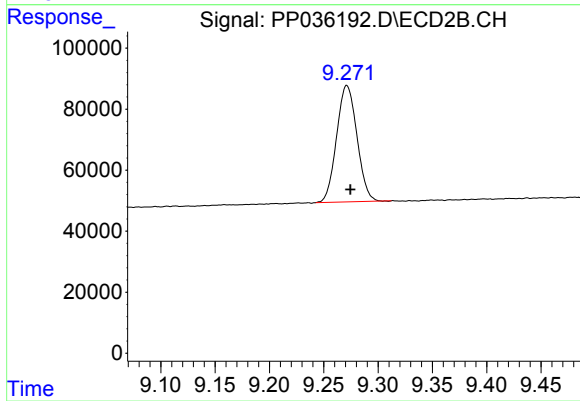

#2 Decachlorobiphenyl


R.T.: 9.271 min
Delta R.T.: -0.003 min
Response: 497870
Conc: 21.70 ng/ml

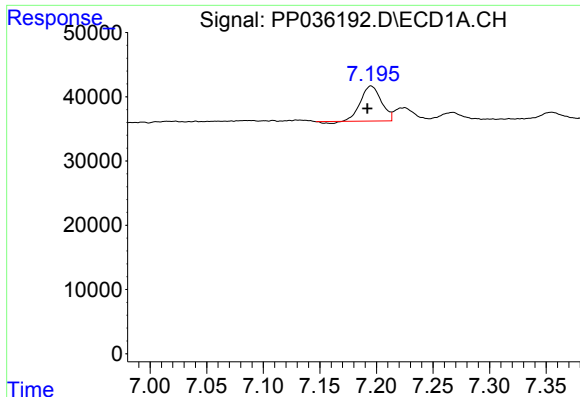

#26 AR-1254-1


R.T.: 7.195 min
Delta R.T.: 0.003 min
Response: 68537
Conc: 42.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2021

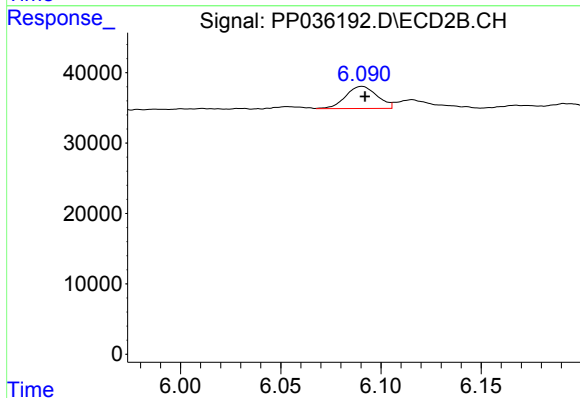


#26 AR-1254-1

R.T.: 6.091 min
Delta R.T.: -0.001 min
Response: 34236
Conc: 26.20 ng/ml

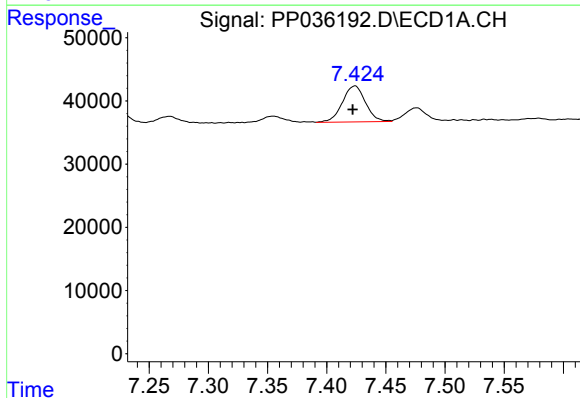


#27 AR-1254-2

R.T.: 7.424 min
Delta R.T.: 0.002 min
Response: 77338
Conc: 31.39 ng/ml

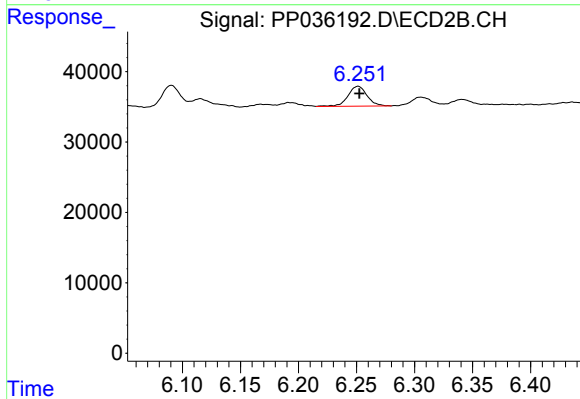

#27 AR-1254-2


R.T.: 6.251 min
Delta R.T.: -0.001 min
Response: 32470
Conc: 28.16 ng/ml

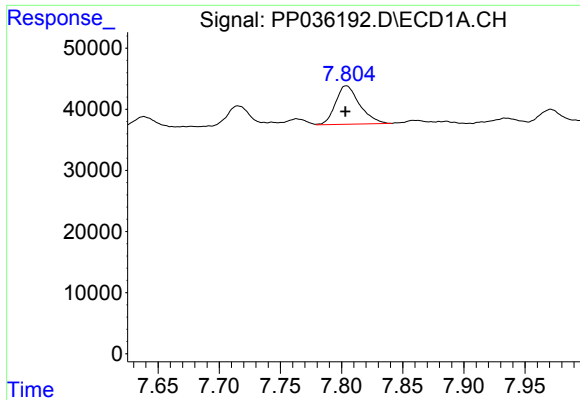

#28 AR-1254-3


R.T.: 7.804 min
Delta R.T.: 0.000 min
Response: 86153
Conc: 32.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2021

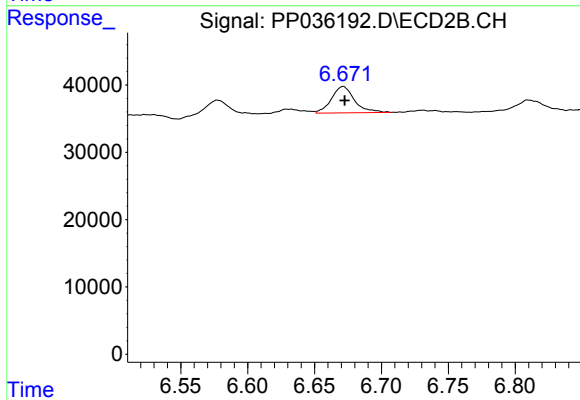


#28 AR-1254-3

R.T.: 6.672 min
Delta R.T.: -0.001 min
Response: 47266
Conc: 24.82 ng/ml

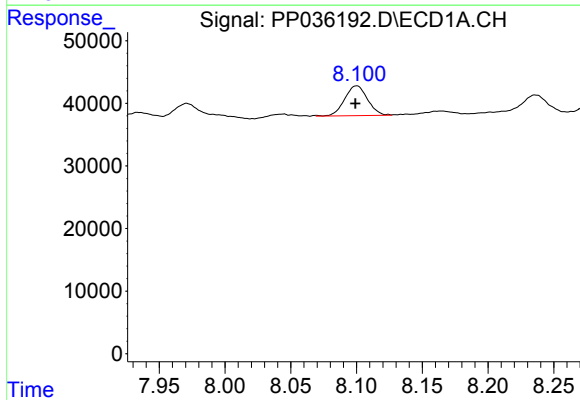


#29 AR-1254-4

R.T.: 8.100 min
Delta R.T.: 0.001 min
Response: 57743
Conc: 28.61 ng/ml

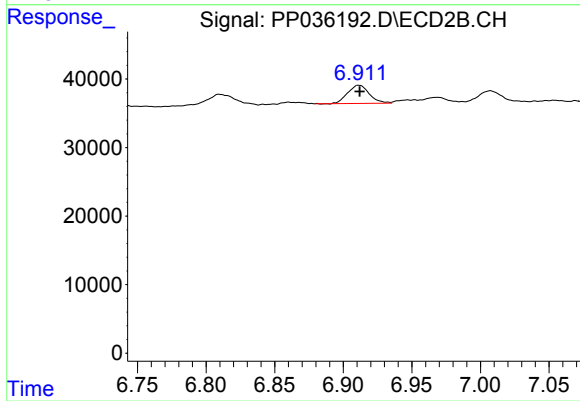

#29 AR-1254-4


R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 29071
Conc: 24.35 ng/ml

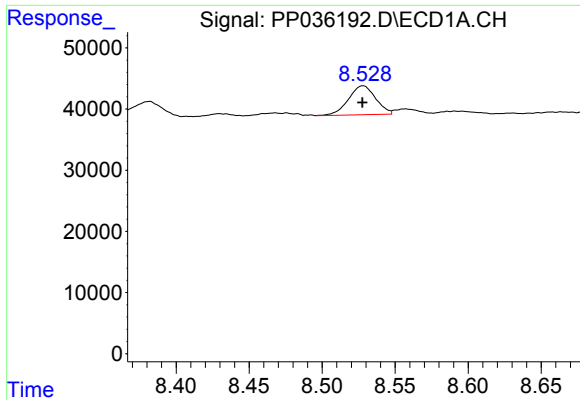

#30 AR-1254-5

R.T.: 8.528 min
Delta R.T.: 0.000 min
Response: 61245
Conc: 26.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT2-2021

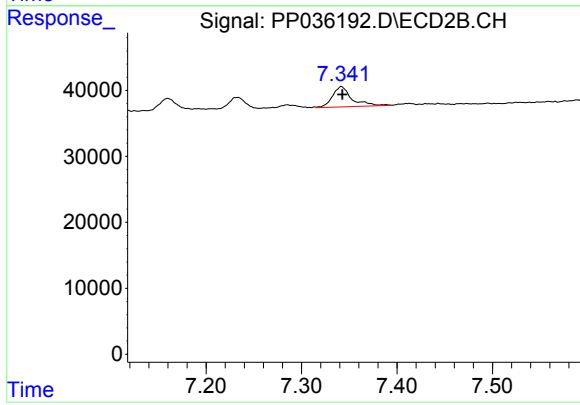

#30 AR-1254-5

R.T.: 7.342 min
Delta R.T.: -0.001 min
Response: 43195
Conc: 25.32 ng/ml